

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR090819\
Data File : PR040818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2019 14:08
Operator : SM\AJ
Sample : K4727-03DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
ECD_R
ClientSampleId :
C0AS1DL

Manual Integrations
APPROVED

Ankita
9/10/2019 8:34:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 04:57:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090619CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 11:15:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

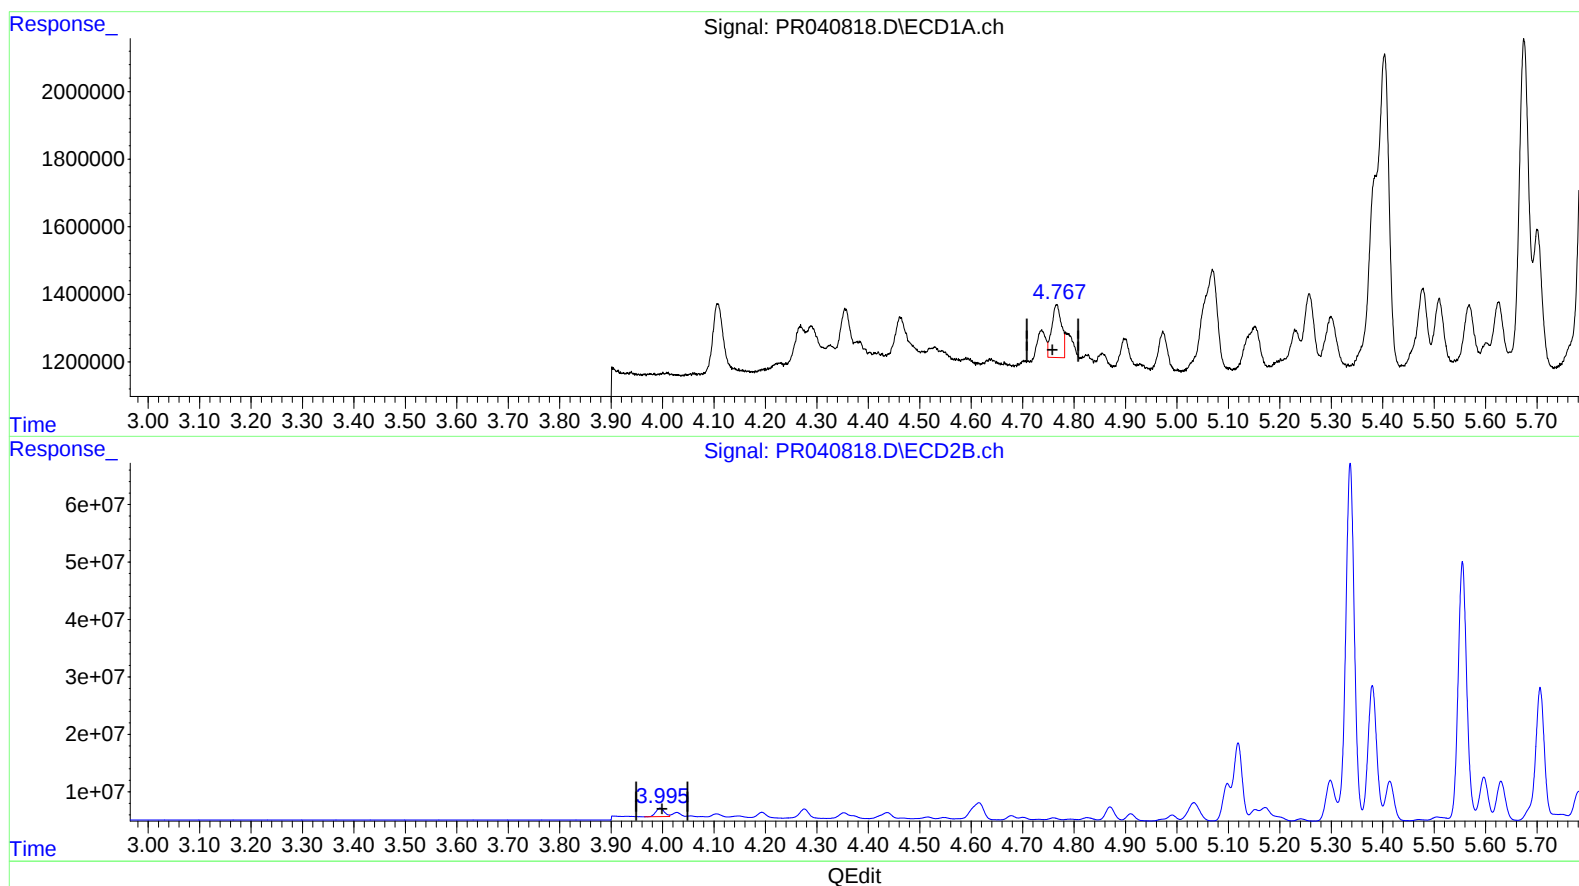

(1) Tetrachloro-m-xylene (SA)

4.767min 0.816 ng/ml m

response 2080009

(1) Tetrachloro-m-xylene #2 (SA)

3.995min 1.187 ng/ml

response 16943999

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR090819\
Data File : PR040818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2019 14:08
Operator : SM\AJ
Sample : K4727-03DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_R
ClientSampleId :
C0AS1DL

Manual Integrations
APPROVED

Ankita
9/10/2019 8:34:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 03:07:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090619CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 06 11:15:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

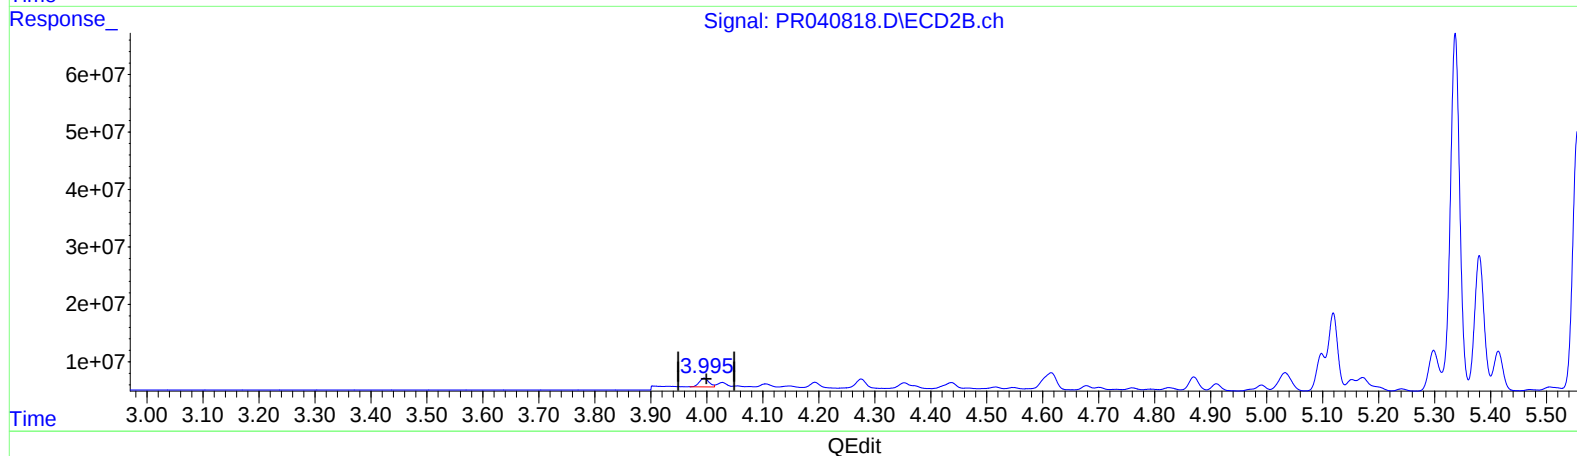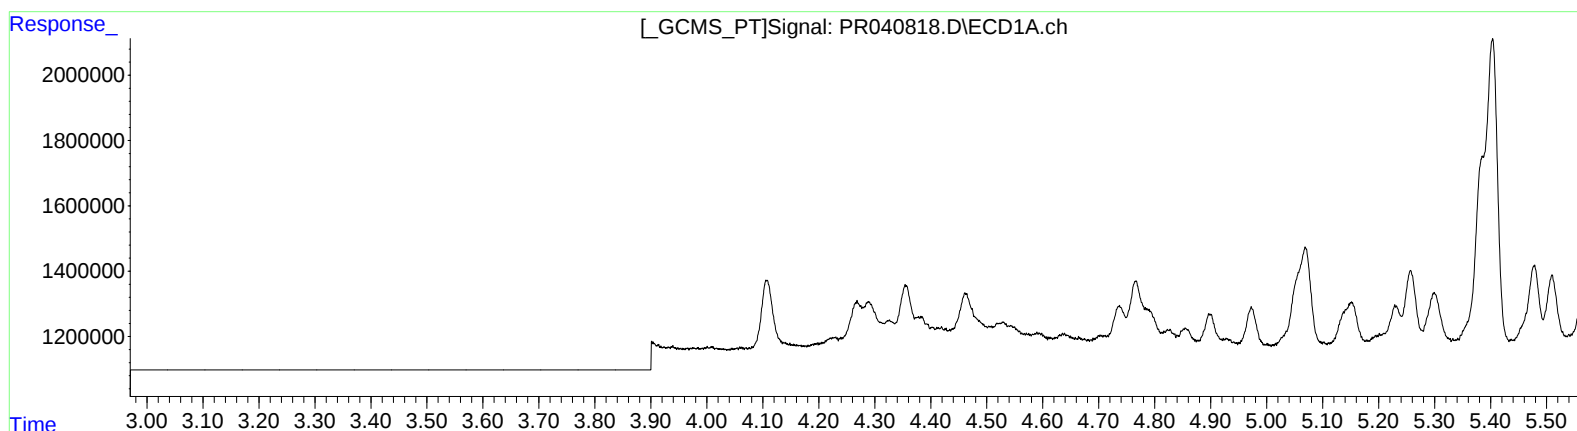

(1) Tetrachloro-m-xylene (SA)

0.000min 0.000 ng/ml

response 0

(1) Tetrachloro-m-xylene #2 (SA)

3.995min 1.265 ng/ml

response 18053951

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR090819\
 Data File : PR040818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2019 14:08
 Operator : SM\AJ
 Sample : K4727-03DL 50X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_R
 Client Sampled :
 C0AS1DL

Manual Integrations
 APPROVED

Ankita
 9/10/2019 8:34:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 04:57:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR090619CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 06 11:15:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.767	3.995	2080009	16943999	0.816m)	1.187 #) A309/10/19
2) SA Decachlor...	10.720	9.134	9396967	31781593	2.737	2.834

Target Compounds

26) L6 AR-1254-1	6.801	5.911	584.9E6	2192.4E6	4983.382	4178.682
27) L6 AR-1254-2	7.019	6.058	978.5E6	2227.3E6	5312.918	4764.370
28) L6 AR-1254-3	7.388	6.467	1191.4E6	4047.0E6	6106.870	5227.911
29) L6 AR-1254-4	7.674	6.695	936.2E6	2883.5E6	6391.557	5466.563
30) L6 AR-1254-5	8.094	7.117	1111.5E6	3965.8E6	7248.015	5987.983

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.