

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091419\
 Data File : PR041088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Sep 2019 08:31
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_R
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 00:45:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 10 13:01:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

28)	L6	AR-1254-3	0.000	6.460	0	4449947	N.D.	5.915 #
29)	L6	AR-1254-4	0.000	6.688	0	2516948	N.D.	4.813 #
31)	L7	AR-1260-1	0.000	6.591	0	6820924	N.D.	13.389 #
38)	L8	AR-1262-3	0.000	7.959	0	9478659	N.D.	15.696 #
39)	L8	AR-1262-4	0.000	8.006	0	4703546	N.D.	4.218 #
40)	L8	AR-1262-5	0.000	8.465f	0	5658694	N.D.	10.829 #
41)	L9	AR-1268-1	0.000	7.959	0	9478659	N.D.	5.911 #
42)	L9	AR-1268-2	0.000	8.006	0	4703546	N.D.	3.147 #
43)	L9	AR-1268-3	0.000	8.209	0	627128	N.D.	0.502 #
44)	L9	AR-1268-4	0.000	8.465f	0	5658694	N.D.	10.866 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR091419\
Data File : PR041088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Sep 2019 08:31
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_R
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 00:45:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR091019CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 10 13:01:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

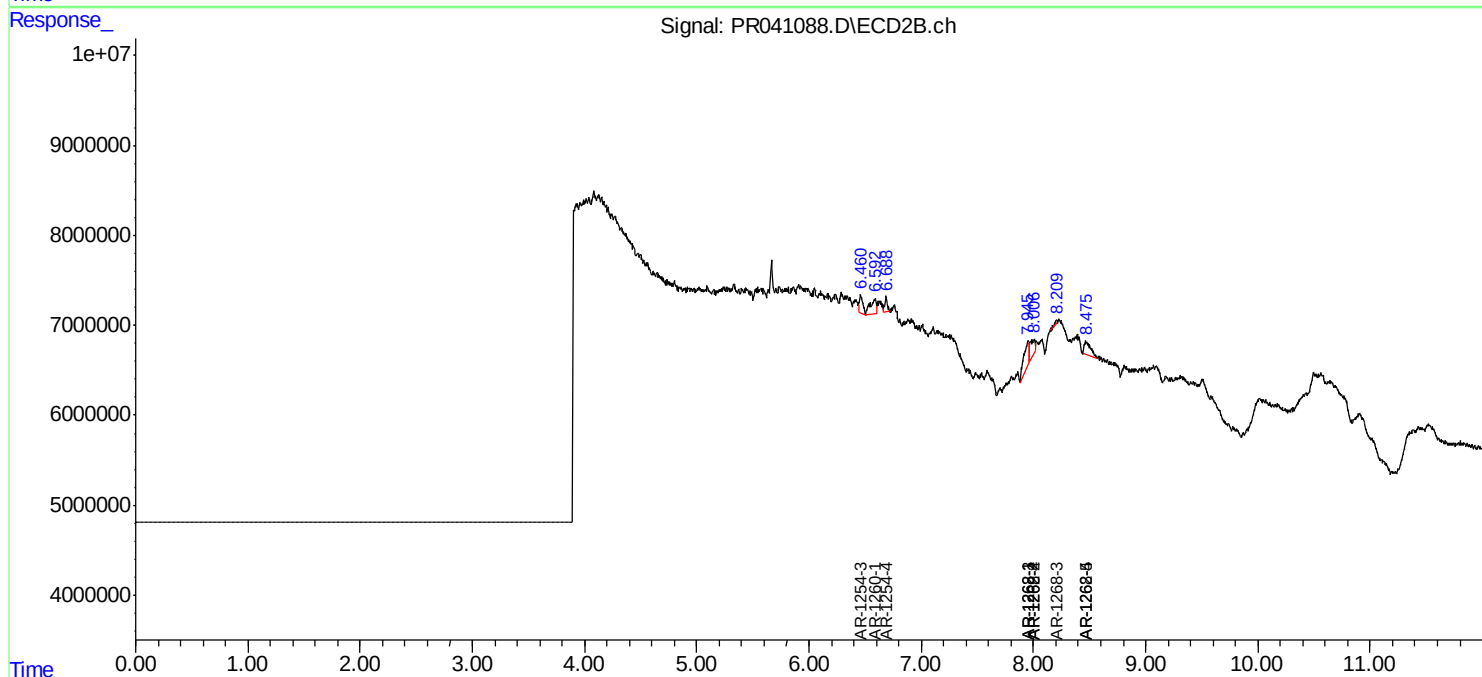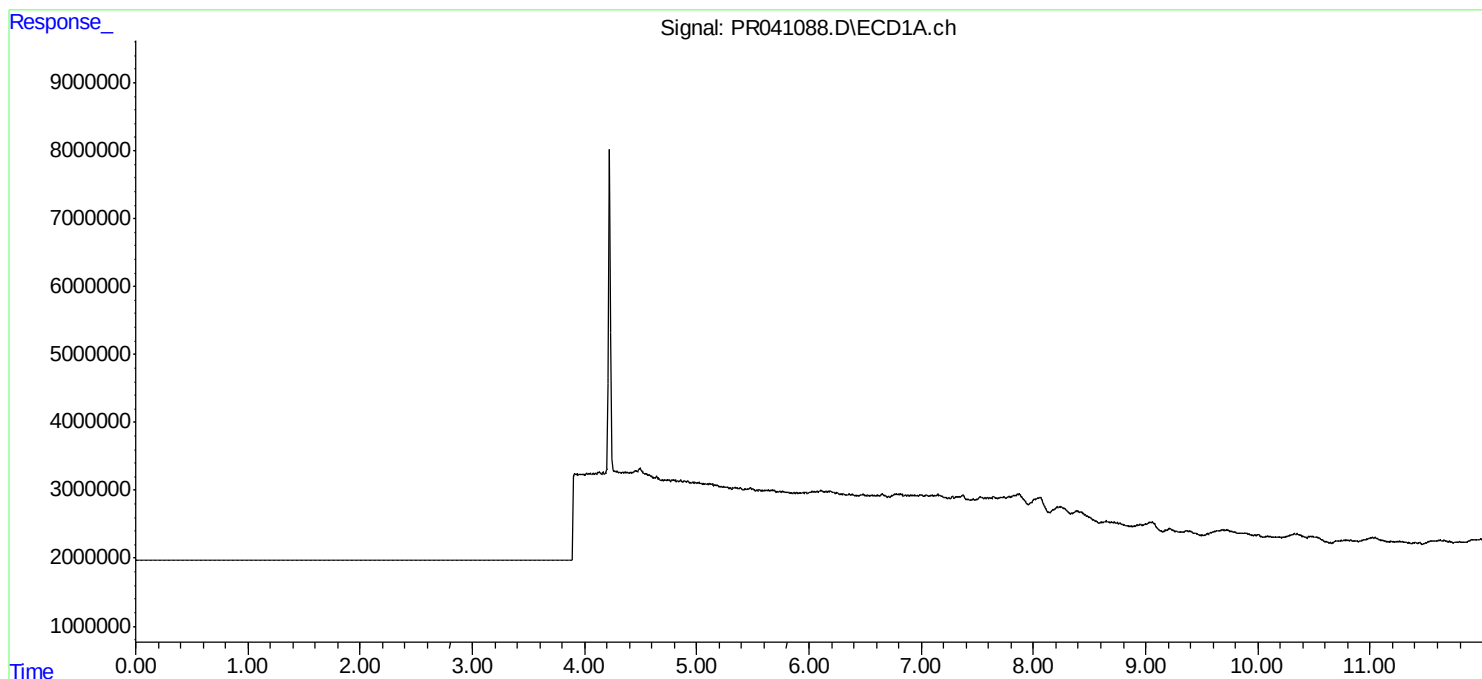


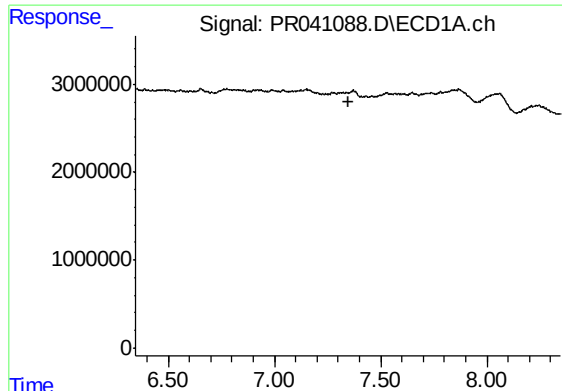

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 7.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

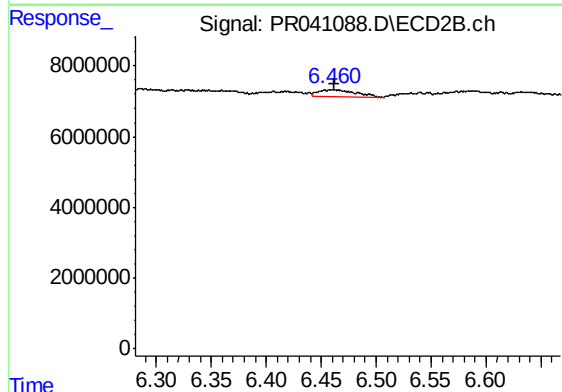


#28 AR-1254-3

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 4449947
Conc: 5.92 ng/ml

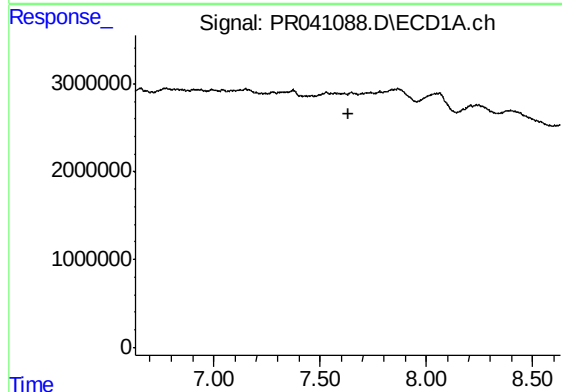


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.631 min
Response: 0
Conc: N.D.

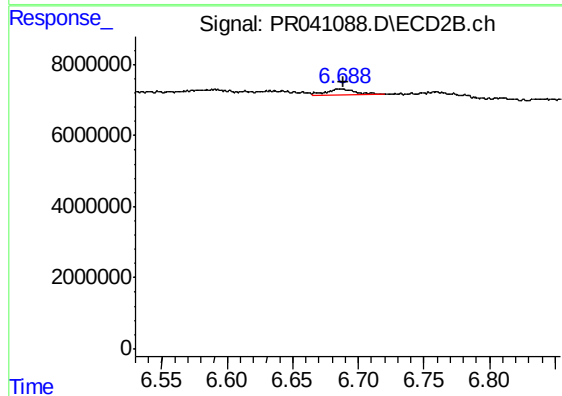

#29 AR-1254-4


R.T.: 6.688 min
Delta R.T.: -0.001 min
Response: 2516948
Conc: 4.81 ng/ml

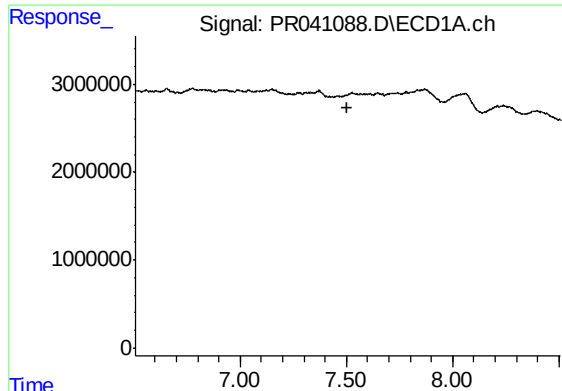

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

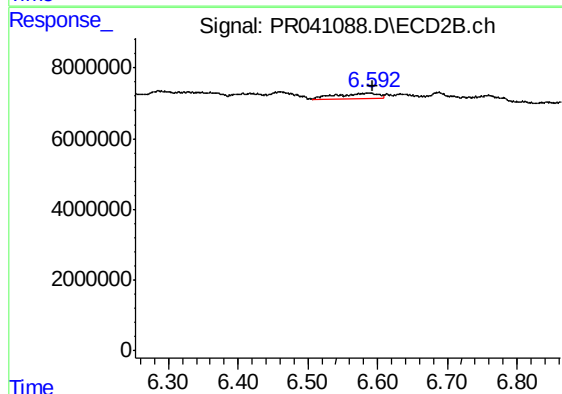


#31 AR-1260-1

R.T.: 6.591 min
Delta R.T.: -0.002 min
Response: 6820924
Conc: 13.39 ng/ml

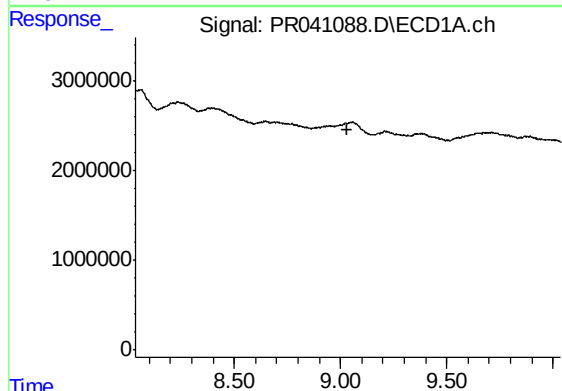


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.035 min
Response: 0
Conc: N.D.

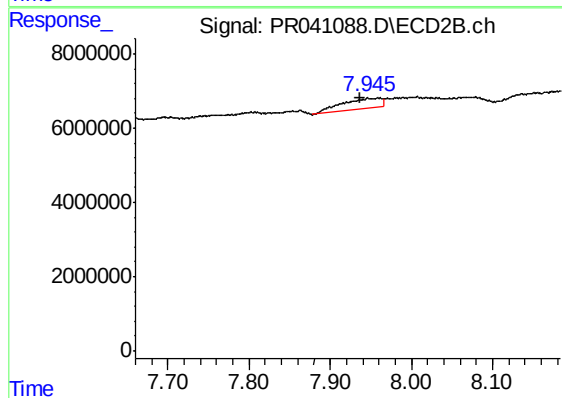

#38 AR-1262-3


R.T.: 7.959 min
Delta R.T.: 0.022 min
Response: 9478659
Conc: 15.70 ng/ml

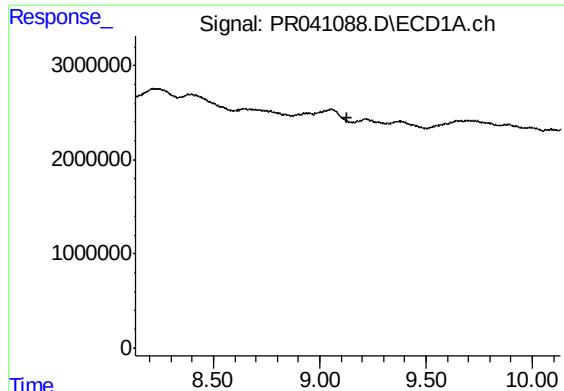

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

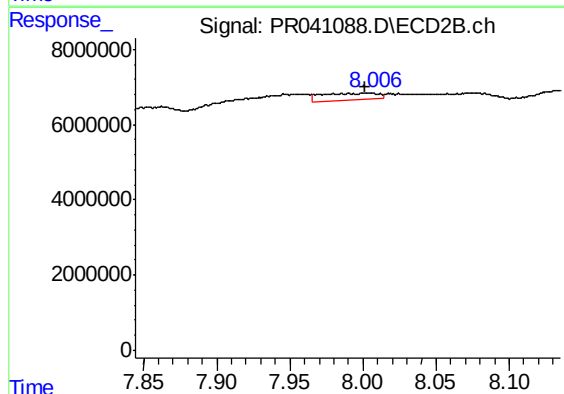


#39 AR-1262-4

R.T.: 8.006 min
Delta R.T.: 0.004 min
Response: 4703546
Conc: 4.22 ng/ml

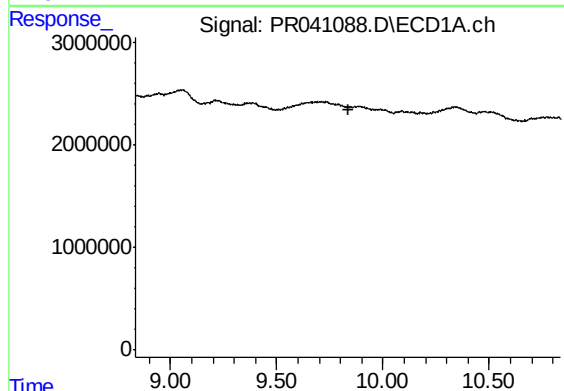


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.835 min
Response: 0
Conc: N.D.

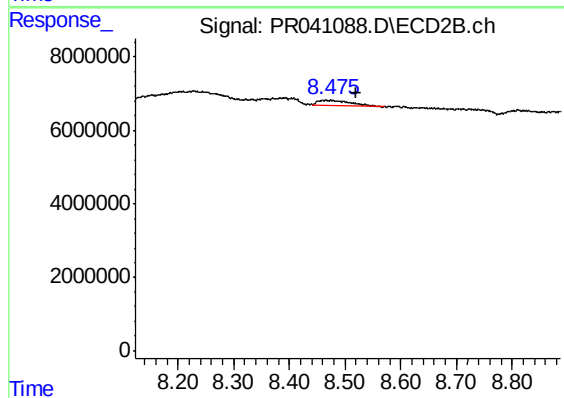

#40 AR-1262-5


R.T.: 8.465 min
Delta R.T.: -0.055 min
Response: 5658694
Conc: 10.83 ng/ml

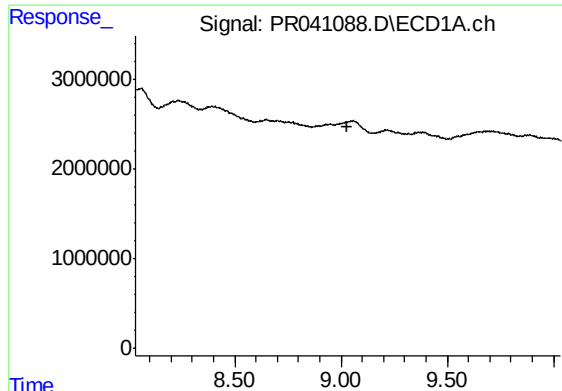

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.032 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

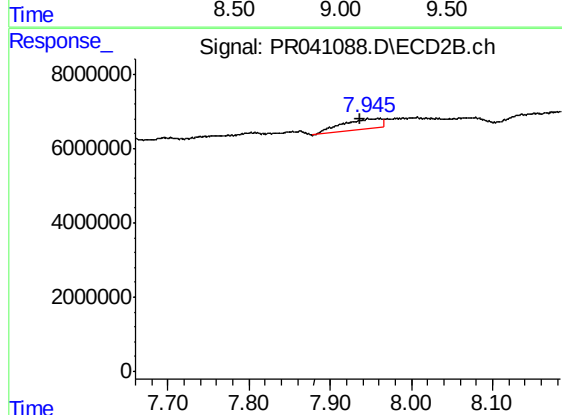


#41 AR-1268-1

R.T.: 7.959 min
Delta R.T.: 0.022 min
Response: 9478659
Conc: 5.91 ng/ml

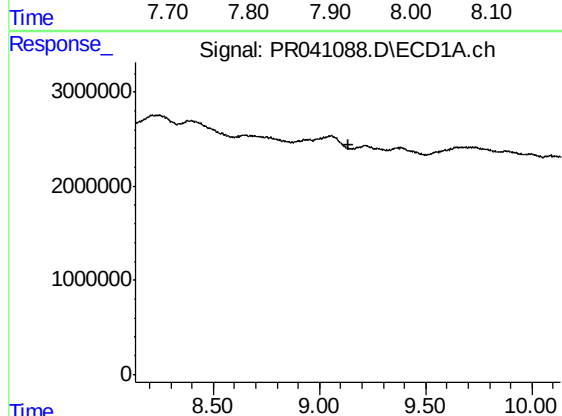


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.134 min
Response: 0
Conc: N.D.

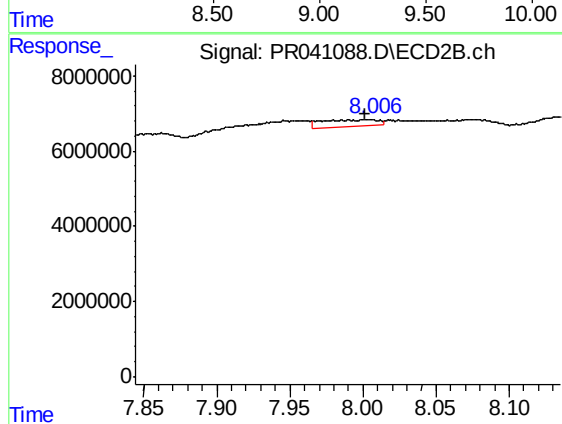

#42 AR-1268-2


R.T.: 8.006 min
Delta R.T.: 0.004 min
Response: 4703546
Conc: 3.15 ng/ml

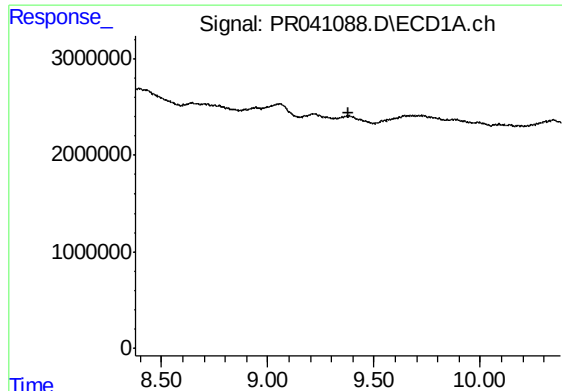

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 9.378 min
Response: 0
Conc: N.D.

Instrument :
ECD_R
ClientSampleId :
HEXANE

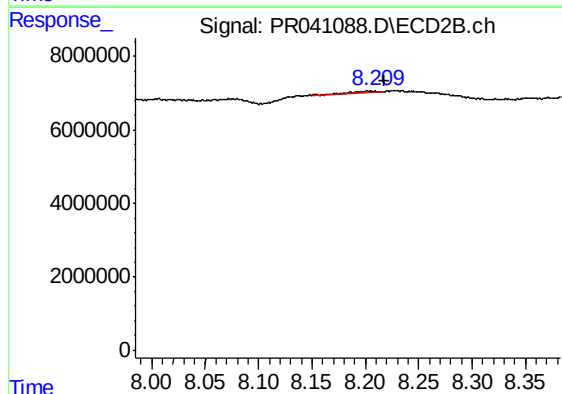


#43 AR-1268-3

R.T.: 8.209 min
Delta R.T.: -0.009 min
Response: 627128
Conc: 0.50 ng/ml

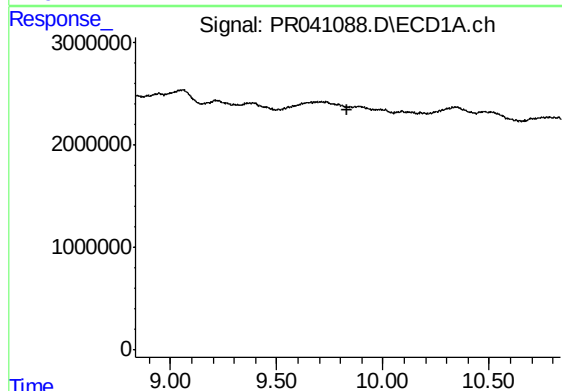

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.835 min
Response: 0
Conc: N.D.

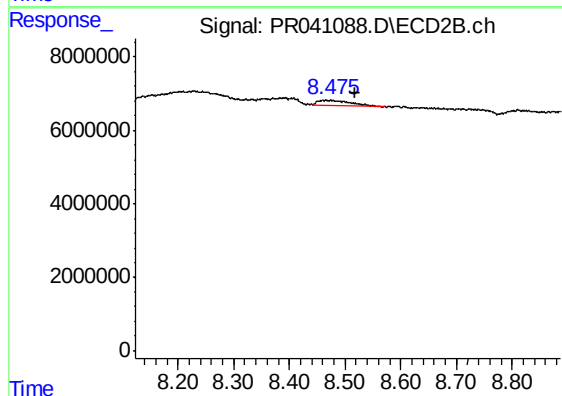

#44 AR-1268-4

R.T.: 8.465 min
Delta R.T.: -0.053 min
Response: 5658694
Conc: 10.87 ng/ml