

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR122818\  
Data File : PR035119.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Dec 2018 22:28  
Operator : SM\SJ  
Sample : J6428-14DL2 50X  
Misc :  
ALS Vial : 47 Sample Multiplier: 1



Instrument :  
ECD\_R  
ClientSampleId :  
A41W7DL2

Manual Integrations  
APPROVED

Sohil  
1/3/2019 2:43:15 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 29 03:20:00 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR121818CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Dec 18 01:56:32 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

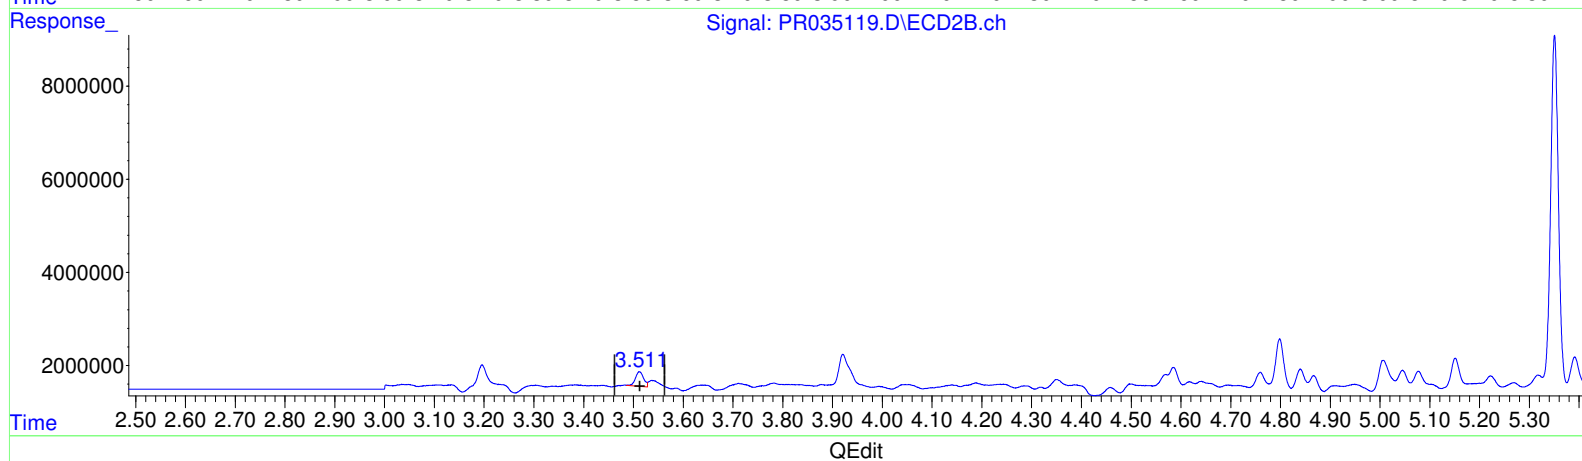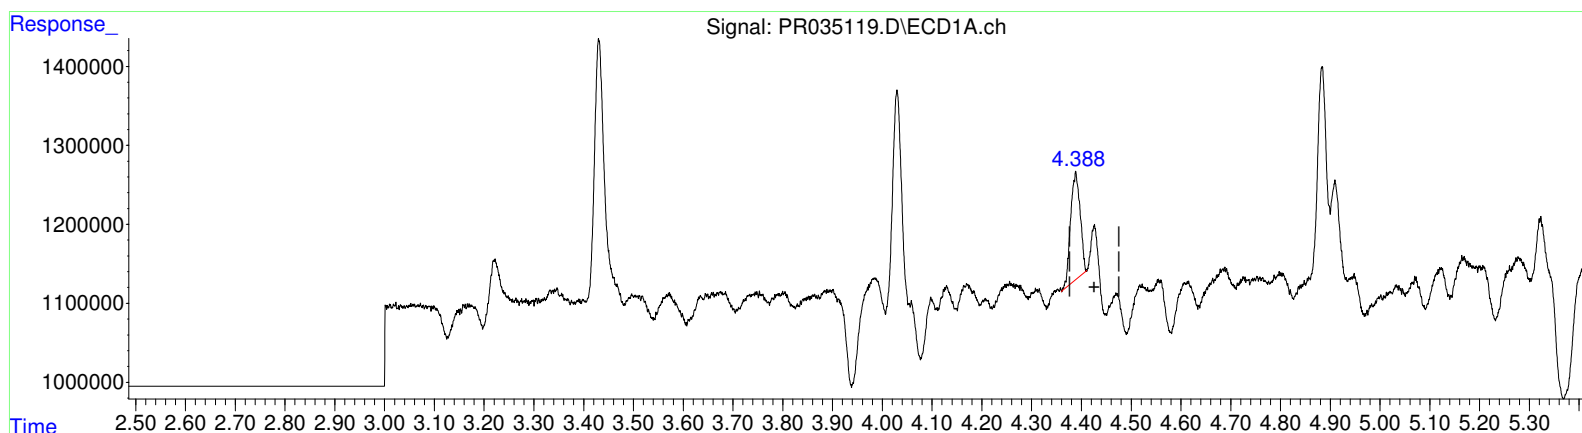

(1) Tetrachloro-m-xylene (SA)

4.389min 0.931 ng/ml

response 1811480

(1) Tetrachloro-m-xylene #2 (SA)

3.512min 1.016 ng/ml

response 3542462

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR122818\  
Data File : PR035119.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 Dec 2018 22:28  
Operator : SM\SJ  
Sample : J6428-14DL2 50X  
Misc :  
ALS Vial : 47 Sample Multiplier: 1


Instrument :  
ECD\_R  
ClientSampleId :  
A41W7DL2

Manual Integrations  
APPROVED

Sohil  
1/3/2019 2:43:15 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 29 03:20:00 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR121818CLP.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Dec 18 01:56:32 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

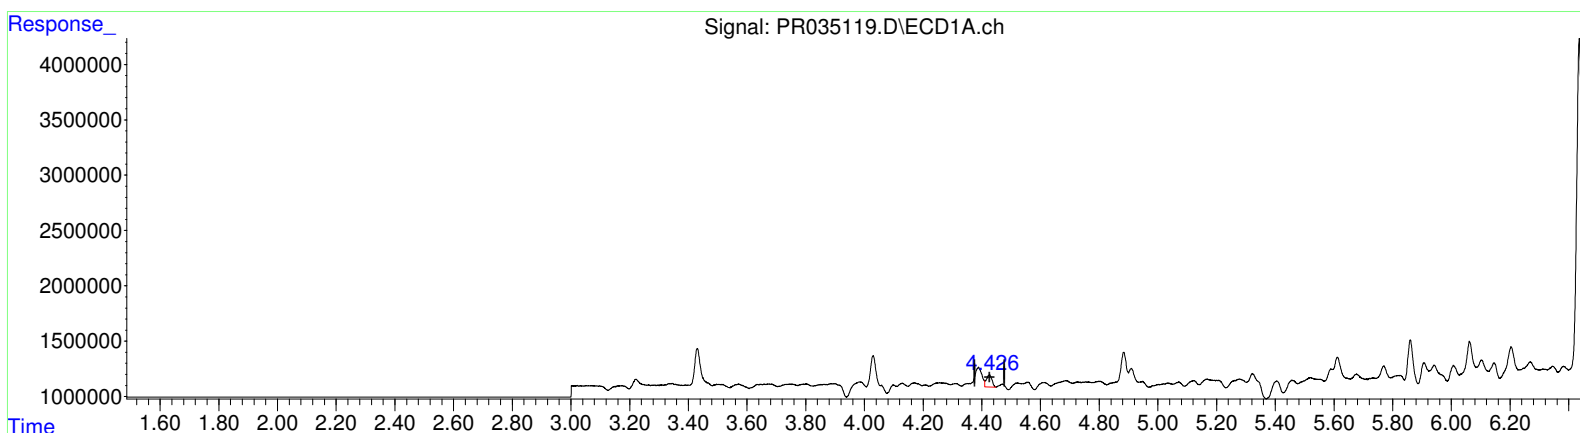

(1) Tetrachloro-m-xylene (SA)

4.426min 0.739 ng/ml m

response 1436949

(1) Tetrachloro-m-xylene #2 (SA)

3.512min 1.016 ng/ml

response 3542462

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Data\PR122818\  
 Data File : PR035119.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 Dec 2018 22:28  
 Operator : SM\SJ  
 Sample : J6428-14DL2 50X  
 Misc :  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 ECD\_R  
 ClientSampleId :  
 A41W7DL2

Manual Integrations  
 APPROVED

Sohil  
 1/3/2019 2:43:15 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 29 03:20:00 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_R\Method\PR121818CLP.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Dec 18 01:56:32 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2  
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml    | ng/ml    |
|-----------------------------|--------|-------|---------|---------|----------|----------|
| -----                       |        |       |         |         |          |          |
| System Monitoring Compounds |        |       |         |         |          |          |
| 1) SA Tetrachlo...          | 4.426  | 3.512 | 1436949 | 3542462 | 0.739m   | 1.016 #  |
| 2) SA Decachlor...          | 10.103 | 8.397 | 3344896 | 5793503 | 1.701    | 1.318    |
| Target Compounds            |        |       |         |         |          |          |
| 31) L7 AR-1260-1            | 7.179  | 6.018 | 143.2E6 | 325.9E6 | 1523.205 | 1516.122 |
| 32) L7 AR-1260-2            | 7.435  | 6.204 | 183.7E6 | 470.6E6 | 1582.291 | 1729.407 |
| 33) L7 AR-1260-3            | 7.719  | 6.354 | 219.4E6 | 364.2E6 | 1572.222 | 1467.011 |
| 34) L7 AR-1260-4            | 8.017  | 6.819 | 116.5E6 | 232.3E6 | 1348.426 | 1358.552 |
| 35) L7 AR-1260-5            | 8.334  | 7.060 | 267.4E6 | 686.6E6 | 1480.771 | 1419.682 |
| -----                       |        |       |         |         |          |          |

) 53  
 12/28/18

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.