

Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
 Data File : PE016879.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 3 Oct 2017 15:27
 Operator : UA/AJ
 Sample : I5432-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 FK-BPM-01-E7-E8-F7-F8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 16:13:00 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 02 15:22:58 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds							
4) S 2,4-DCAA	10.064	10.643	20674	-6365	223.595	N.D.	#
Target Compounds							
1) T Dalapon	2.856	0.000	17145	0	73.020	N.D.	#
5) T DICAMBA	10.064	0.000	20674	0	49.297	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
Data File : PE016879.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 3 Oct 2017 15:27
Operator : UA/AJ
Sample : I5432-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
FK-BPM-01-E7-E8-F7-F8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 16:13:00 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
Quant Title : 8080.M
QLast Update : Mon Oct 02 15:22:58 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

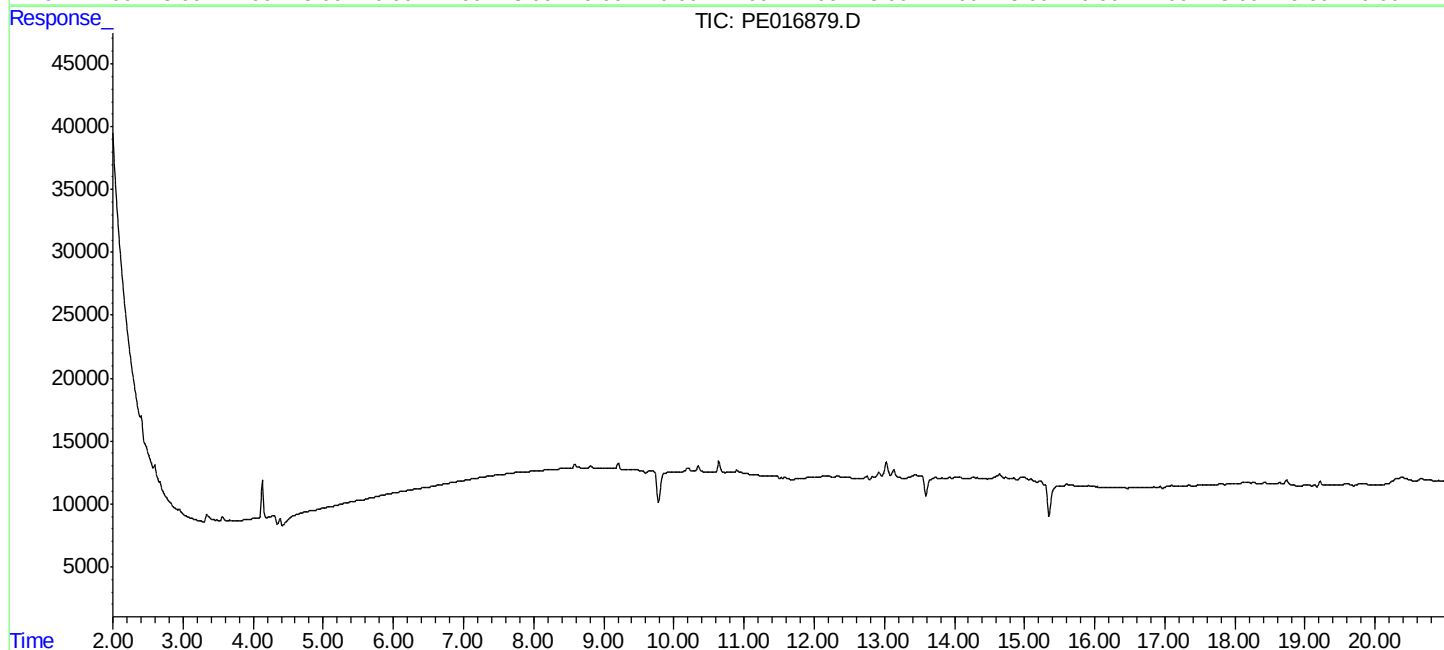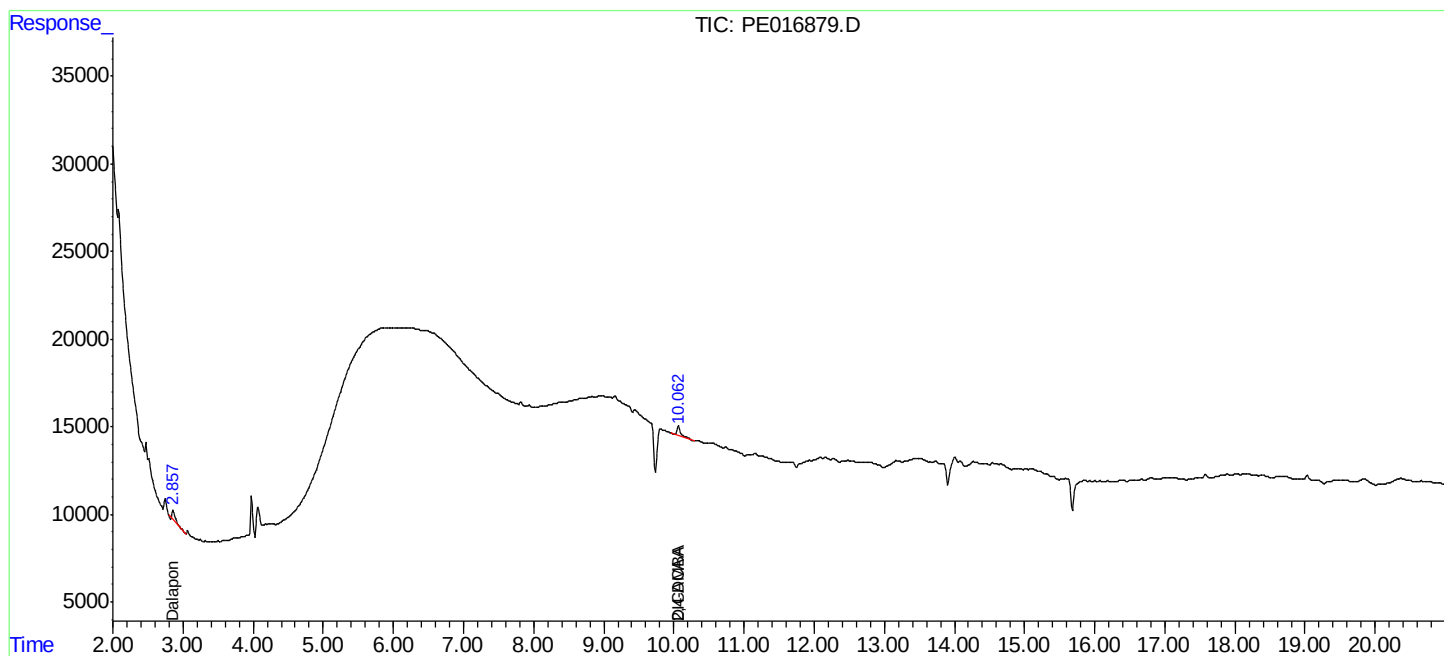


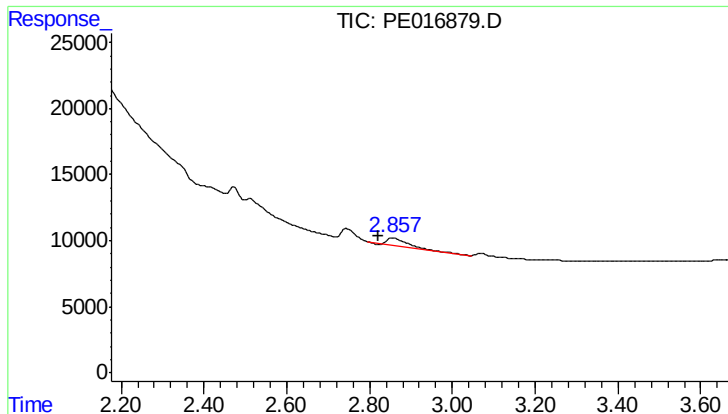

#1 Dalapon


R.T.: 2.856 min
Delta R.T.: 0.033 min
Response: 17145
Conc: 73.02 ng/ml

Instrument :
ECD_E
ClientSampleId :
FK-BPM-01-E7-E8-F7-F8

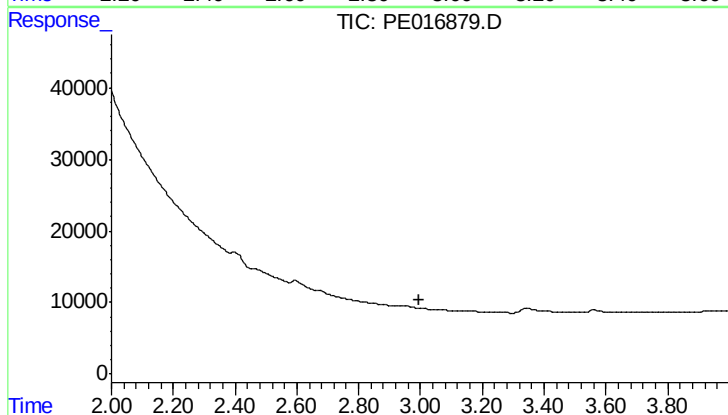


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.998 min
Response: 0
Conc: N.D.

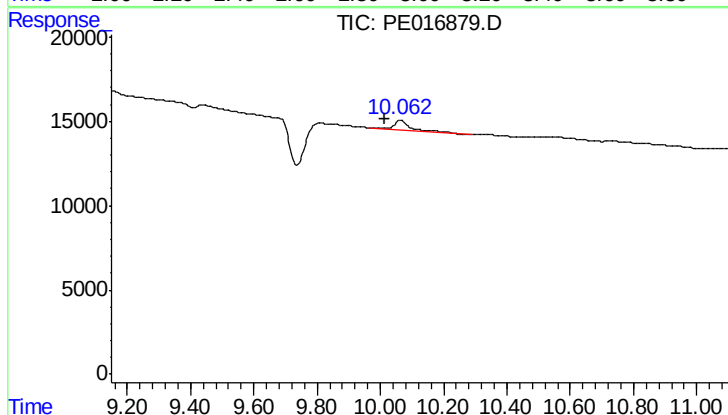


#4 2,4-DCAA

R.T.: 10.064 min
Delta R.T.: 0.052 min
Response: 20674
Conc: 223.60 ng/ml

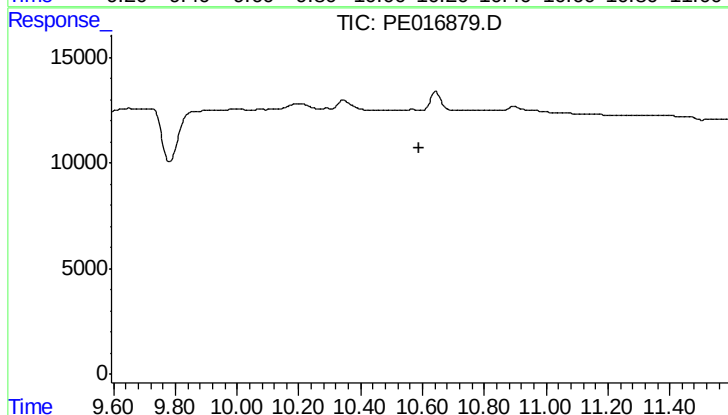

#4 2,4-DCAA


R.T.: 10.643 min
Delta R.T.: 0.051 min
Response: -6365
Conc: N.D.

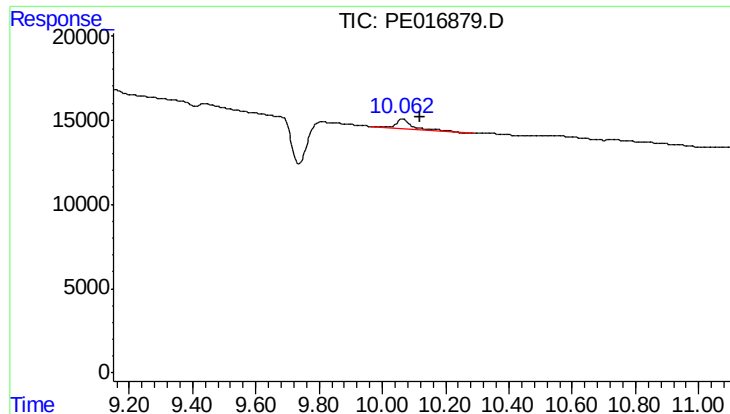

#5 DICAMBA

R.T.: 10.064 min
Delta R.T.: -0.054 min
Response: 20674
Conc: 49.30 ng/ml

Instrument :
ECD_E
ClientSampleId :
FK-BPM-01-E7-E8-F7-F8

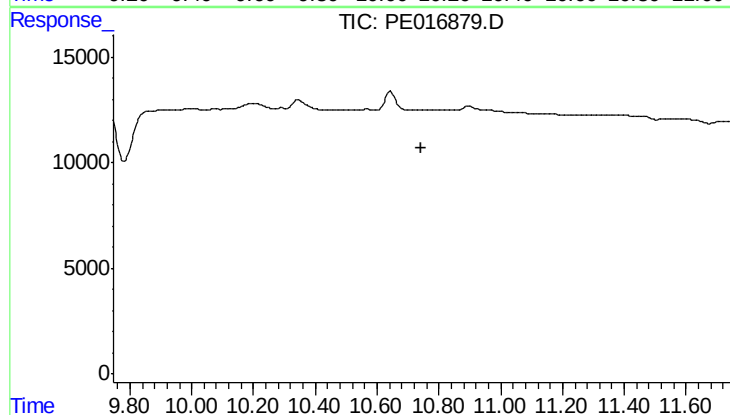

#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 10.744 min
Response: 0
Conc: N.D.