

Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
 Data File : PE016912.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 4 Oct 2017 7:39
 Operator : UA/AJ
 Sample : I5563-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 NYSEG-PH4-SB-ESMI-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:37:50 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 04 13:20:47 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x 0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	10.058	0.000	4971	0	51.731	N.D.	#
Target Compounds								
3) T	4-Nitroph...	0.000	9.964	0	328493	N.D.	2229.355	#
5) T	DICAMBA	10.207	0.000	9225	0	21.453	N.D.	#
9) T	2,4-D	11.658	0.000	73191	0	452.098	N.D.	#
10) T	Pentachlo...	0.000	13.064	0	49461	N.D.	21.309	#
11) T	2,4,5-TP ...	12.719	0.000	31726	0	55.822	N.D.	#
12) T	2,4,5-T	13.199	0.000	64252	0	99.796	N.D.	#
13) T	2,4-DB	0.000	14.466	0	32513	N.D.	250.956	#
14) T	DINOSEB	0.000	14.348	0	78043	N.D.	88.102	#
15) T	Picloram	14.792	0.000	18739	0	17.378	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
Data File : PE016912.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 4 Oct 2017 7:39
Operator : UA/AJ
Sample : I5563-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:37:50 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
Quant Title : 8080.M
QLast Update : Wed Oct 04 13:20:47 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

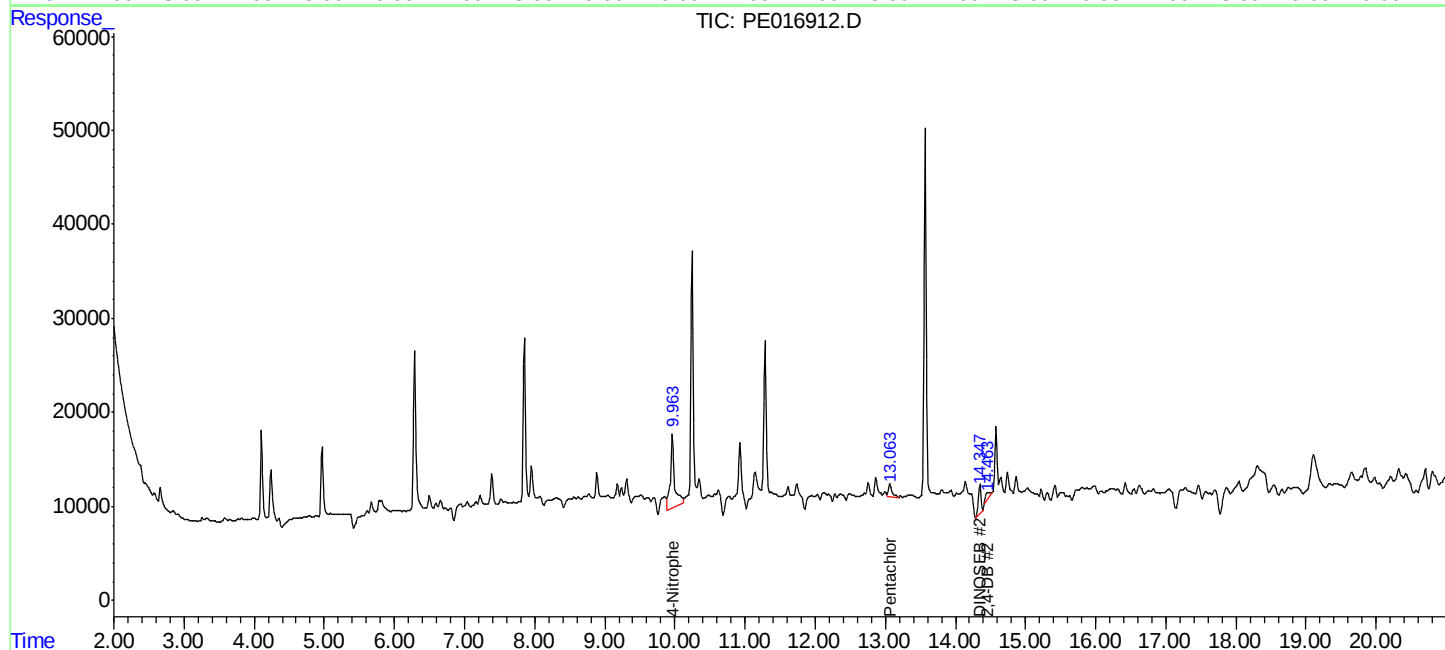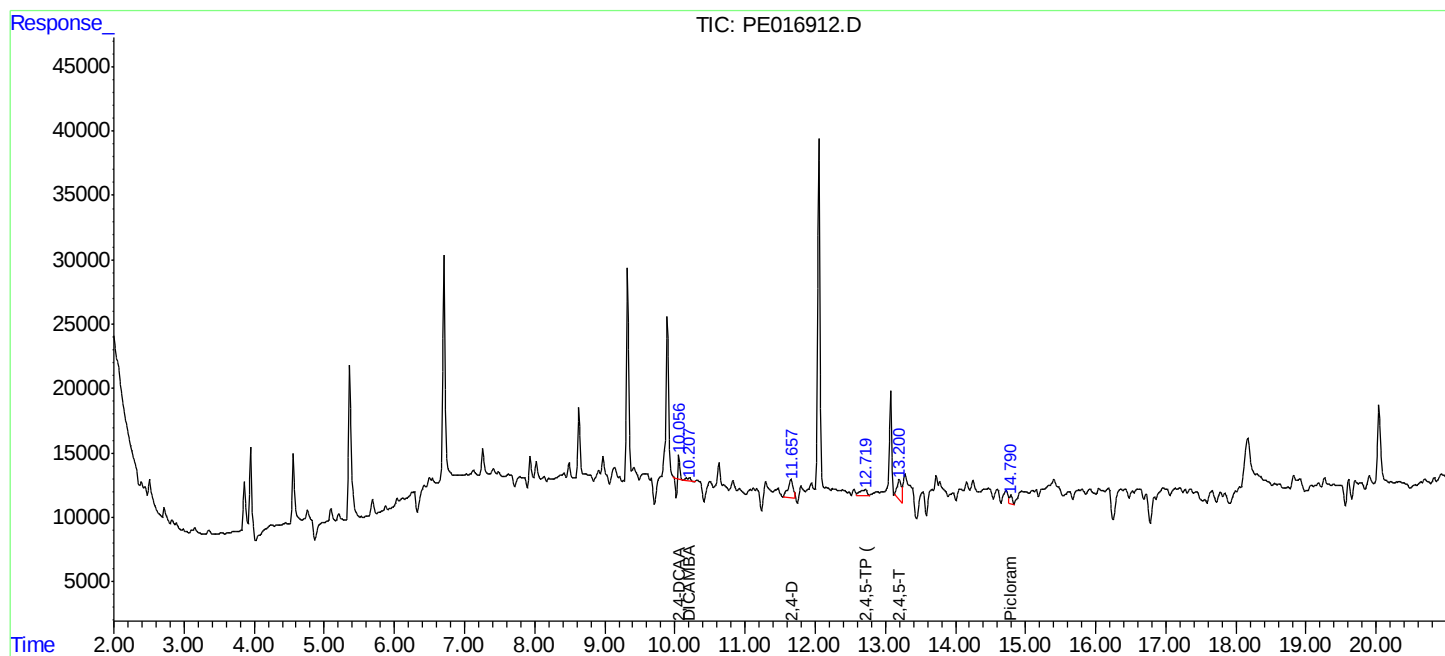


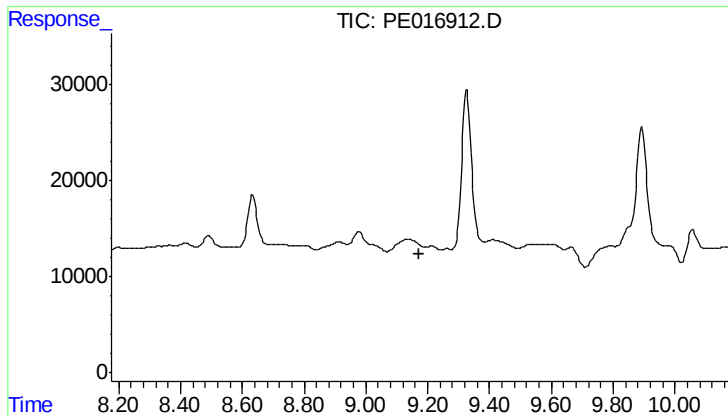

#3 4-Nitrophenol


R.T.: 0.000 min
 Exp R.T.: 9.174 min
 Response: 0
 Conc: N.D.

Instrument :
 ECD_E
 ClientSampleId :
 NYSEG-PH4-SB-ESMI-4

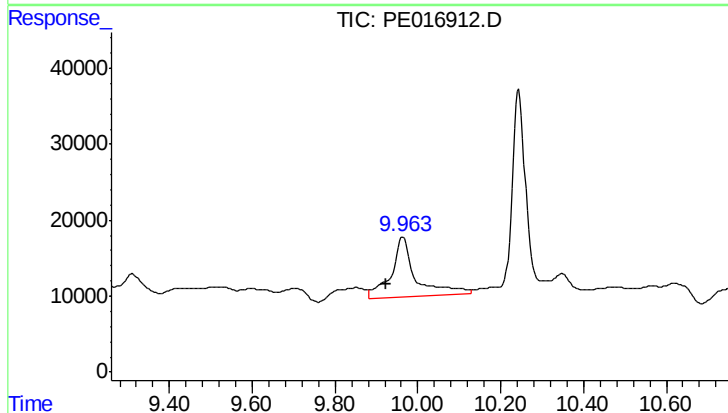


#3 4-Nitrophenol

R.T.: 9.964 min
 Delta R.T.: 0.040 min
 Response: 328493
 Conc: 2229.35 ng/ml

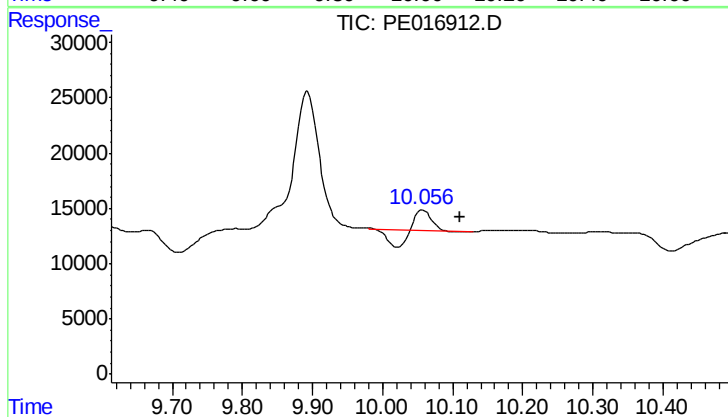


#4 2,4-DCAA

R.T.: 10.058 min
 Delta R.T.: -0.052 min
 Response: 4971
 Conc: 51.73 ng/ml

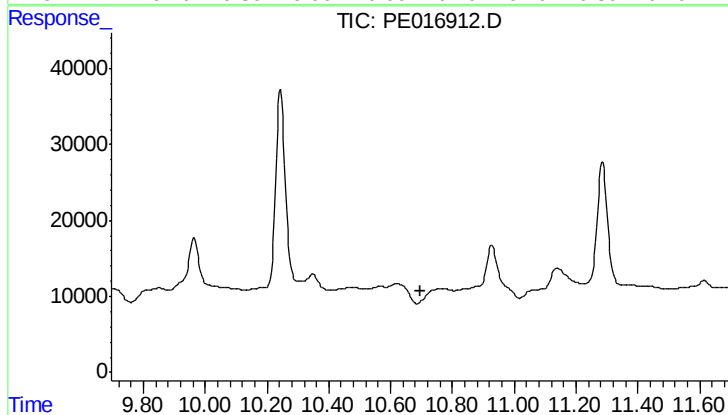

#4 2,4-DCAA


R.T.: 0.000 min
 Exp R.T.: 10.696 min
 Response: 0
 Conc: N.D.

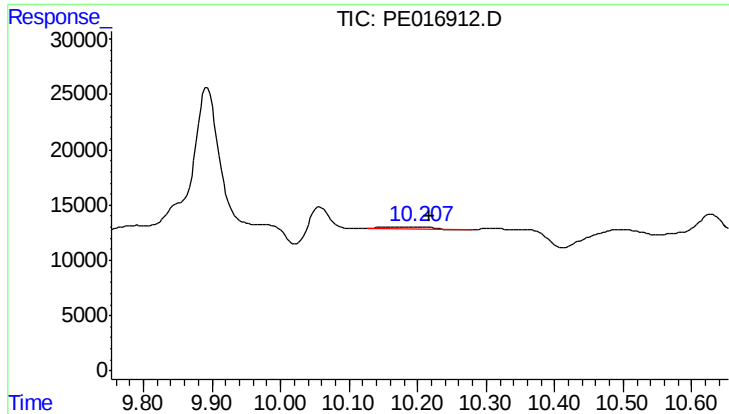

#5 DICAMBA


R.T.: 10.207 min
Delta R.T.: -0.010 min
Response: 9225
Conc: 21.45 ng/ml

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-4

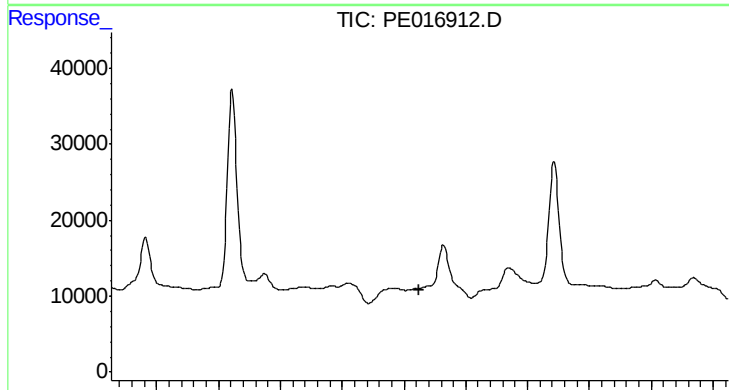


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 10.851 min
Response: 0
Conc: N.D.

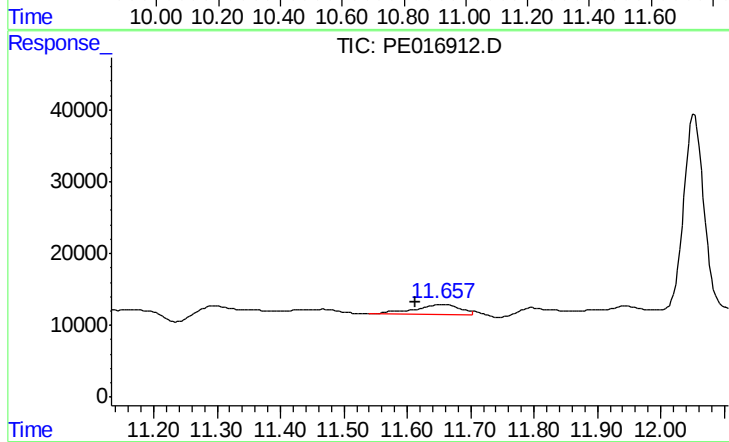


#9 2,4-D

R.T.: 11.658 min
Delta R.T.: 0.046 min
Response: 73191
Conc: 452.10 ng/ml

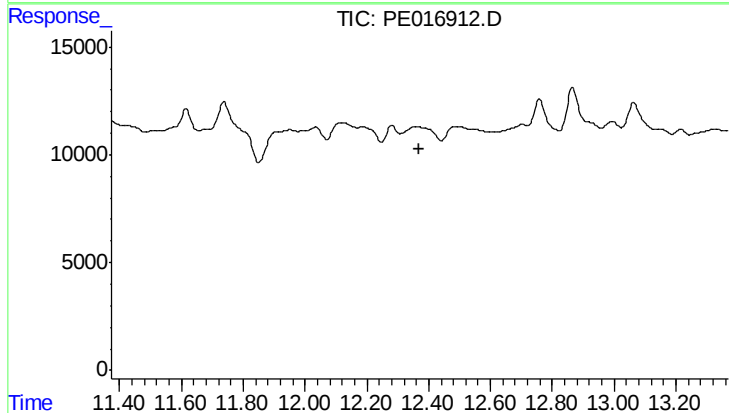

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.371 min
Response: 0
Conc: N.D.

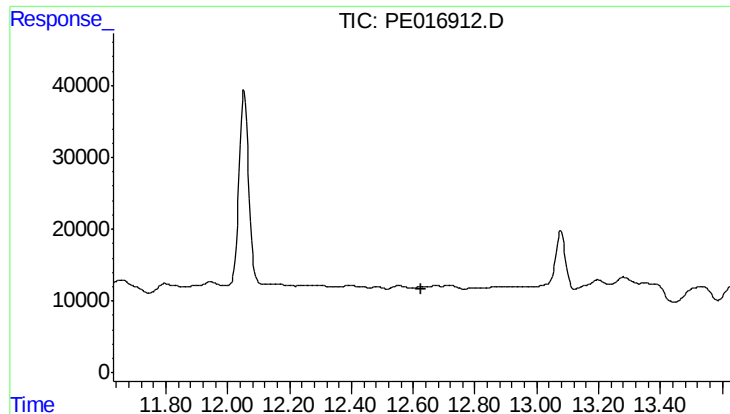

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 12.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-4

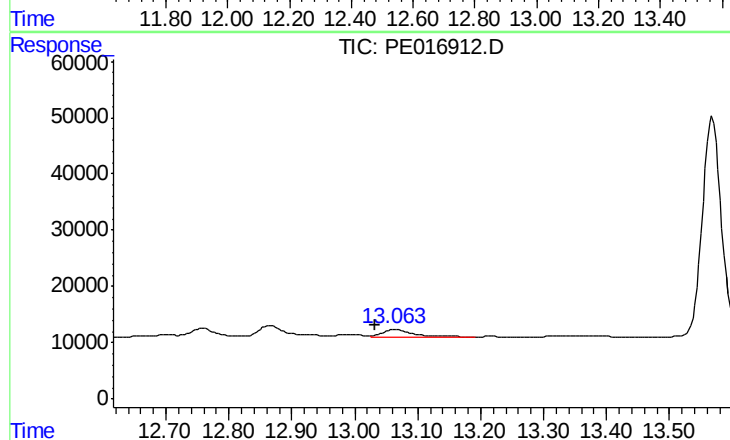


#10 Pentachlorophenol

R.T.: 13.064 min
Delta R.T.: 0.032 min
Response: 49461
Conc: 21.31 ng/ml

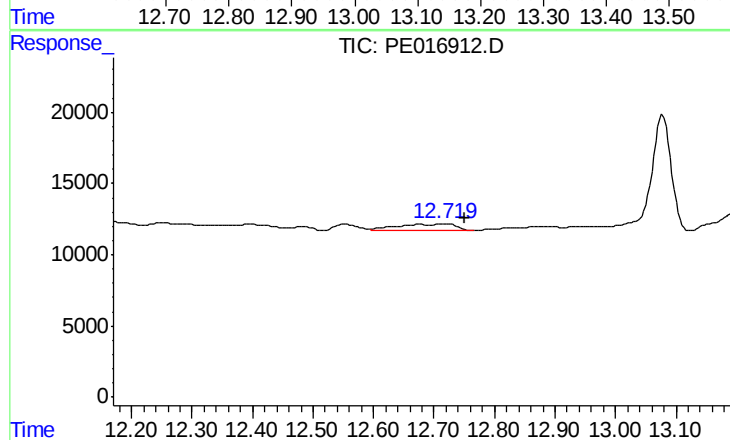


#11 2,4,5-TP (SILVEX)

R.T.: 12.719 min
Delta R.T.: -0.031 min
Response: 31726
Conc: 55.82 ng/ml

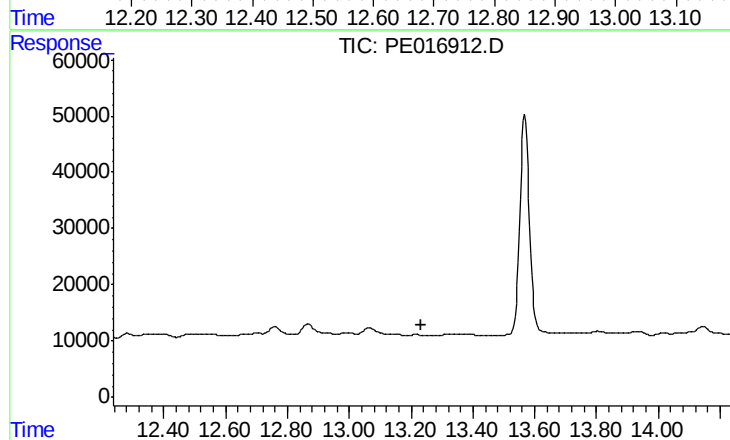

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 13.234 min
Response: 0
Conc: N.D.

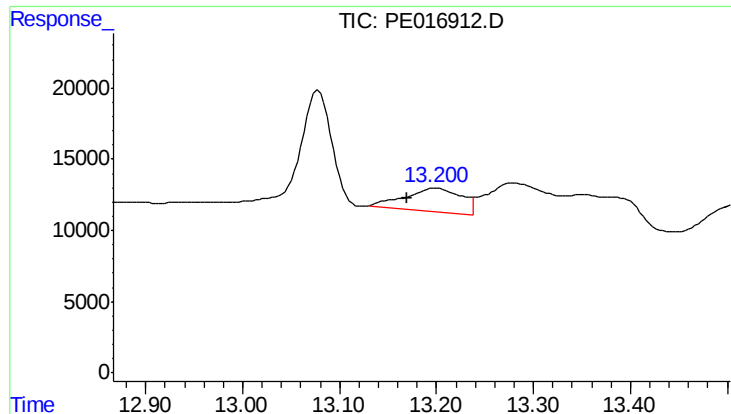

#12 2,4,5-T


R.T.: 13.199 min
Delta R.T.: 0.029 min
Response: 64252
Conc: 99.80 ng/ml

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-4

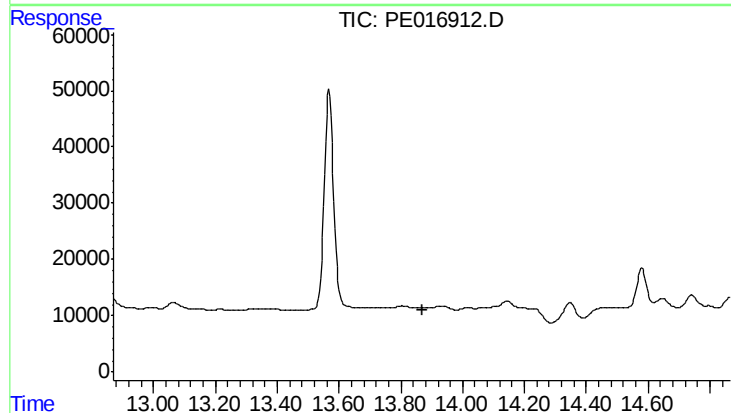


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 13.869 min
Response: 0
Conc: N.D.

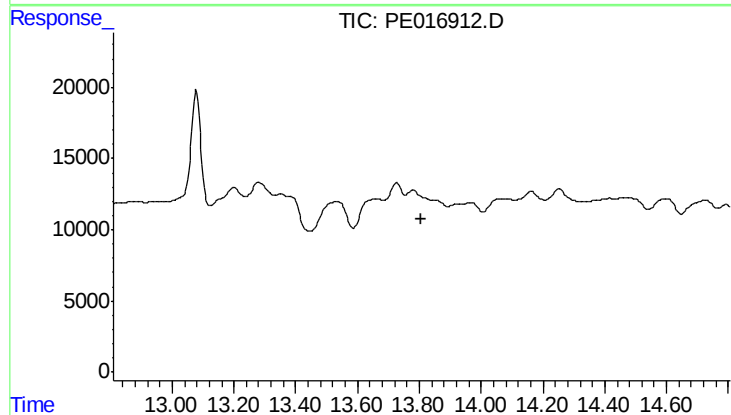


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 13.808 min
Response: 0
Conc: N.D.

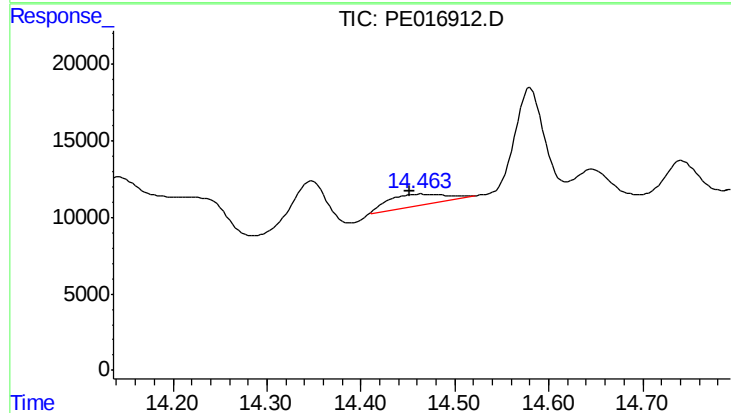

#13 2,4-DB


R.T.: 14.466 min
Delta R.T.: 0.014 min
Response: 32513
Conc: 250.96 ng/ml

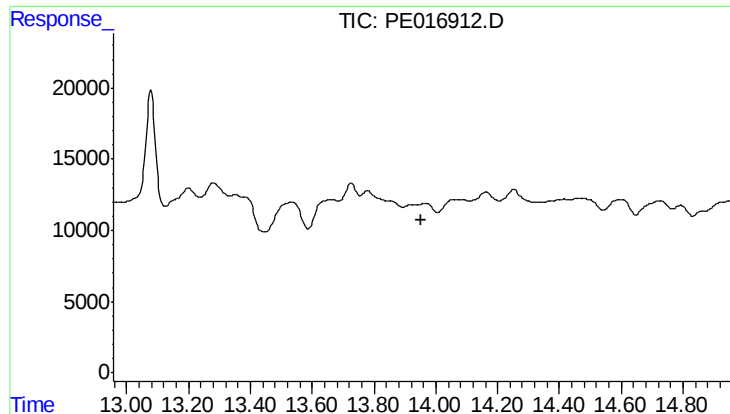

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 13.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-4

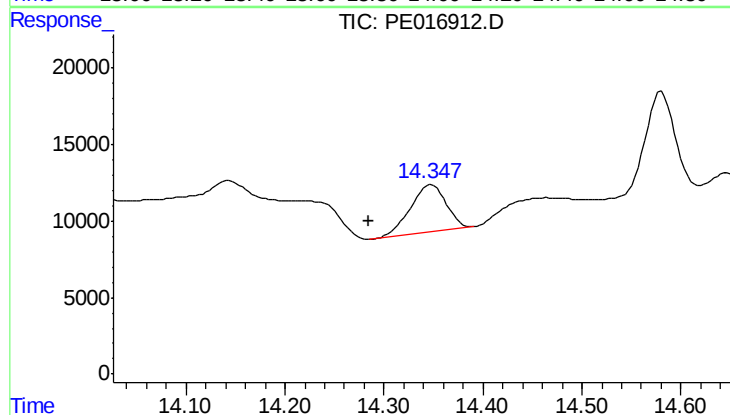


#14 DINOSEB

R.T.: 14.348 min
Delta R.T.: 0.064 min
Response: 78043
Conc: 88.10 ng/ml

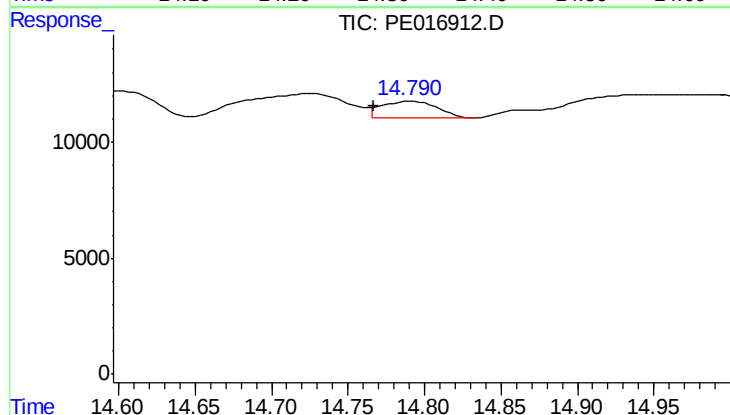

#15 Picloram

R.T.: 14.792 min
Delta R.T.: 0.025 min
Response: 18739
Conc: 17.38 ng/ml

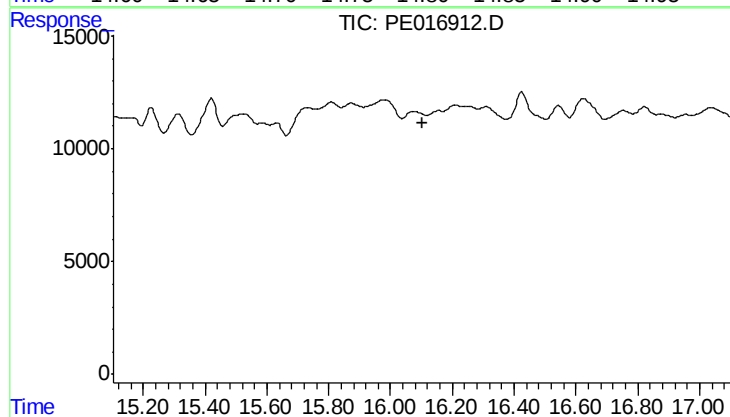

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.103 min
Response: 0
Conc: N.D.