

Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
 Data File : PE016918.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 4 Oct 2017 10:35
 Operator : UA/AJ
 Sample : I5563-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 NYSEG-PH4-SB-ESMI-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 16:40:29 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 04 13:20:47 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) T	4-Nitroph...	0.000	9.971	0	250056	N.D.	1697.035 #
8) T	DICHLORPROP	11.306	11.748	-15918	84273	N.D.	402.449
9) T	2,4-D	11.674	0.000	41721	0	257.707	N.D. #
10) T	Pentachlo...	0.000	13.074	0	26776	N.D.	11.536 #
12) T	2,4,5-T	13.209	0.000	12292	0	19.092	N.D. #
13) T	2,4-DB	13.787	0.000	29399	0	325.711	N.D. #
14) T	DINOSEB	13.992	0.000	13727	0	25.564	N.D. #
15) T	Picloram	14.734	0.000	40465	0	37.526	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE100217\
Data File : PE016918.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 4 Oct 2017 10:35
Operator : UA/AJ
Sample : I5563-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 16:40:29 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE100117.M
Quant Title : 8080.M
QLast Update : Wed Oct 04 13:20:47 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

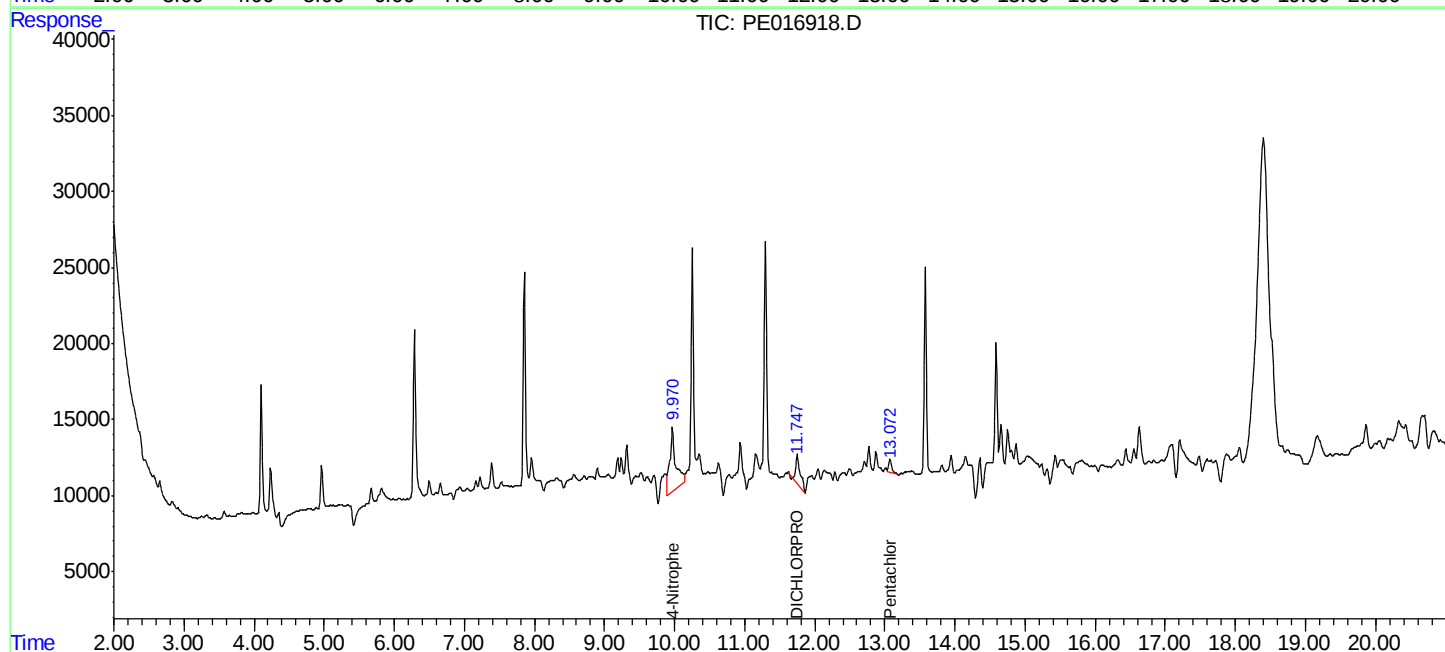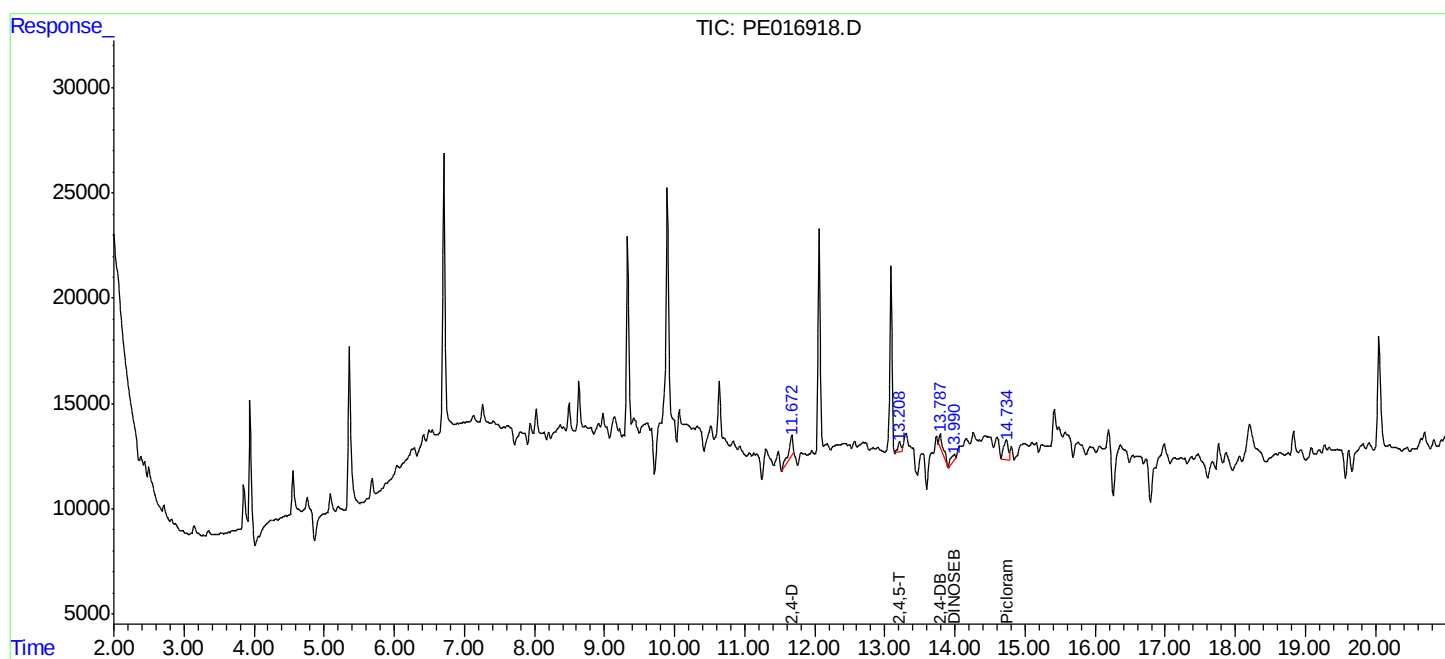


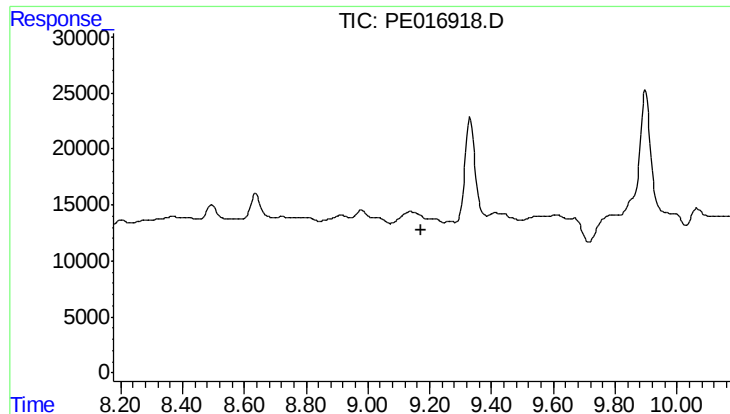

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 9.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

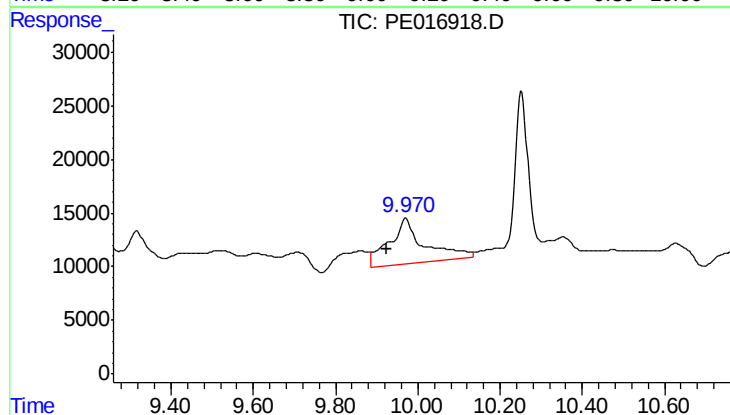


#3 4-Nitrophenol

R.T.: 9.971 min
Delta R.T.: 0.047 min
Response: 250056
Conc: 1697.03 ng/ml

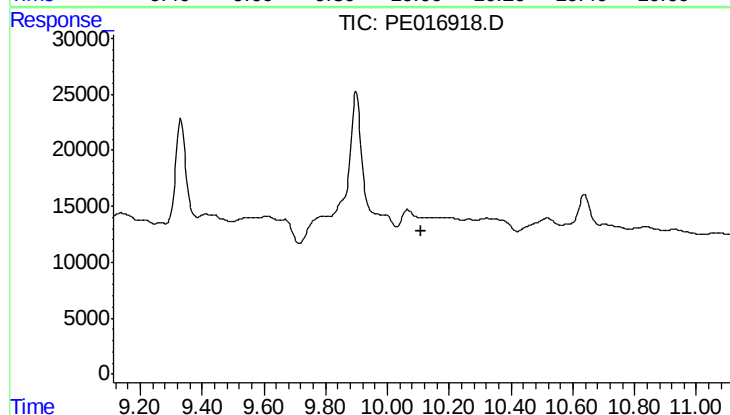


#4 2,4-DCAA

R.T.: 10.065 min
Delta R.T.: -0.046 min
Response: -7519
Conc: N.D.

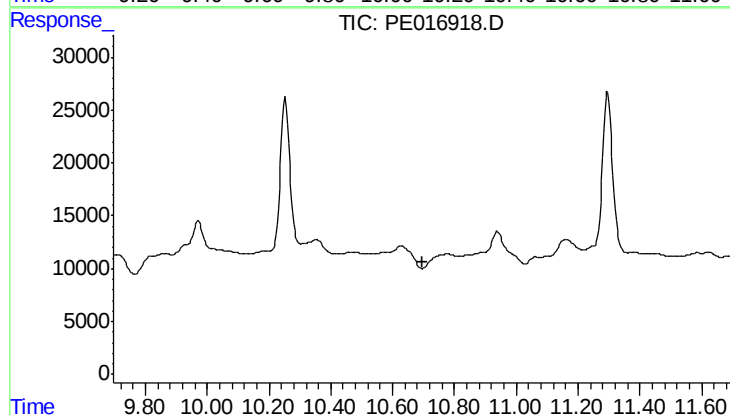

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.696 min
Response: 0
Conc: N.D.

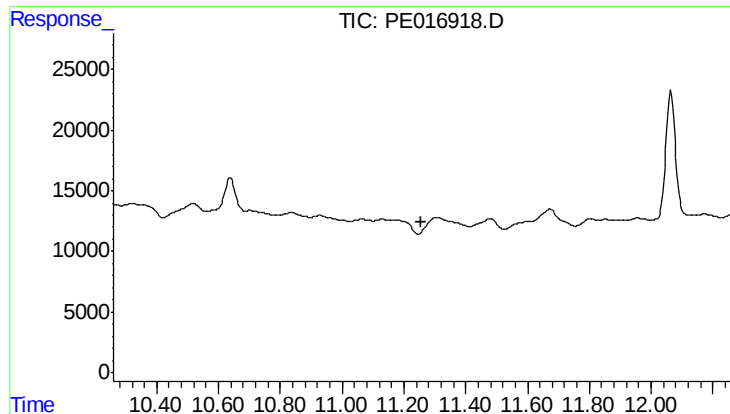

#8 DICHLORPROP


R.T.: 11.306 min
Delta R.T.: 0.048 min
Response: -15918
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

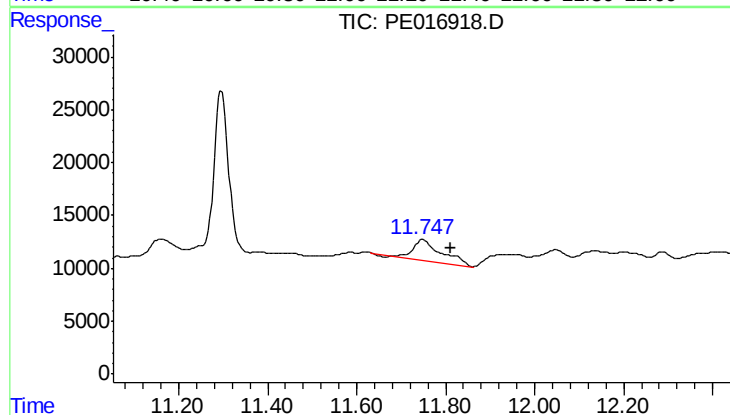


#8 DICHLORPROP

R.T.: 11.748 min
Delta R.T.: -0.062 min
Response: 84273
Conc: 402.45 ng/ml

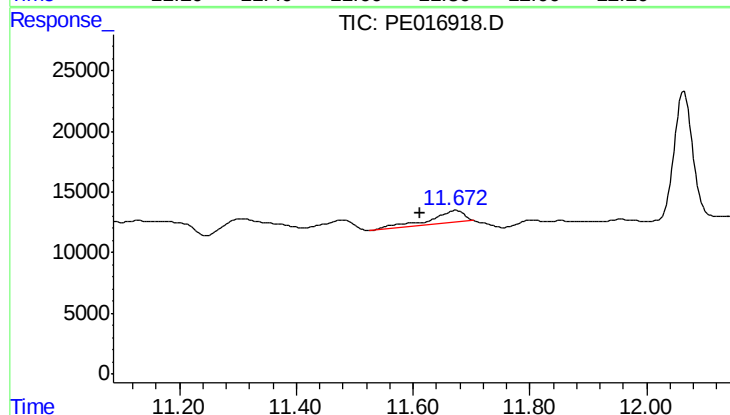


#9 2,4-D

R.T.: 11.674 min
Delta R.T.: 0.062 min
Response: 41721
Conc: 257.71 ng/ml

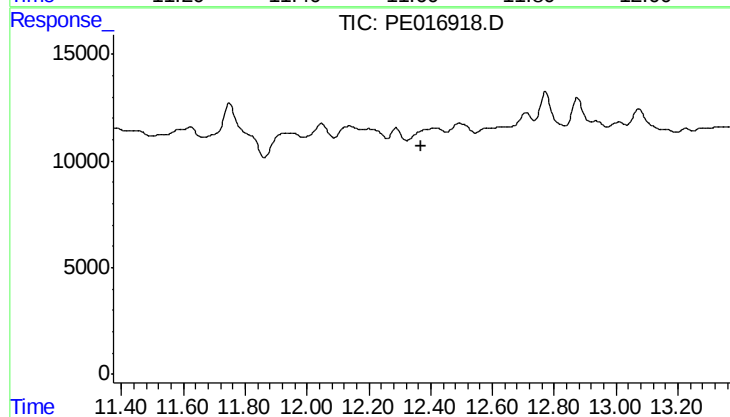

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 12.371 min
Response: 0
Conc: N.D.

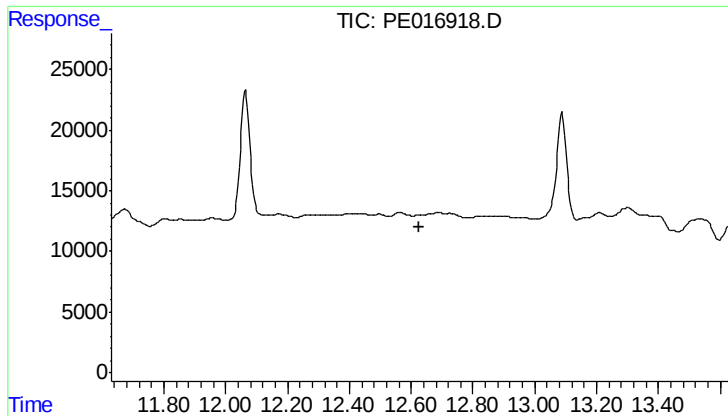

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 12.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

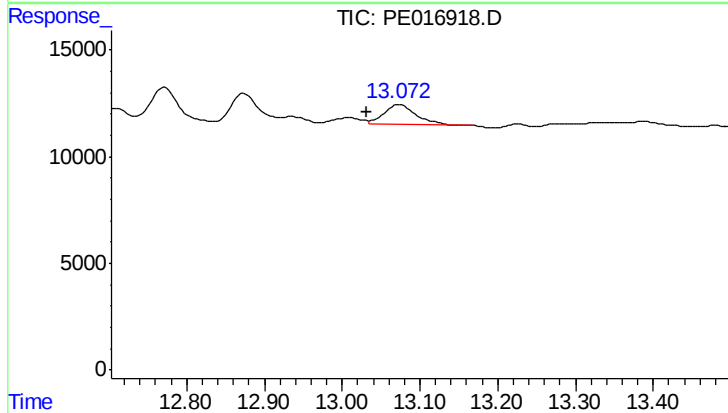


#10 Pentachlorophenol

R.T.: 13.074 min
Delta R.T.: 0.042 min
Response: 26776
Conc: 11.54 ng/ml

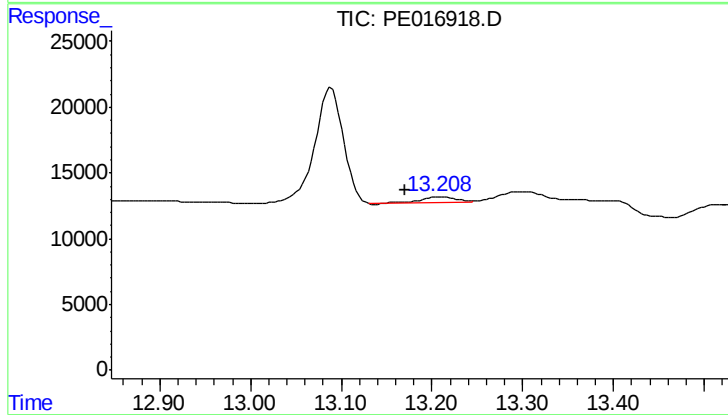


#12 2,4,5-T

R.T.: 13.209 min
Delta R.T.: 0.039 min
Response: 12292
Conc: 19.09 ng/ml

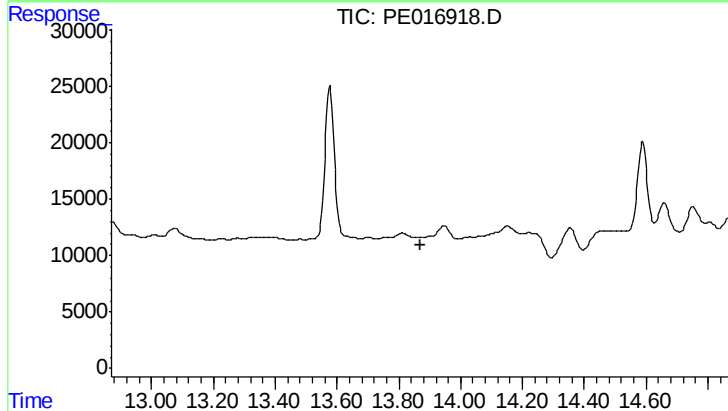

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 13.869 min
Response: 0
Conc: N.D.

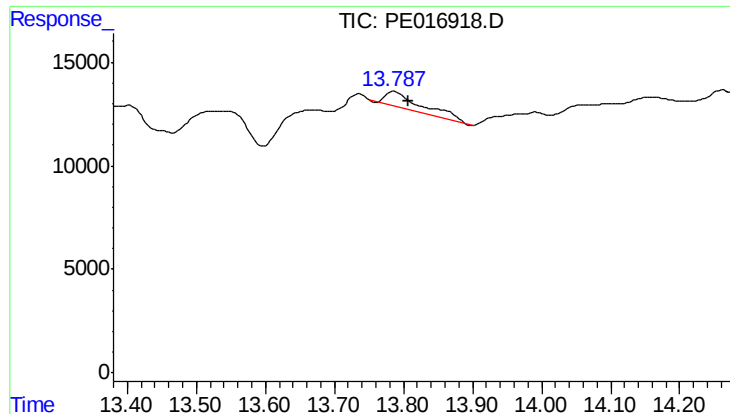

#13 2,4-DB


R.T.: 13.787 min
Delta R.T.: -0.021 min
Response: 29399
Conc: 325.71 ng/ml

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

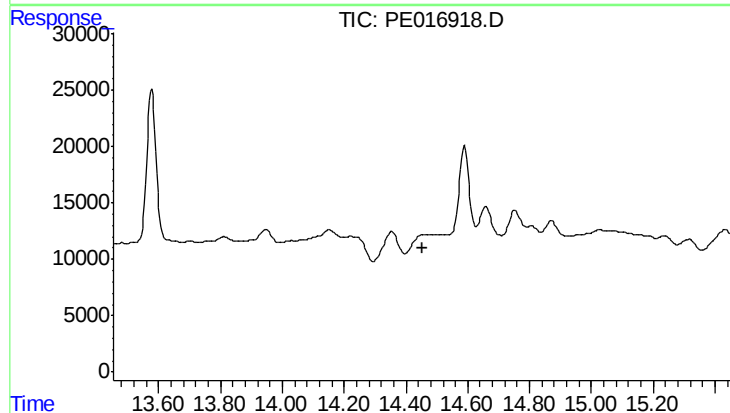


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 14.452 min
Response: 0
Conc: N.D.

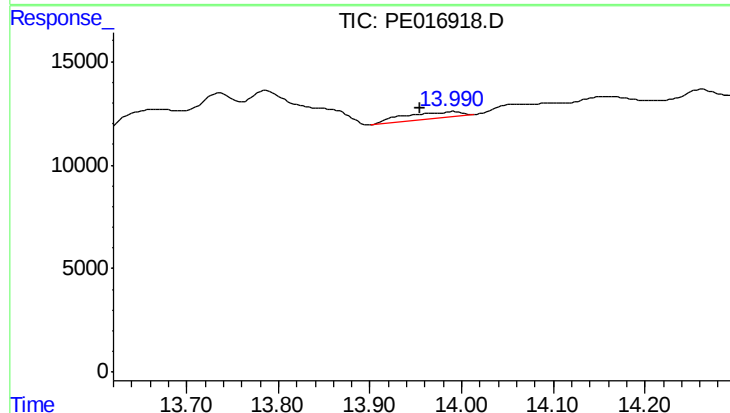


#14 DINOSEB

R.T.: 13.992 min
Delta R.T.: 0.037 min
Response: 13727
Conc: 25.56 ng/ml

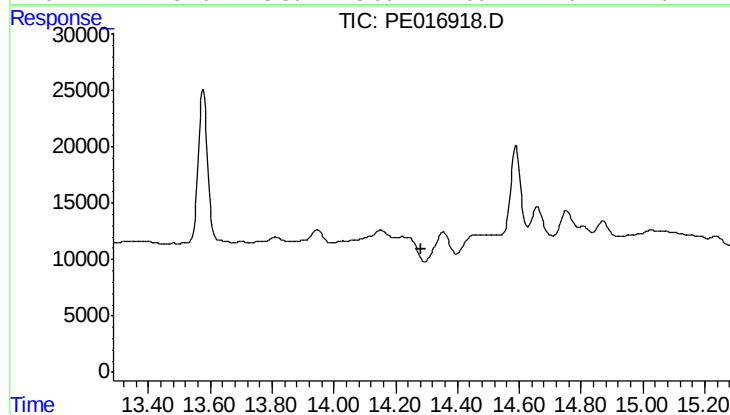

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 14.284 min
Response: 0
Conc: N.D.

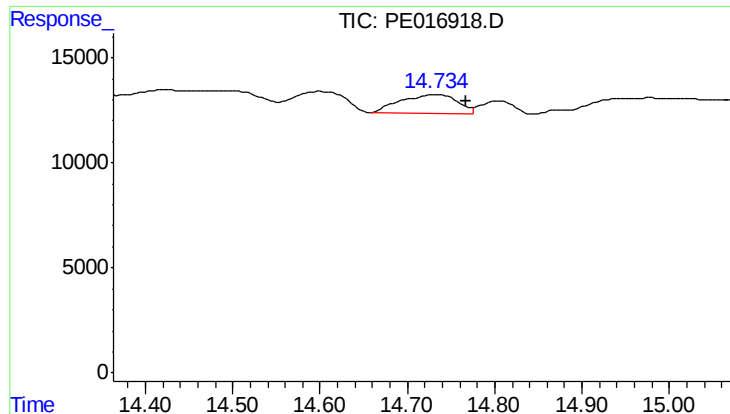

#15 Picloram

R.T.: 14.734 min
Delta R.T.: -0.033 min
Response: 40465
Conc: 37.53 ng/ml

Instrument :
ECD_E
ClientSampleId :
NYSEG-PH4-SB-ESMI-8

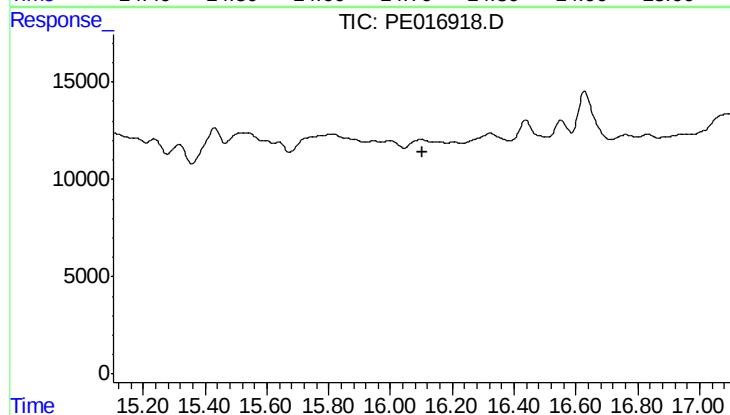

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.103 min
Response: 0
Conc: N.D.