

Data Path : P:\HPCHEM1\ECD E\Data\PE012618\
 Data File : PE018922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2018 9:02
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 02:52:12 2018
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE012618.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 27 02:21:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

10) T	Pentachlo...	0.000	13.149	0	428331	N.D.	134.627 #
15) T	Picloram	0.000	16.312	0	92114	N.D.	87.022 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD E\Data\PE012618\
Data File : PE018922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2018 9:02
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 02:52:12 2018
Quant Method : P:\HPCHEM1\ECD_E\Method\PE012618.M
Quant Title : 8080.M
QLast Update : Sat Jan 27 02:21:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Ini. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

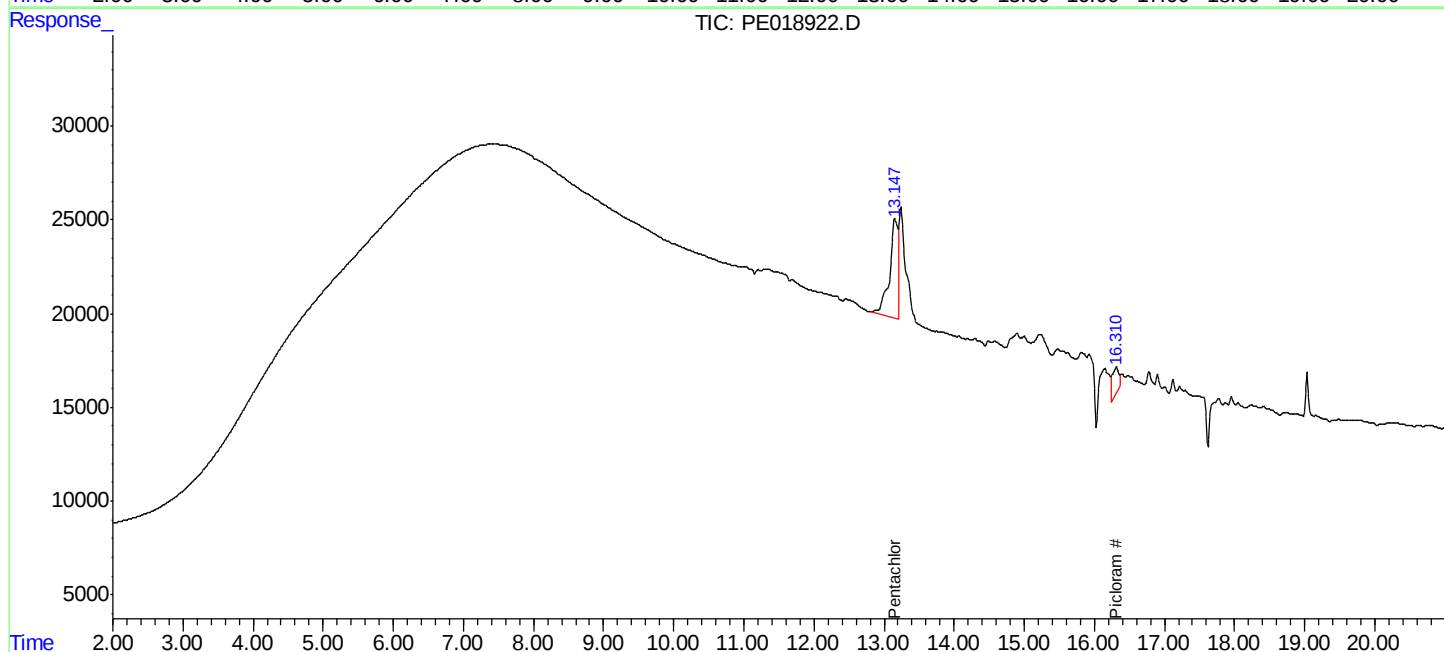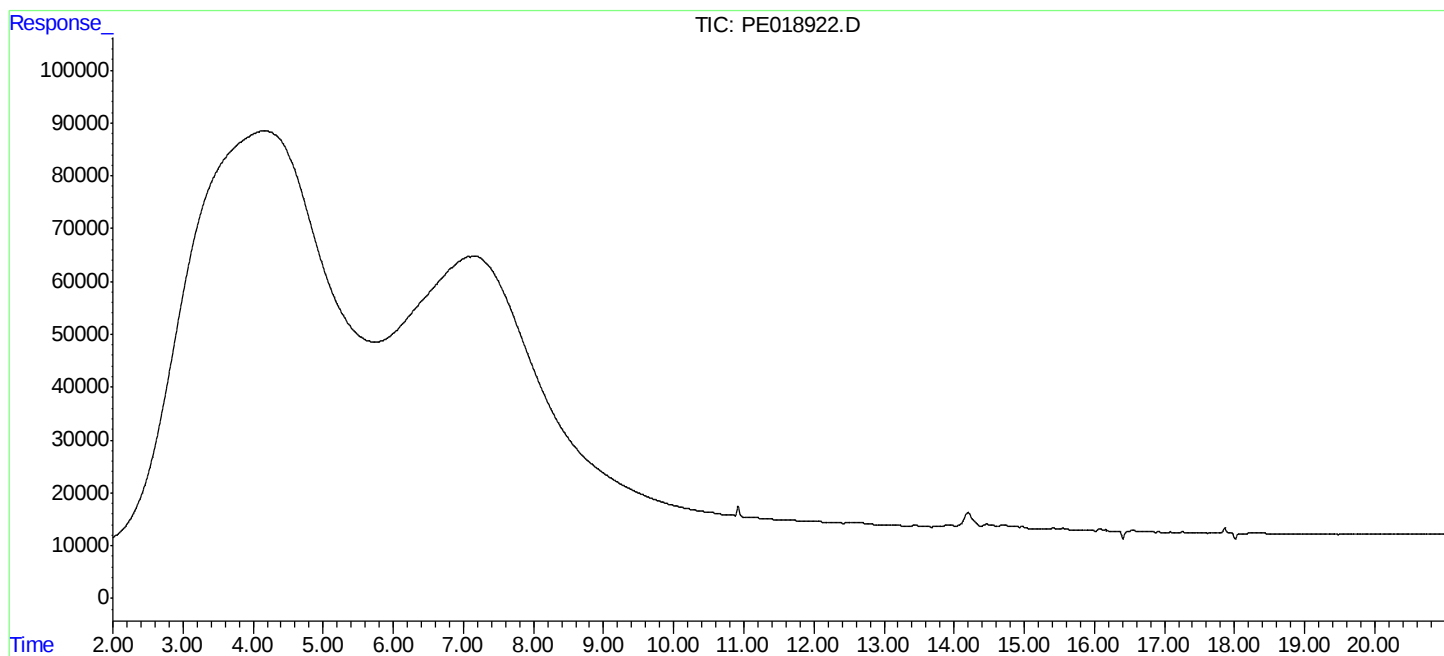


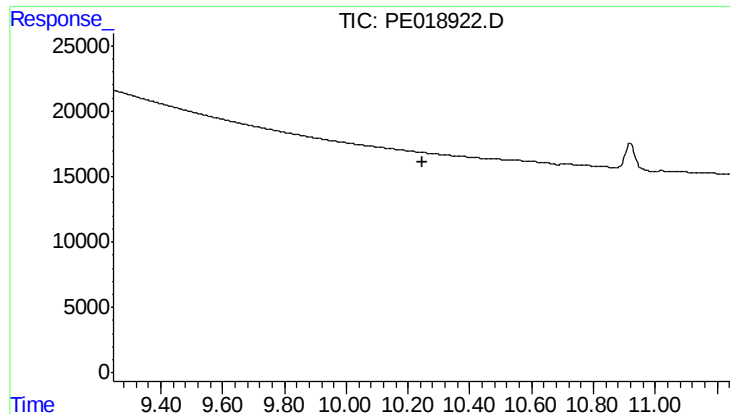

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.245 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

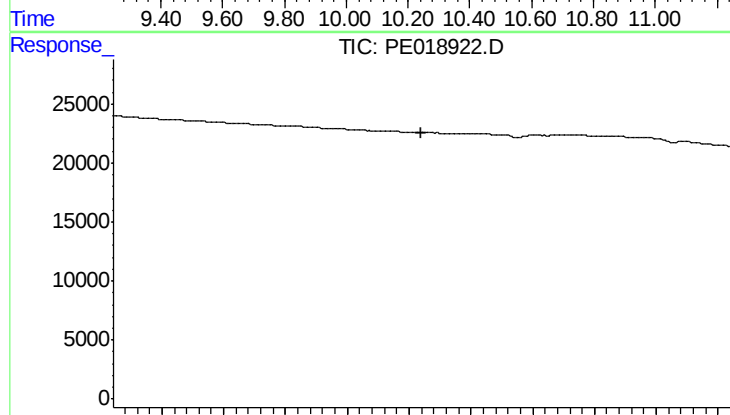


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 10.841 min
Response: 0
Conc: N.D.

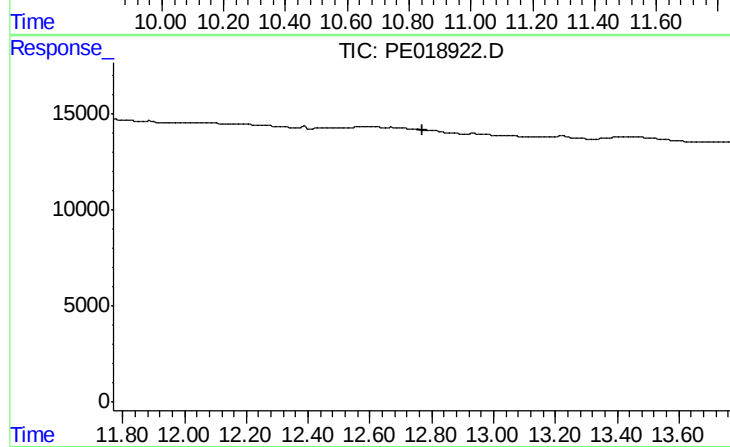


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 12.769 min
Response: 0
Conc: N.D.

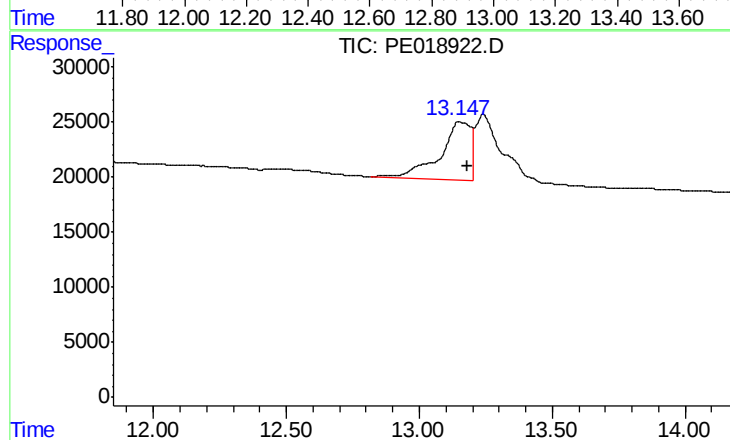

#10 Pentachlorophenol


R.T.: 13.149 min
Delta R.T.: -0.034 min
Response: 428331
Conc: 134.63 ng/ml

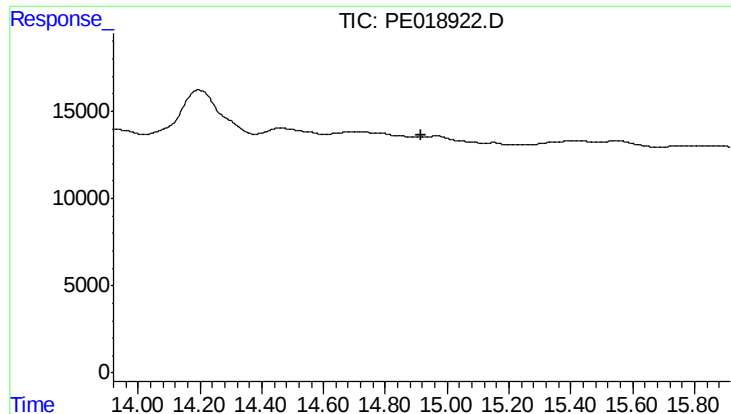

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

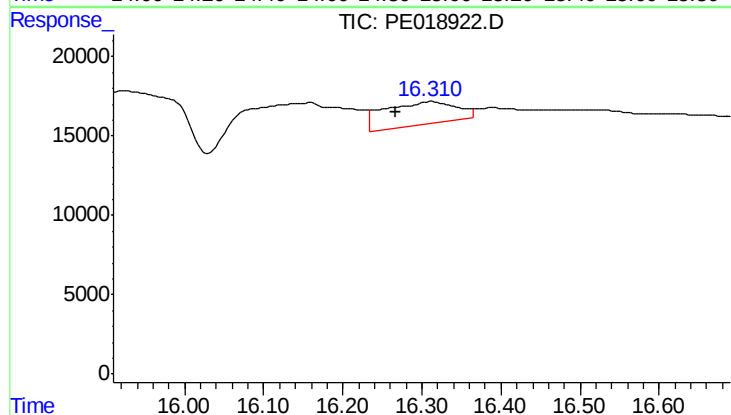

#15 Picloram

R.T.: 16.312 min
Delta R.T.: 0.046 min
Response: 92114
Conc: 87.02 ng/ml