

Data Path : P:\HPCHEM1\ECD_E\Data\PE012918\
 Data File : PE019000.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2018 9:41
 Operator : UA/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:15:54 2018
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE012618.M
 Quant Title : 8080.M
 QLast Update : Sat Jan 27 02:21:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

14) T	DINOSEB	14.067	0.000	97731	0	195.197	N.D.	#
15) T	Picloram	0.000	16.253	0	563236	N.D.	532.096	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE012918\
Data File : PE019000.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 9:41
Operator : UA/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:15:54 2018
Quant Method : P:\HPCHEM1\ECD_E\Method\PE012618.M
Quant Title : 8080.M
QLast Update : Sat Jan 27 02:21:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25 μ m

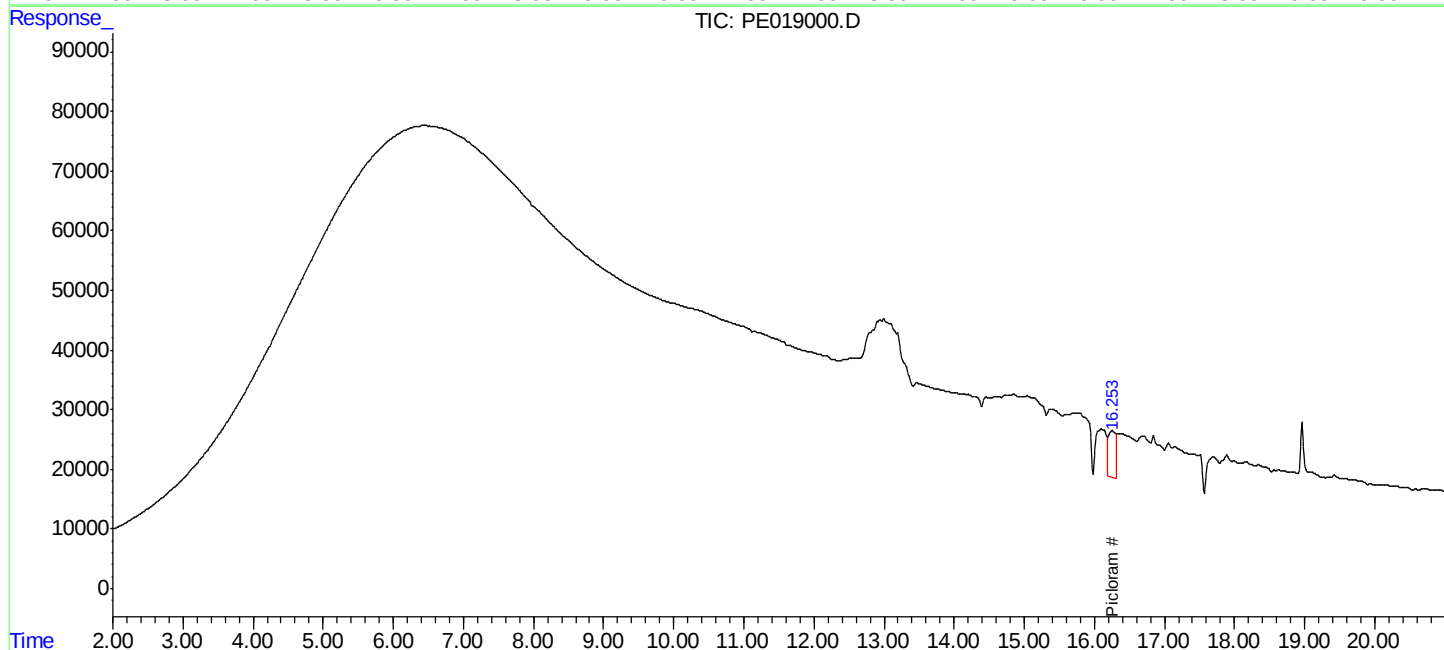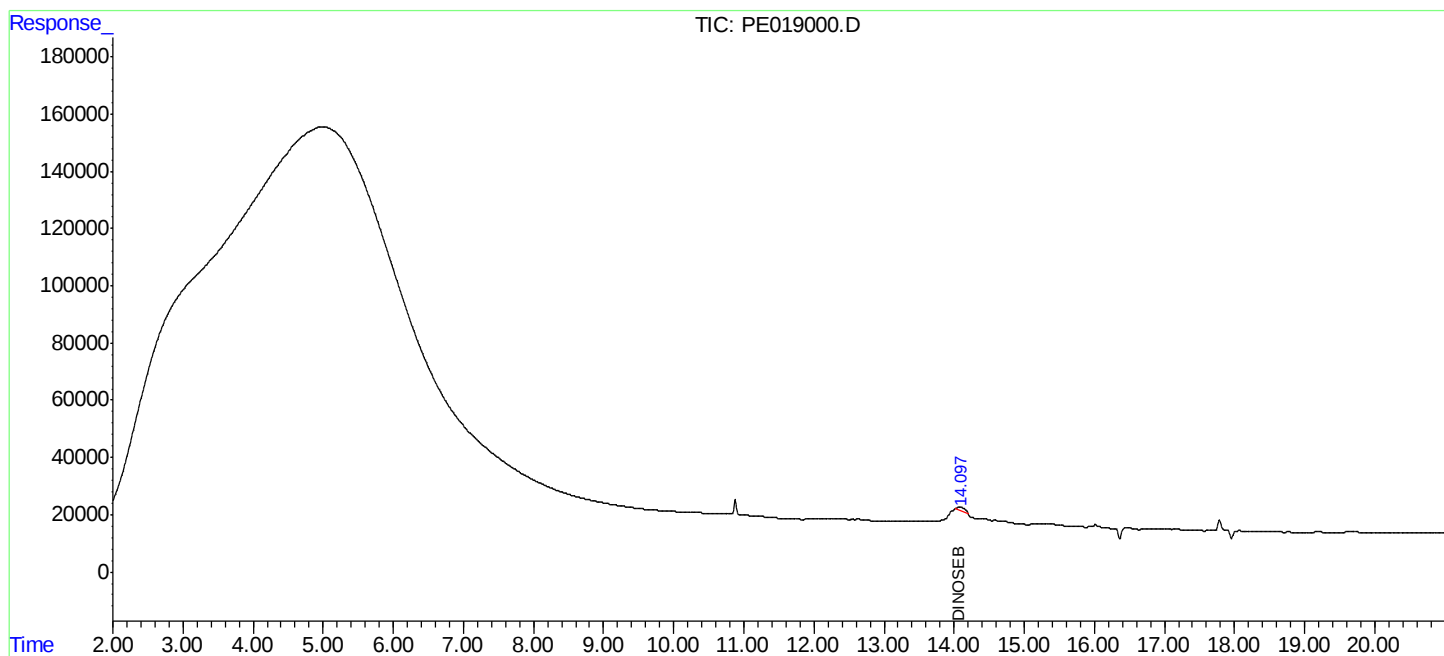


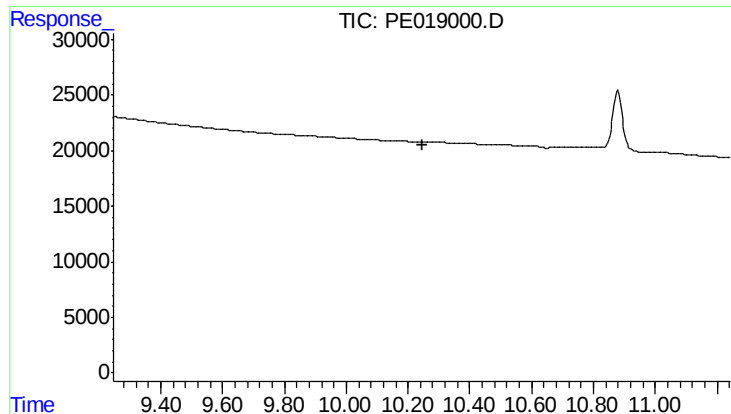

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.245 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HEXANE

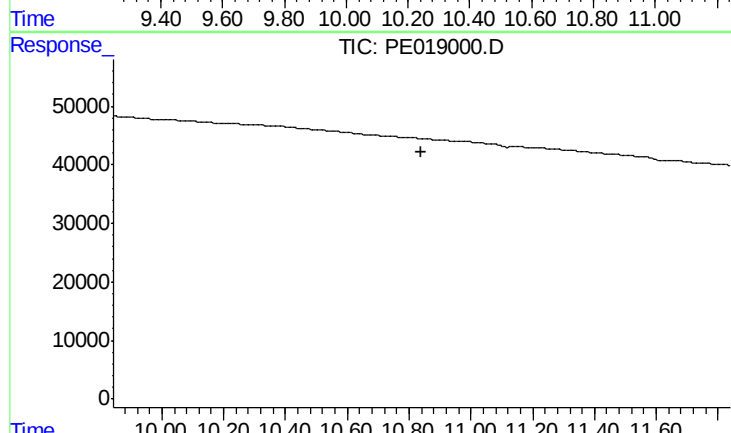


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 10.841 min
Response: 0
Conc: N.D.

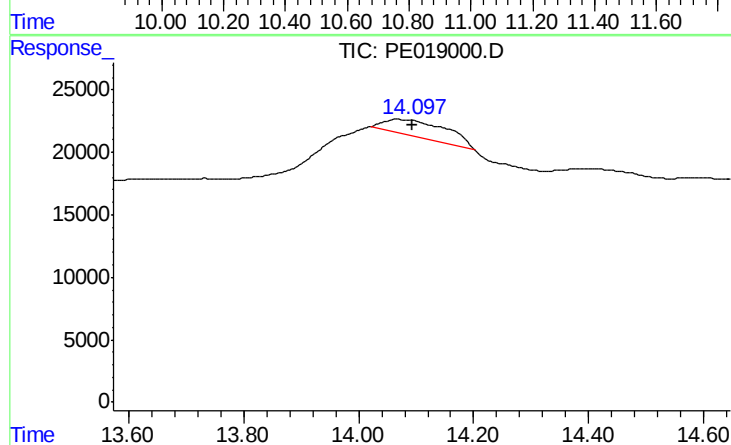


#14 DINOSEB

R.T.: 14.067 min
Delta R.T.: -0.026 min
Response: 97731
Conc: 195.20 ng/ml

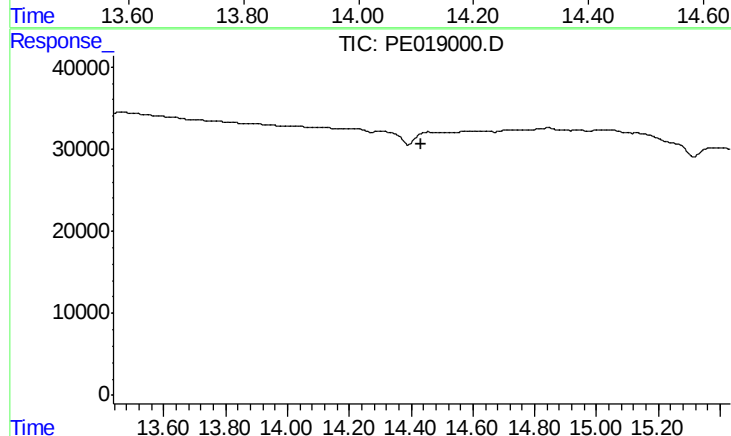

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 14.435 min
Response: 0
Conc: N.D.

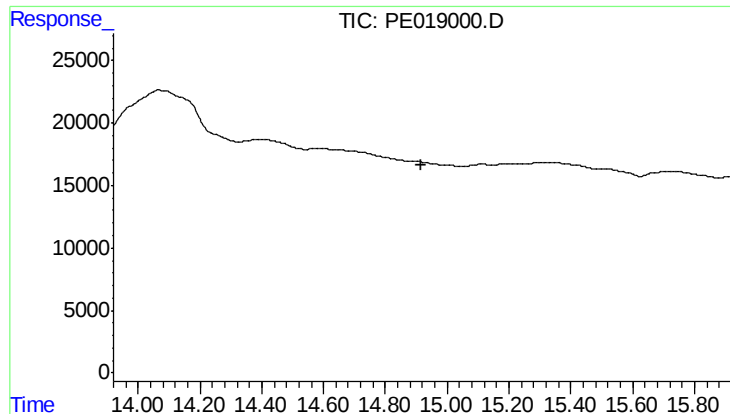

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HEXANE

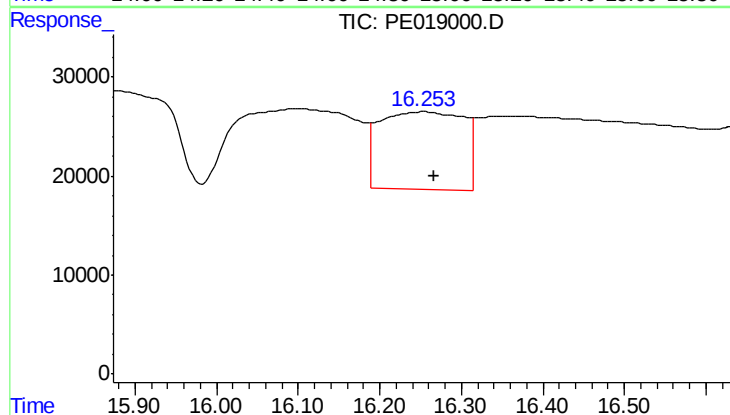

#15 Picloram

R.T.: 16.253 min
Delta R.T.: -0.013 min
Response: 563236
Conc: 532.10 ng/ml