

Data Path : P:\HPCHEM1\ECD_E\Data\PE101017\
 Data File : PE017083.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Oct 2017 18:57
 Operator : UA/AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 10 19:29:06 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE100417.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 05 09:47:18 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
Target Compounds						
1) T Dalapon	2.733	2.911	134908	185278	525.612	582.369
2) T 3,5-DICHL...	8.648	0.000	118841	0	714.184	N.D. #
10) T Pentachlo...	12.566	0.000	601241	0	370.005	N.D. #
13) T 2,4-DB	13.768	0.000	536492	0	5184.338	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE101017\
Data File : PE017083.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Oct 2017 18:57
Operator : UA/AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 10 19:29:06 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE100417.M
Quant Title : 8080.M
QLast Update : Thu Oct 05 09:47:18 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

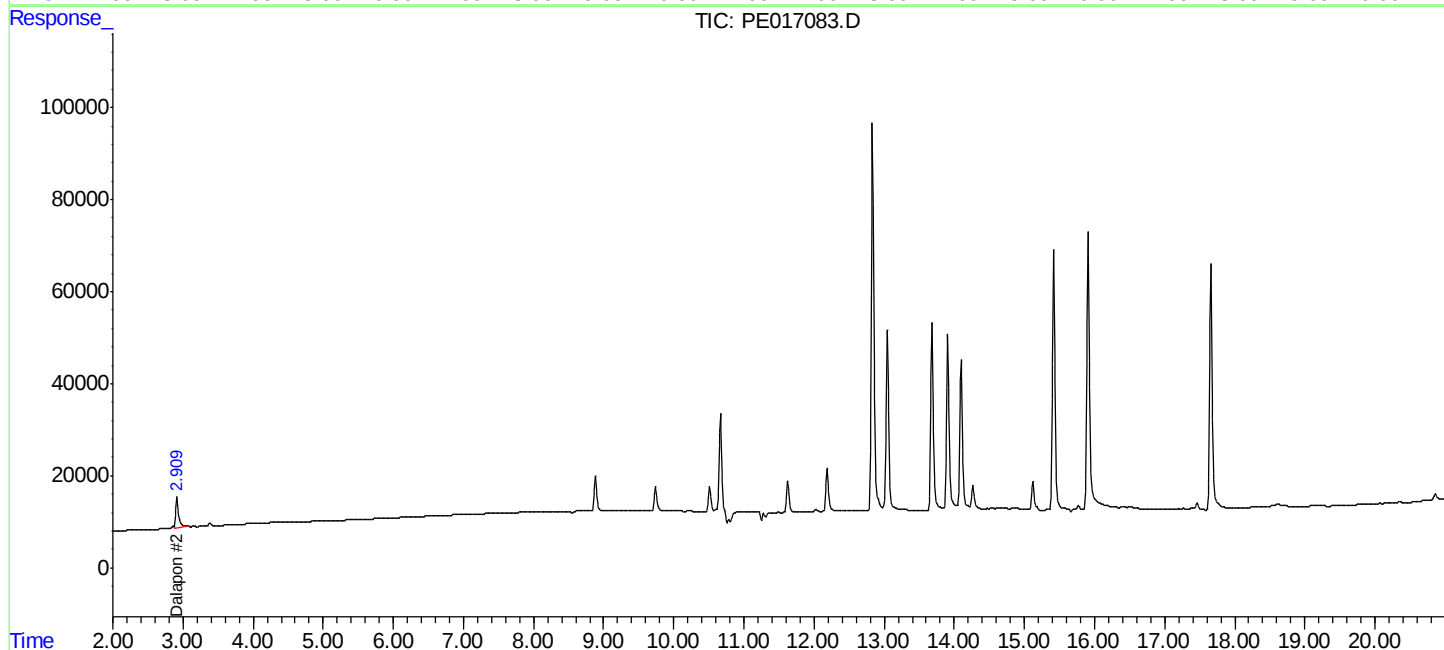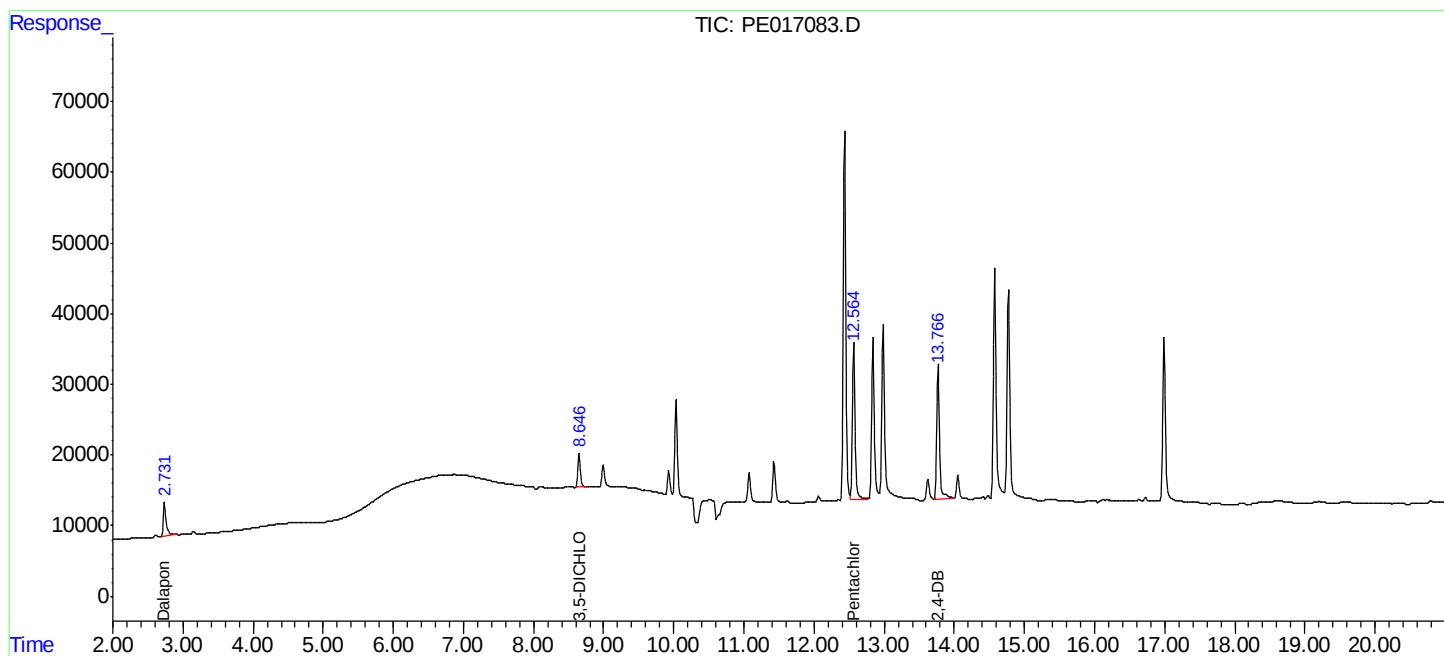


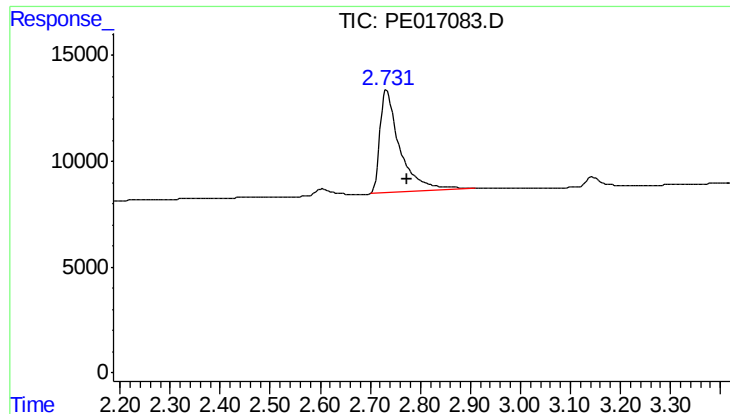

#1 Dalapon


R.T.: 2.733 min
Delta R.T.: -0.042 min
Response: 134908
Conc: 525.61 ng/ml

Instrument :
ECD_E
ClientSampleId :
HSTDCCC750

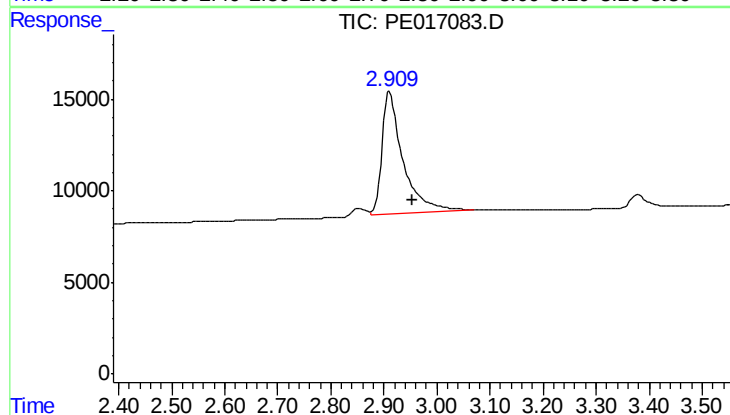


#1 Dalapon

R.T.: 2.911 min
Delta R.T.: -0.043 min
Response: 185278
Conc: 582.37 ng/ml

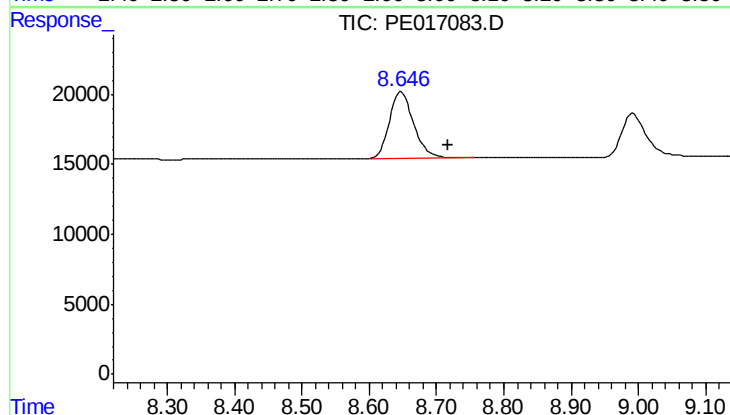


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.648 min
Delta R.T.: -0.069 min
Response: 118841
Conc: 714.18 ng/ml

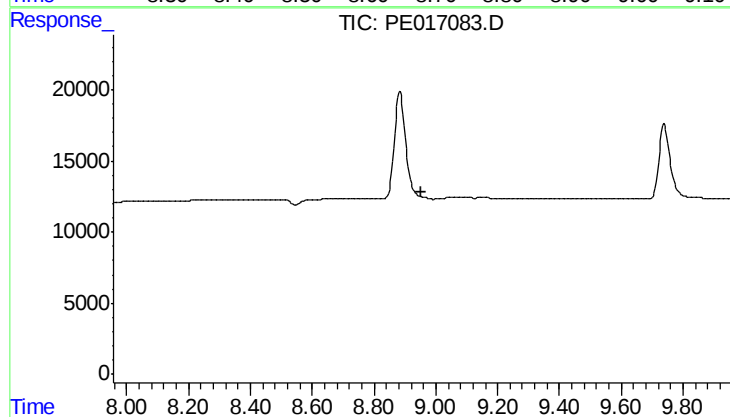

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 8.954 min
Response: 0
Conc: N.D.

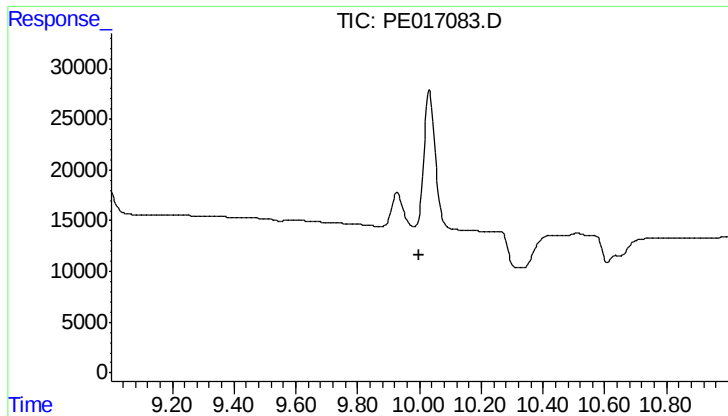

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.001 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HSTDCCC750

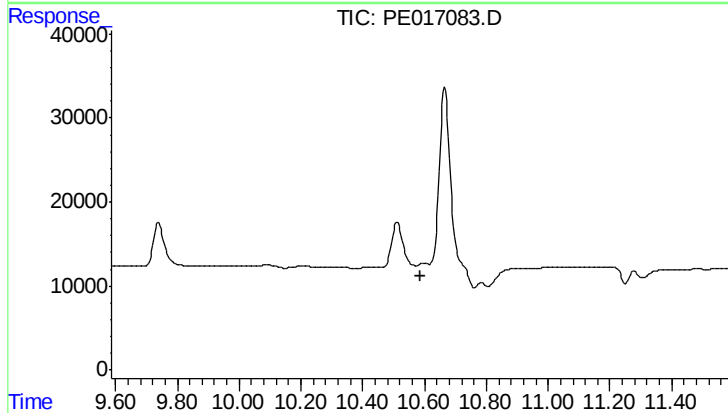


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 10.586 min
Response: 0
Conc: N.D.

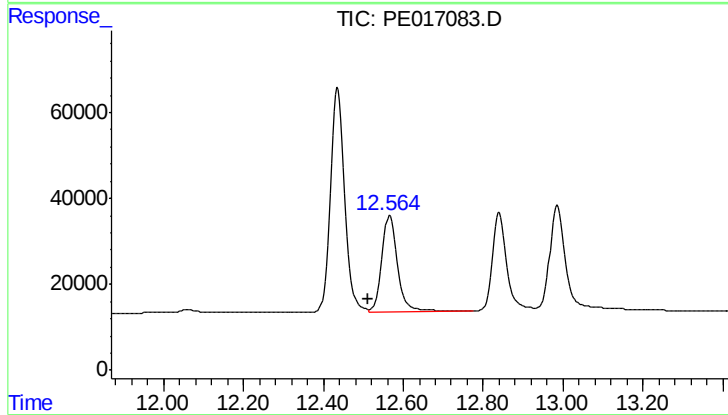


#10 Pentachlorophenol

R.T.: 12.566 min
Delta R.T.: 0.054 min
Response: 601241
Conc: 370.00 ng/ml

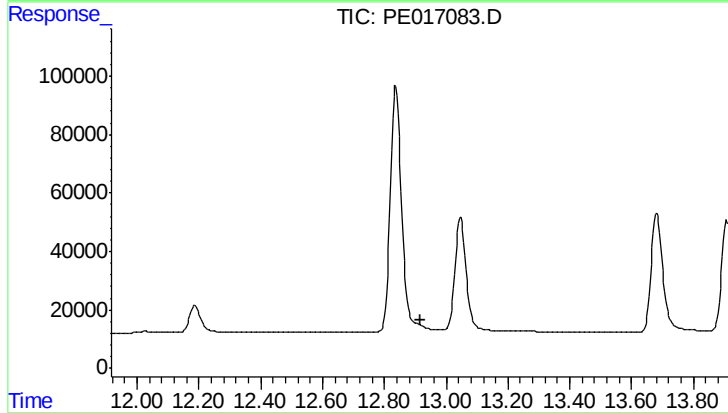

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 12.916 min
Response: 0
Conc: N.D.

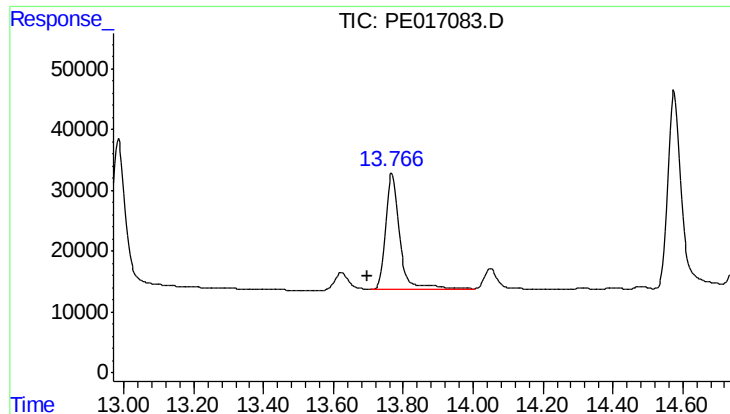

#13 2,4-DB

R.T.: 13.768 min
Delta R.T.: 0.070 min
Response: 536492
Conc: 5184.34 ng/ml

Instrument :
ECD_E
ClientSampleId :
HSTDCCC750

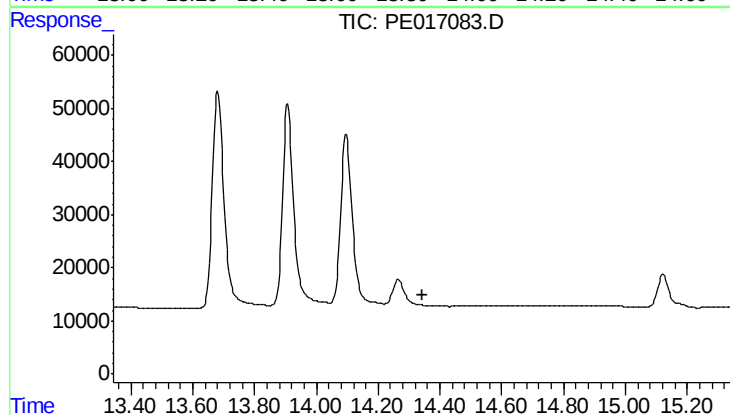

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 14.342 min
Response: 0
Conc: N.D.