

Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
 Data File : PE017150.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2017 8:43
 Operator : UA/AJ
 Sample : I5567-04MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 HP-RR2MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 17:35:38 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 13 07:26:24 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	10.478	0.000	5758630	0	61141.580	N.D. #
Target Compounds							
3) T	4-Nitroph...	0.000	10.315	0	172318	N.D.	1653.235 #
5) T	DICAMBA	0.000	11.204	0	6204647	N.D.	12191.095 #
8) T	DICHLORPROP	0.000	12.174	0	161367	N.D.	969.805 #
10) T	Pentachlo...	13.024	13.425	569726	677107	427.934	308.324 #
11) T	2,4,5-TP ...	0.000	13.602	0	171877	N.D.	208.993 #
12) T	2,4,5-T	13.518	14.264	162958	18805	345.250	20.703 #
13) T	2,4-DB	14.182	14.836	27342	30099	374.093	284.675
15) T	Picloram	15.207	16.512	499046	150160	936.858	132.378 #
16) T	DCPA	15.393	16.003	-1489	34196	N.D.	23.678



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
Data File : PE017150.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2017 8:43
Operator : UA/AJ
Sample : I5567-04MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 17:35:38 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
Quant Title : 8080.M
QLast Update : Fri Oct 13 07:26:24 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

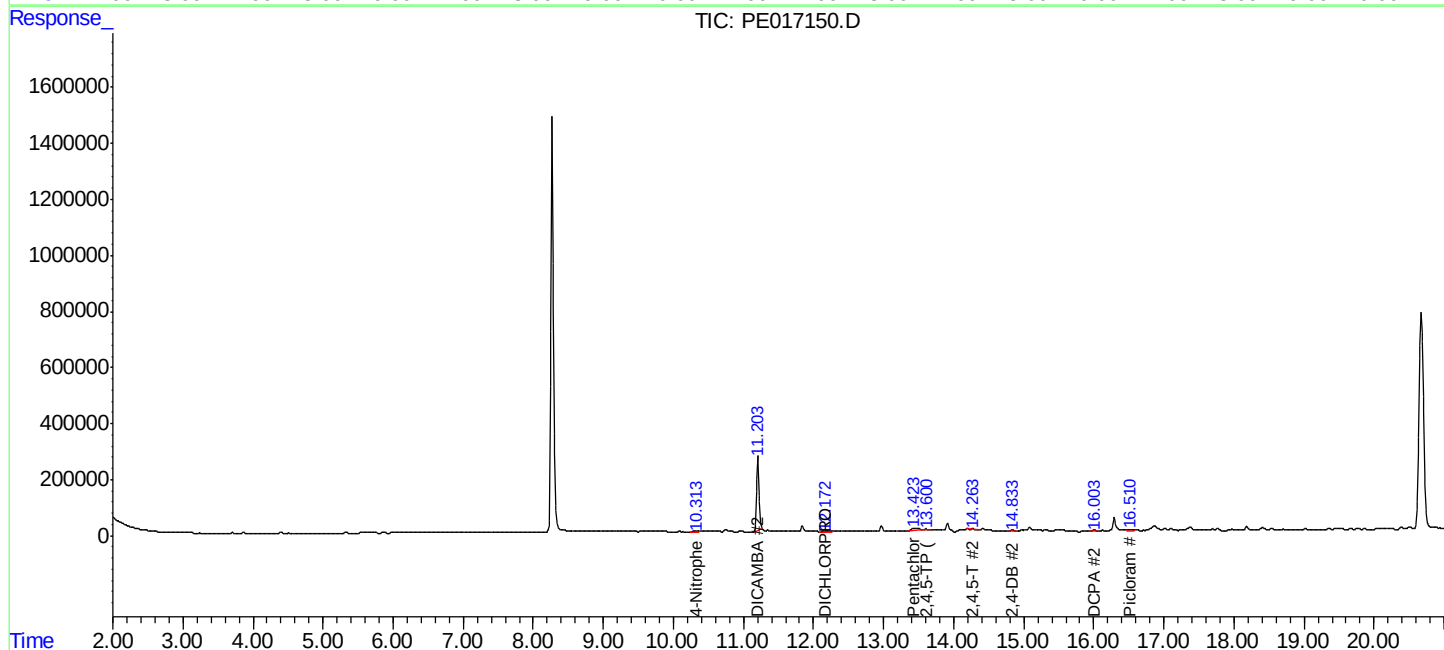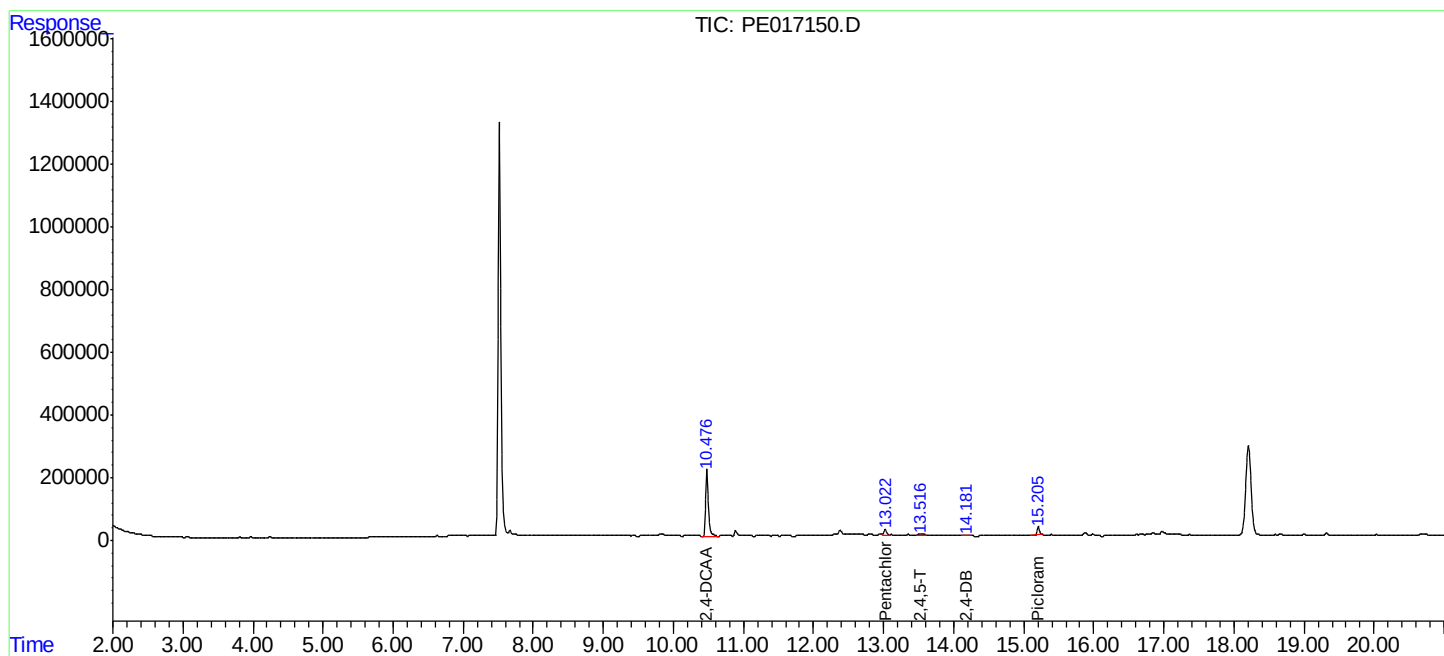


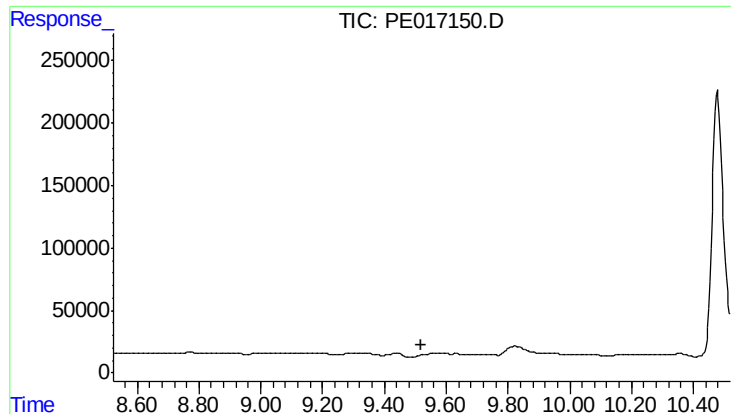

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 9.521 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

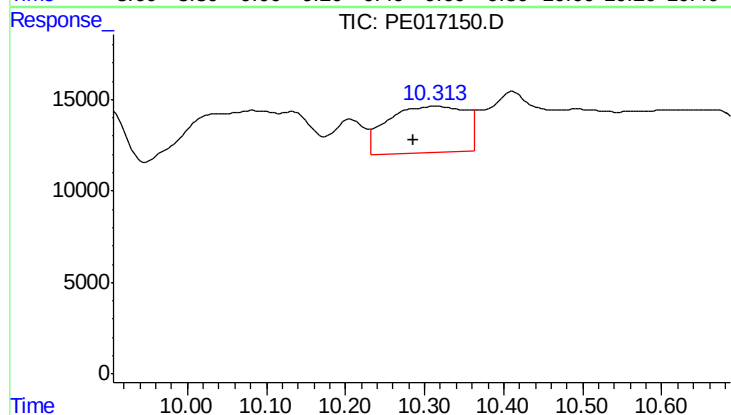


#3 4-Nitrophenol

R.T.: 10.315 min
Delta R.T.: 0.030 min
Response: 172318
Conc: 1653.23 ng/ml

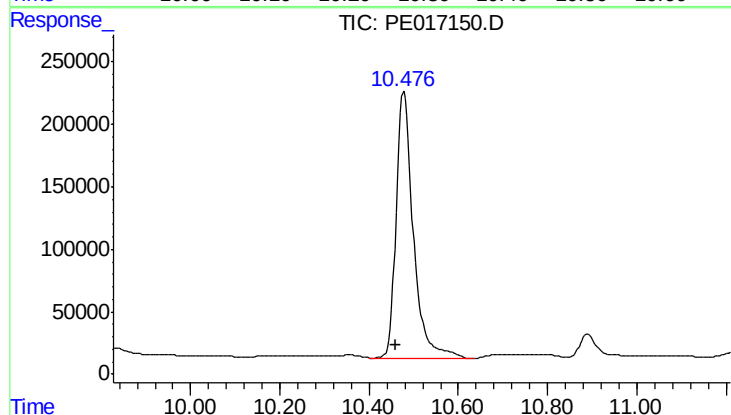


#4 2,4-DCAA

R.T.: 10.478 min
Delta R.T.: 0.017 min
Response: 5758630
Conc: 61141.58 ng/ml

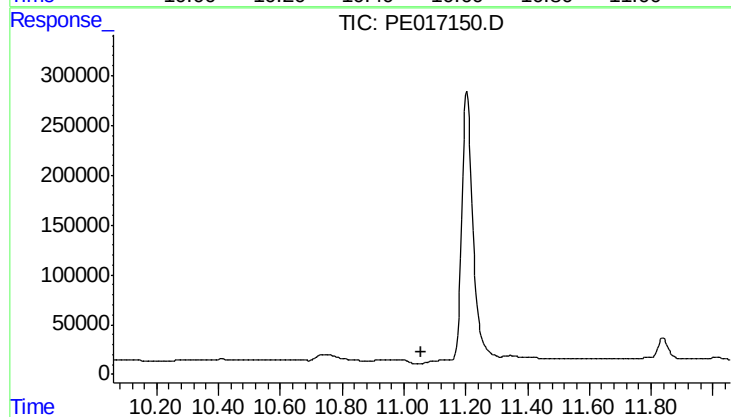

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.058 min
Response: 0
Conc: N.D.

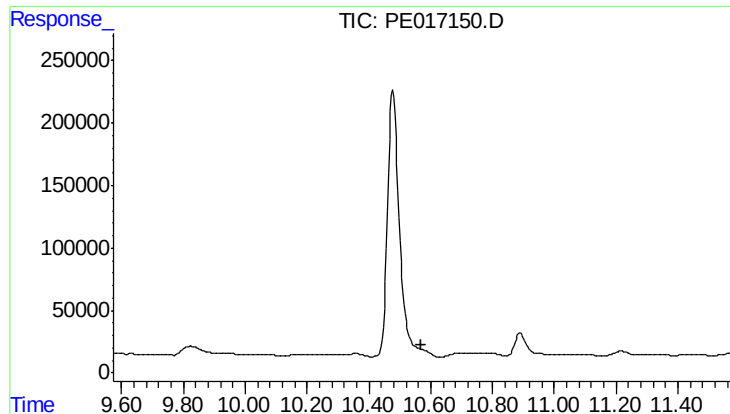

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 10.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

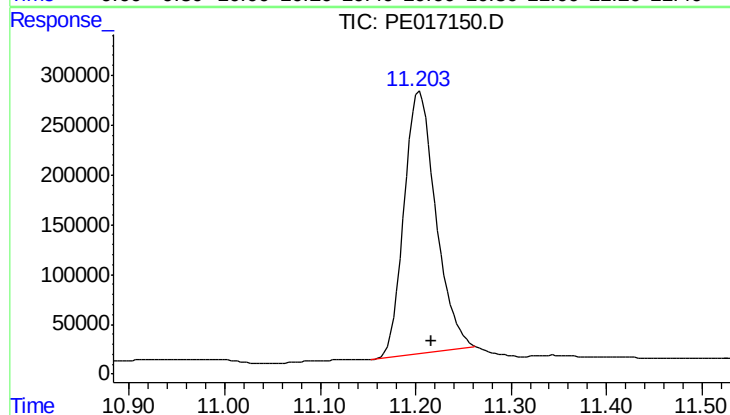


#5 DICAMBA

R.T.: 11.204 min
Delta R.T.: -0.013 min
Response: 6204647
Conc: 12191.09 ng/ml

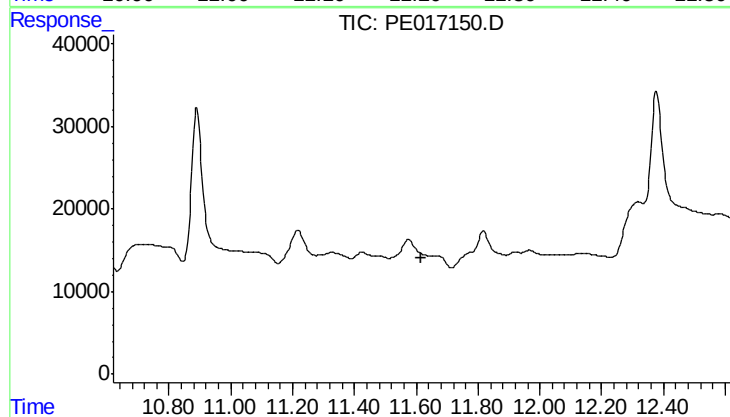


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 11.617 min
Response: 0
Conc: N.D.

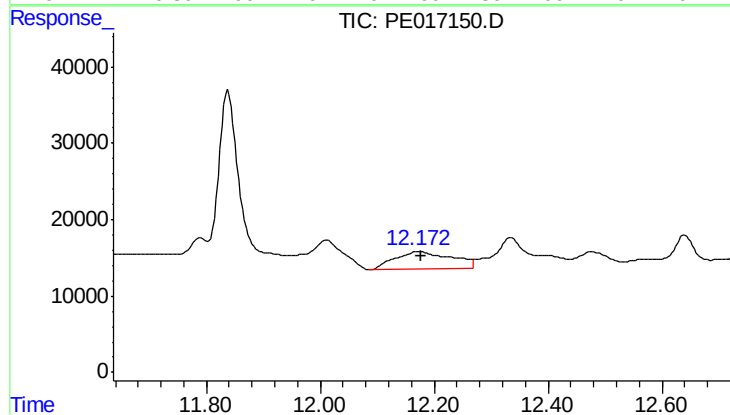

#8 DICHLORPROP


R.T.: 12.174 min
Delta R.T.: -0.003 min
Response: 161367
Conc: 969.80 ng/ml

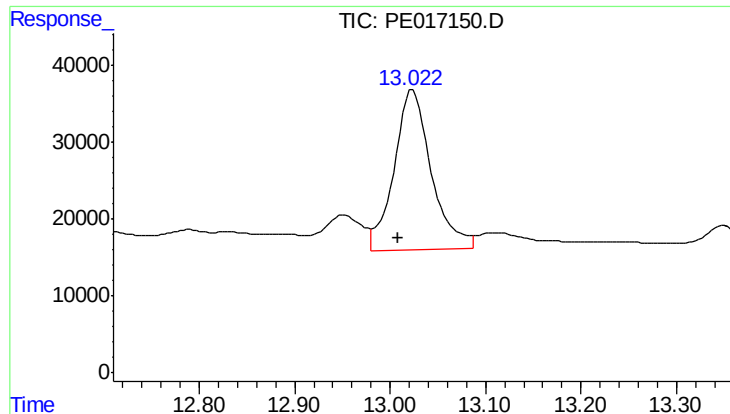

#10 Pentachlorophenol


R.T.: 13.024 min
Delta R.T.: 0.015 min
Response: 569726
Conc: 427.93 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

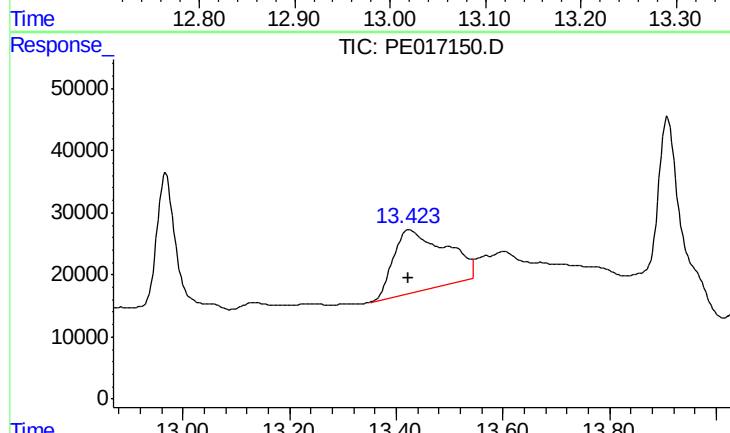


#10 Pentachlorophenol

R.T.: 13.425 min
Delta R.T.: 0.003 min
Response: 677107
Conc: 308.32 ng/ml

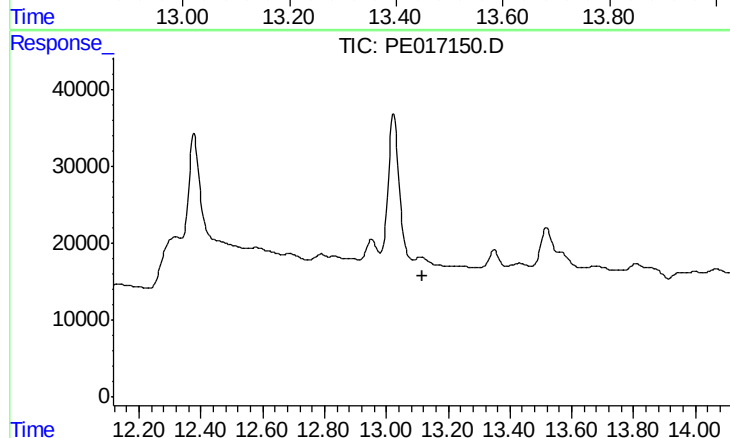


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 13.115 min
Response: 0
Conc: N.D.

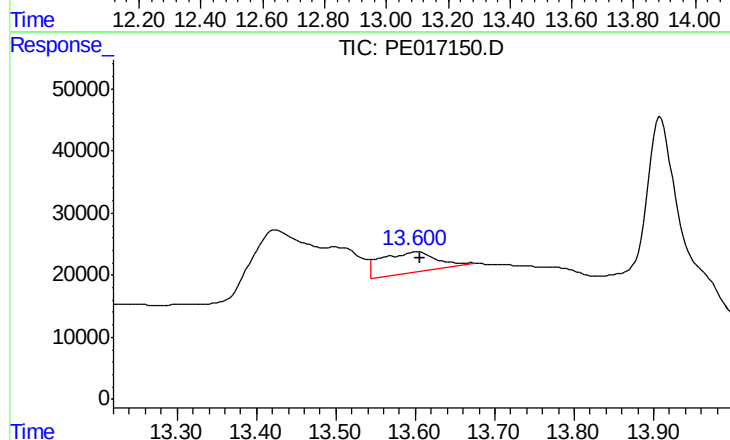

#11 2,4,5-TP (SILVEX)


R.T.: 13.602 min
Delta R.T.: -0.004 min
Response: 171877
Conc: 208.99 ng/ml

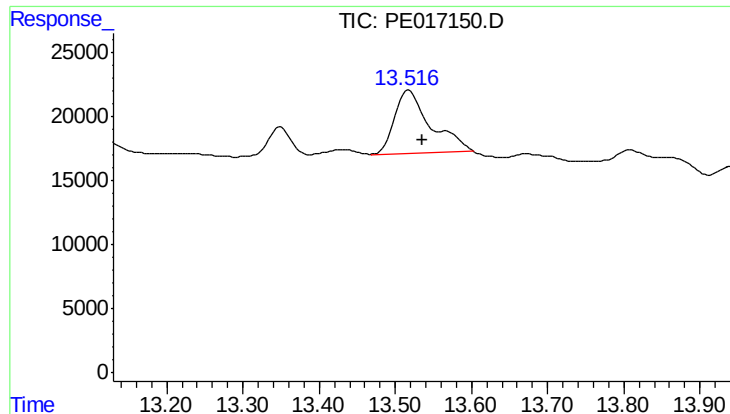

#12 2,4,5-T


R.T.: 13.518 min
Delta R.T.: -0.018 min
Response: 162958
Conc: 345.25 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

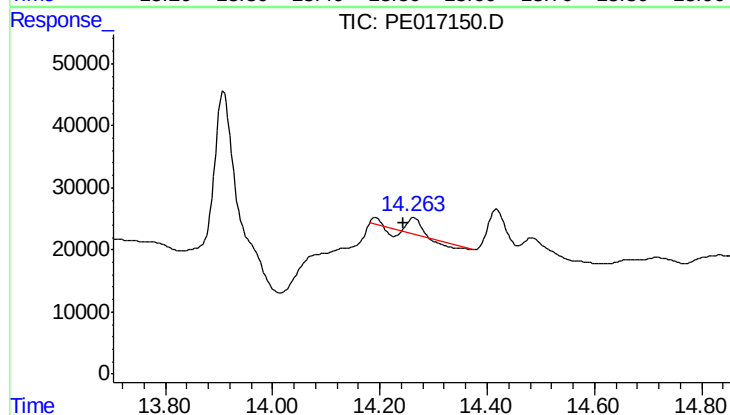


#12 2,4,5-T

R.T.: 14.264 min
Delta R.T.: 0.021 min
Response: 18805
Conc: 20.70 ng/ml

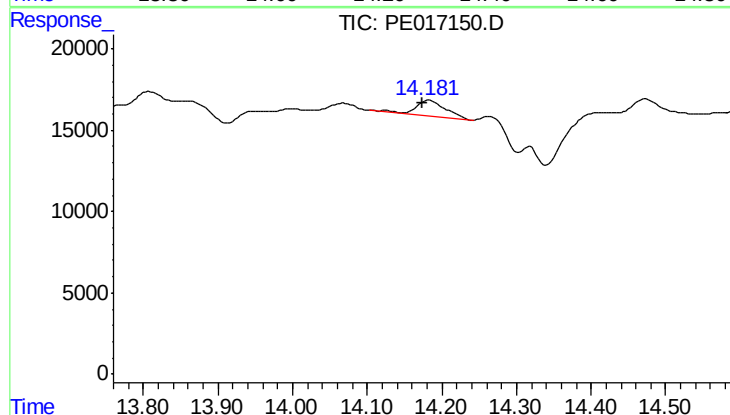


#13 2,4-DB

R.T.: 14.182 min
Delta R.T.: 0.008 min
Response: 27342
Conc: 374.09 ng/ml

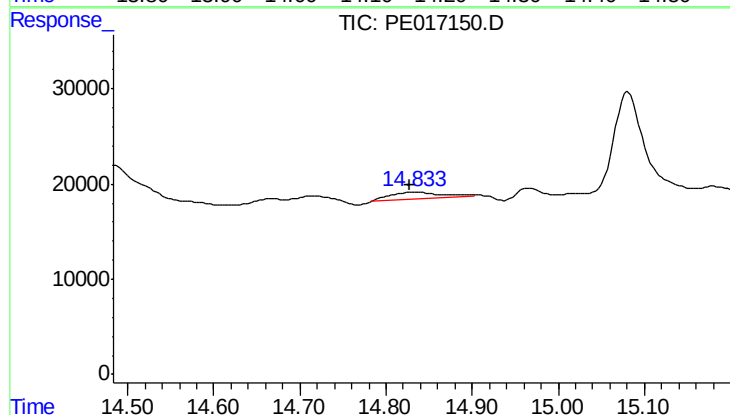

#13 2,4-DB


R.T.: 14.836 min
Delta R.T.: 0.008 min
Response: 30099
Conc: 284.67 ng/ml

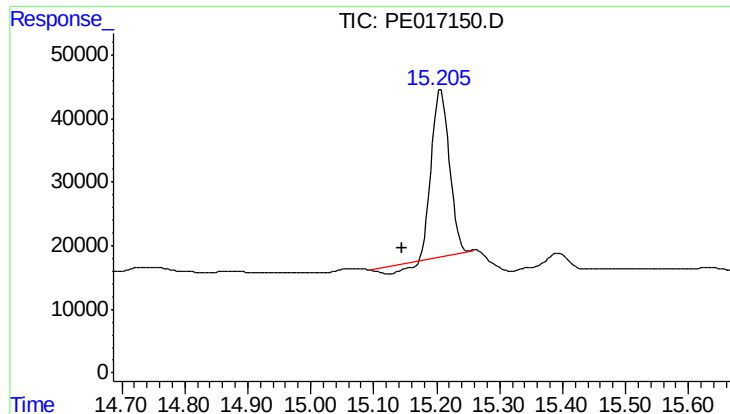

#15 Picloram


R.T.: 15.207 min
Delta R.T.: 0.061 min
Response: 499046
Conc: 936.86 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-RR2MS

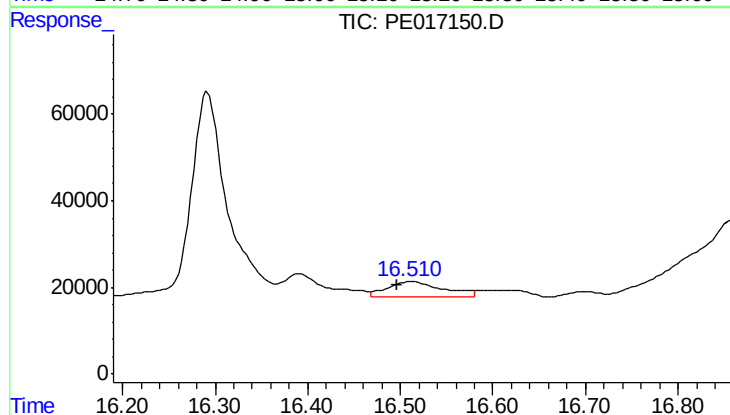


#15 Picloram

R.T.: 16.512 min
Delta R.T.: 0.016 min
Response: 150160
Conc: 132.38 ng/ml

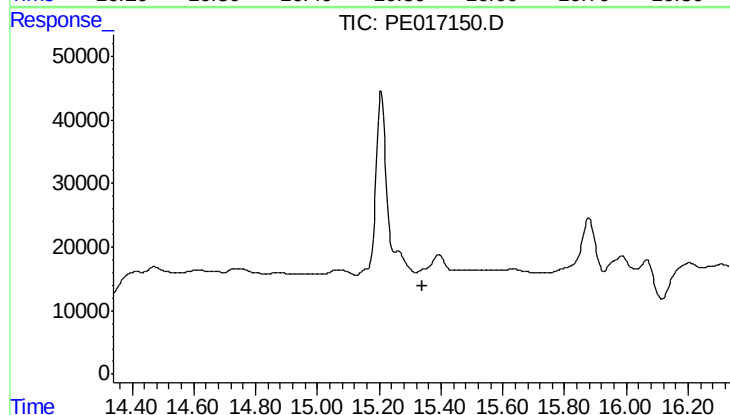

#16 DCPA

R.T.: 15.393 min
Delta R.T.: 0.054 min
Response: -1489
Conc: N.D.

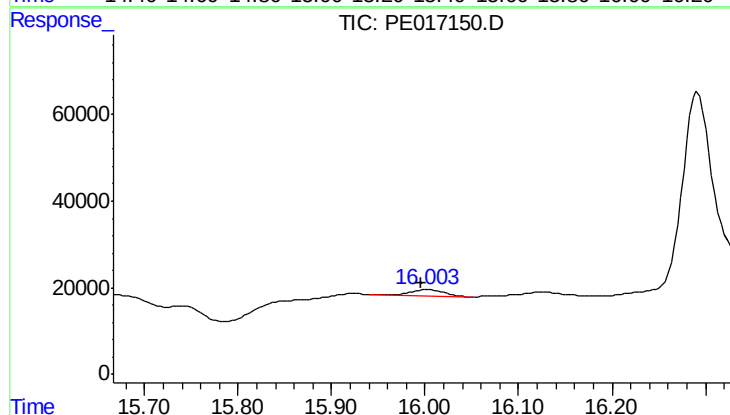

#16 DCPA

R.T.: 16.003 min
Delta R.T.: 0.007 min
Response: 34196
Conc: 23.68 ng/ml