

Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
 Data File : PE017152.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2017 9:41
 Operator : UA/AJ
 Sample : I5567-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 HP-FL1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 17:35:57 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 13 07:26:24 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
 Signal #1 Info : 30M x 0.25mm x 0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	10.437	0.000	30822	0	327.247	N.D.	#
Target Compounds								
3) T	4-Nitroph...	9.518	0.000	82302	0	1368.777	N.D.	#
8) T	DICHLORPROP	0.000	12.161	0	88961	N.D.	534.648	#
9) T	2,4-D	0.000	12.709	0	49062	N.D.	244.287	#
10) T	Pentachlo...	13.008	13.409	37083	32874	27.854	14.970	#
12) T	2,4,5-T	13.504	14.238	41768	32851	88.492	36.166	#
13) T	2,4-DB	14.178	14.833	25311	35458	346.300	335.356	#
14) T	DINOSEB	0.000	14.704	0	44784	N.D.	60.777	#
15) T	Picloram	15.162	16.513	16652	201638	31.261	177.760	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
Data File : PE017152.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2017 9:41
Operator : UA/AJ
Sample : I5567-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
HP-FL1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 17:35:57 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
Quant Title : 8080.M
QLast Update : Fri Oct 13 07:26:24 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

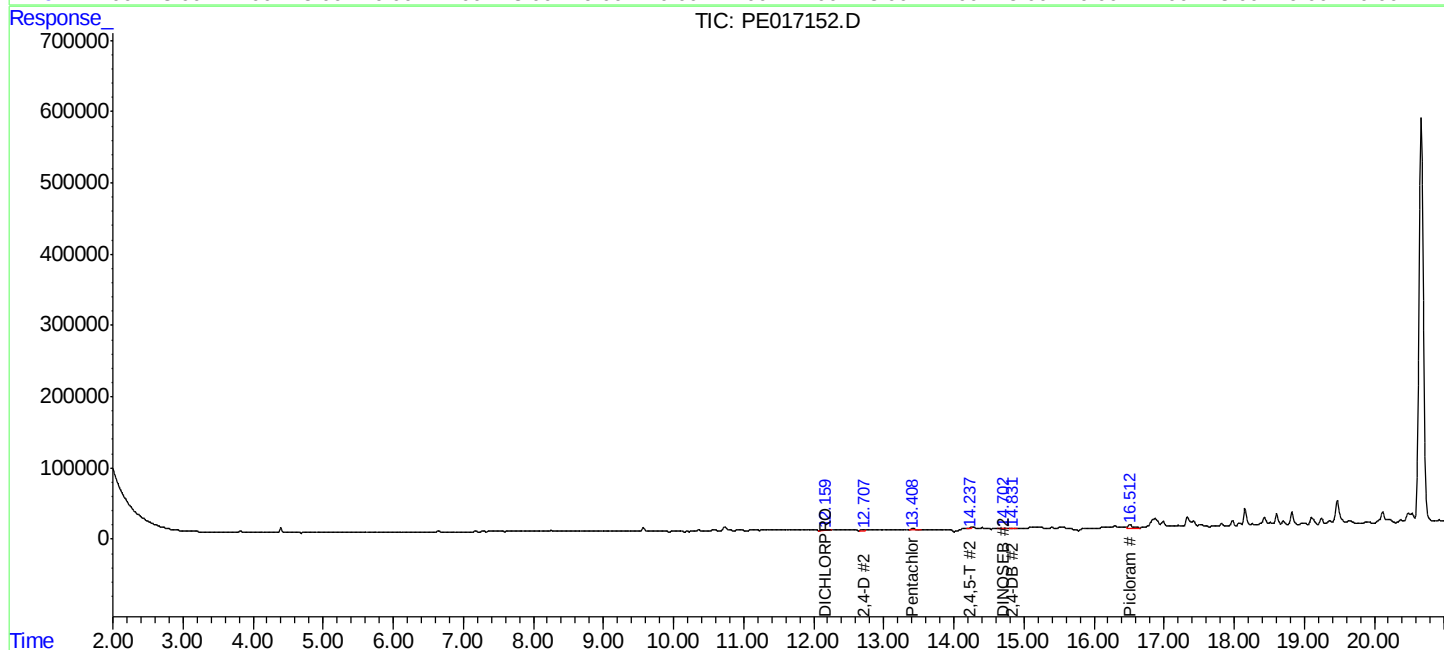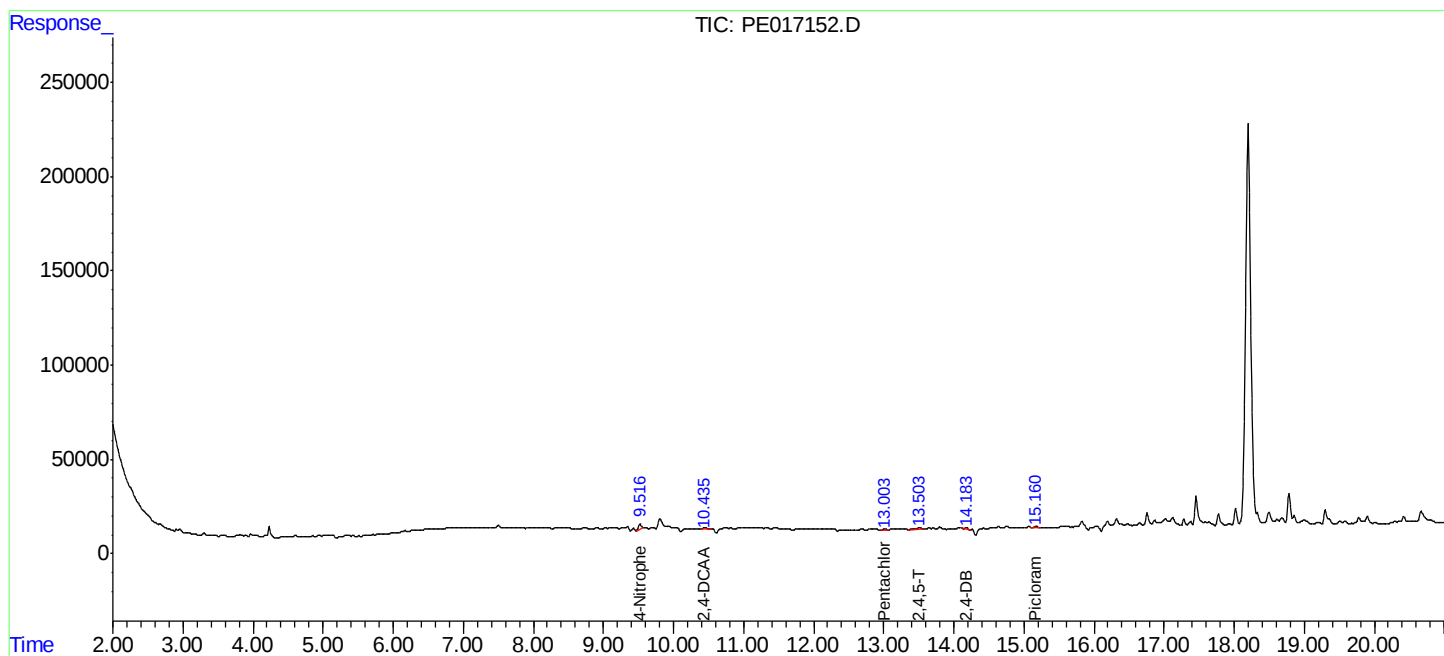


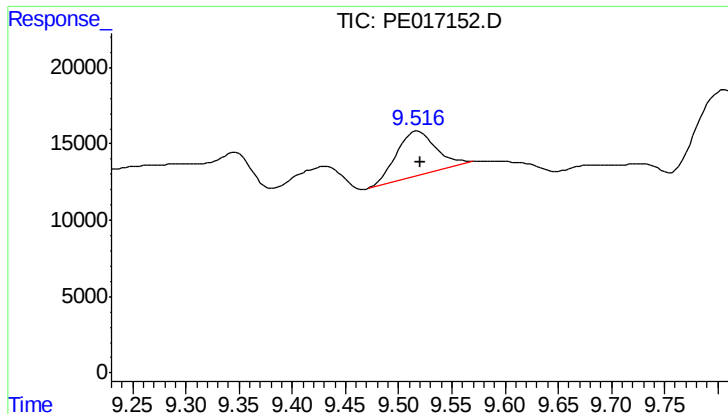

#3 4-Nitrophenol


R.T.: 9.518 min
Delta R.T.: -0.003 min
Response: 82302
Conc: 1368.78 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-FL1

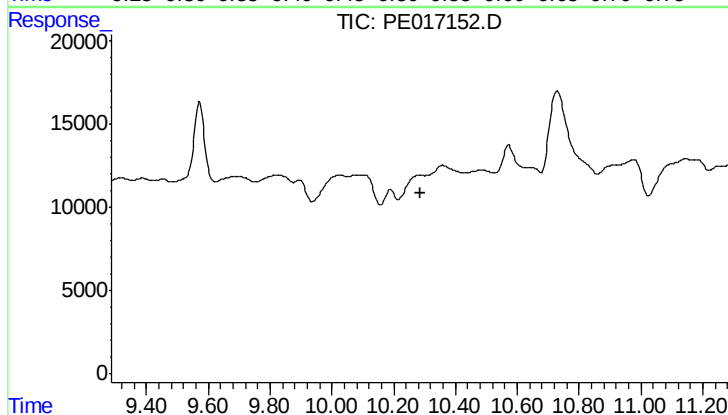


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.286 min
Response: 0
Conc: N.D.

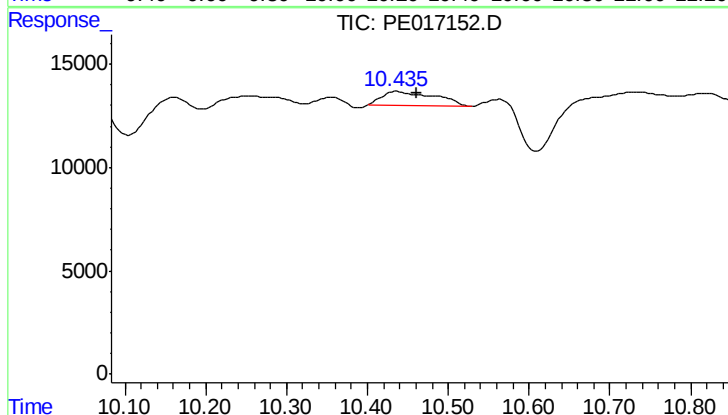


#4 2,4-DCAA

R.T.: 10.437 min
Delta R.T.: -0.024 min
Response: 30822
Conc: 327.25 ng/ml

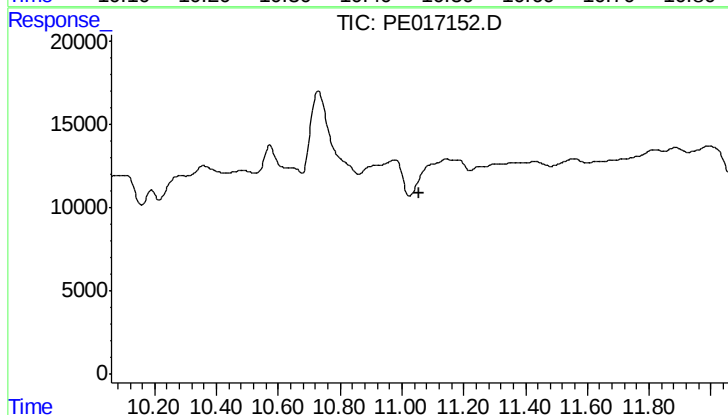

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.058 min
Response: 0
Conc: N.D.

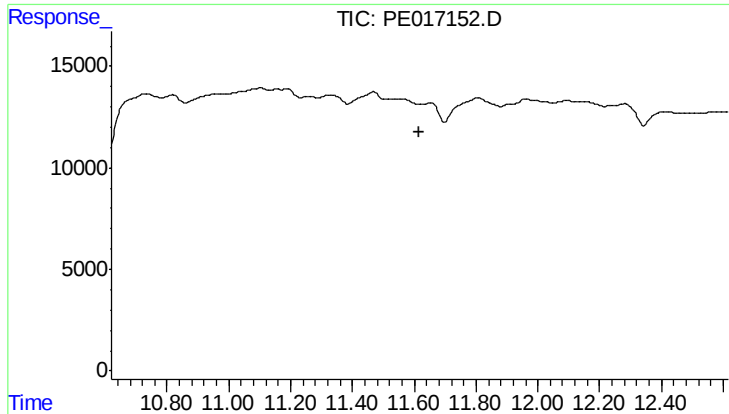

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 11.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HP-FL1

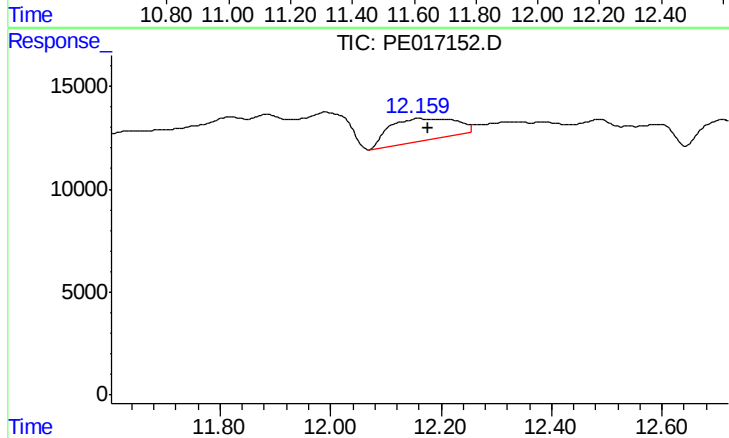


#8 DICHLORPROP

R.T.: 12.161 min
Delta R.T.: -0.015 min
Response: 88961
Conc: 534.65 ng/ml

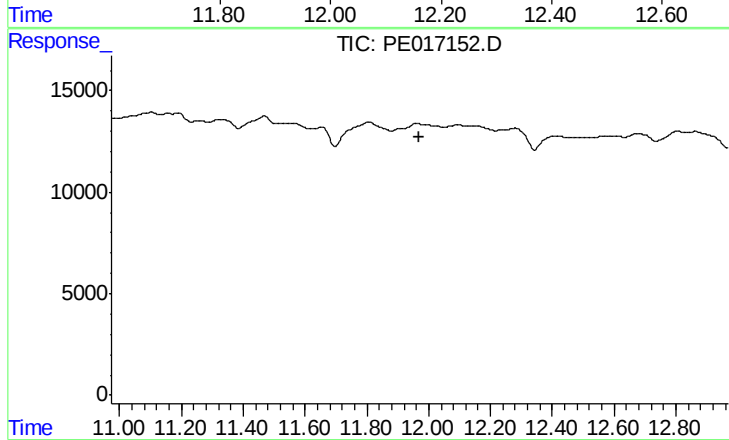


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 11.971 min
Response: 0
Conc: N.D.

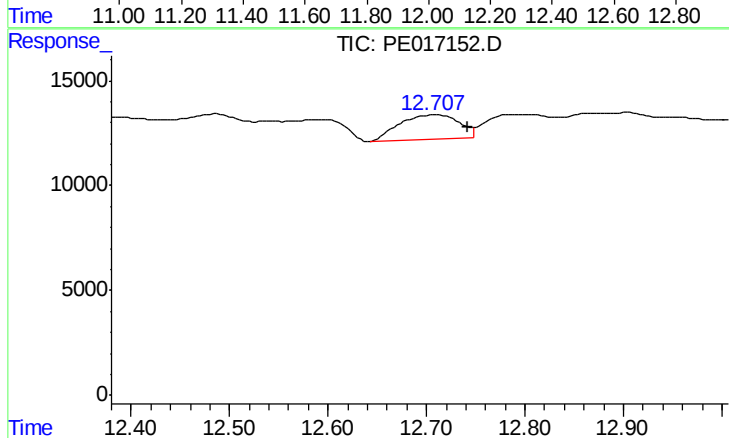

#9 2,4-D


R.T.: 12.709 min
Delta R.T.: -0.033 min
Response: 49062
Conc: 244.29 ng/ml

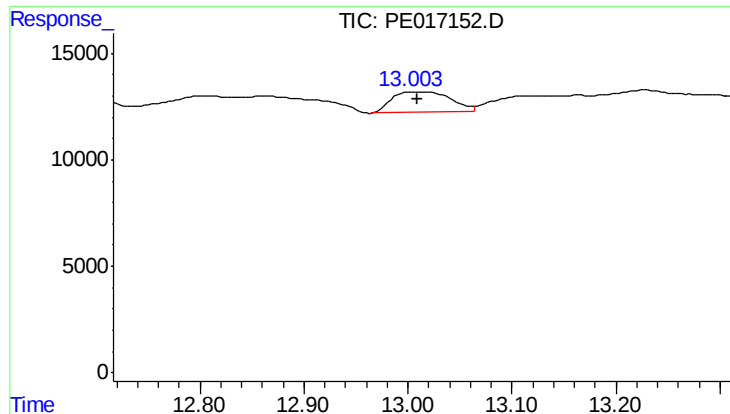

#10 Pentachlorophenol


R.T.: 13.008 min
Delta R.T.: -0.001 min
Response: 37083
Conc: 27.85 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-FL1

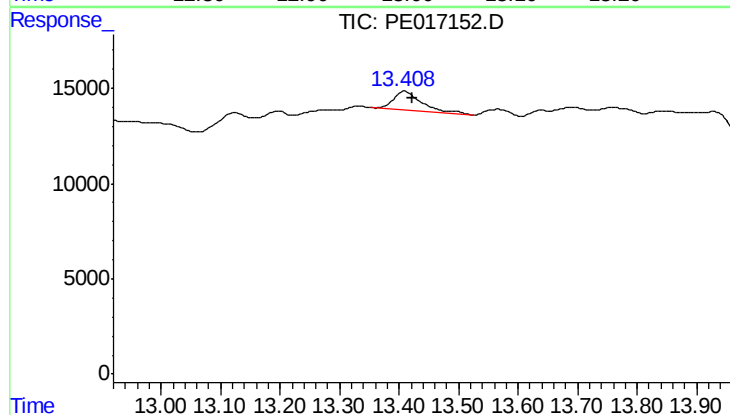


#10 Pentachlorophenol

R.T.: 13.409 min
Delta R.T.: -0.013 min
Response: 32874
Conc: 14.97 ng/ml

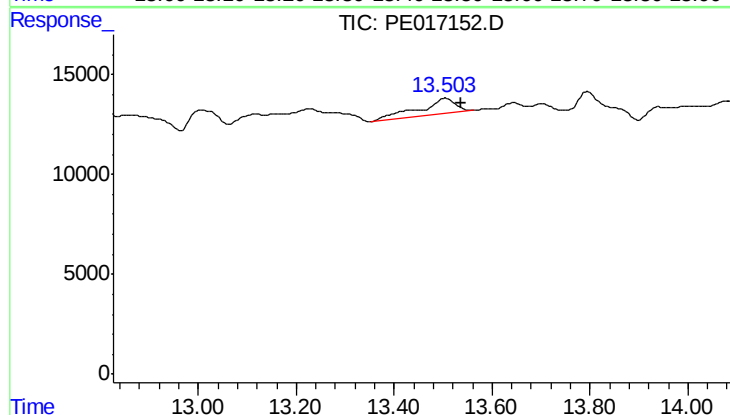


#12 2,4,5-T

R.T.: 13.504 min
Delta R.T.: -0.032 min
Response: 41768
Conc: 88.49 ng/ml

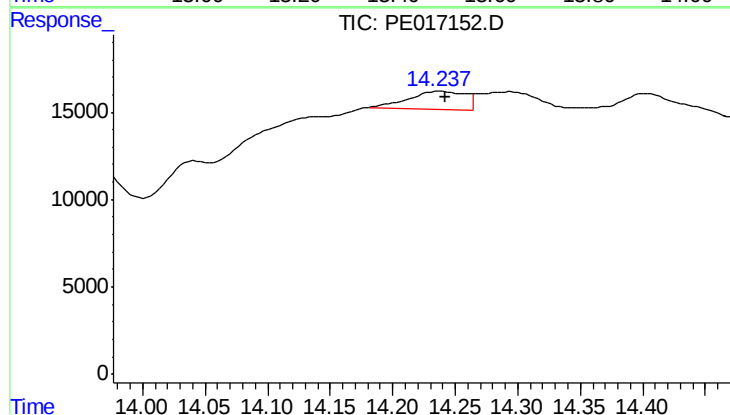

#12 2,4,5-T


R.T.: 14.238 min
Delta R.T.: -0.005 min
Response: 32851
Conc: 36.17 ng/ml

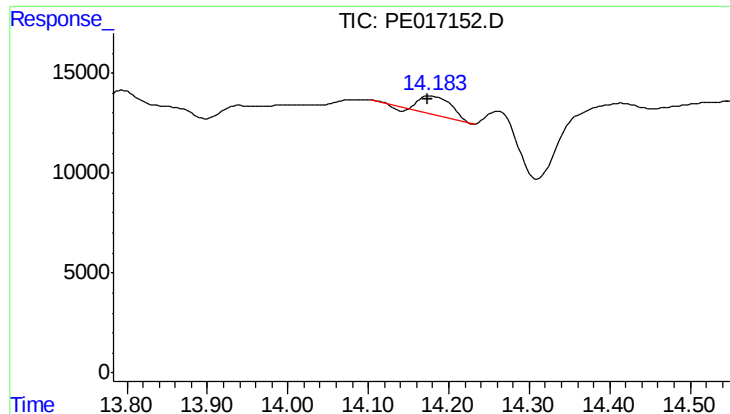

#13 2,4-DB


R.T.: 14.178 min
Delta R.T.: 0.003 min
Response: 25311
Conc: 346.30 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-FL1

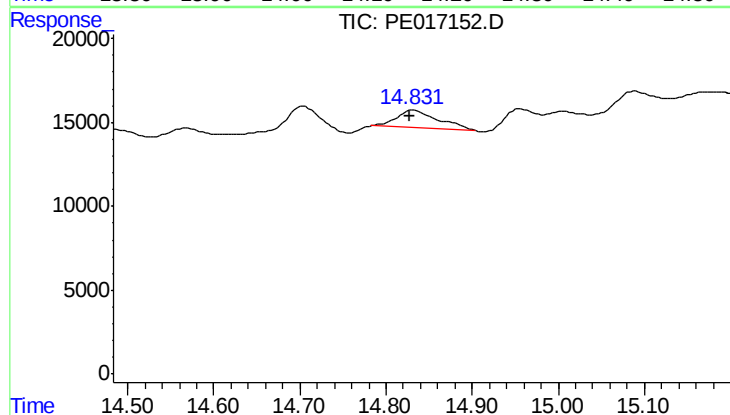


#13 2,4-DB

R.T.: 14.833 min
Delta R.T.: 0.005 min
Response: 35458
Conc: 335.36 ng/ml

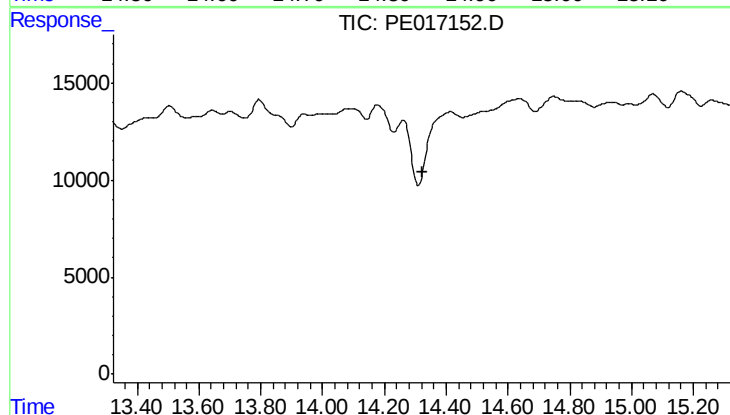


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 14.322 min
Response: 0
Conc: N.D.

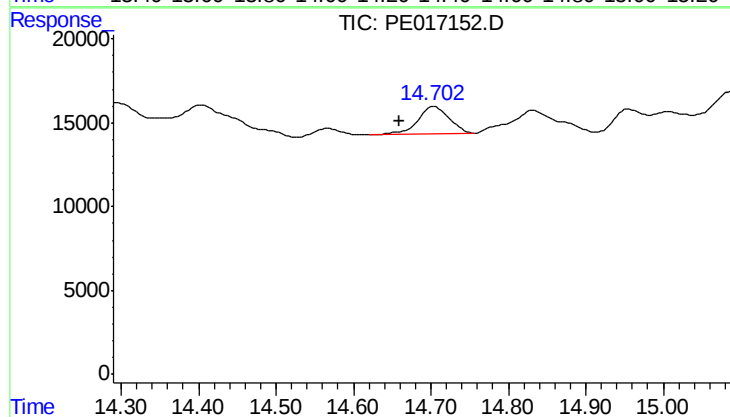

#14 DINOSEB


R.T.: 14.704 min
Delta R.T.: 0.044 min
Response: 44784
Conc: 60.78 ng/ml

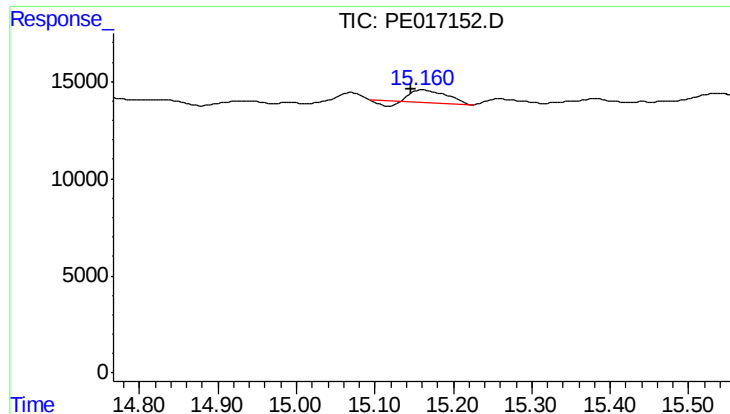

#15 Picloram

R.T.: 15.162 min
Delta R.T.: 0.016 min
Response: 16652
Conc: 31.26 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-FL1

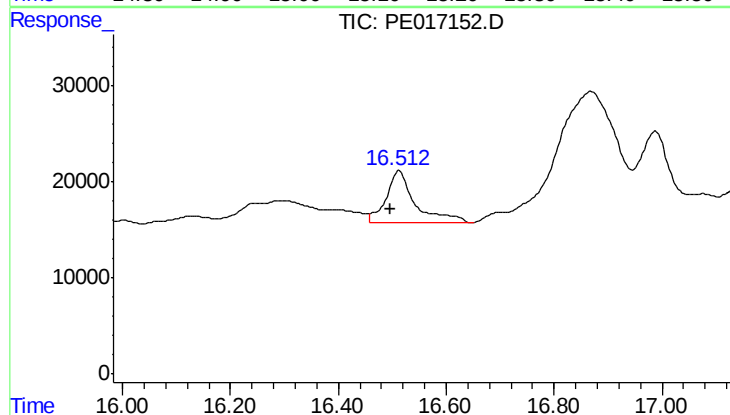

#15 Picloram

R.T.: 16.513 min
Delta R.T.: 0.017 min
Response: 201638
Conc: 177.76 ng/ml