

Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
 Data File : PE017153.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Oct 2017 10:10
 Operator : UA/AJ
 Sample : I5567-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :
 HP-FL2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 13 17:36:09 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 13 07:26:24 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Infernon
 Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	10.440	0.000	15598	0	165.608	N.D. #
Target Compounds							
3) T	4-Nitroph...	9.519	0.000	30419	0	505.897	N.D. #
15) T	Picloram	0.000	16.490	0	32911	N.D.	29.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_E\Data\PE101217\
Data File : PE017153.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Oct 2017 10:10
Operator : UA/AJ
Sample : I5567-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :
HP-FL2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 13 17:36:09 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
Quant Title : 8080.M
QLast Update : Fri Oct 13 07:26:24 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

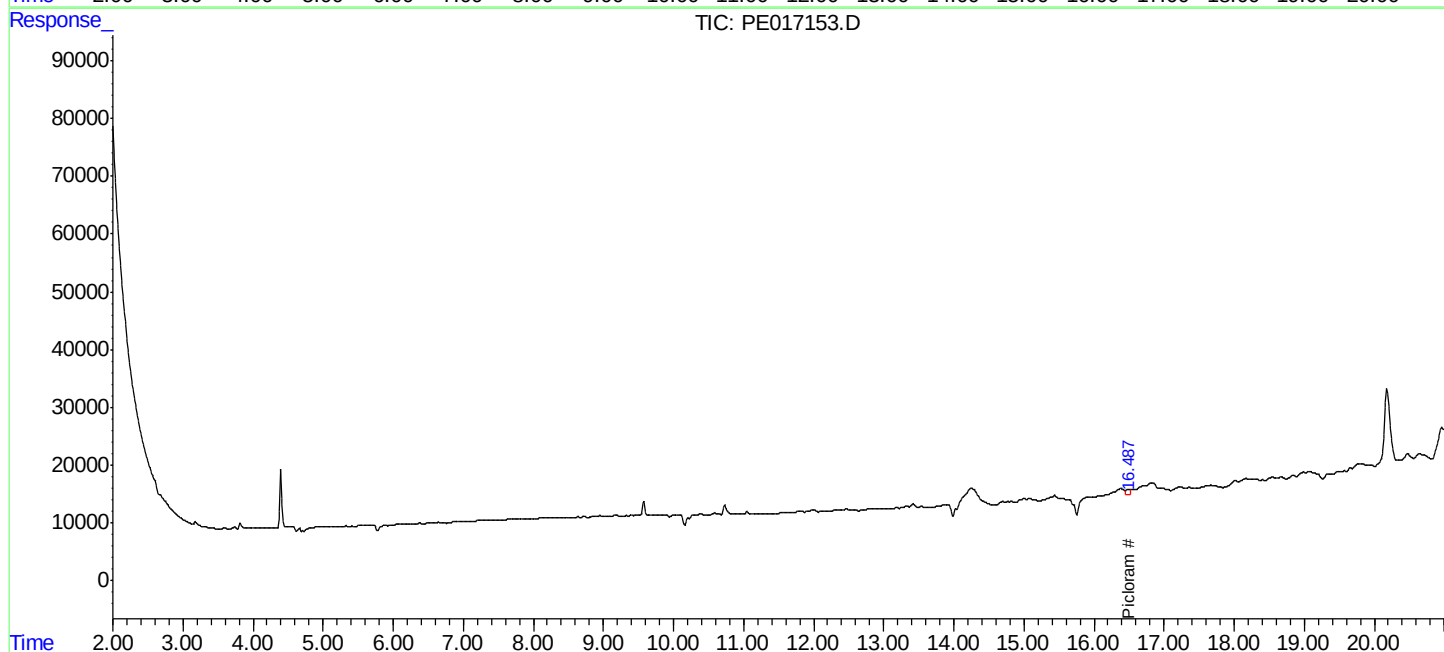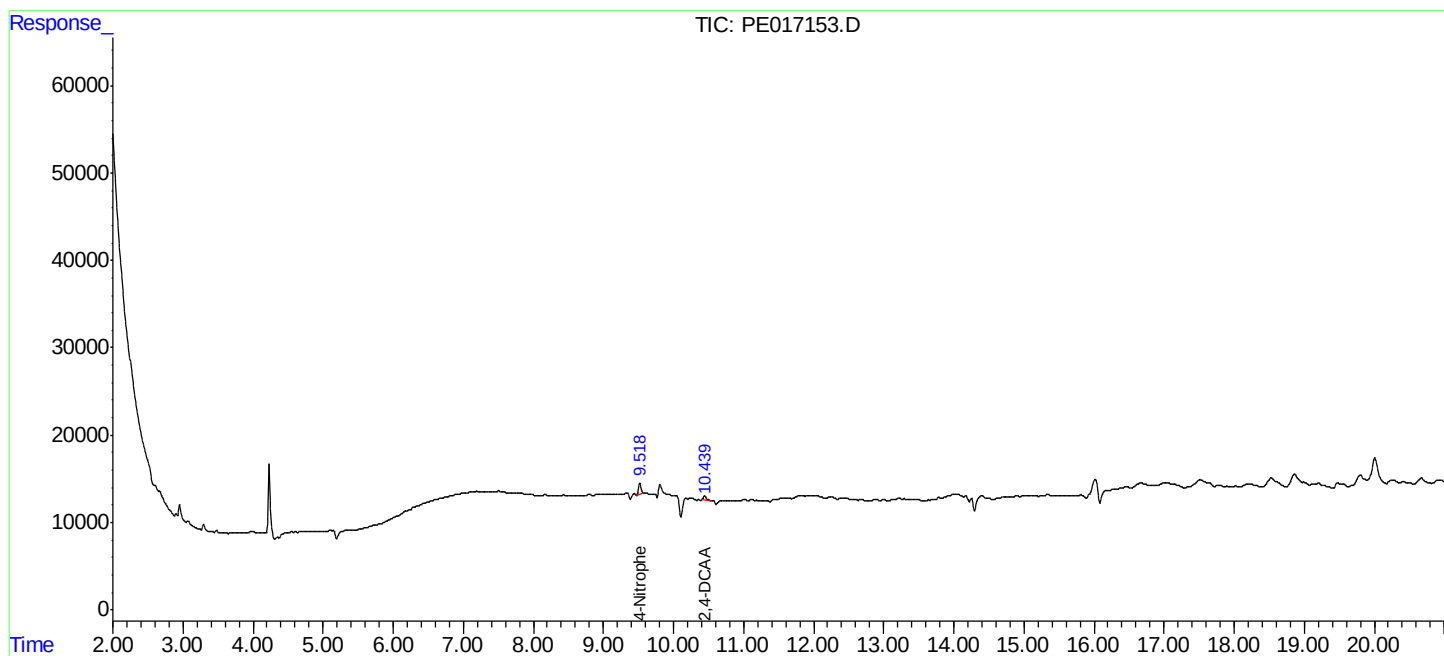


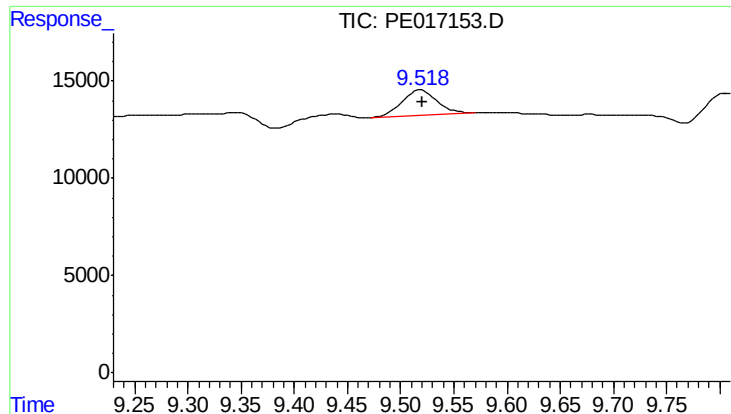

#3 4-Nitrophenol


R.T.: 9.519 min
Delta R.T.: -0.001 min
Response: 30419
Conc: 505.90 ng/ml

Instrument :
ECD_E
ClientSampleId :
HP-FL2

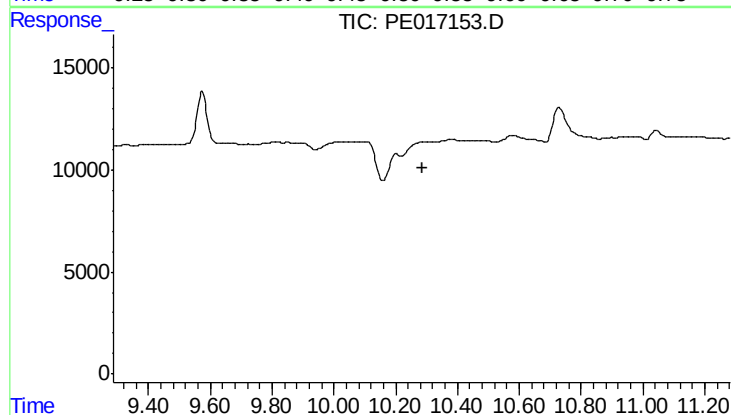


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.286 min
Response: 0
Conc: N.D.

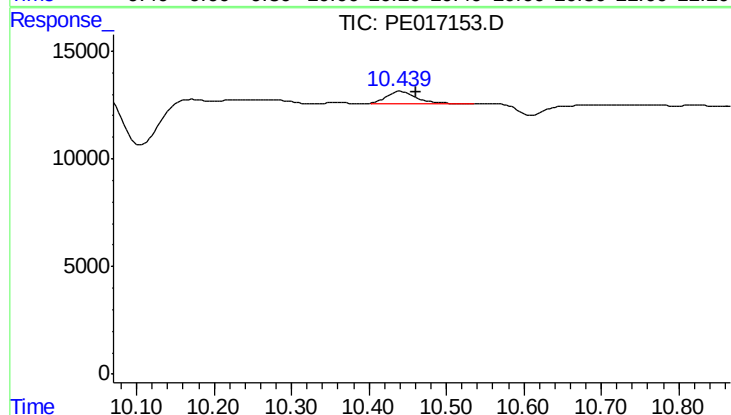


#4 2,4-DCAA

R.T.: 10.440 min
Delta R.T.: -0.021 min
Response: 15598
Conc: 165.61 ng/ml

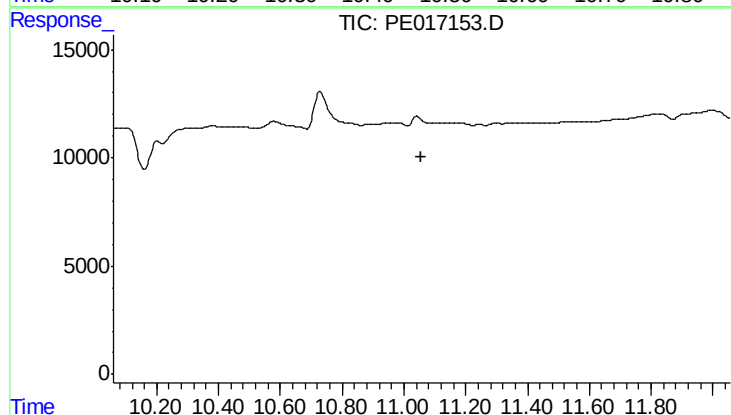

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.058 min
Response: 0
Conc: N.D.

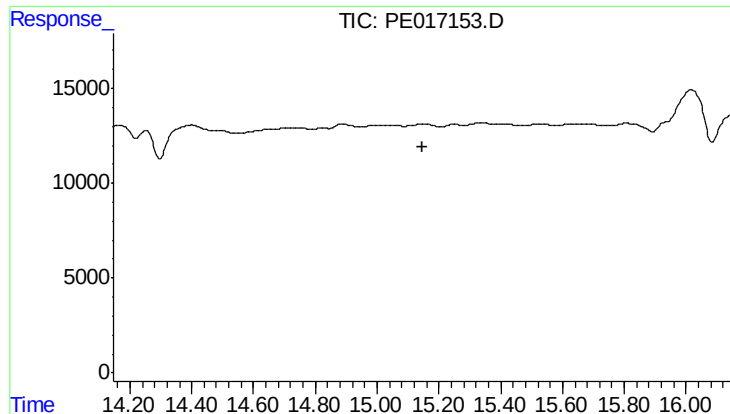

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 15.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :
HP-FL2

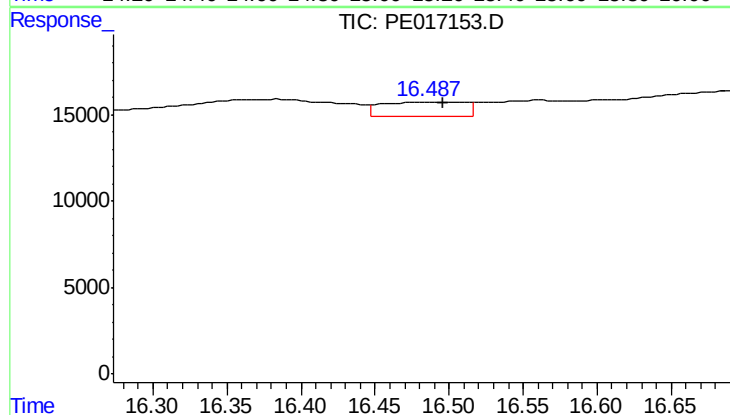

#15 Picloram

R.T.: 16.490 min
Delta R.T.: -0.006 min
Response: 32911
Conc: 29.01 ng/ml