

Data Path : P:\HPCHEM1\ECD E\Data\PE101417\
 Data File : PE017177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Oct 2017 3:14
 Operator : UA/AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 04:51:49 2017
 Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 13 07:26:24 2017
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
 Signal #1 Info : 30M x 0.25mm x 0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	10.515	0.000	100864	0	1070.908	N.D. #
Target Compounds							
1) T	Dalapon	0.000	3.203	0	74982	N.D.	285.363 #
2) T	3,5-DICHL...	0.000	9.354	0	163915	N.D.	700.071 #
3) T	4-Nitroph...	0.000	10.228	0	79781	N.D.	765.427 #
5) T	DICAMBA	10.515	0.000	100864	0	286.913	N.D. #
8) T	DICHLORPROP	0.000	12.120	0	131466	N.D.	790.099 #
9) T	2,4-D	0.000	12.685	0	164427	N.D.	818.714 #
10) T	Pentachlo...	13.062	0.000	467991	0	351.518	N.D. #
11) T	2,4,5-TP ...	13.062	13.552	467991	686856	810.925	835.177
12) T	2,4,5-T	13.484	0.000	441760	0	935.933	N.D. #
14) T	DINOSEB	0.000	14.611	0	560762	N.D.	761.026 #
15) T	Picloram	0.000	16.448	0	843274	N.D.	743.415 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD E\Data\PE101417\
Data File : PE017177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Oct 2017 3:14
Operator : UA/AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 04:51:49 2017
Quant Method : P:\HPCHEM1\ECD_E\Method\PE101217.M
Quant Title : 8080.M
QLast Update : Fri Oct 13 07:26:24 2017
Response via : Initial Calibration
Integrator: ChemStation

Volume Ini. : 2 µl
Signal #1 Phase : ZB-35-HT Inferno Signal #2 Phase: ZB-XLB-HT Inferno
Signal #1 Info : 30M x 0.25mm x0.2 Signal #2 Info : 30M x 0.25mm x 0.25µm

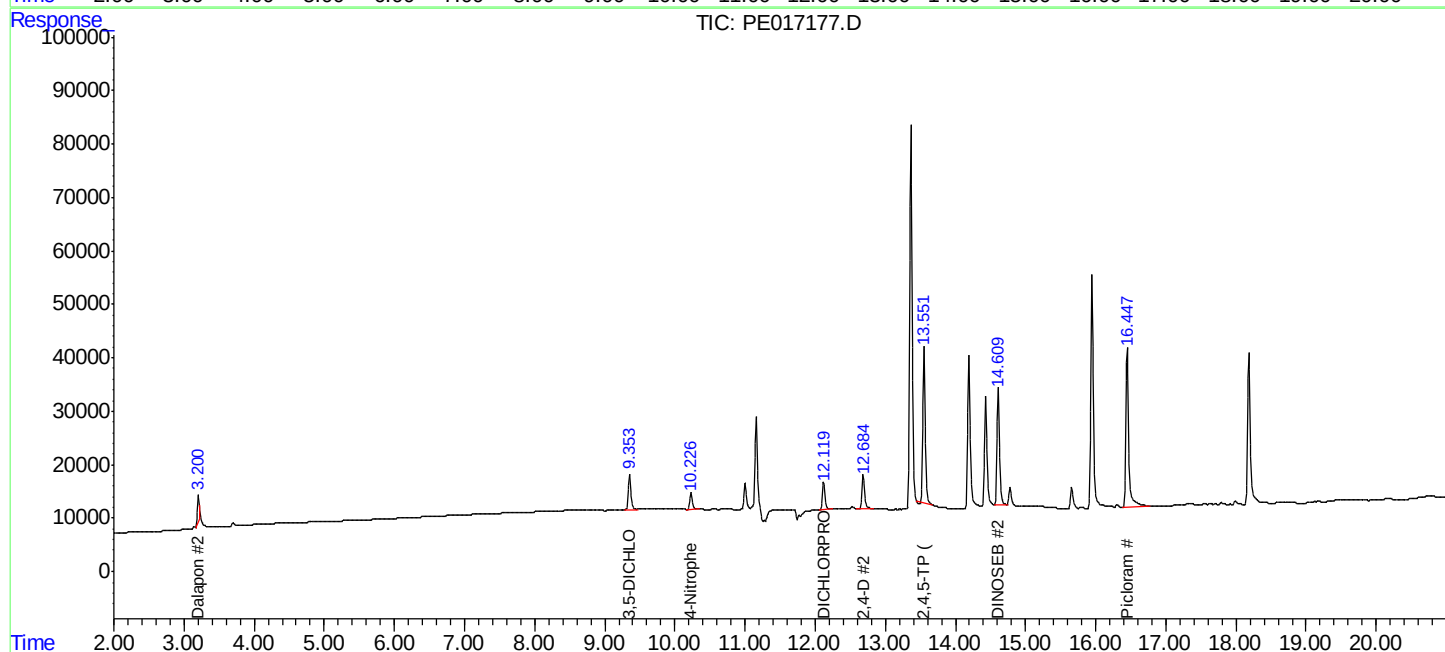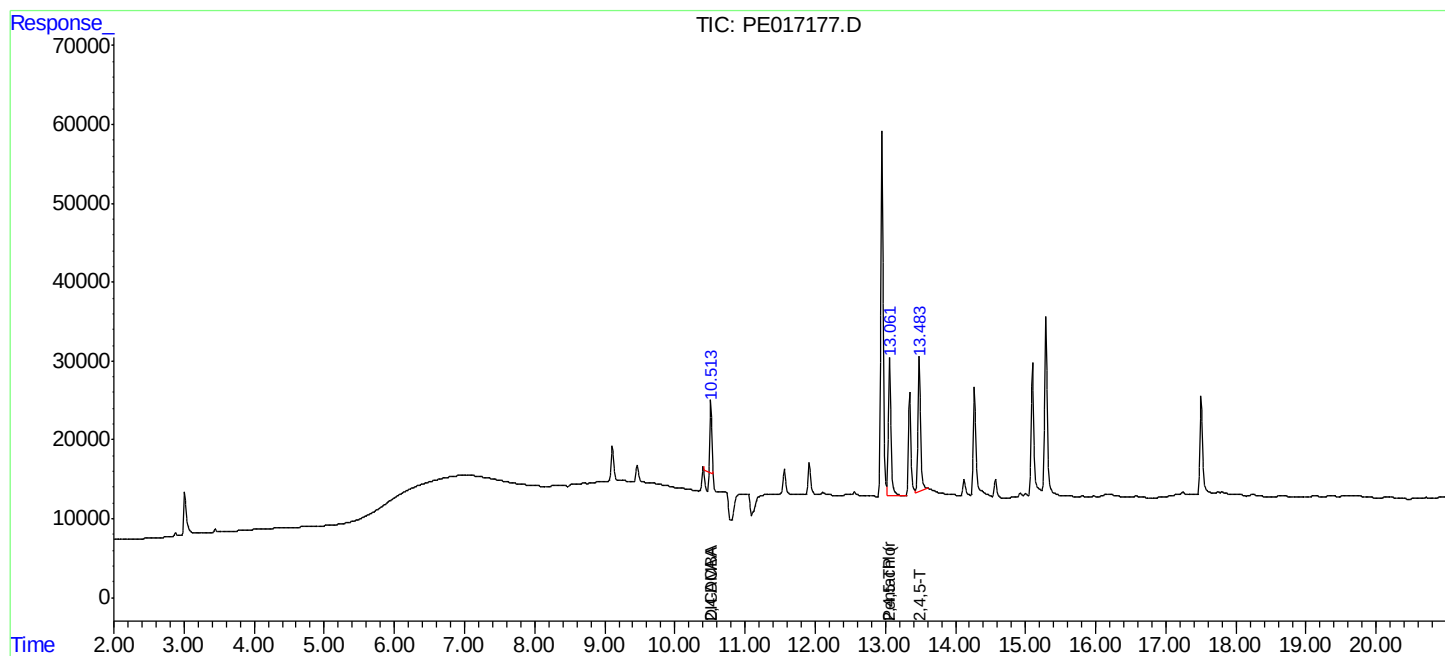


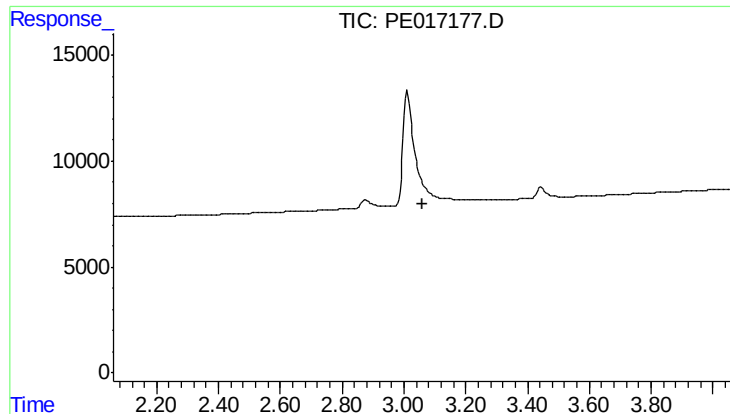

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

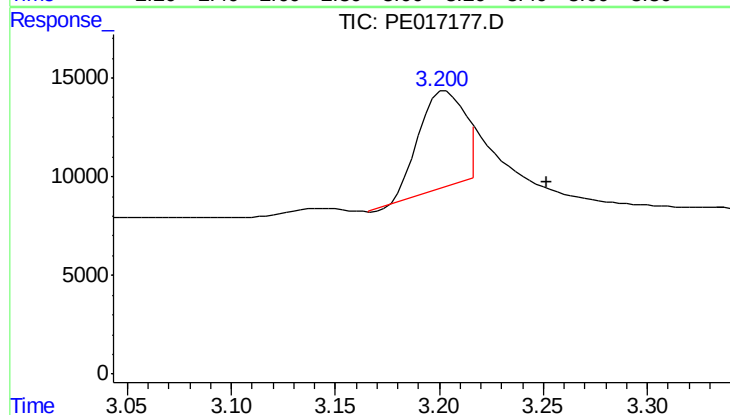


#1 Dalapon

R.T.: 3.203 min
Delta R.T.: -0.048 min
Response: 74982
Conc: 285.36 ng/ml

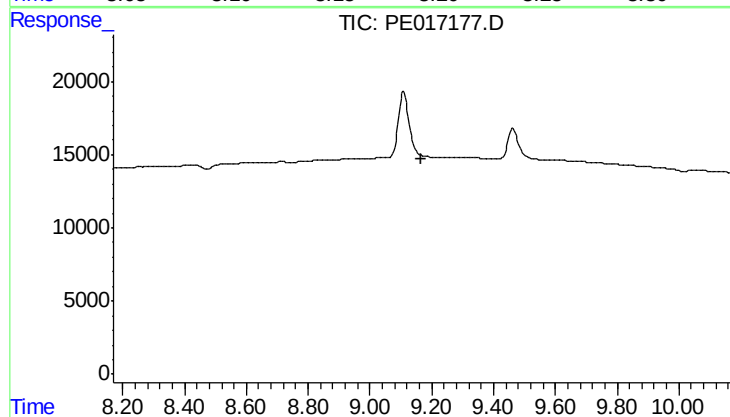


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.167 min
Response: 0
Conc: N.D.

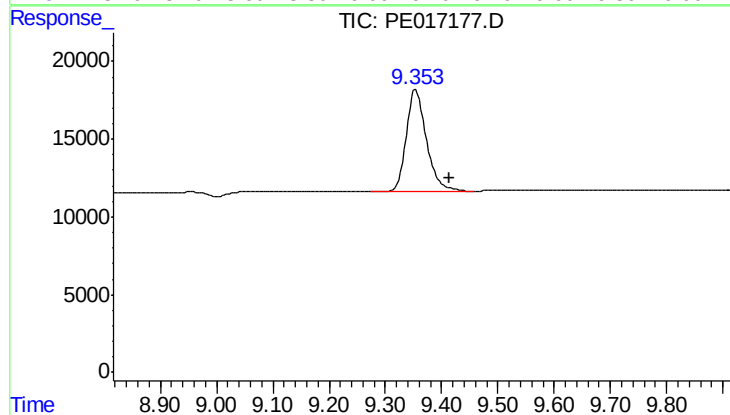

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.354 min
Delta R.T.: -0.059 min
Response: 163915
Conc: 700.07 ng/ml

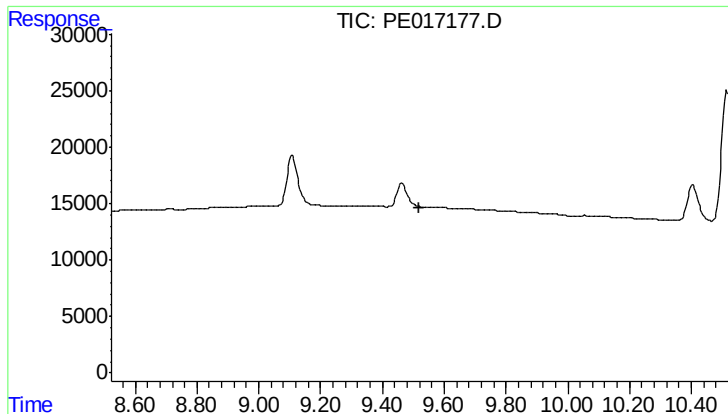

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 9.521 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

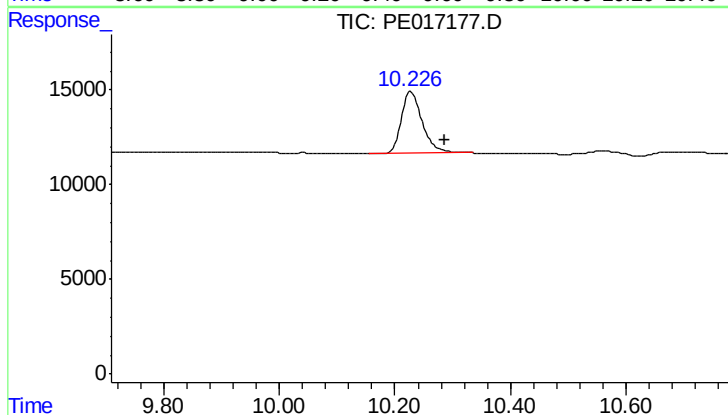


#3 4-Nitrophenol

R.T.: 10.228 min
Delta R.T.: -0.058 min
Response: 79781
Conc: 765.43 ng/ml

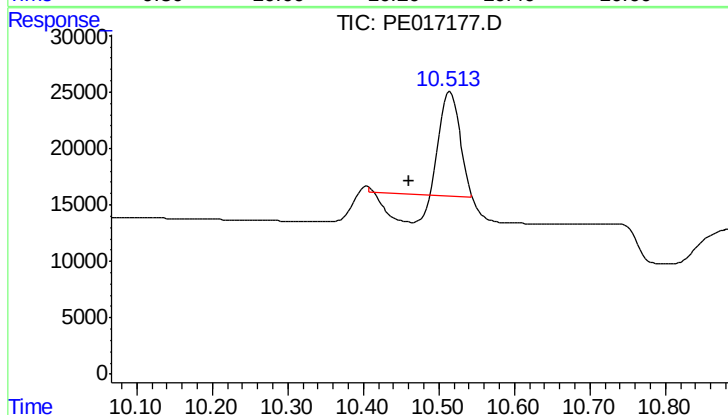


#4 2,4-DCAA

R.T.: 10.515 min
Delta R.T.: 0.054 min
Response: 100864
Conc: 1070.91 ng/ml

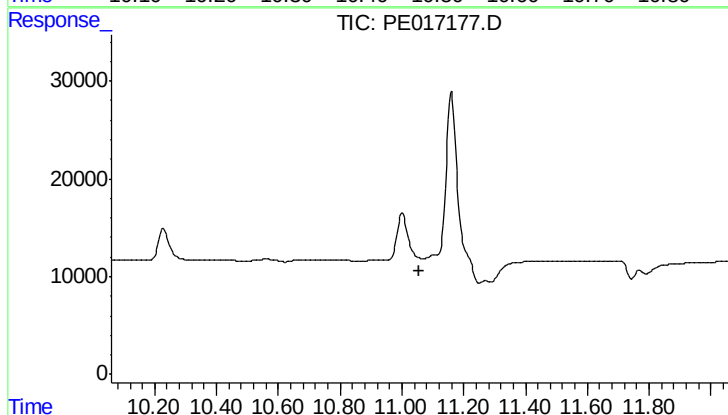

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.058 min
Response: 0
Conc: N.D.

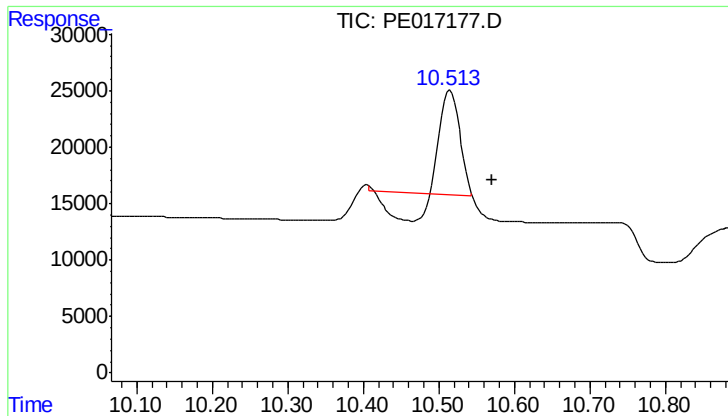

#5 DICAMBA


R.T.: 10.515 min
Delta R.T.: -0.056 min
Response: 100864
Conc: 286.91 ng/ml

Instrument :
ECD_E
ClientSampleId :

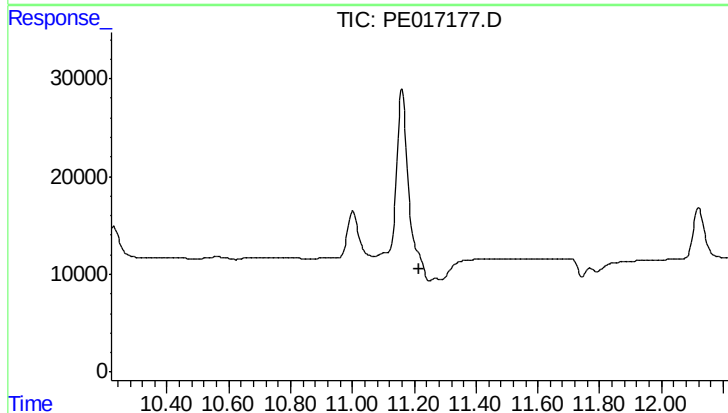


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.217 min
Response: 0
Conc: N.D.

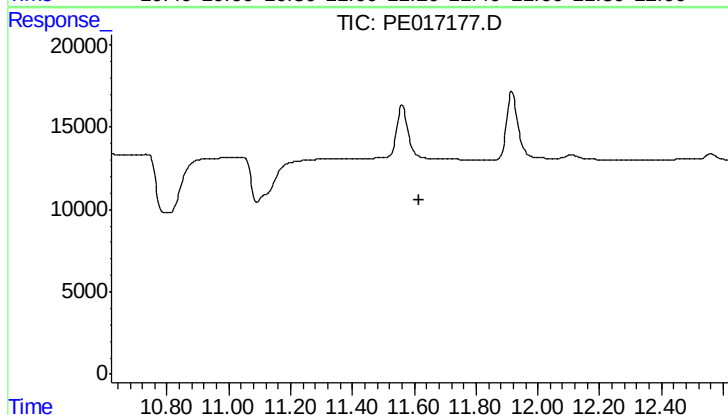


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 11.617 min
Response: 0
Conc: N.D.

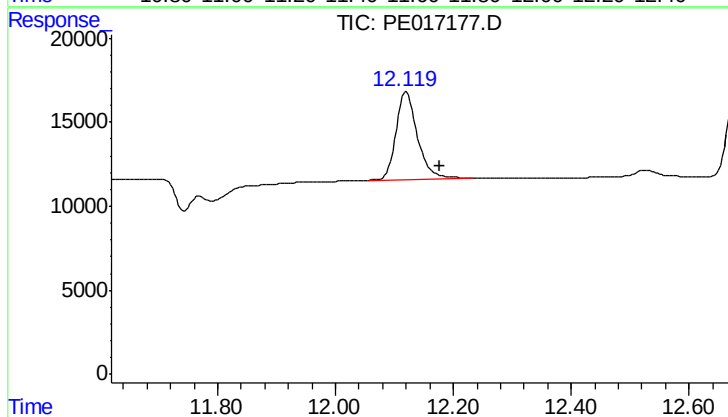

#8 DICHLORPROP


R.T.: 12.120 min
Delta R.T.: -0.056 min
Response: 131466
Conc: 790.10 ng/ml

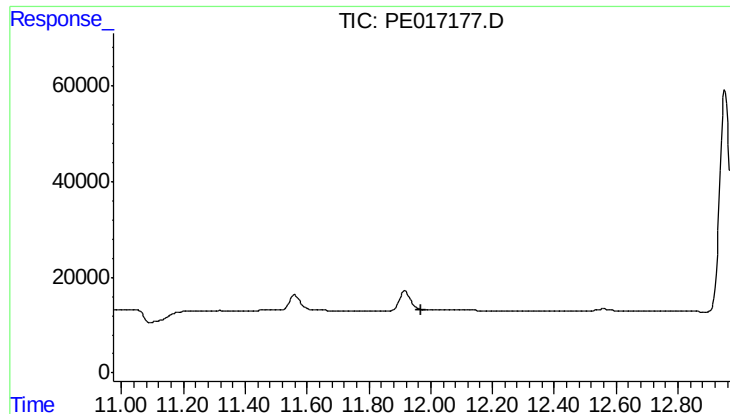

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 11.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

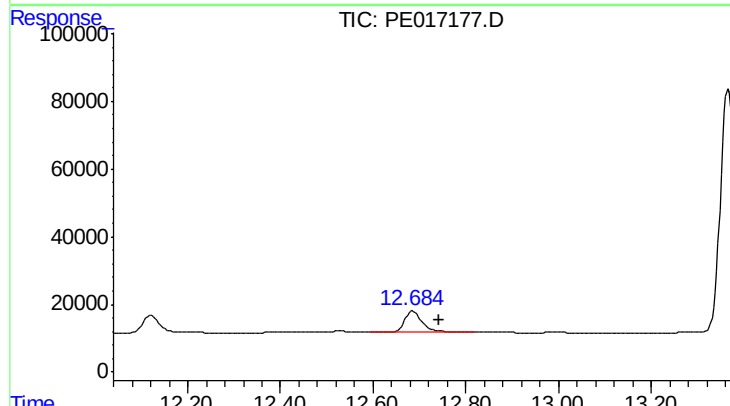


#9 2,4-D

R.T.: 12.685 min
Delta R.T.: -0.057 min
Response: 164427
Conc: 818.71 ng/ml

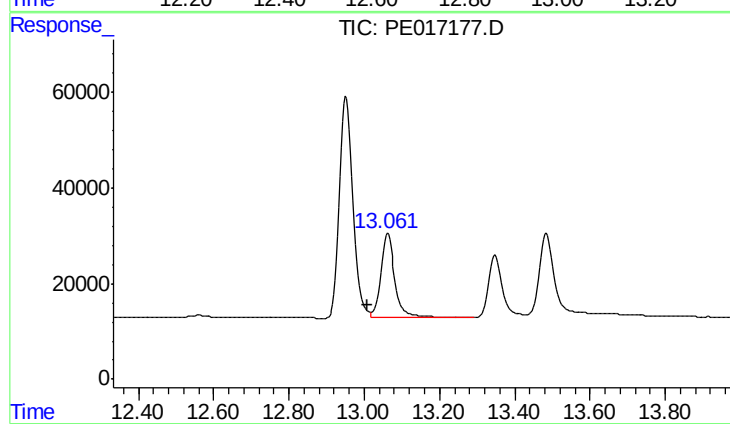


#10 Pentachlorophenol

R.T.: 13.062 min
Delta R.T.: 0.053 min
Response: 467991
Conc: 351.52 ng/ml

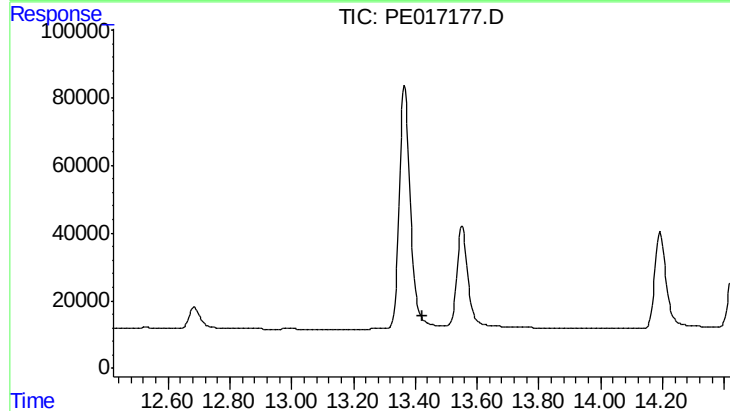

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.423 min
Response: 0
Conc: N.D.

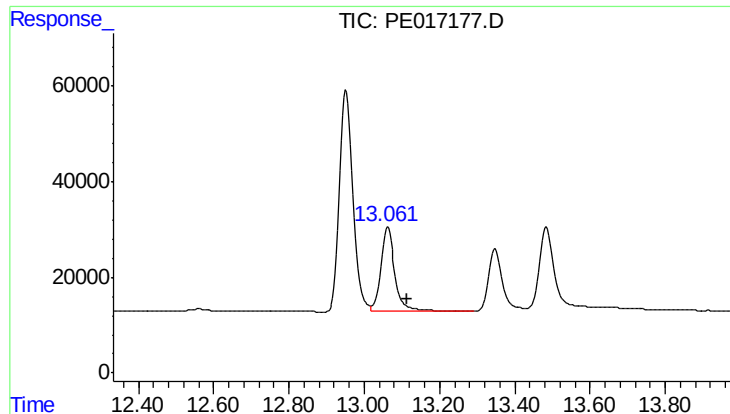

#11 2,4,5-TP (SILVEX)


R.T.: 13.062 min
Delta R.T.: -0.053 min
Response: 467991
Conc: 810.93 ng/ml

Instrument :
ECD_E
ClientSampleId :

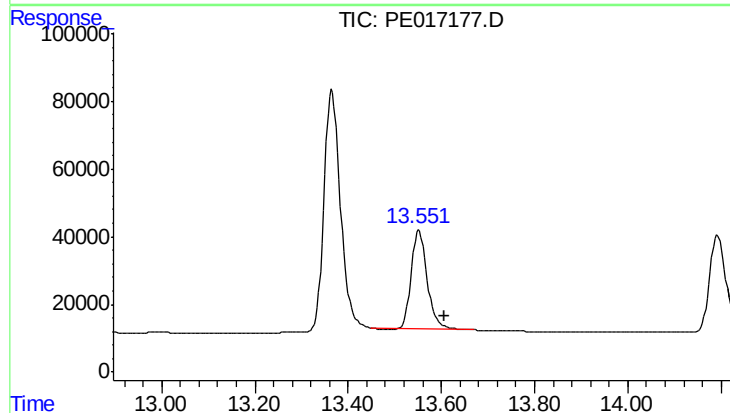


#11 2,4,5-TP (SILVEX)

R.T.: 13.552 min
Delta R.T.: -0.053 min
Response: 686856
Conc: 835.18 ng/ml

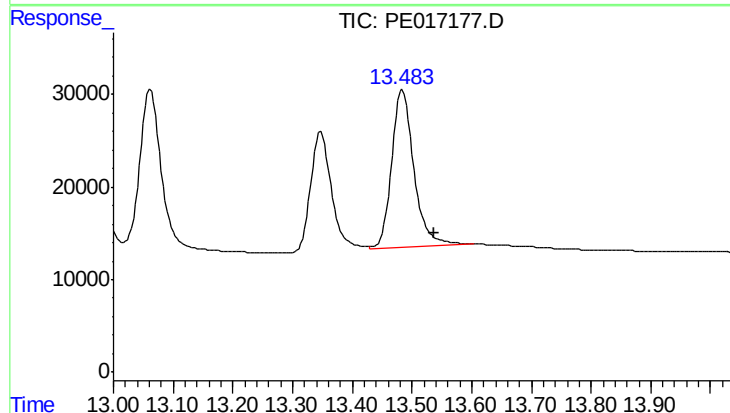


#12 2,4,5-T

R.T.: 13.484 min
Delta R.T.: -0.052 min
Response: 441760
Conc: 935.93 ng/ml

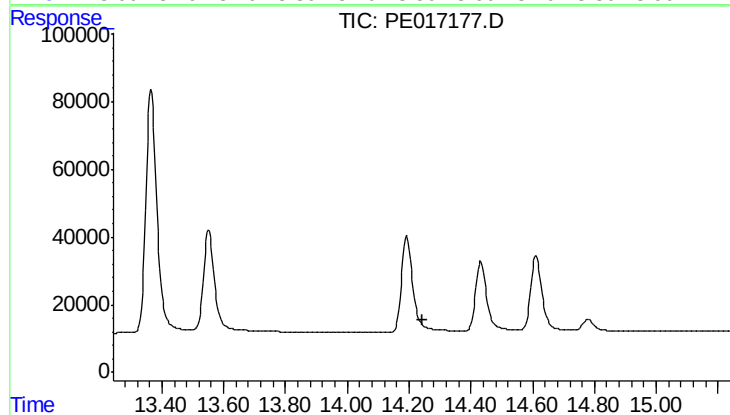

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.243 min
Response: 0
Conc: N.D.

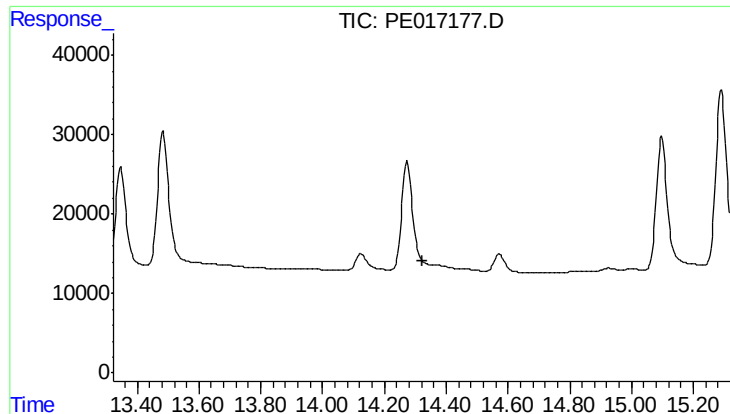

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 14.322 min
Response: 0
Conc: N.D.

Instrument :
ECD_E
ClientSampleId :

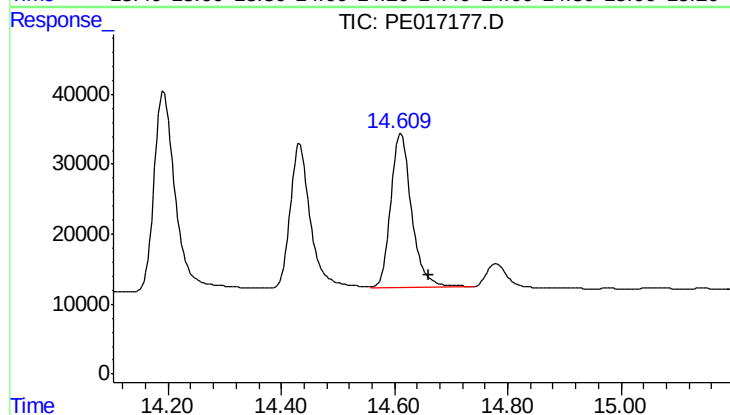


#14 DINOSEB

R.T.: 14.611 min
Delta R.T.: -0.049 min
Response: 560762
Conc: 761.03 ng/ml

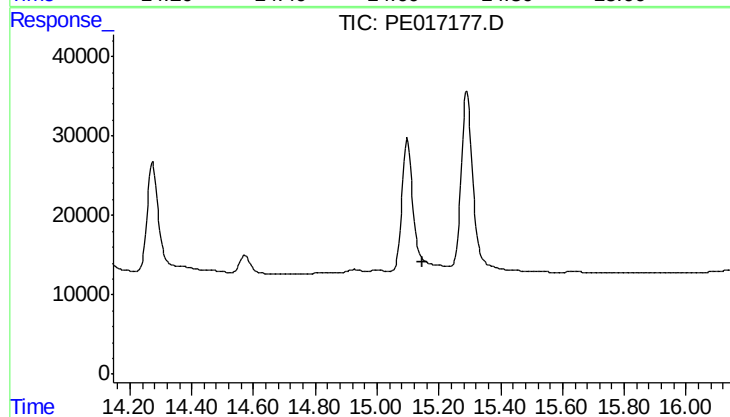

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 15.145 min
Response: 0
Conc: N.D.

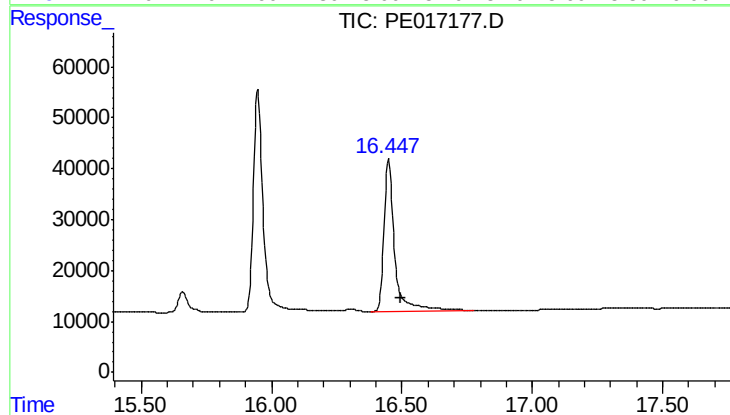

#15 Picloram

R.T.: 16.448 min
Delta R.T.: -0.048 min
Response: 843274
Conc: 743.41 ng/ml