

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010319\
 Data File : FB019246.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jan 2019 9:08
 Operator : MJ/SJ
 Sample : BSF0103S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 03 12:56:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.107	169532	19.396 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	457468	29.924 ng/ml
2) t 2,2,4-Trimethylpentane	7.723	472666	30.681 ng/ml
3) t n-Heptane	8.061	152228	10.242 ng/ml
4) t Benzene	8.201	185037	10.273 ng/ml
6) t Toluene	10.955	470076	30.969 ng/ml
7) t Ethylbenzene	13.405	162705	10.473 ng/ml
8) t m-Xylene	13.538	346121	21.245 ng/ml
9) t O-Xylene	14.270	365157	21.596 ng/ml
10) t 1,2,4-Trimethylbenzene	16.553	426938	21.096 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010319\
Data File : FB019246.D
Signal(s) : FID2B.CH
Acq On : 3 Jan 2019 9:08
Operator : MJ/SJ
Sample : BSF0103S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 03 12:56:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

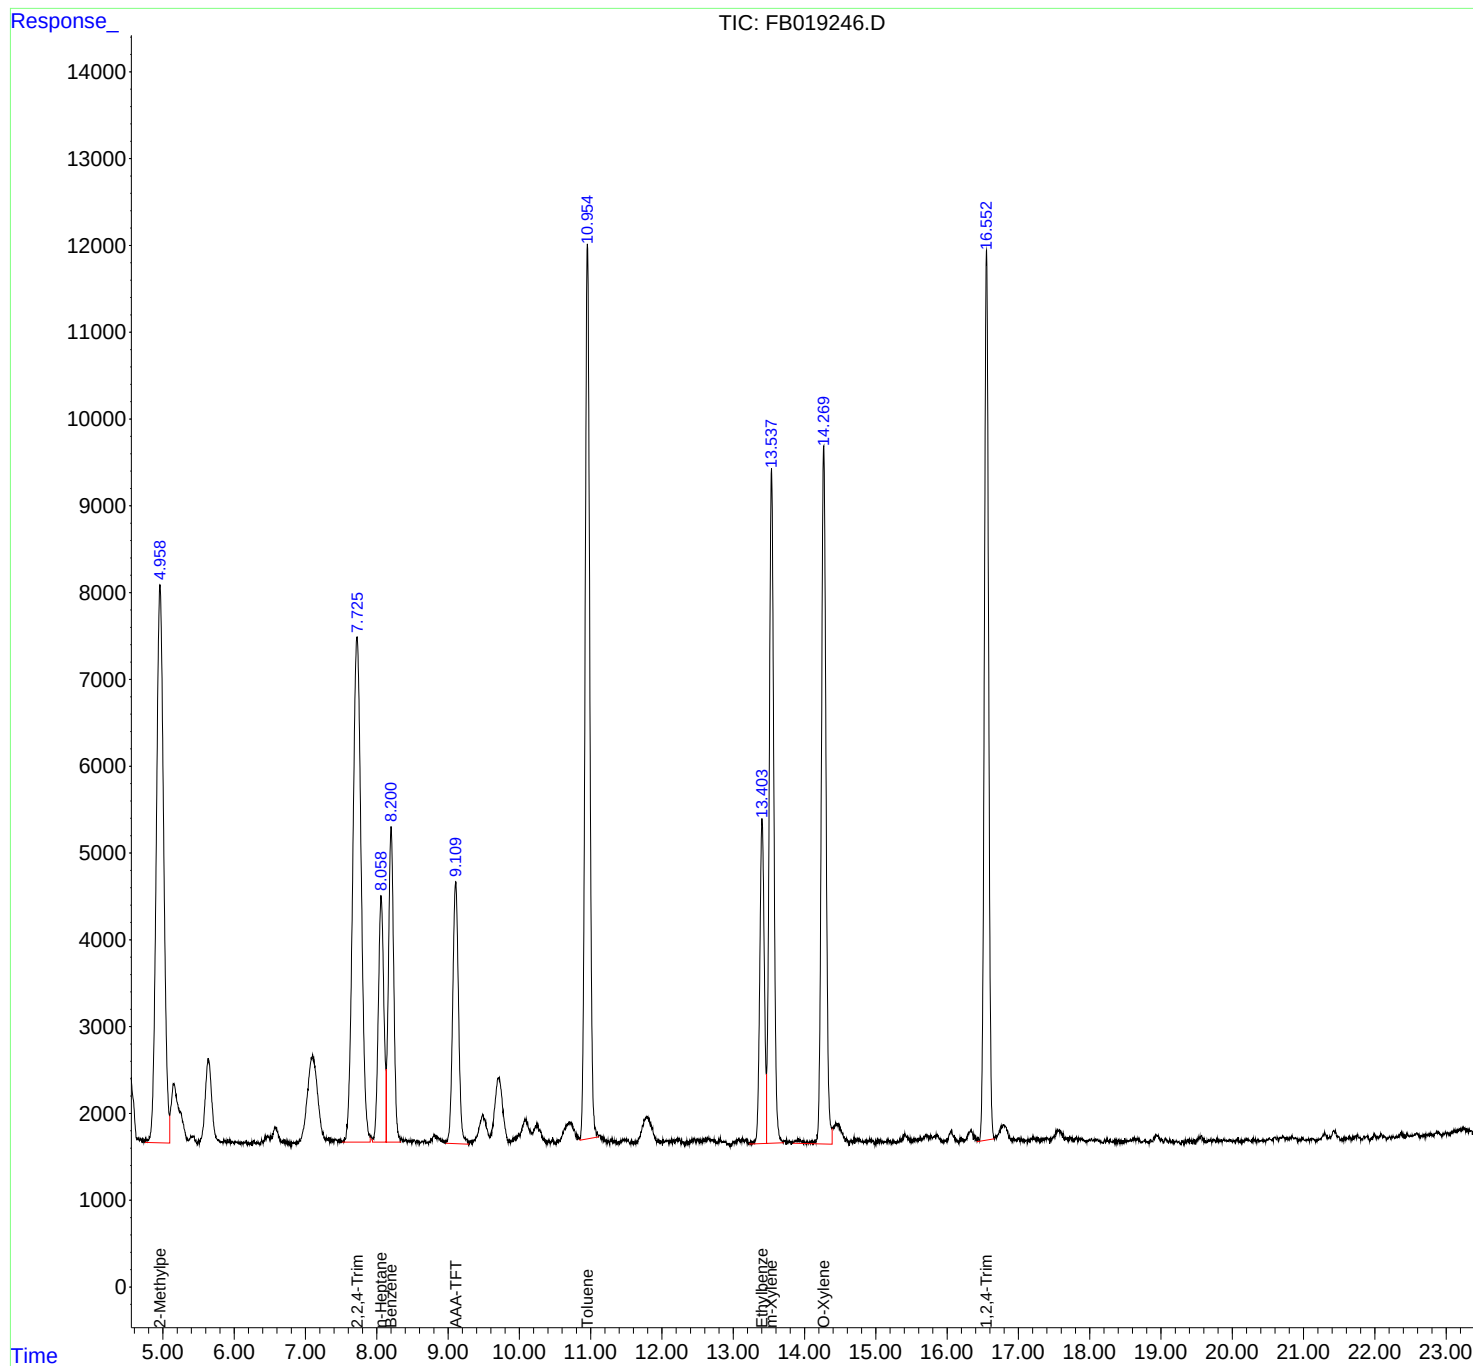


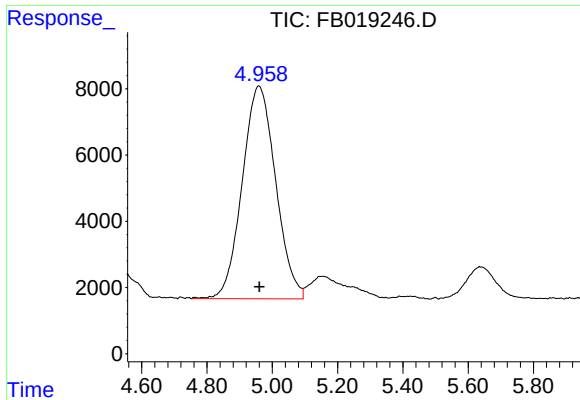

#1 2-Methylpentane


R.T.: 4.960 min
Delta R.T.: -0.001 min
Response: 457468
Conc: 29.92 ng/ml

Instrument :
FID_B
ClientSampleId :

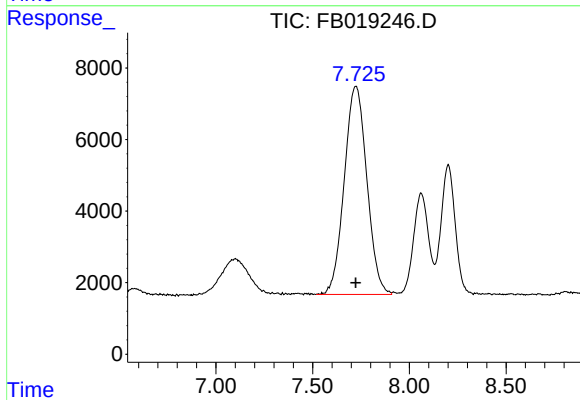


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: 0.000 min
Response: 472666
Conc: 30.68 ng/ml

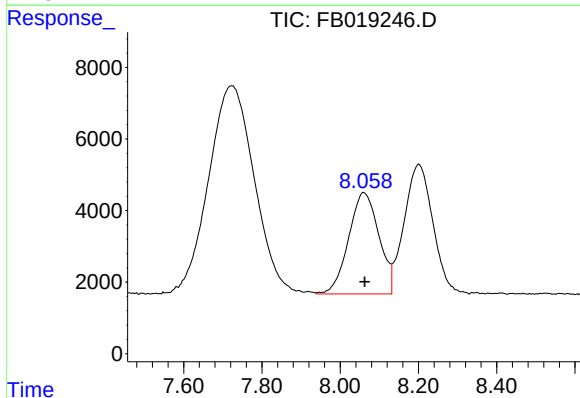


#3 n-Heptane

R.T.: 8.061 min
Delta R.T.: -0.001 min
Response: 152228
Conc: 10.24 ng/ml

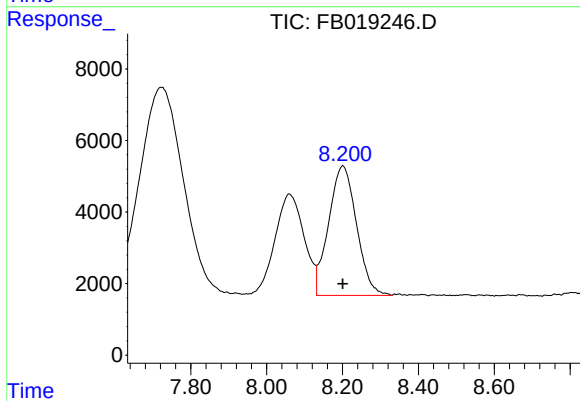

#4 Benzene


R.T.: 8.201 min
Delta R.T.: 0.000 min
Response: 185037
Conc: 10.27 ng/ml

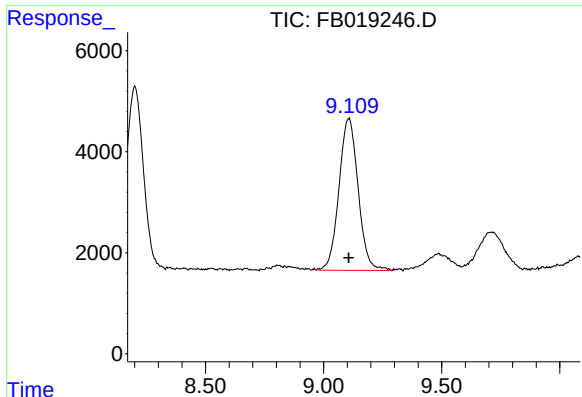

#5 AAA-TFT


R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 169532
Conc: 19.40 ng/ml

Instrument :
FID_B
ClientSampleId :

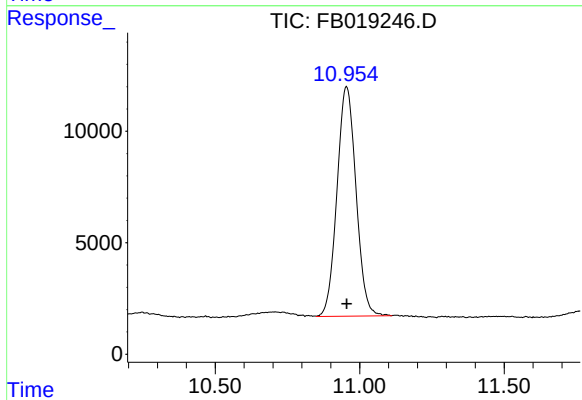


#6 Toluene

R.T.: 10.955 min
Delta R.T.: 0.000 min
Response: 470076
Conc: 30.97 ng/ml

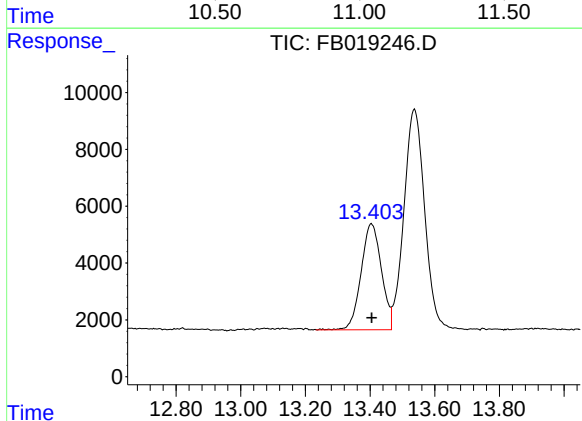


#7 Ethylbenzene

R.T.: 13.405 min
Delta R.T.: 0.000 min
Response: 162705
Conc: 10.47 ng/ml

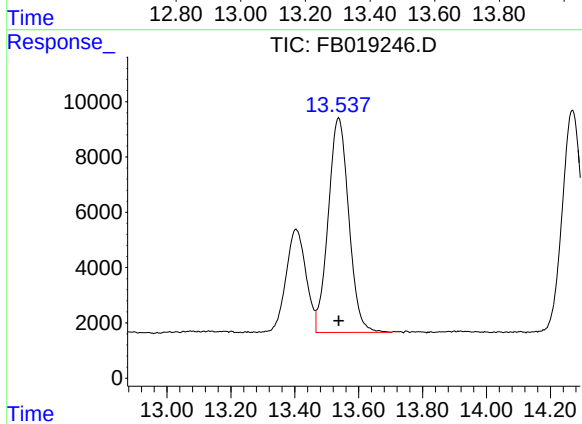

#8 m-Xylene


R.T.: 13.538 min
Delta R.T.: 0.000 min
Response: 346121
Conc: 21.25 ng/ml

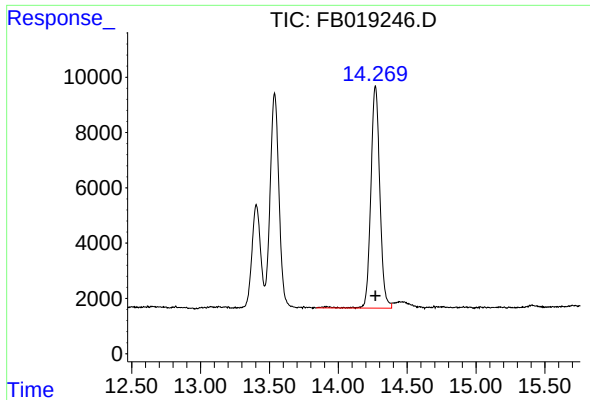

#9 O-Xylene

R.T.: 14.270 min
Delta R.T.: 0.000 min
Response: 365157
Conc: 21.60 ng/ml

Instrument :
FID_B
ClientSampleId :

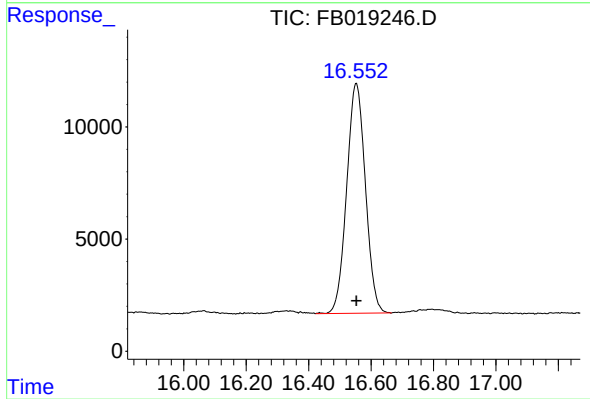

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 426938
Conc: 21.10 ng/ml