

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010325\
 Data File : FB031306.D
 Signal(s) : FID2B.CH
 Acq On : 3 Jan 2025 15:28
 Operator : YP/AJ
 Sample : FB010325GROICV
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 03 14:37:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010325.M
 Quant Title :
 QLast Update : Fri Jan 03 14:30:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	529234	21.048 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	993171	27.199 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1241792	27.170 ng/ml
3) t n-Heptane	7.751	344691	8.536 ng/ml
4) t Benzene	7.889	465910	8.811 ng/ml
6) t Toluene	10.618	1293677	26.394 ng/ml
7) t Ethylbenzene	13.056	391426	8.839 ng/ml
8) t m-Xylene	13.190	840013	17.620 ng/ml
9) t O-Xylene	13.918	791052	17.792 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	646329	17.776 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010325\
Data File : FB031306.D
Signal(s) : FID2B.CH
Acq On : 3 Jan 2025 15:28
Operator : YP/AJ
Sample : FB010325GR0ICV
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 03 14:37:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010325.M
Quant Title :
QLast Update : Fri Jan 03 14:30:31 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

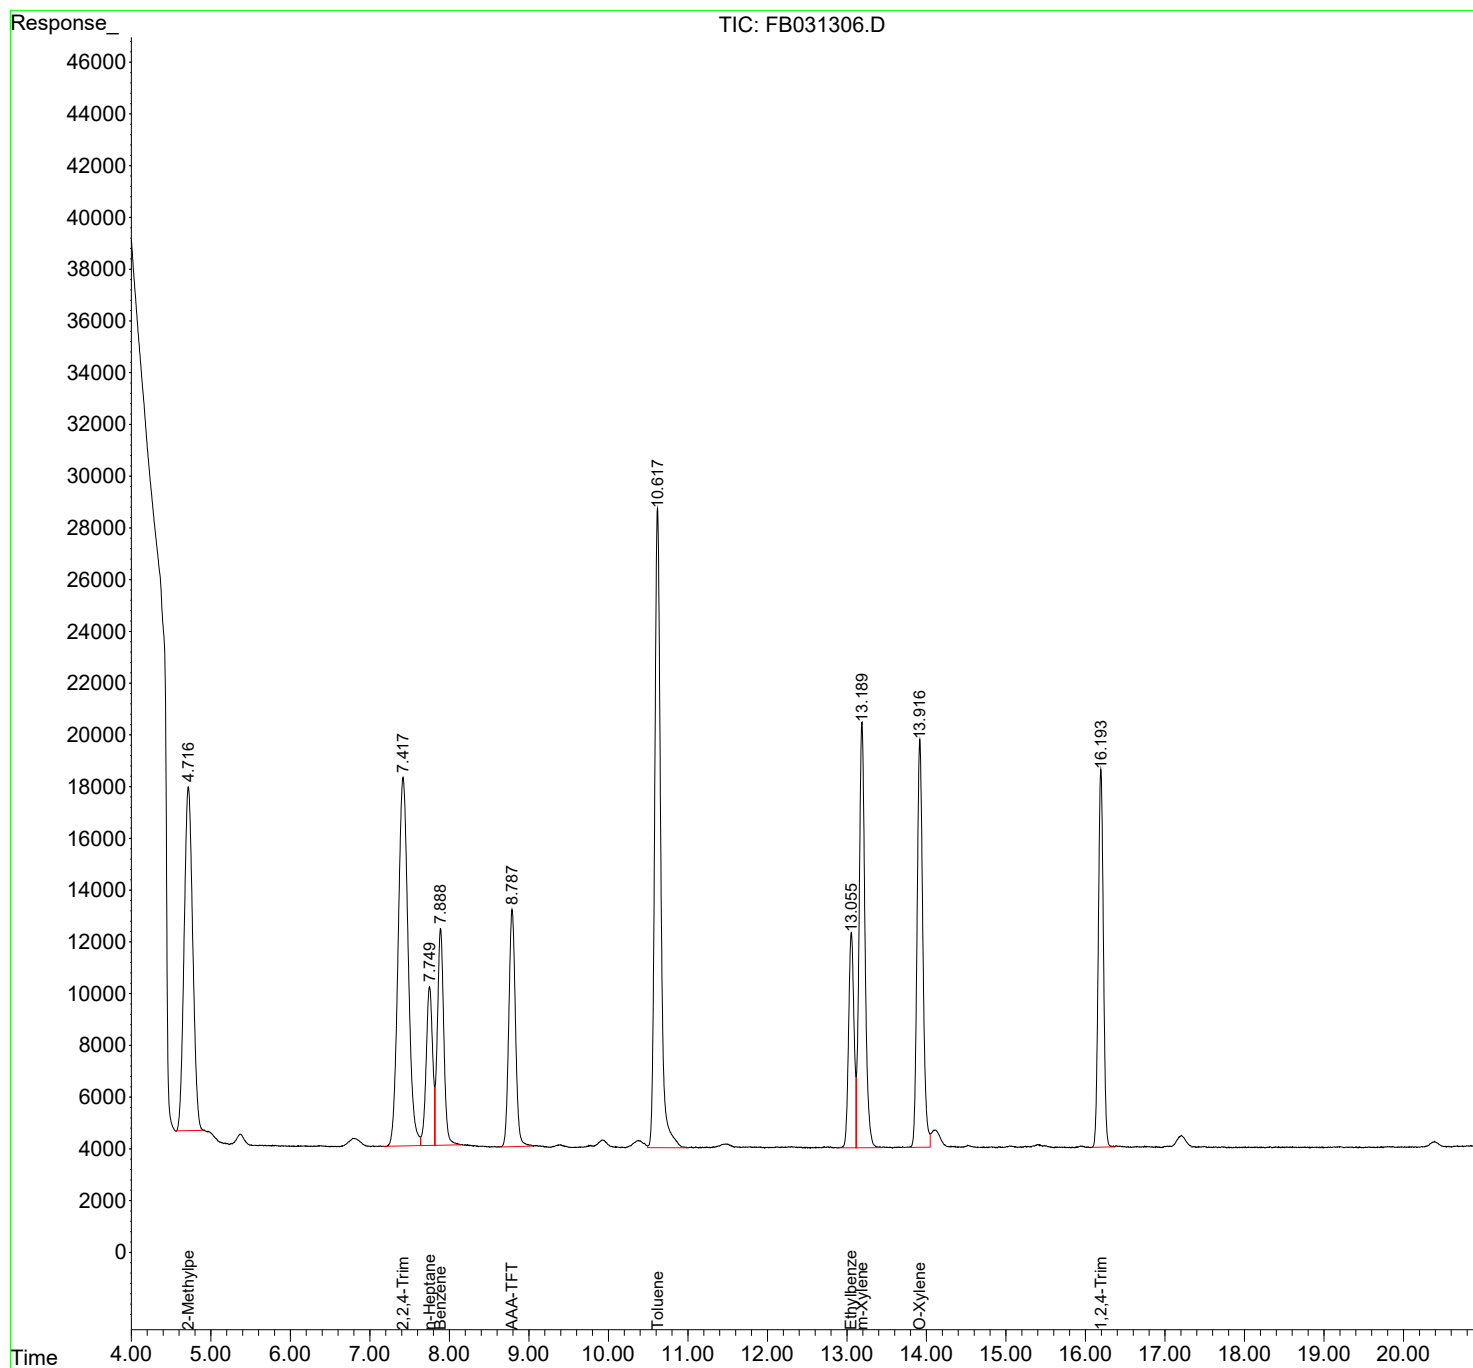


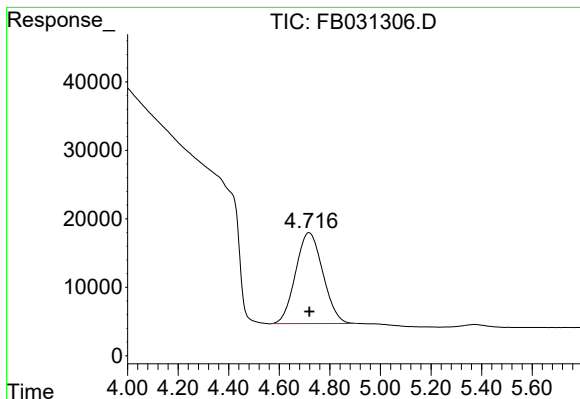

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: -0.002 min
Response: 993171
Conc: 27.20 ng/ml

Instrument :
FID_B
ClientSampleId :

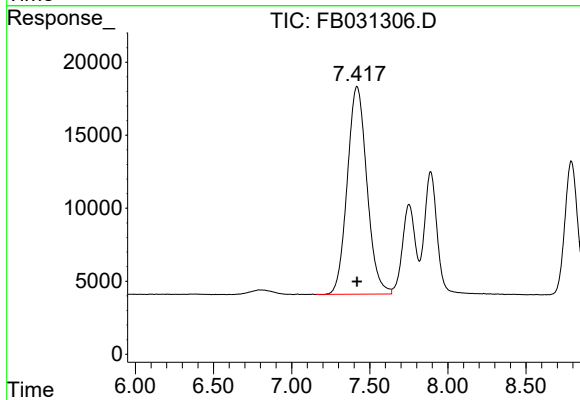


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1241792
Conc: 27.17 ng/ml

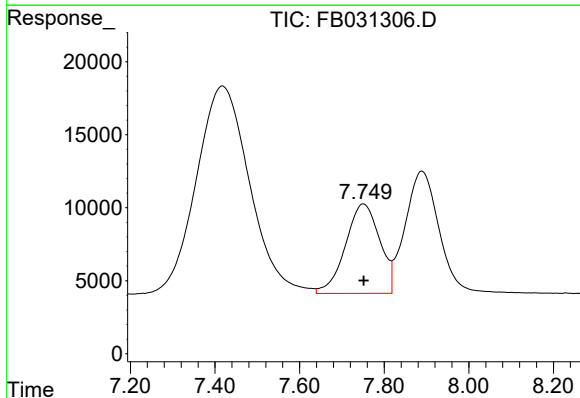


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.001 min
Response: 344691
Conc: 8.54 ng/ml

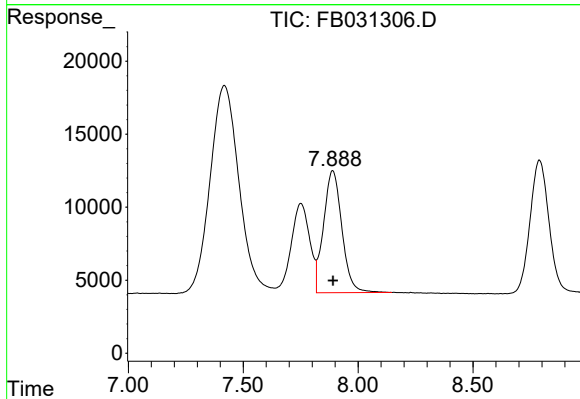

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.001 min
Response: 465910
Conc: 8.81 ng/ml

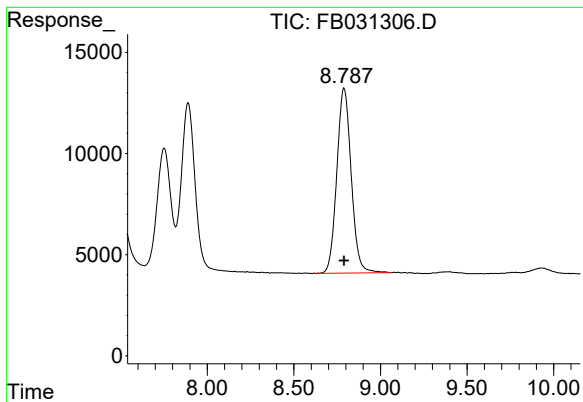

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 529234
Conc: 21.05 ng/ml

Instrument :
FID_B
ClientSampleId :

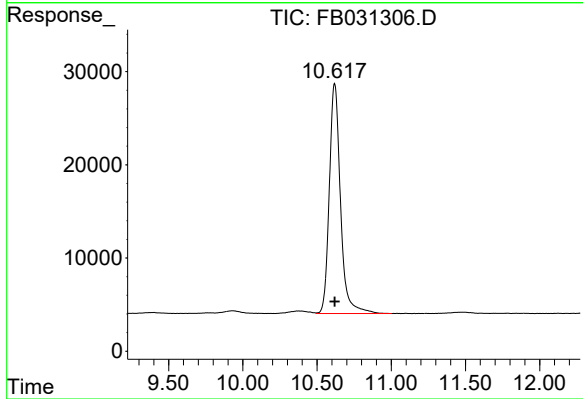


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.001 min
Response: 1293677
Conc: 26.39 ng/ml

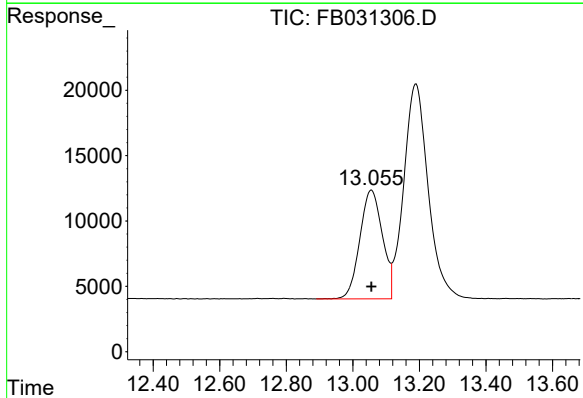


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 391426
Conc: 8.84 ng/ml

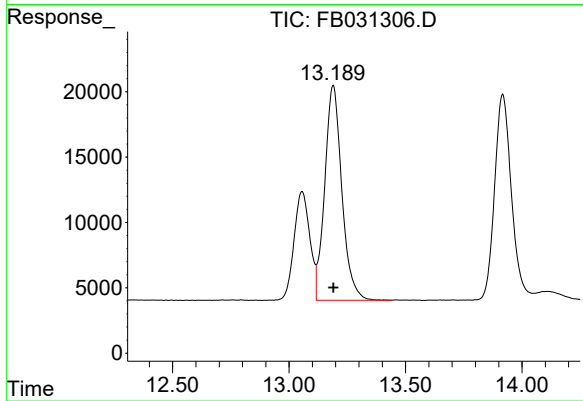

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 840013
Conc: 17.62 ng/ml

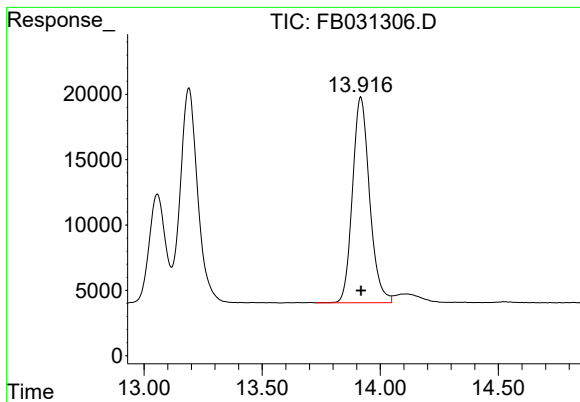

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 791052
Conc: 17.79 ng/ml

Instrument :
FID_B
ClientSampleId :

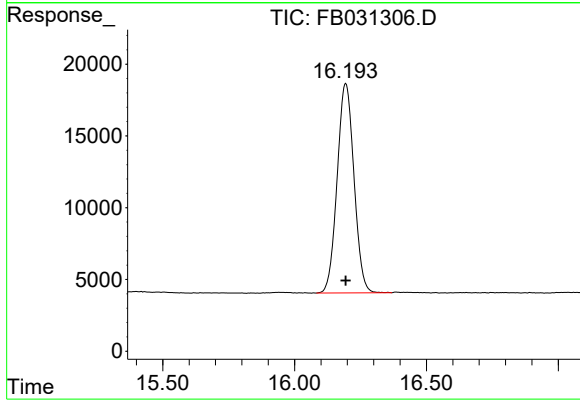

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 646329
Conc: 17.78 ng/ml