

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010421\
 Data File : FB025379.D
 Signal(s) : FID2B.CH
 Acq On : 4 Jan 2021 11:31
 Operator : DD/AJ
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 100 GRO STD

Integration File: Calibration.e
 Quant Time: Jan 04 13:08:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:06:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	2060035	93.616 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.682	4431933	141.220 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	4707532	150.666 ng/ml
3) t n-Heptane	7.755	1550739	49.871 ng/ml
4) t Benzene	7.891	1906642	48.303 ng/ml
6) t Toluene	10.630	5413882	143.492 ng/ml
7) t Ethylbenzene	13.071	1683449	48.863 ng/ml
8) t m-Xylene	13.204	3253306	93.558 ng/ml
9) t O-Xylene	13.932	3161708	94.079 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	2883846	99.701 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010421\
Data File : FB025379.D
Signal(s) : FID2B.CH
Acq On : 4 Jan 2021 11:31
Operator : DD/AJ
Sample : 100 GRO STD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
100 GRO STD

Integration File: Calibration.e
Quant Time: Jan 04 13:08:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:06:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

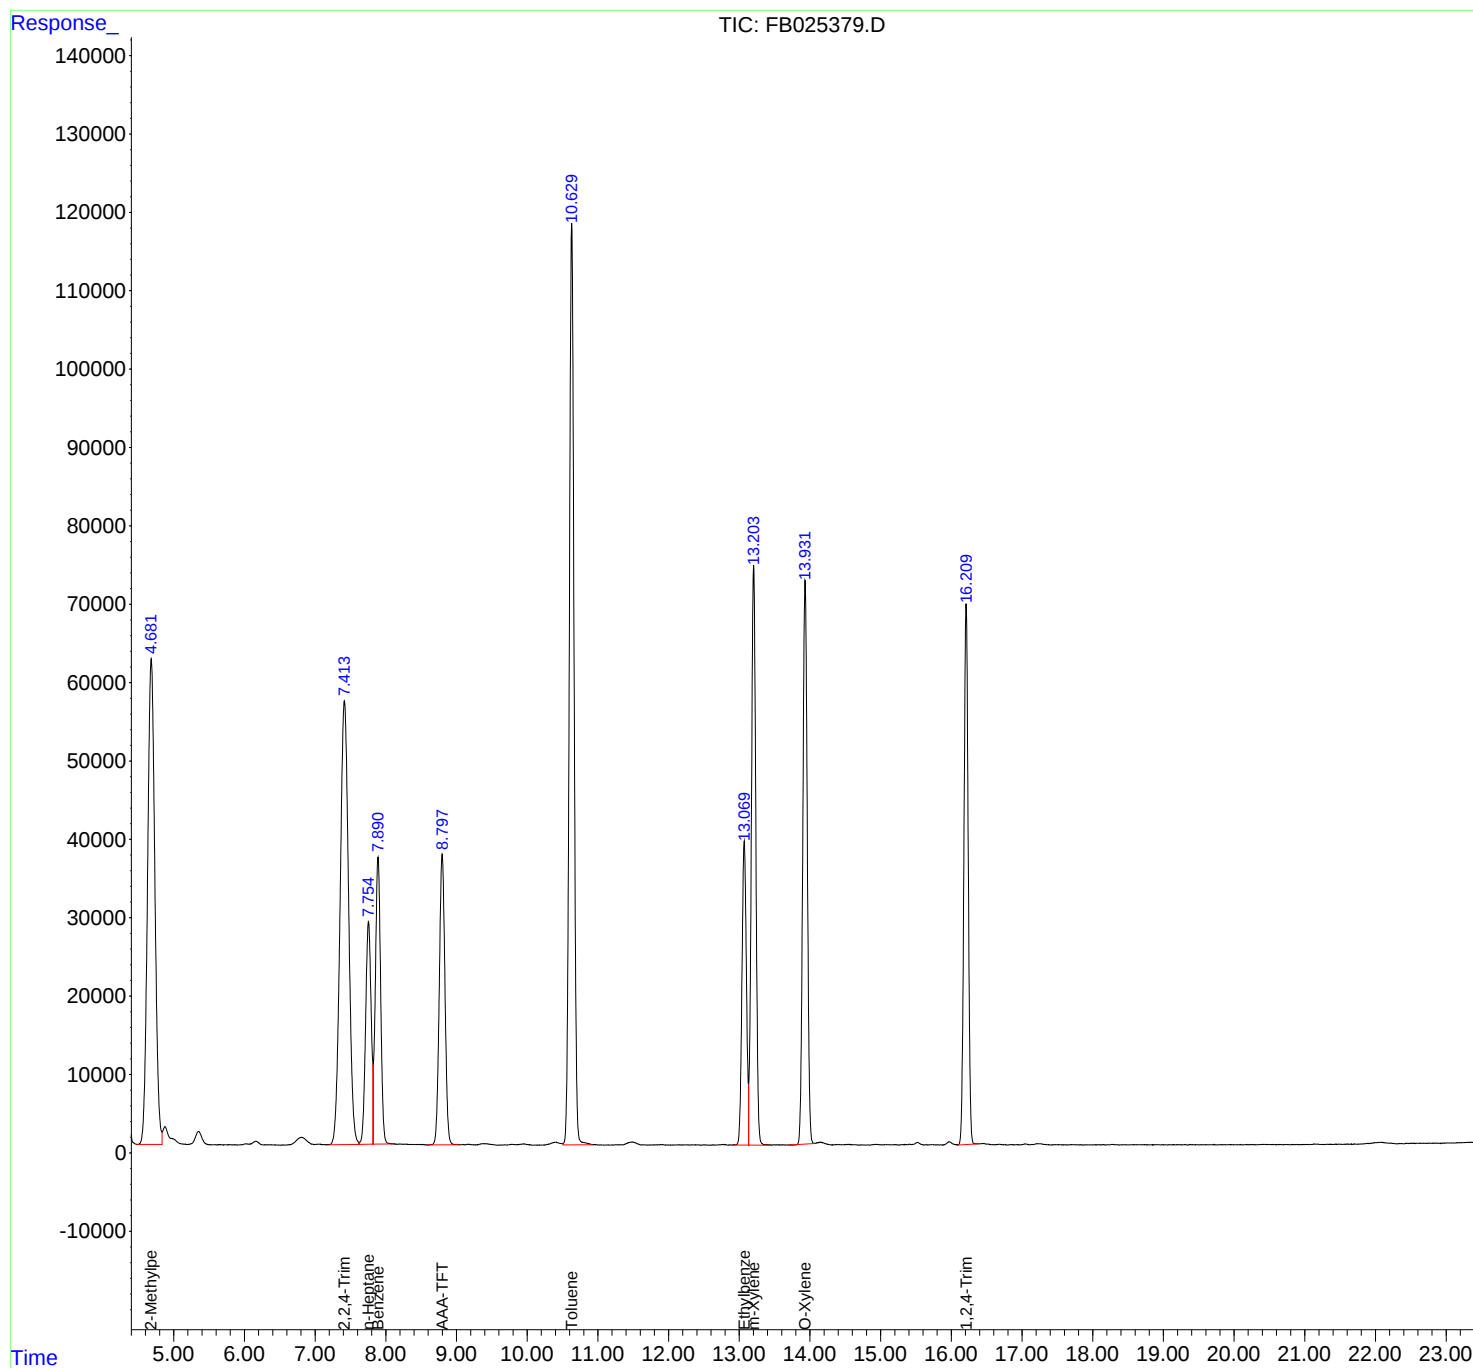


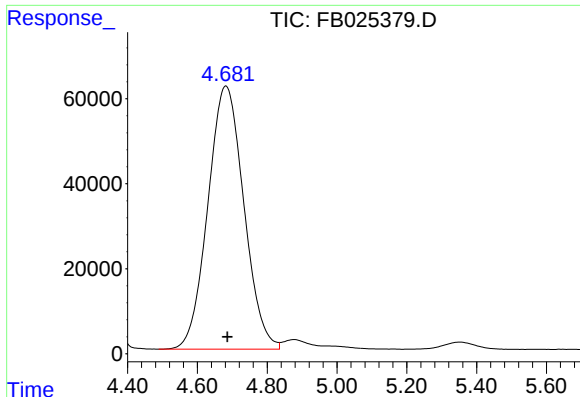

#1 2-Methylpentane


R.T.: 4.682 min
Delta R.T.: -0.004 min
Response: 4431933
Conc: 141.22 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

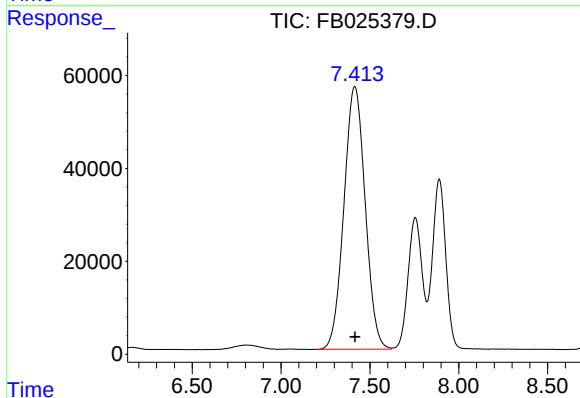


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 4707532
Conc: 150.67 ng/ml

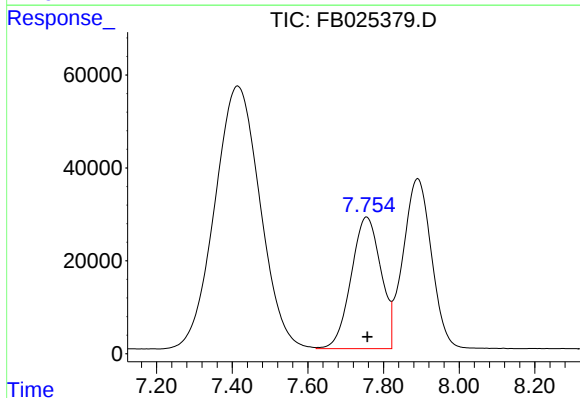


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.002 min
Response: 1550739
Conc: 49.87 ng/ml

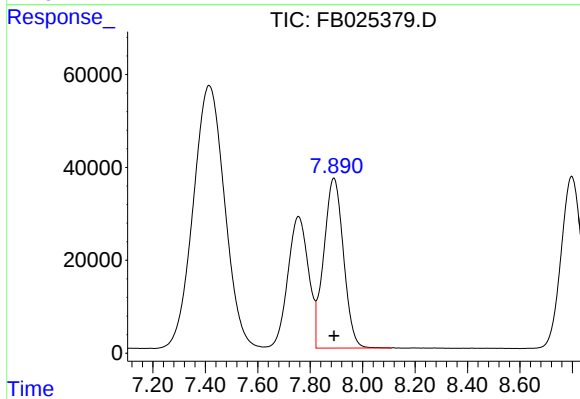

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 1906642
Conc: 48.30 ng/ml

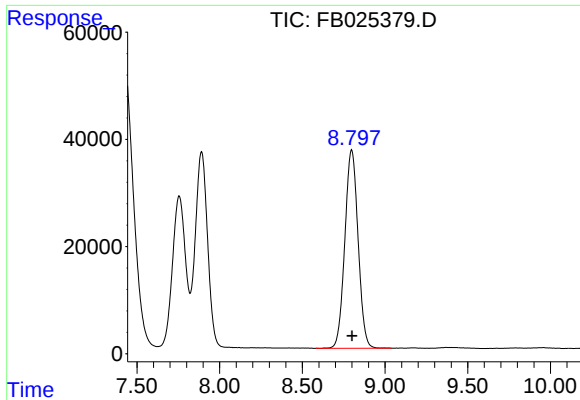

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: -0.002 min
Response: 2060035
Conc: 93.62 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

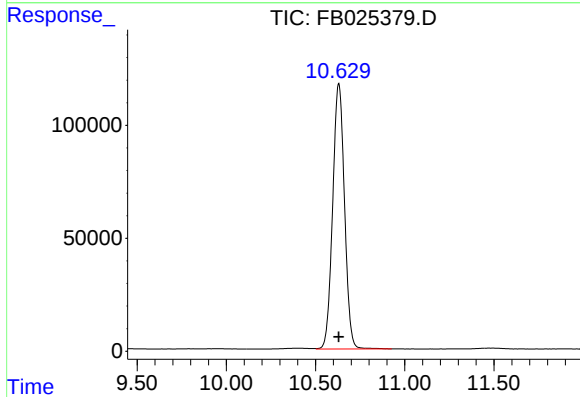


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 5413882
Conc: 143.49 ng/ml

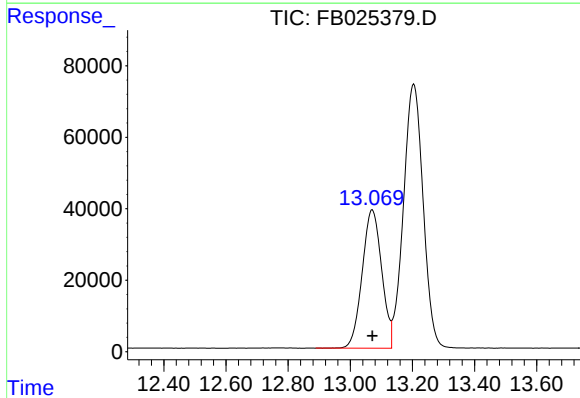


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 1683449
Conc: 48.86 ng/ml

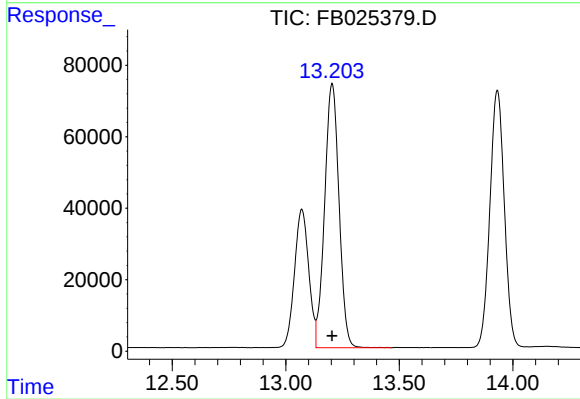

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 3253306
Conc: 93.56 ng/ml

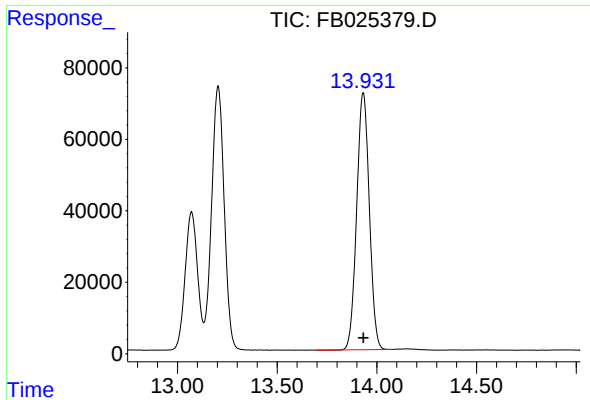

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 3161708
Conc: 94.08 ng/ml

Instrument :
FID_B
ClientSampleId :
100 GRO STD

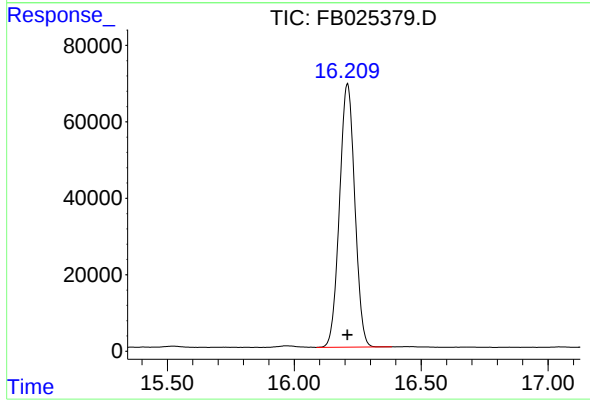

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 2883846
Conc: 99.70 ng/ml