

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010421\
 Data File : FB025385.D
 Signal(s) : FID2B.CH
 Acq On : 4 Jan 2021 15:02
 Operator : DD/AJ
 Sample : L5249-02MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-123120MS

Integration File: Calibration.e
 Quant Time: Jan 05 00:16:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	438791	19.506 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	877077	27.864 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	874743	27.591 ng/ml
3) t n-Heptane	7.758	281252	8.994 ng/ml
4) t Benzene	7.893	378952	9.639 ng/ml
6) t Toluene	10.631	1077757	28.710 ng/ml
7) t Ethylbenzene	13.072	322989	9.430 ng/ml
8) t m-Xylene	13.205	651820	19.052 ng/ml
9) t O-Xylene	13.932	631362	18.994 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	529072	18.398 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010421\
Data File : FB025385.D
Signal(s) : FID2B.CH
Acq On : 4 Jan 2021 15:02
Operator : DD/AJ
Sample : L5249-02MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-123120MS

Integration File: Calibration.e
Quant Time: Jan 05 00:16:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

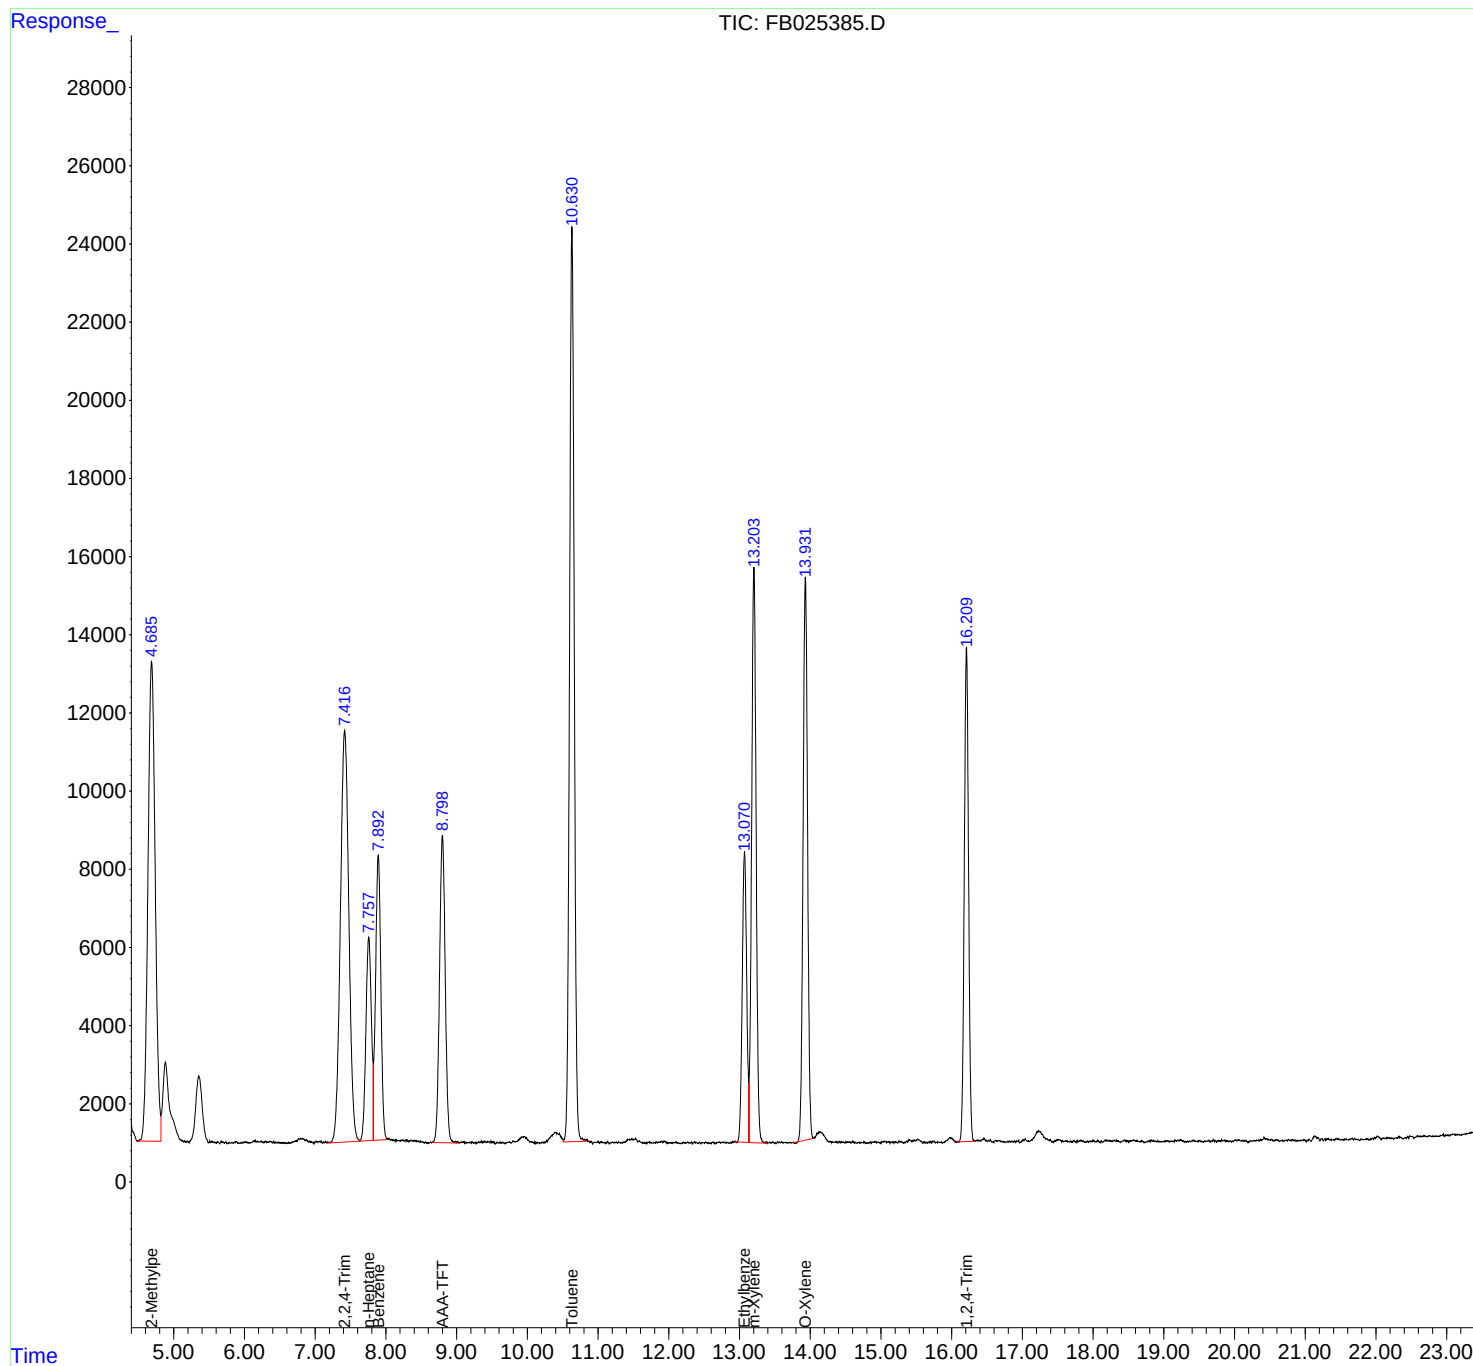


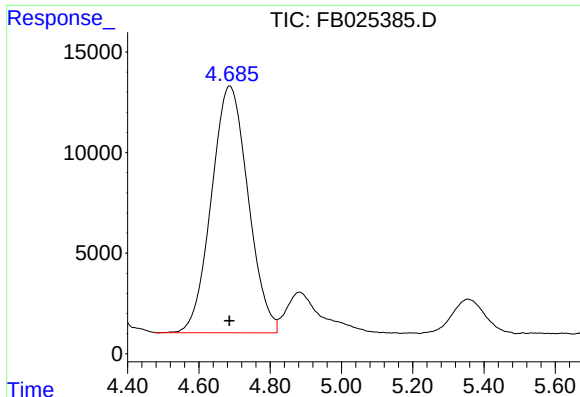

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 877077
Conc: 27.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-123120MS

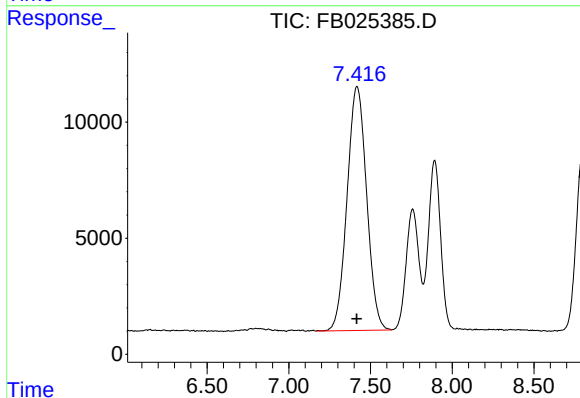


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 874743
Conc: 27.59 ng/ml

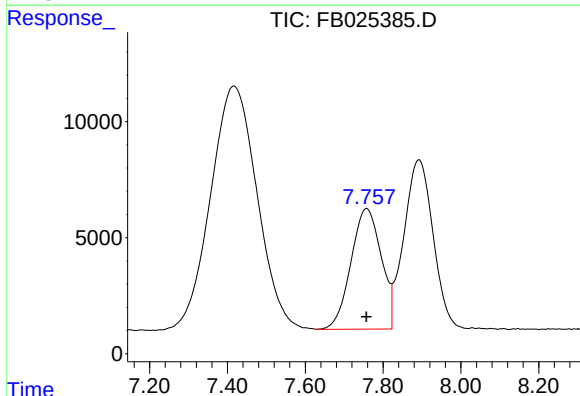


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.001 min
Response: 281252
Conc: 8.99 ng/ml

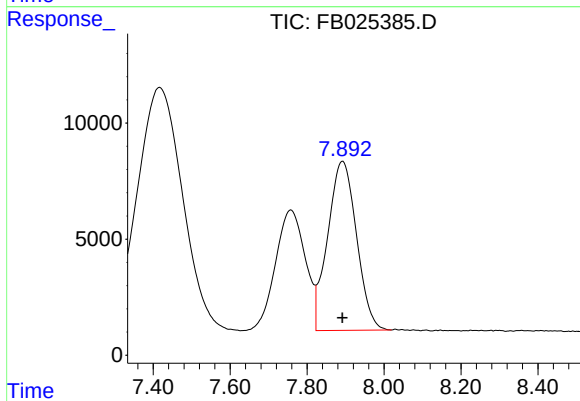

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 378952
Conc: 9.64 ng/ml

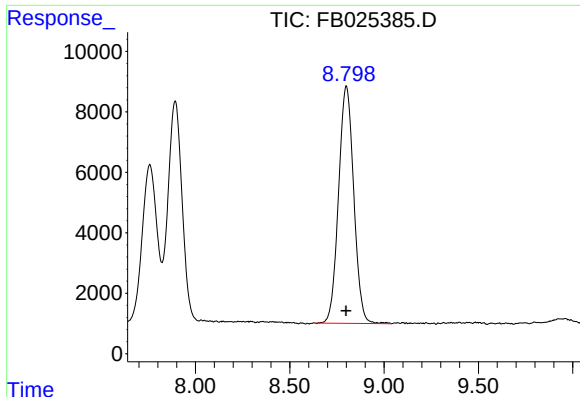

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 438791
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-123120MS

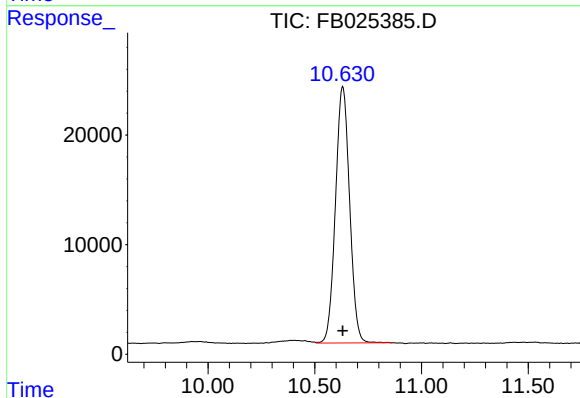


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1077757
Conc: 28.71 ng/ml

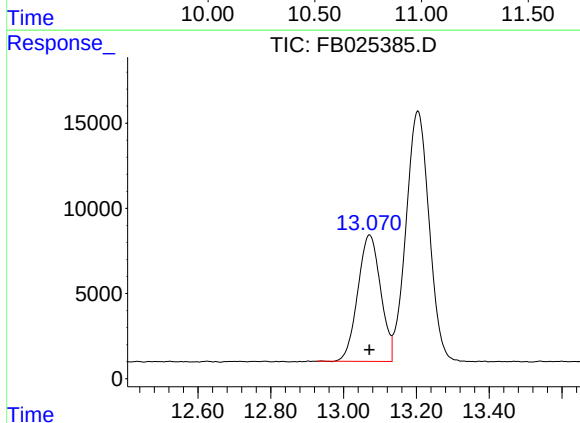


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 322989
Conc: 9.43 ng/ml

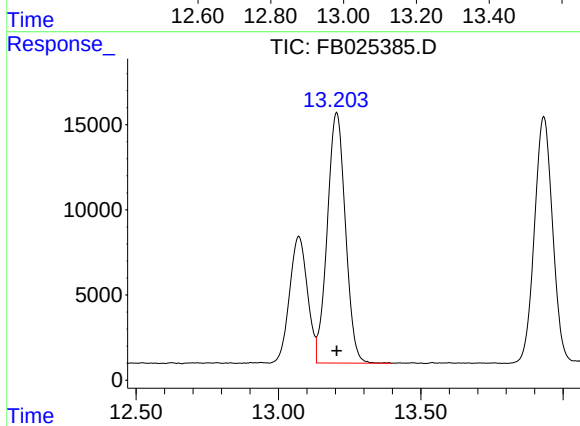

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 651820
Conc: 19.05 ng/ml

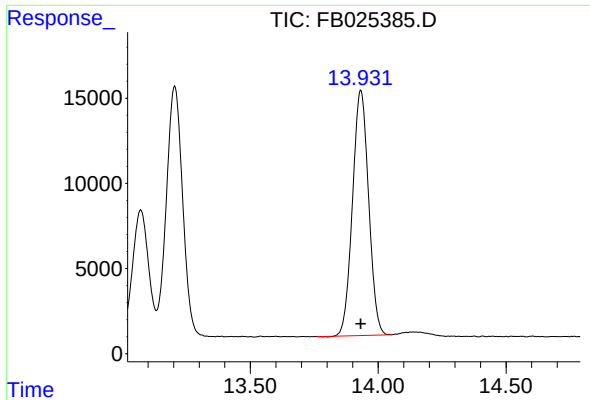

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 631362
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-123120MS

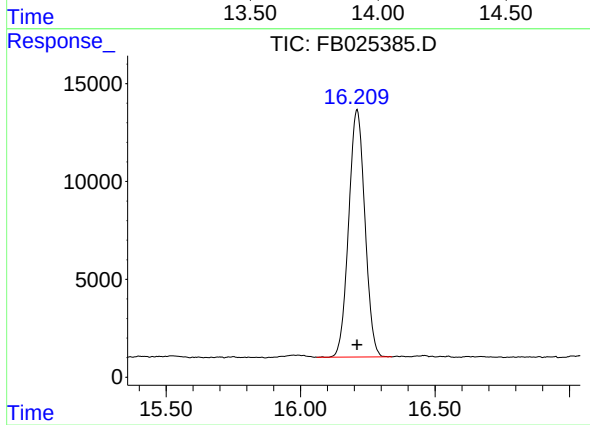

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 529072
Conc: 18.40 ng/ml