

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010920\
 Data File : FB023392.D
 Signal(s) : FID2B.CH
 Acq On : 9 Jan 2020 16:44
 Operator : DD/AJ
 Sample : L1070-02MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 10 00:18:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	476538	20.095 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.683	747756	24.160 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	800393	23.960 ng/ml
3) t n-Heptane	7.750	255049	7.732 ng/ml
4) t Benzene	7.884	369346	9.249 ng/ml
6) t Toluene	10.622	1025528	26.635 ng/ml
7) t Ethylbenzene	13.062	313223	8.630 ng/ml
8) t m-Xylene	13.195	593195	17.089 ng/ml
9) t O-Xylene	13.923	578151	17.165 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	488982	17.427 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB010920\
Data File : FB023392.D
Signal(s) : FID2B.CH
Acq On : 9 Jan 2020 16:44
Operator : DD/AJ
Sample : L1070-02MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 10 00:18:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

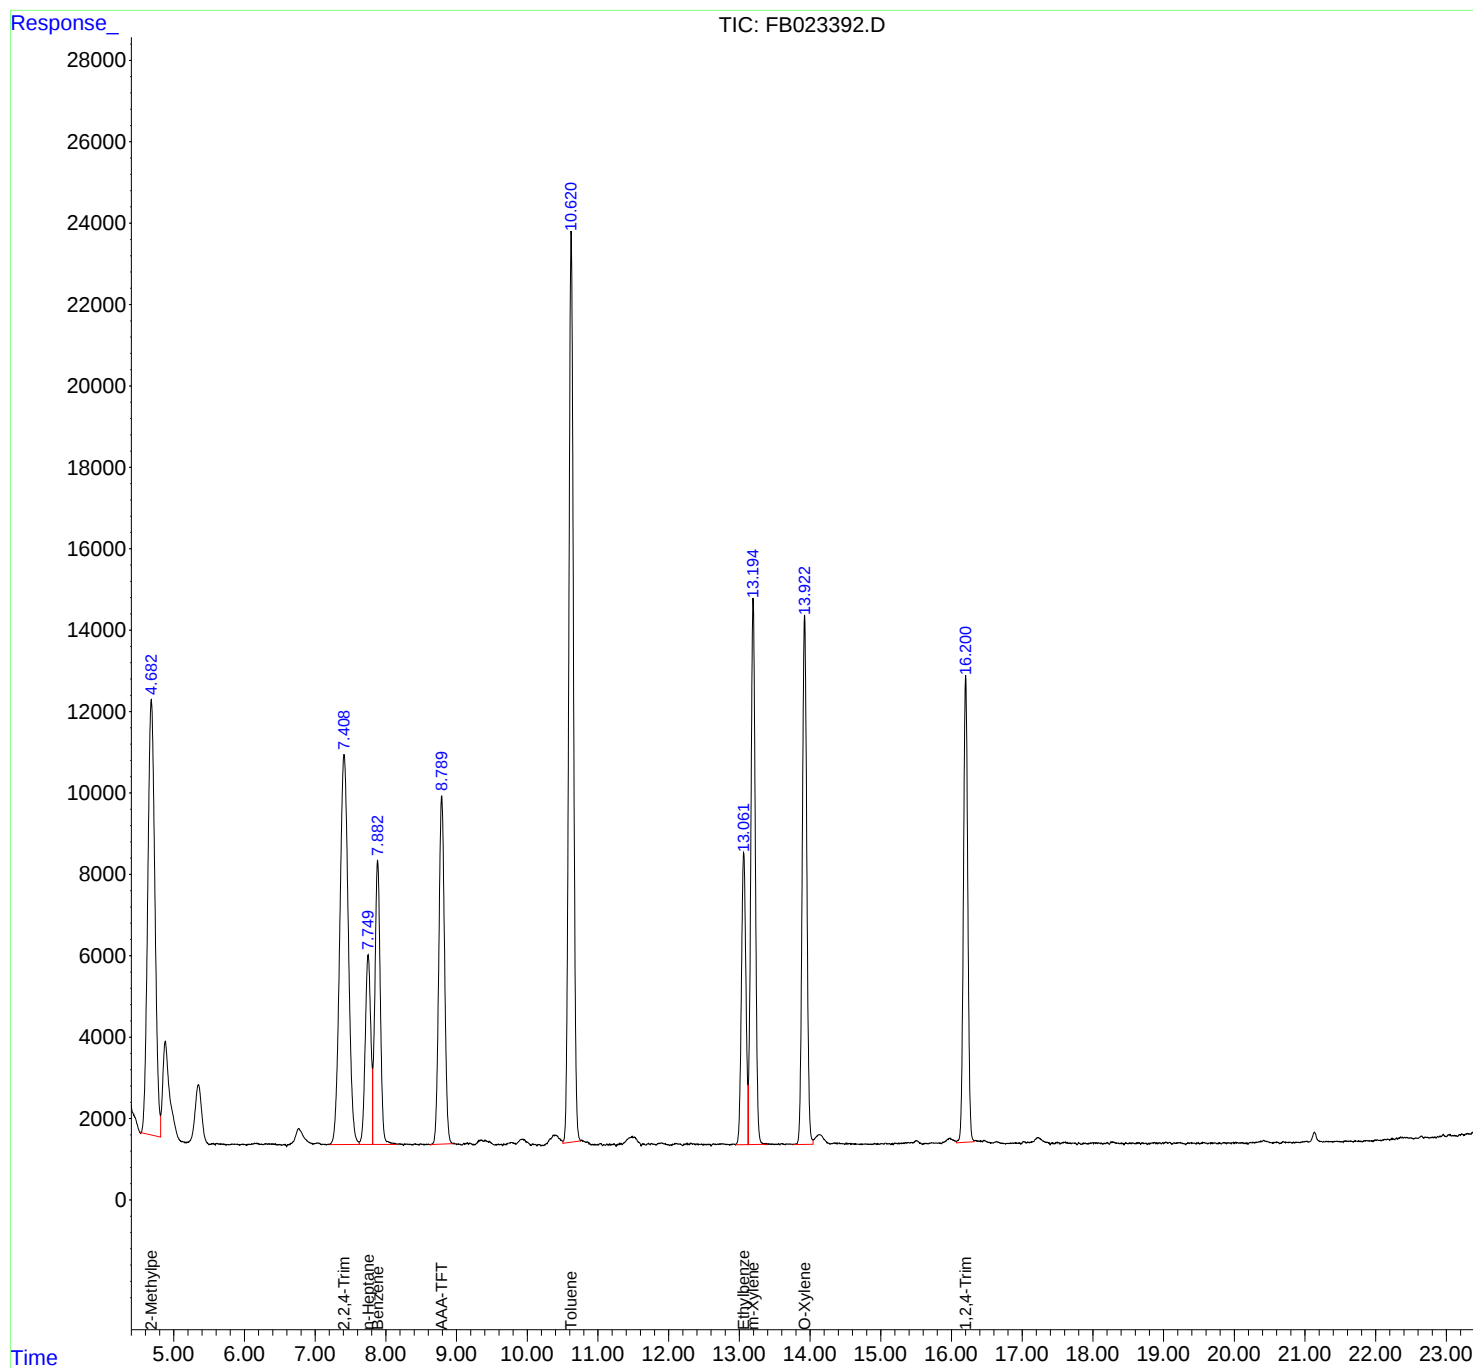

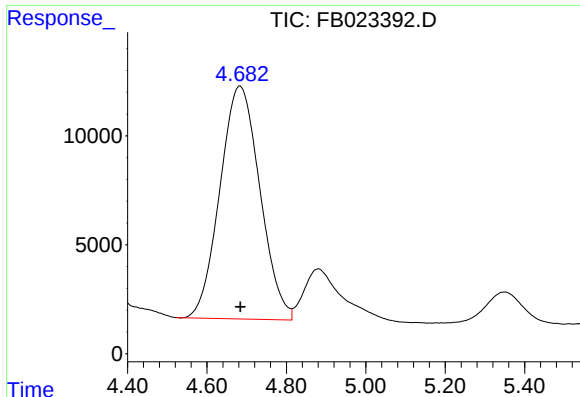


#1 2-Methylpentane

R.T.: 4.683 min
Delta R.T.: 0.000 min
Response: 747756
Conc: 24.16 ng/ml

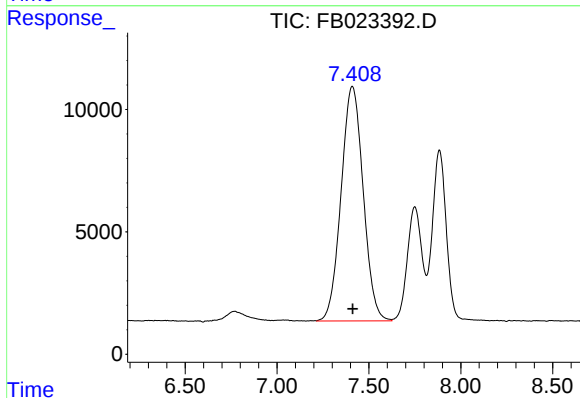


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.002 min
Response: 800393
Conc: 23.96 ng/ml

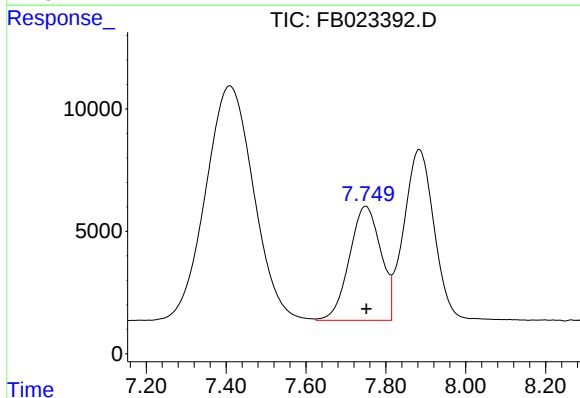


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 255049
Conc: 7.73 ng/ml

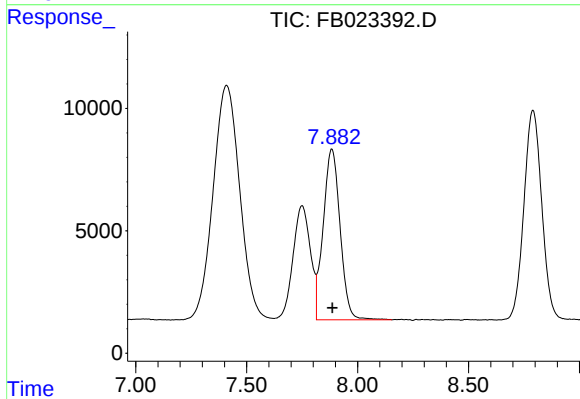


#4 Benzene

R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 369346
Conc: 9.25 ng/ml

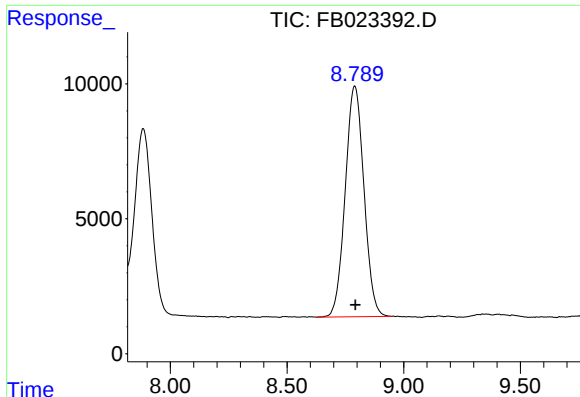


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 476538
Conc: 20.10 ng/ml

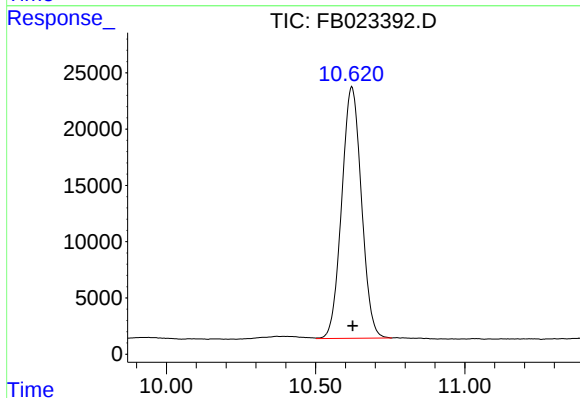


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.002 min
Response: 1025528
Conc: 26.63 ng/ml

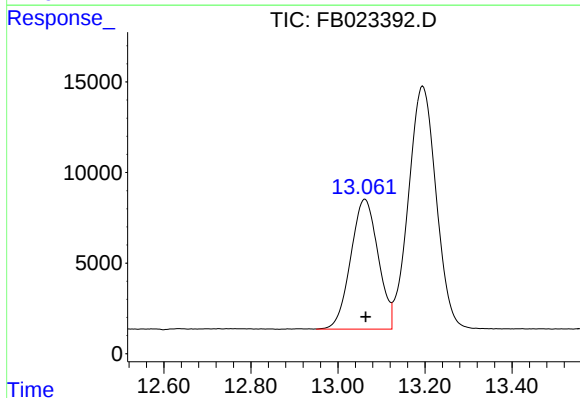


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.001 min
Response: 313223
Conc: 8.63 ng/ml

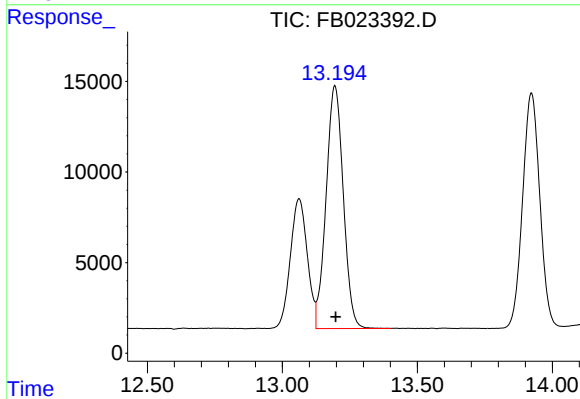


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 593195
Conc: 17.09 ng/ml

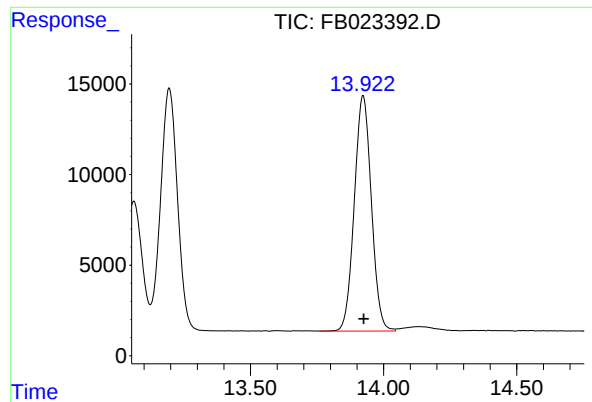

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.002 min
Response: 578151
Conc: 17.16 ng/ml

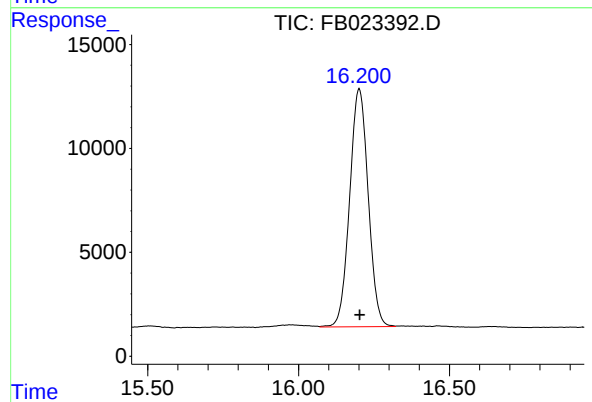

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.002 min
Response: 488982
Conc: 17.43 ng/ml