

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
 Data File : FB019361.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jan 2019 18:06
 Operator : MJ/SJ
 Sample : K1011-01
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 11 04:53:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.046	152345	17.144 ng/ml
Target Compounds			
6) t Toluene	10.889	17275	0.955 ng/ml
7) t Ethylbenzene	13.338	7335	0.331 ng/ml
8) t m-Xylene	13.475	11961	0.521 ng/ml
9) t O-Xylene	14.210	7563	0.337 ng/ml
10) t 1,2,4-Trimethylbenzene	16.487	10220	0.448 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
Data File : FB019361.D
Signal(s) : FID2B.CH
Acq On : 10 Jan 2019 18:06
Operator : MJ/SJ
Sample : K1011-01
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 04:53:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

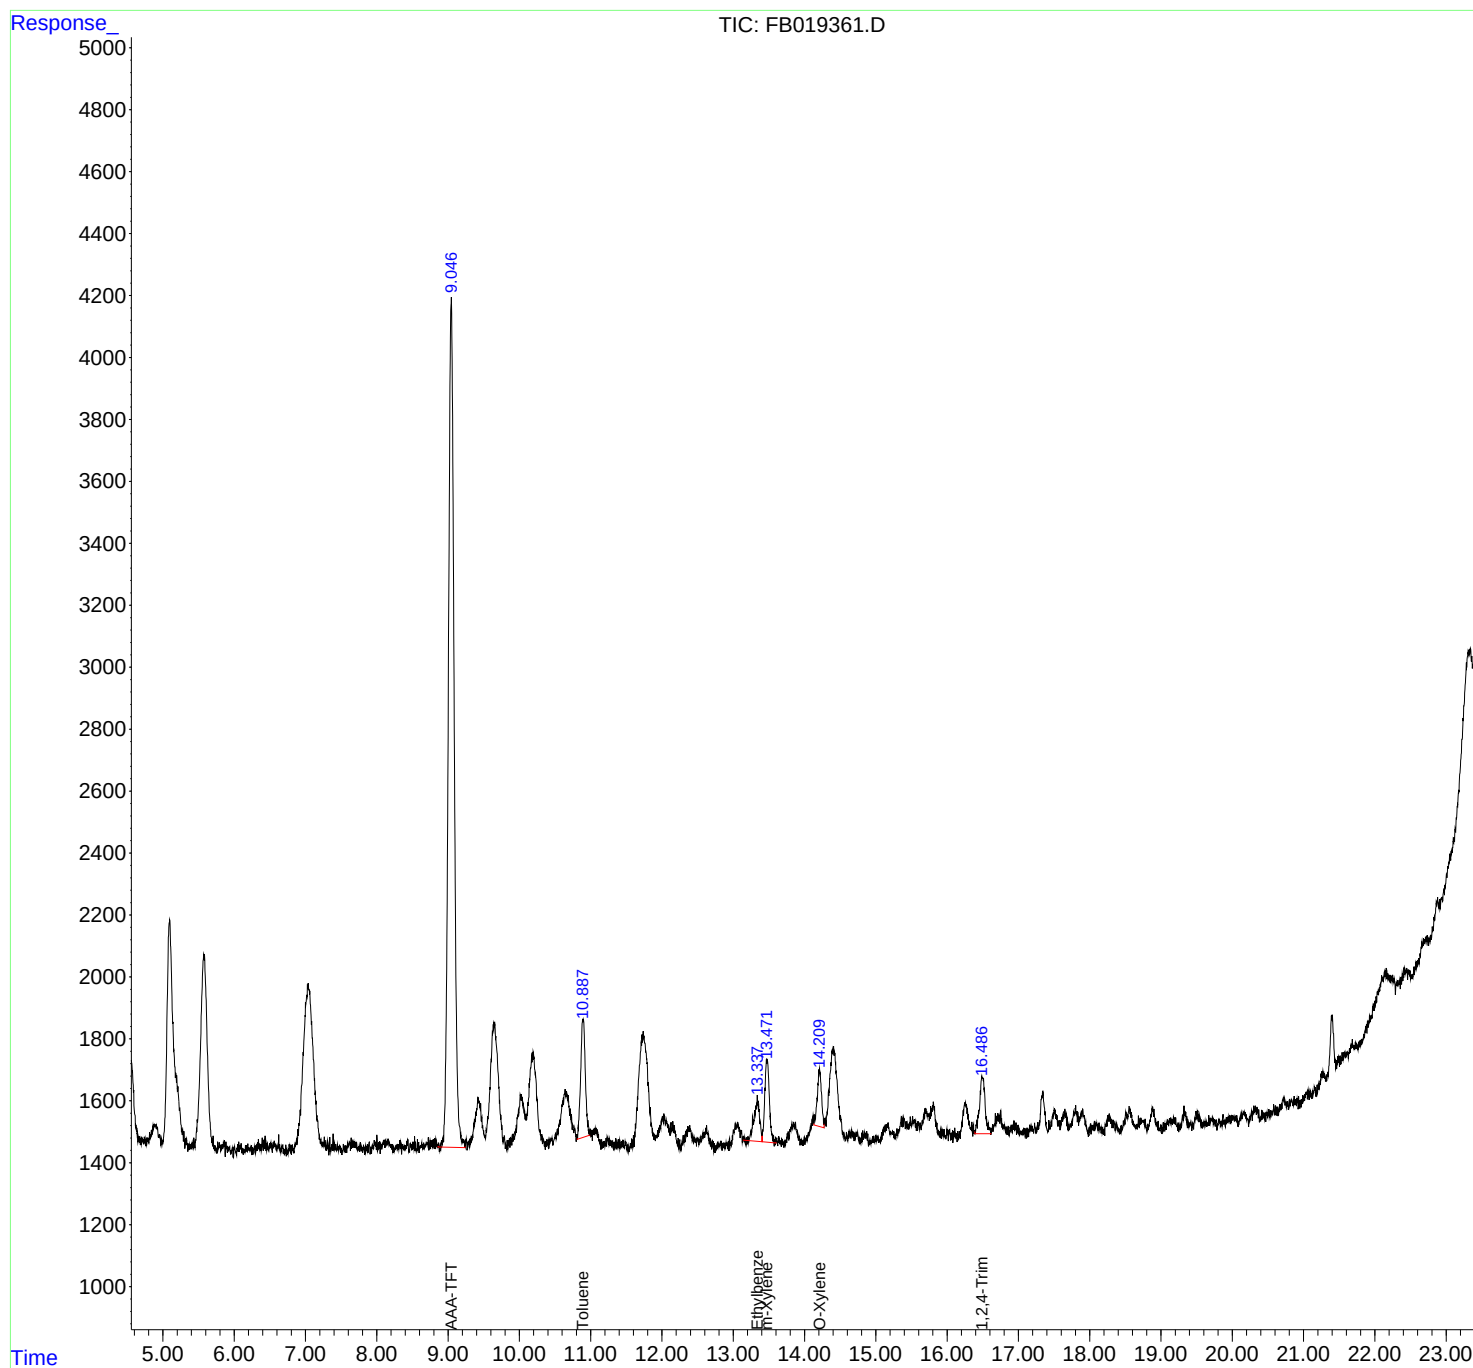


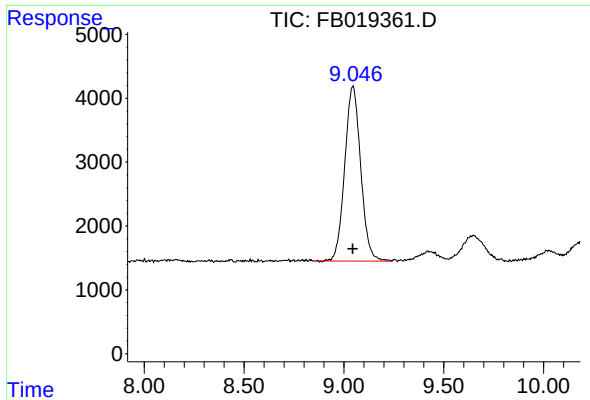

#5 AAA-TFT


R.T.: 9.046 min
Delta R.T.: 0.002 min
Response: 152345
Conc: 17.14 ng/ml

Instrument :
FID_B
ClientSampleId :

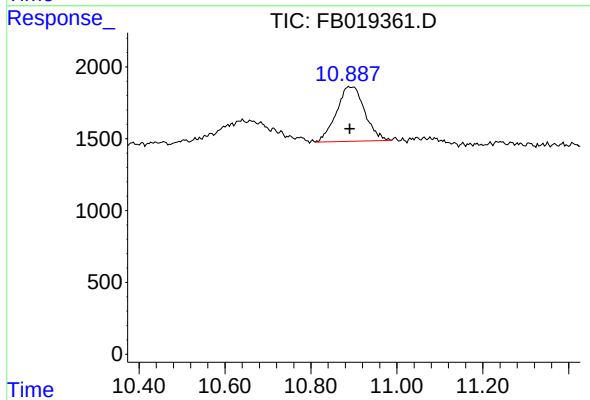


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.001 min
Response: 17275
Conc: 0.95 ng/ml

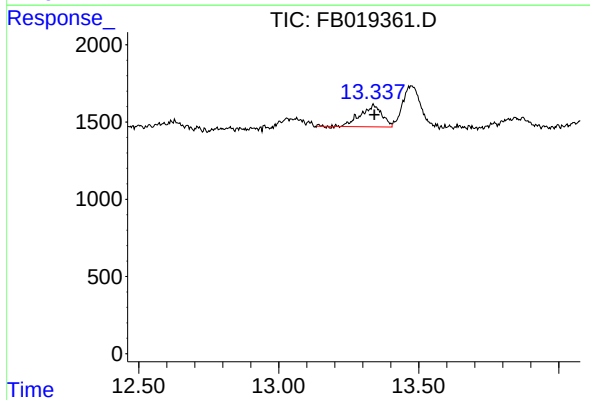


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.004 min
Response: 7335
Conc: 0.33 ng/ml

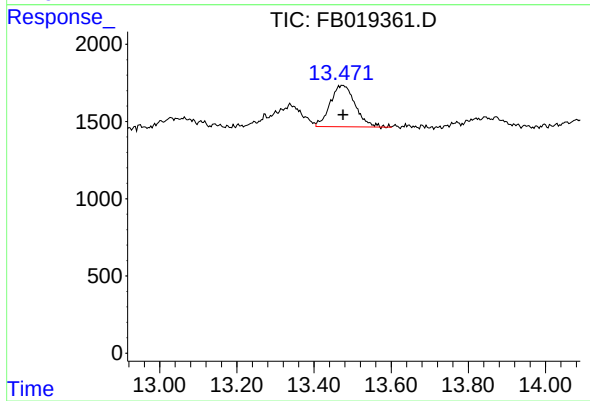

#8 m-Xylene


R.T.: 13.475 min
Delta R.T.: 0.000 min
Response: 11961
Conc: 0.52 ng/ml

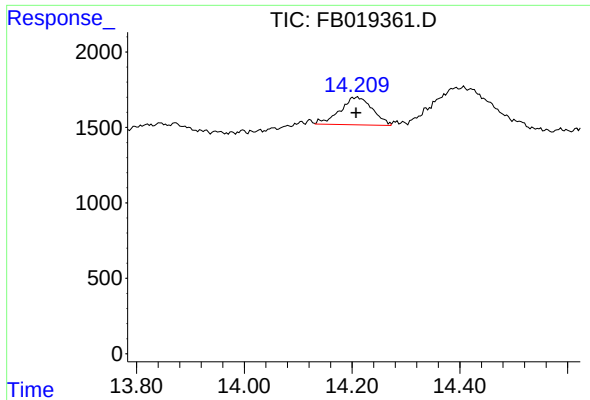

#9 O-Xylene

R.T.: 14.210 min
Delta R.T.: 0.003 min
Response: 7563
Conc: 0.34 ng/ml

Instrument :
FID_B
ClientSampleId :

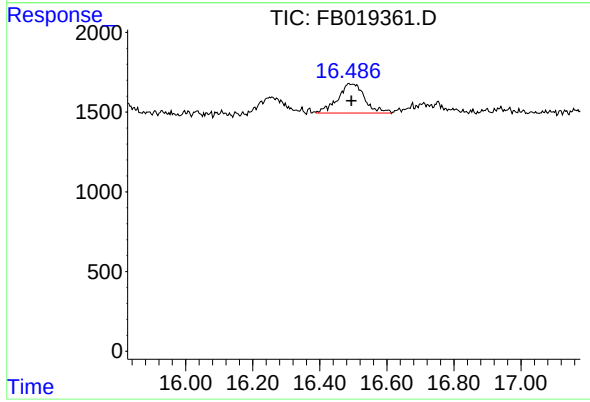

#10 1,2,4-Trimethylbenzene

R.T.: 16.487 min
Delta R.T.: -0.007 min
Response: 10220
Conc: 0.45 ng/ml