

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
Data File : FB019365.D
Signal(s) : FID2B.CH
Acq On : 10 Jan 2019 20:05
Operator : MJ/SJ
Sample : K1119-05
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 04:53:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	163170	18.363 ng/ml
Target Compounds			
6) t Toluene	10.892	8940	0.494 ng/ml
7) t Ethylbenzene	13.329	232534	10.496 ng/ml
8) t m-Xylene	13.472	245990	10.719 ng/ml
9) t O-Xylene	14.208	92275	4.113 ng/ml
10) t 1,2,4-Trimethylbenzene	16.494	642656	28.184 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
Data File : FB019365.D
Signal(s) : FID2B.CH
Acq On : 10 Jan 2019 20:05
Operator : MJ/SJ
Sample : K1119-05
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 04:53:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

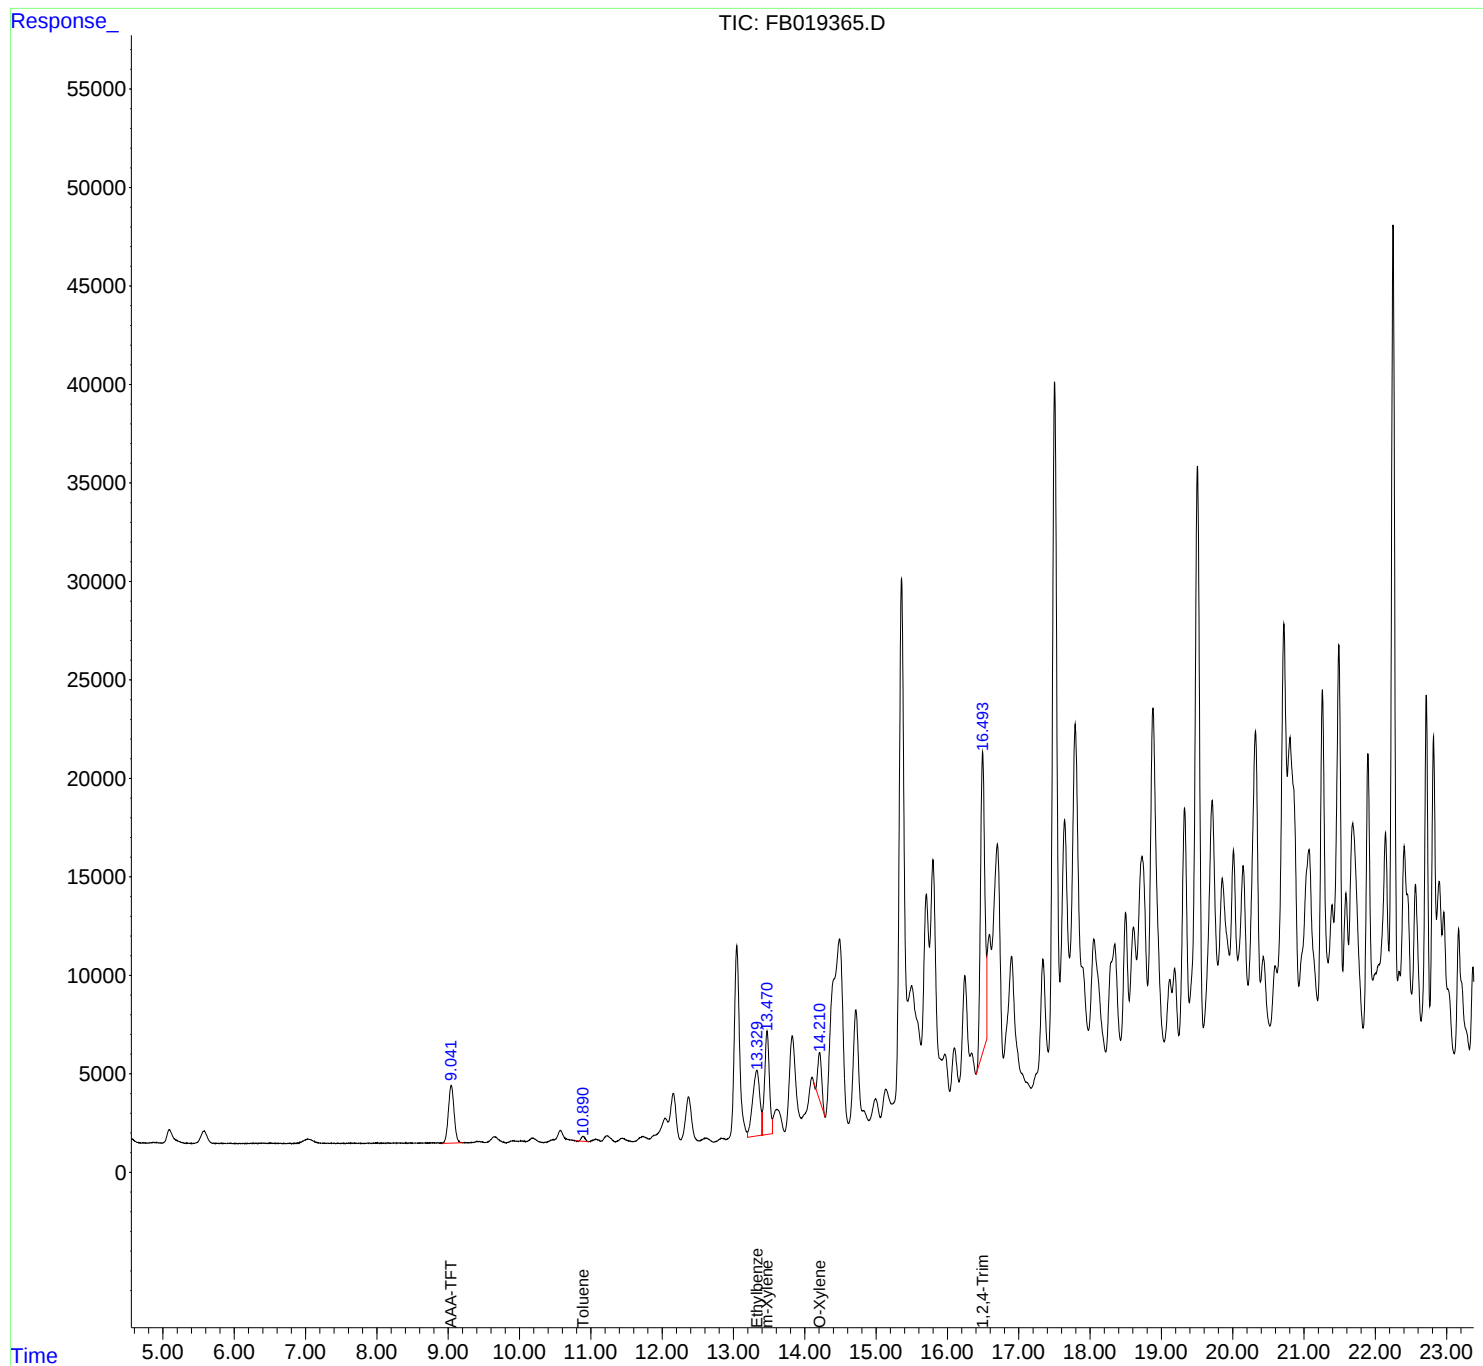


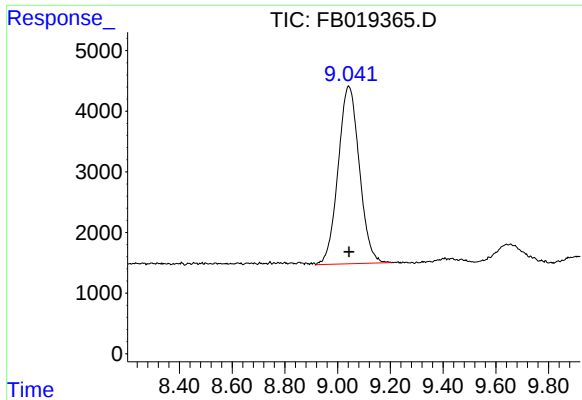

#5 AAA-TFT


R.T.: 9.042 min
Delta R.T.: -0.001 min
Response: 163170
Conc: 18.36 ng/ml

Instrument :
FID_B
ClientSampleId :

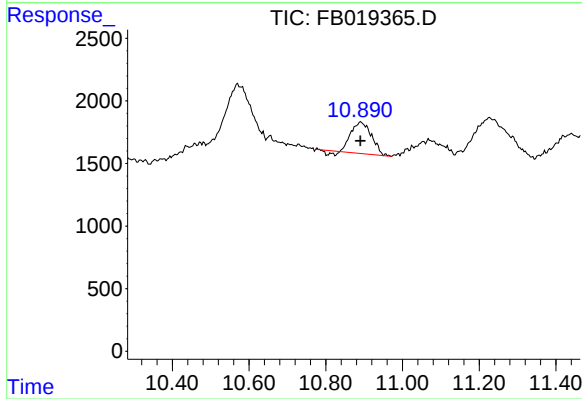


#6 Toluene

R.T.: 10.892 min
Delta R.T.: 0.001 min
Response: 8940
Conc: 0.49 ng/ml

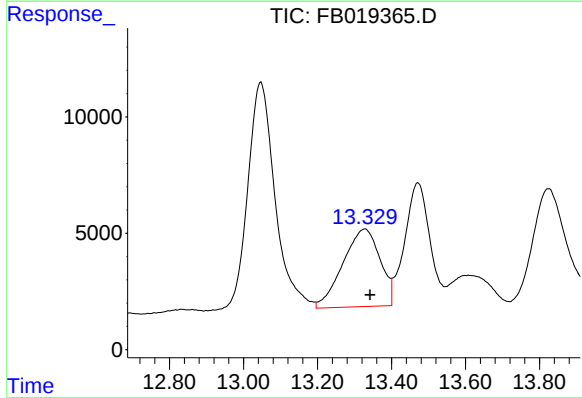


#7 Ethylbenzene

R.T.: 13.329 min
Delta R.T.: -0.013 min
Response: 232534
Conc: 10.50 ng/ml

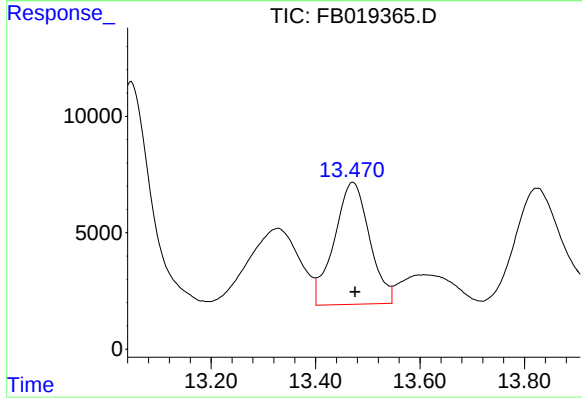

#8 m-Xylene


R.T.: 13.472 min
Delta R.T.: -0.004 min
Response: 245990
Conc: 10.72 ng/ml

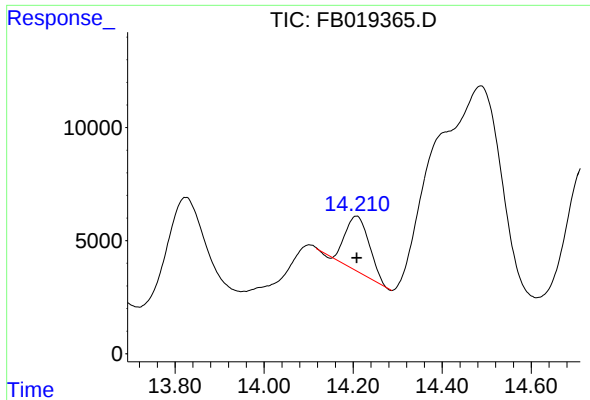

#9 O-Xylene

R.T.: 14.208 min
Delta R.T.: 0.000 min
Response: 92275
Conc: 4.11 ng/ml

Instrument :
FID_B
ClientSampleId :

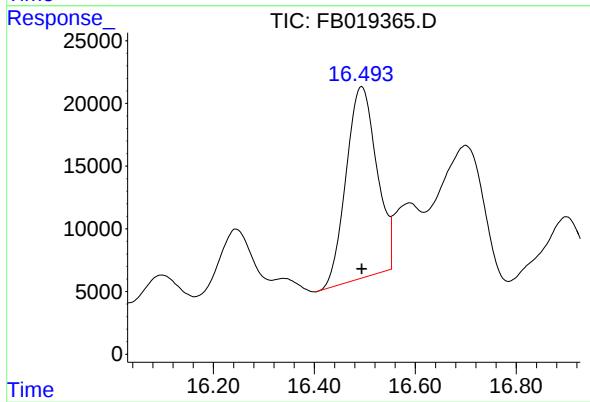

#10 1,2,4-Trimethylbenzene

R.T.: 16.494 min
Delta R.T.: 0.000 min
Response: 642656
Conc: 28.18 ng/ml