

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
 Data File : FB019368.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jan 2019 21:34
 Operator : MJ/SJ
 Sample : K1124-02
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 11 04:54:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	132440	14.904 ng/ml
Target Compounds			
6) t Toluene	10.892	21988	1.216 ng/ml
8) t m-Xylene	13.478	8028	0.350 ng/ml
9) t O-Xylene	14.265	18697	0.833 ng/ml
10) t 1,2,4-Trimethylbenzene	16.524	184040	8.071 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011019\
Data File : FB019368.D
Signal(s) : FID2B.CH
Acq On : 10 Jan 2019 21:34
Operator : MJ/SJ
Sample : K1124-02
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 04:54:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

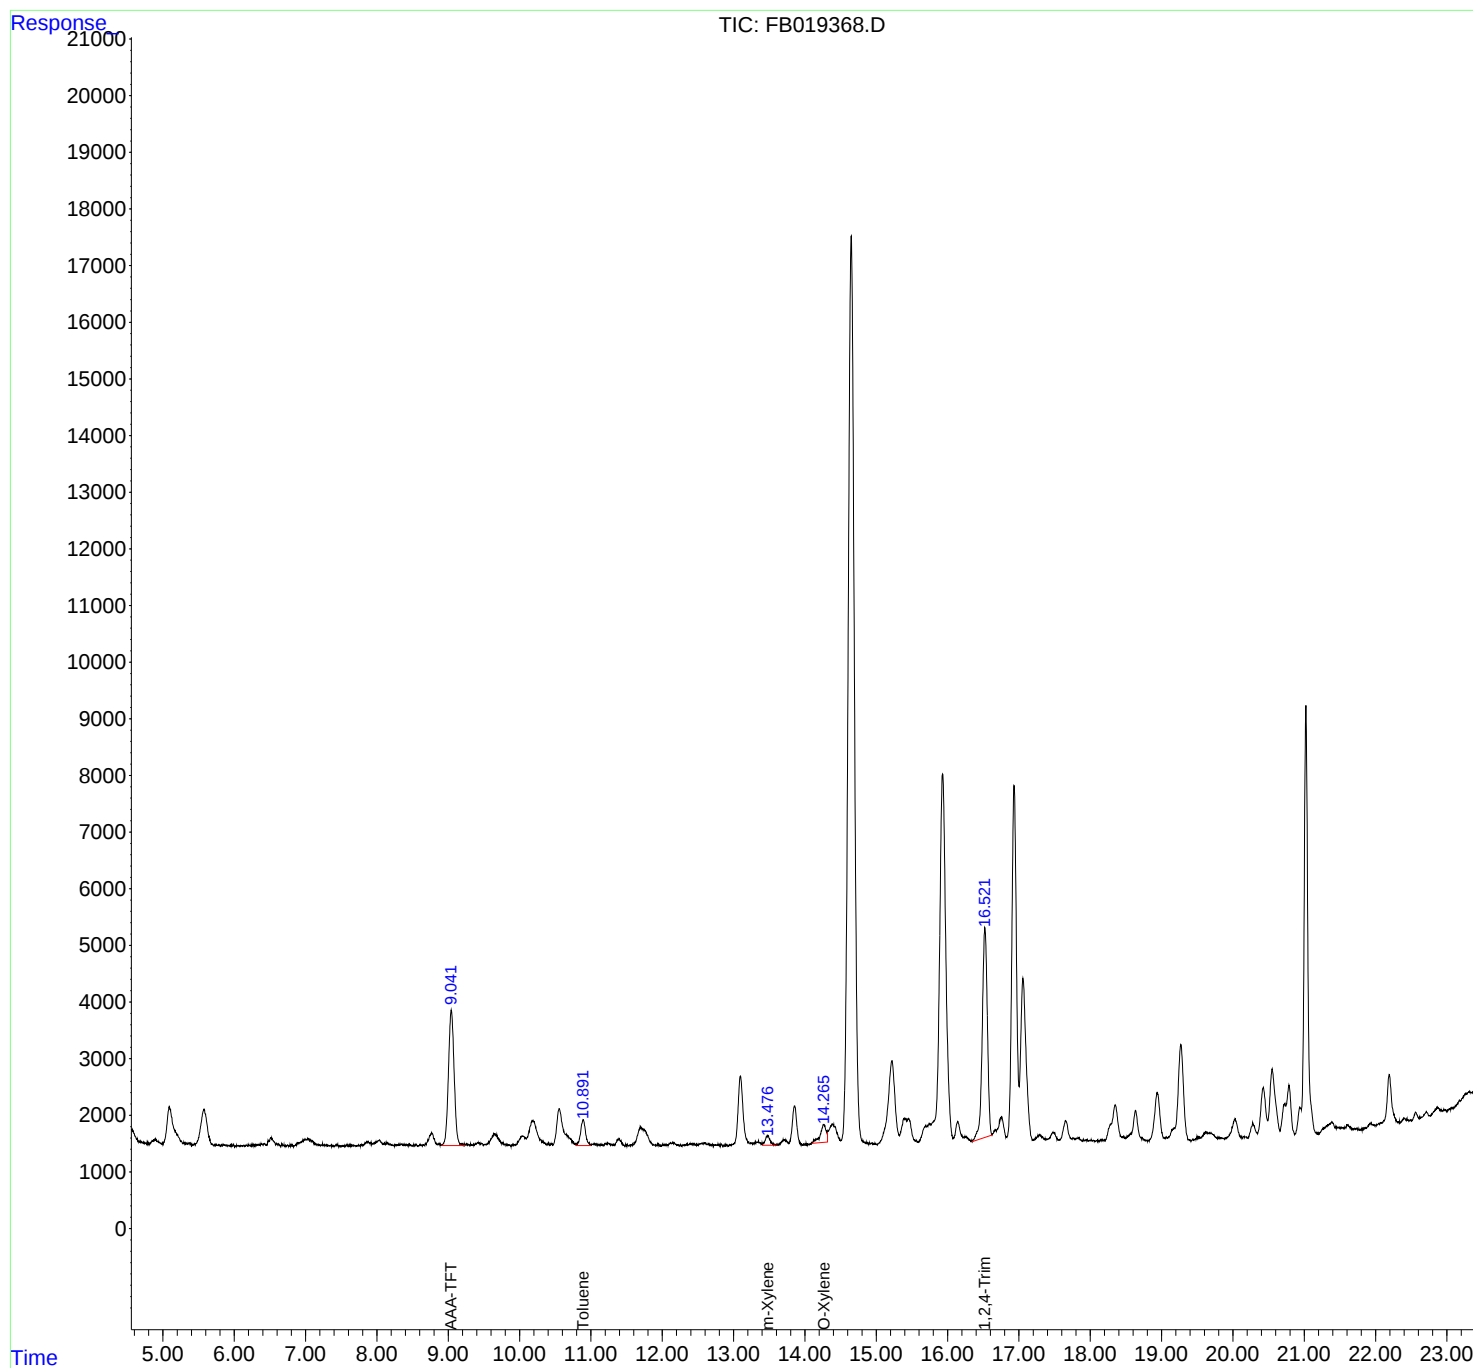


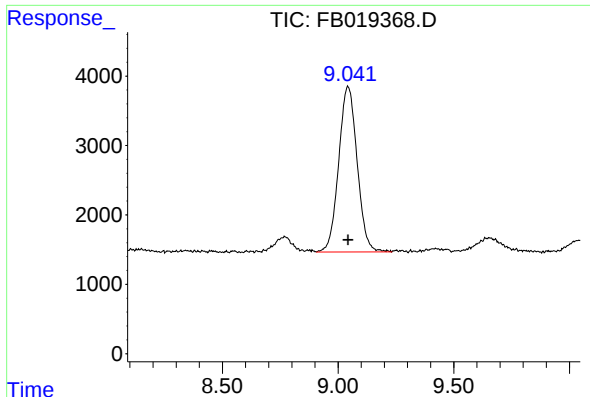

#5 AAA-TFT


R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 132440
Conc: 14.90 ng/ml

Instrument :
FID_B
ClientSampleId :

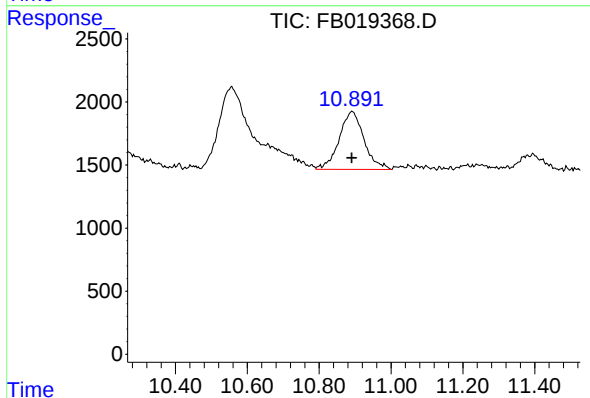


#6 Toluene

R.T.: 10.892 min
Delta R.T.: 0.002 min
Response: 21988
Conc: 1.22 ng/ml

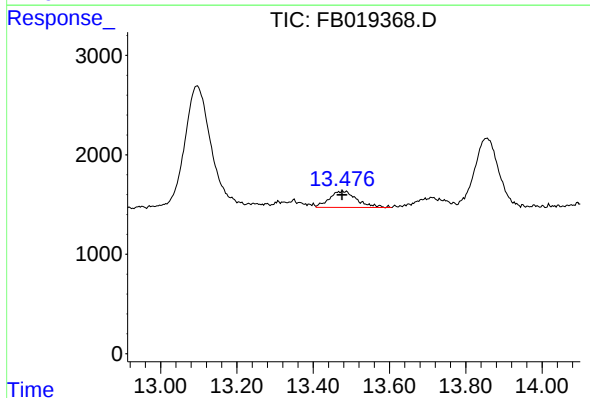


#8 m-Xylene

R.T.: 13.478 min
Delta R.T.: 0.002 min
Response: 8028
Conc: 0.35 ng/ml

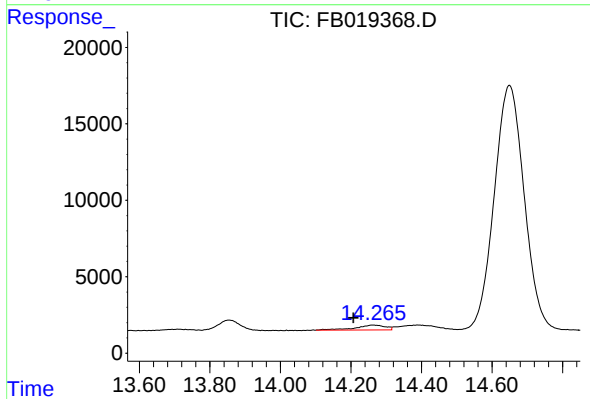

#9 O-Xylene

R.T.: 14.265 min
Delta R.T.: 0.057 min
Response: 18697
Conc: 0.83 ng/ml

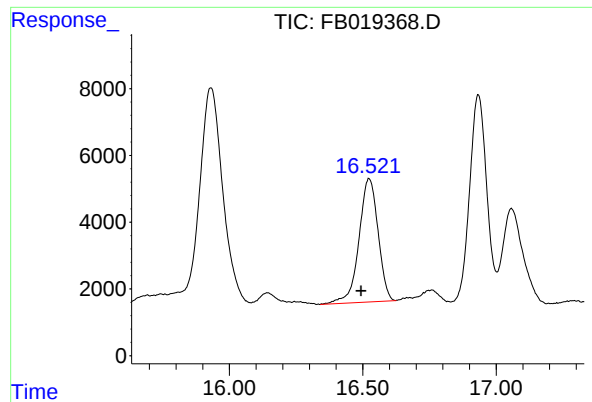

#10 1,2,4-Trimethylbenzene

R.T.: 16.524 min
Delta R.T.: 0.030 min
Response: 184040
Conc: 8.07 ng/ml

Instrument :
FID_B
ClientSampleId :