

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011022\
 Data File : FB026586.D
 Signal(s) : FID2B.CH
 Acq On : 10 Jan 2022 12:23
 Operator : AJ/MA
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 10 13:01:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
 Quant Title :
 QLast Update : Mon Jan 10 12:32:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	525404	51.318 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	1149803	73.206 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	1368351	74.775 ng/ml
3) t n-Heptane	7.744	439011	24.752 ng/ml
4) t Benzene	7.881	507462	24.912 ng/ml
6) t Toluene	10.614	1457626	74.330 ng/ml
7) t Ethylbenzene	13.051	454787	24.642 ng/ml
8) t m-Xylene	13.183	901787	48.933 ng/ml
9) t O-Xylene	13.911	869732	48.872 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	878656	47.973 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011022\
Data File : FB026586.D
Signal(s) : FID2B.CH
Acq On : 10 Jan 2022 12:23
Operator : AJ/MA
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 10 13:01:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011022.M
Quant Title :
QLast Update : Mon Jan 10 12:32:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

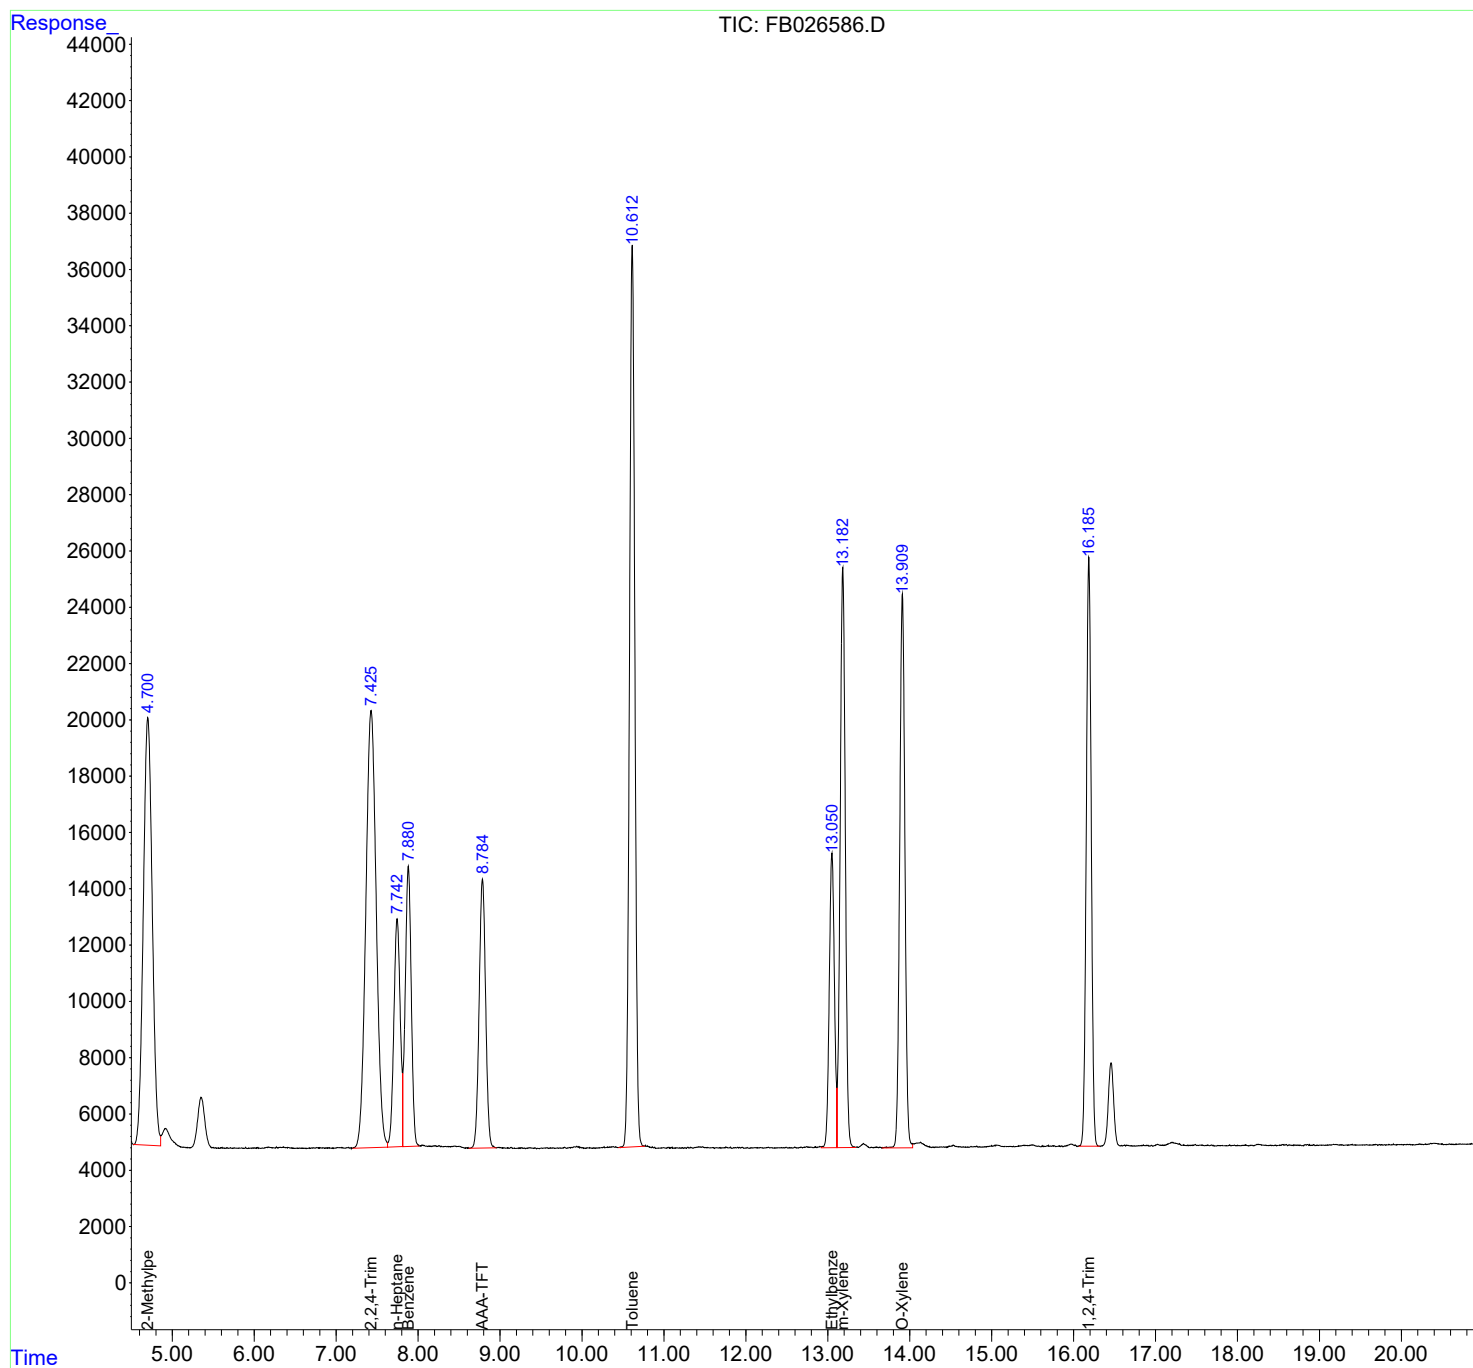


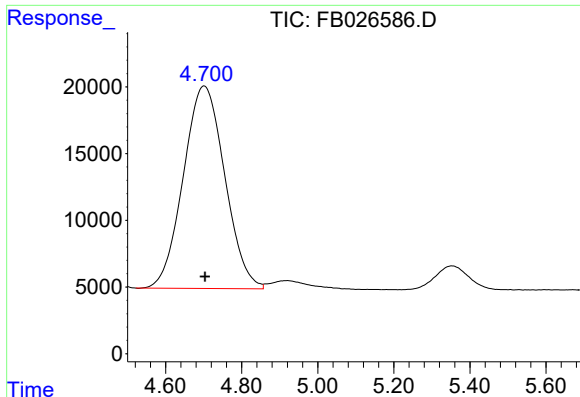

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 1149803
Conc: 73.21 ng/ml

Instrument :
FID_B
ClientSampleId :

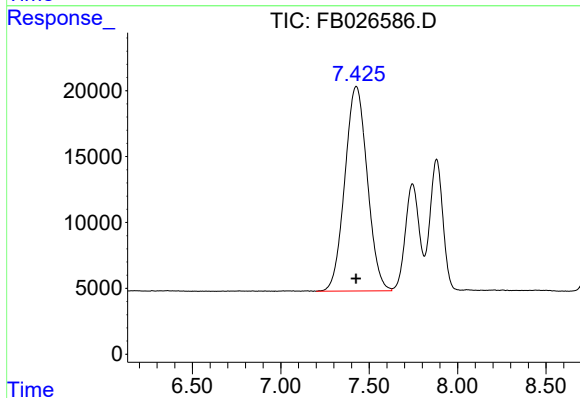


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: 0.002 min
Response: 1368351
Conc: 74.77 ng/ml

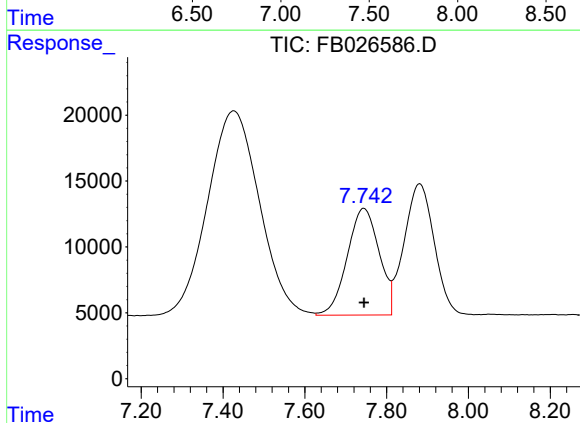


#3 n-Heptane

R.T.: 7.744 min
Delta R.T.: -0.001 min
Response: 439011
Conc: 24.75 ng/ml

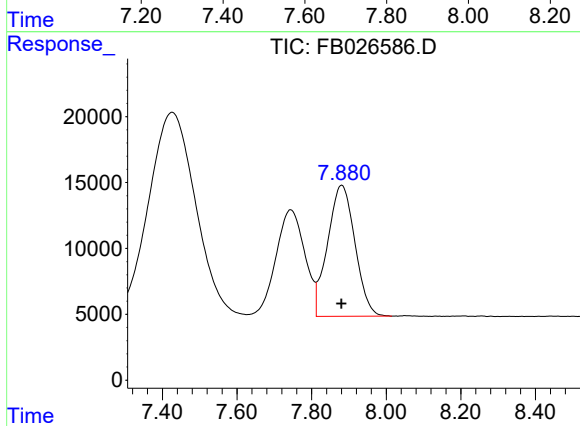

#4 Benzene


R.T.: 7.881 min
Delta R.T.: 0.000 min
Response: 507462
Conc: 24.91 ng/ml

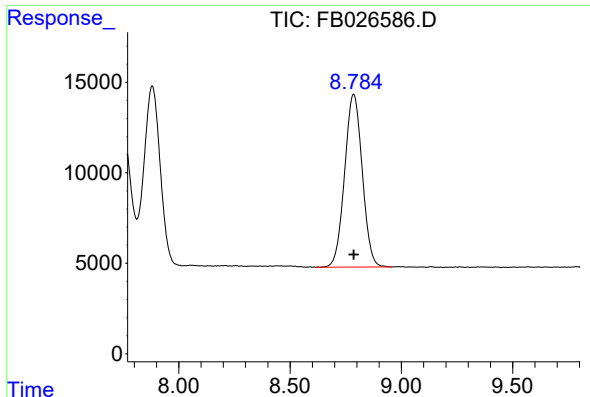

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 525404
Conc: 51.32 ng/ml

Instrument :
FID_B
ClientSampleId :

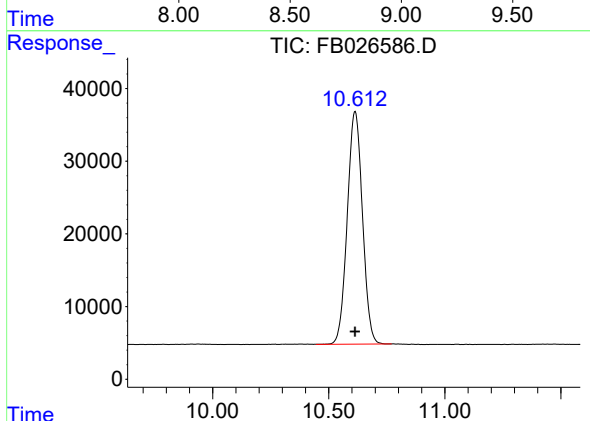


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 1457626
Conc: 74.33 ng/ml

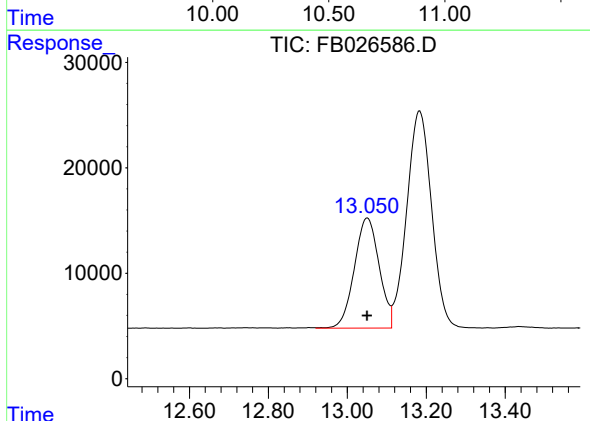


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.000 min
Response: 454787
Conc: 24.64 ng/ml

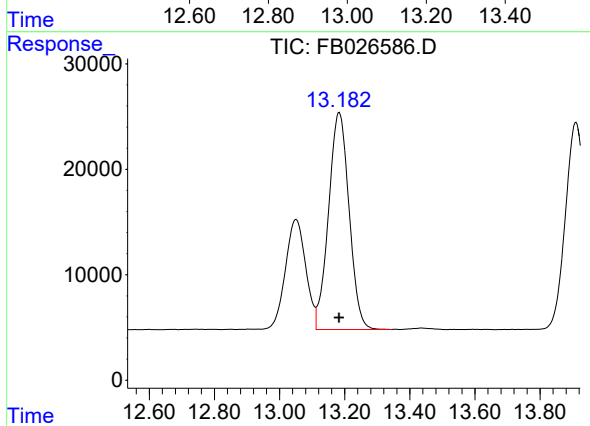

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 901787
Conc: 48.93 ng/ml

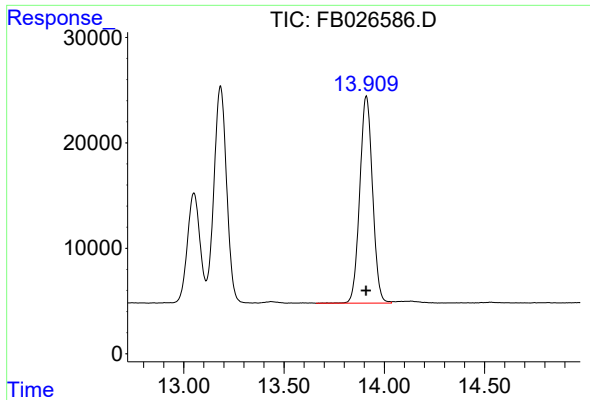

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.000 min
Response: 869732
Conc: 48.87 ng/ml

Instrument :
FID_B
ClientSampleId :

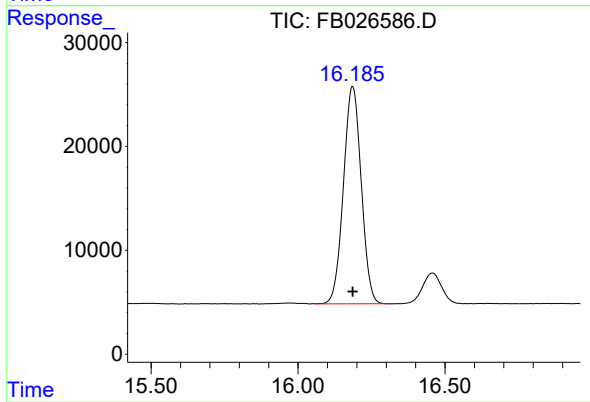

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.000 min
Response: 878656
Conc: 47.97 ng/ml