

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
 Data File : FB019378.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jan 2019 18:47
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 11 23:50:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.042	158810	17.872 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	534448	26.834 ng/ml
2) t 2,2,4-Trimethylpentane	7.655	527581	27.695 ng/ml
3) t n-Heptane	7.996	161255	9.242 ng/ml
4) t Benzene	8.134	185543	9.449 ng/ml
6) t Toluene	10.888	520353	28.766 ng/ml
7) t Ethylbenzene	13.339	216032	9.751 ng/ml
8) t m-Xylene	13.473	445949	19.433 ng/ml
9) t O-Xylene	14.205	440595	19.637 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	435146	19.084 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
Data File : FB019378.D
Signal(s) : FID2B.CH
Acq On : 11 Jan 2019 18:47
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 23:50:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

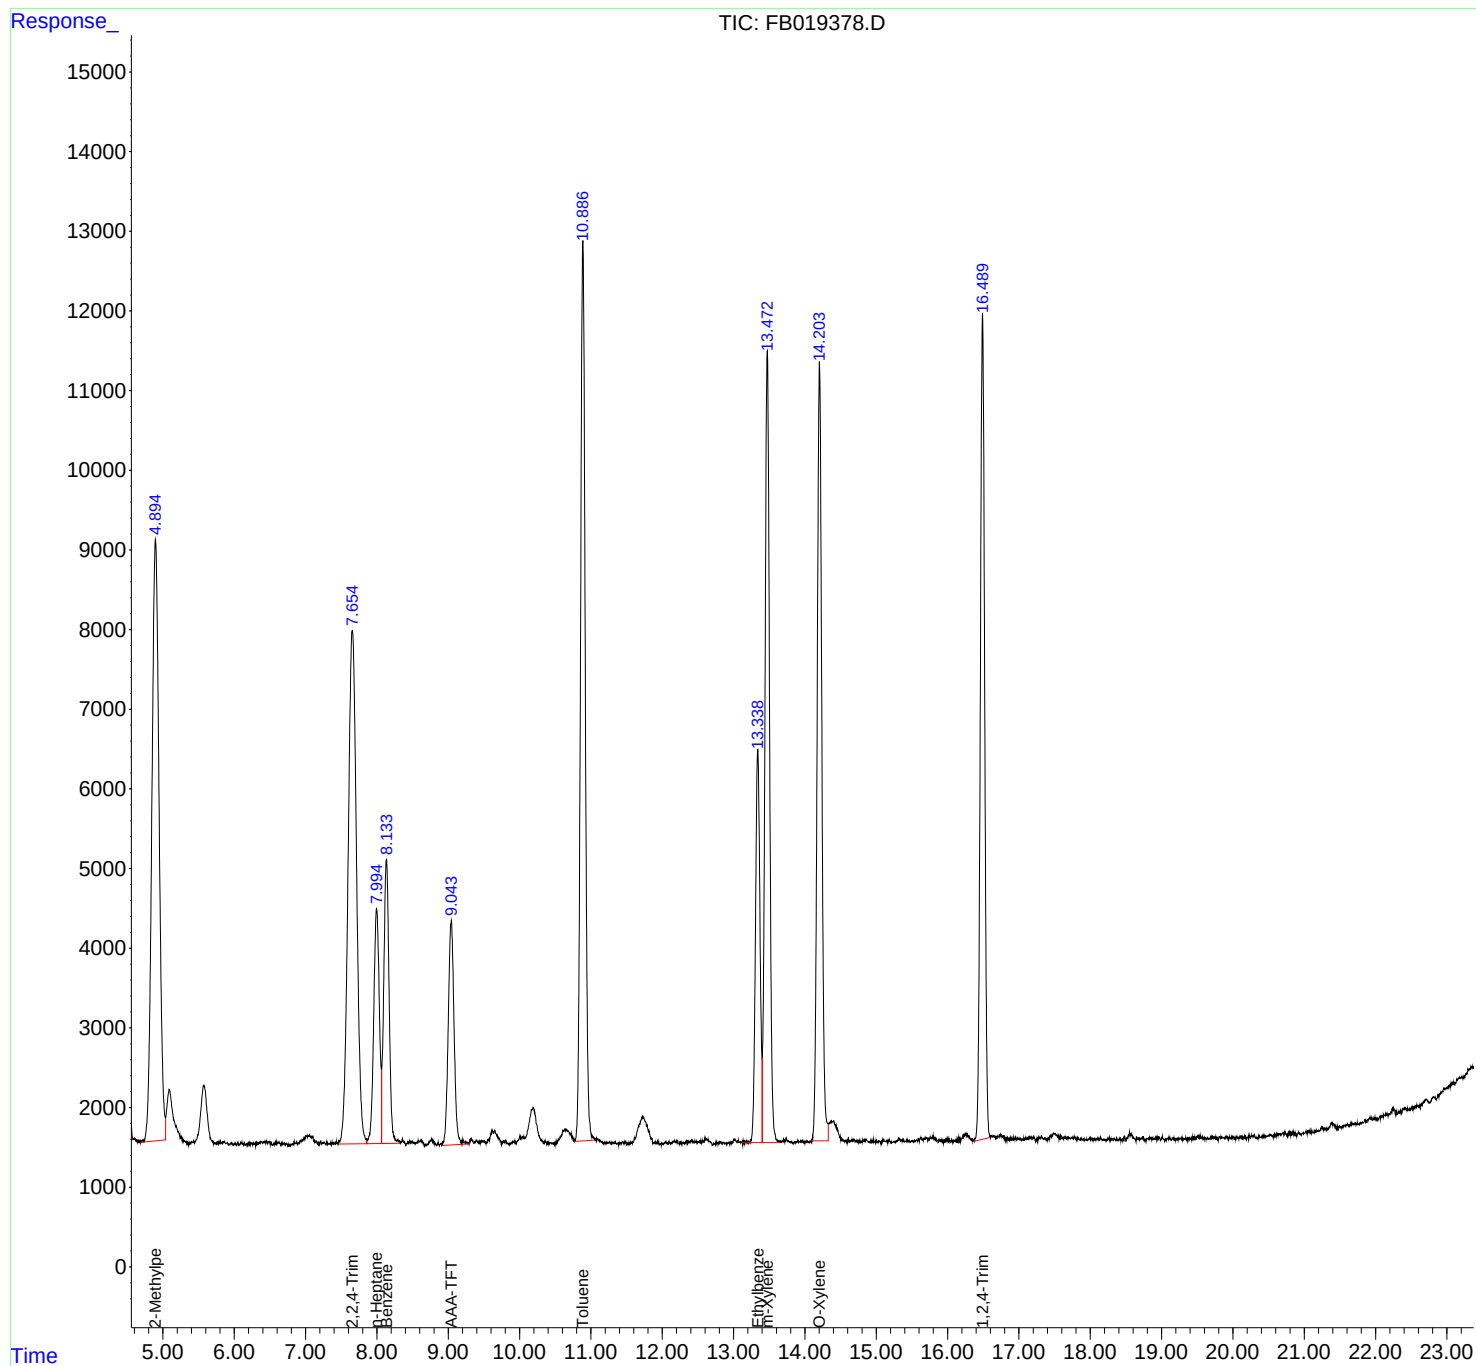


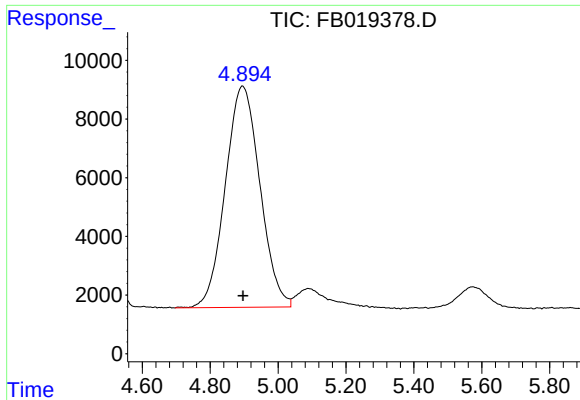

#1 2-Methylpentane


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 534448
Conc: 26.83 ng/ml

Instrument :
FID_B
ClientSampleId :

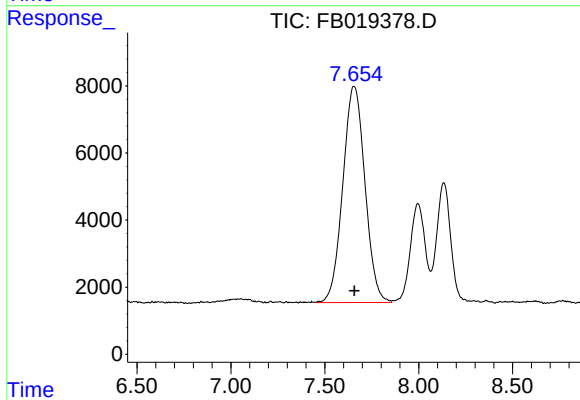


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.003 min
Response: 527581
Conc: 27.69 ng/ml

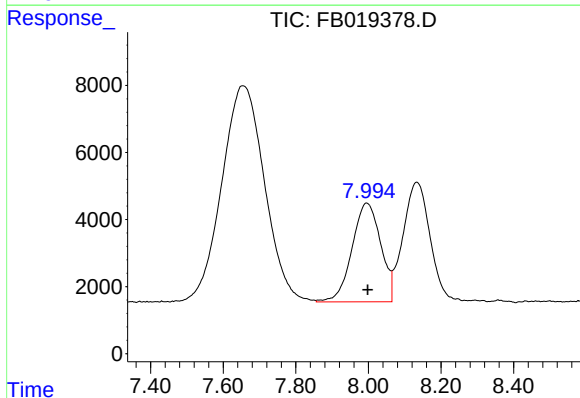


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 161255
Conc: 9.24 ng/ml

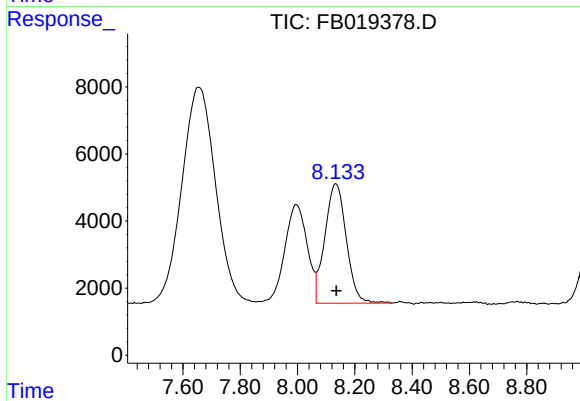

#4 Benzene


R.T.: 8.134 min
Delta R.T.: -0.001 min
Response: 185543
Conc: 9.45 ng/ml

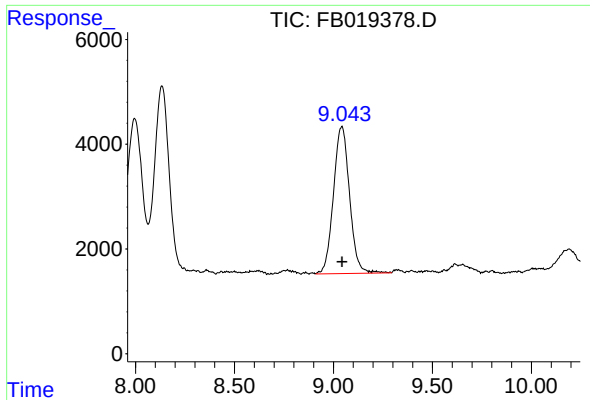

#5 AAA-TFT


R.T.: 9.042 min
Delta R.T.: -0.001 min
Response: 158810
Conc: 17.87 ng/ml

Instrument :
FID_B
ClientSampleId :

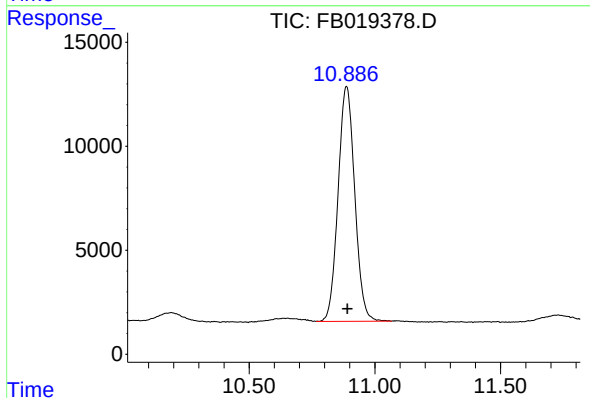


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.003 min
Response: 520353
Conc: 28.77 ng/ml

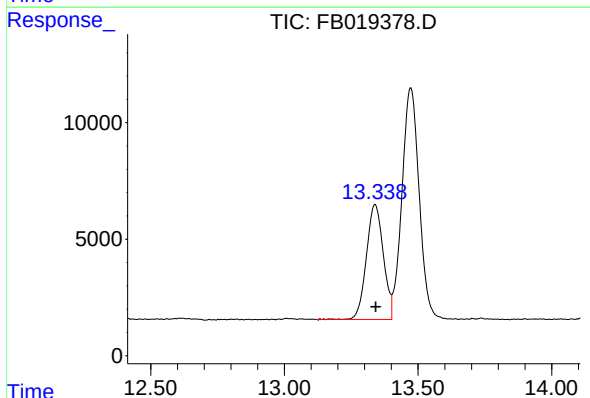


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.003 min
Response: 216032
Conc: 9.75 ng/ml

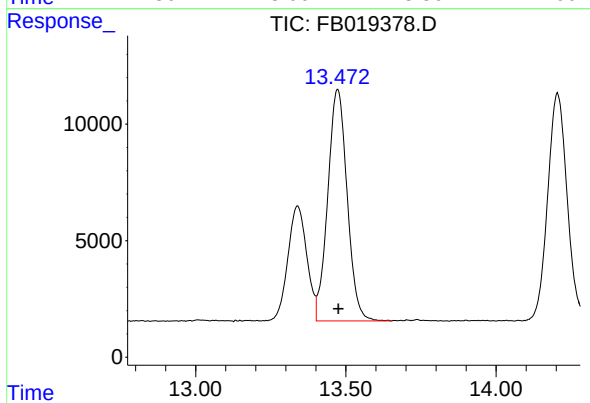

#8 m-Xylene


R.T.: 13.473 min
Delta R.T.: -0.003 min
Response: 445949
Conc: 19.43 ng/ml

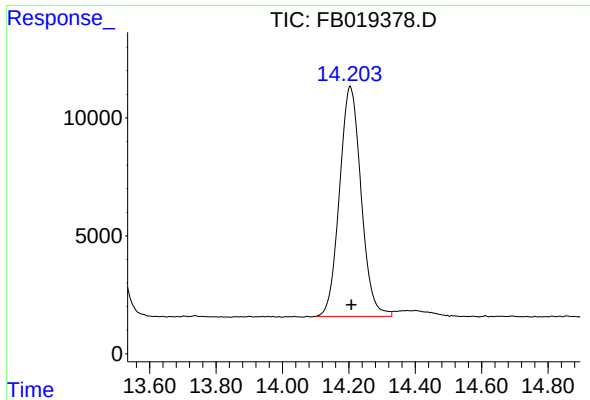

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: -0.003 min
Response: 440595
Conc: 19.64 ng/ml

Instrument :
FID_B
ClientSampleId :

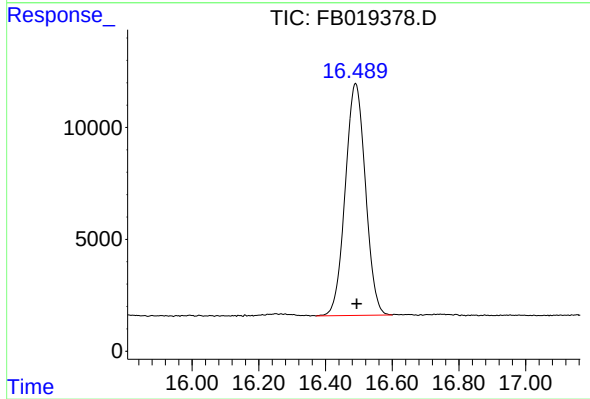

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: -0.003 min
Response: 435146
Conc: 19.08 ng/ml