

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
 Data File : FB019381.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jan 2019 20:16
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 11 23:50:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	164231	18.482 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	500393	25.125 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	484203	25.418 ng/ml
3) t n-Heptane	7.995	149273	8.555 ng/ml
4) t Benzene	8.132	178708	9.101 ng/ml
6) t Toluene	10.887	525698	29.062 ng/ml
7) t Ethylbenzene	13.338	207426	9.362 ng/ml
8) t m-Xylene	13.472	430678	18.767 ng/ml
9) t O-Xylene	14.204	419847	18.712 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	416302	18.257 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
Data File : FB019381.D
Signal(s) : FID2B.CH
Acq On : 11 Jan 2019 20:16
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 23:50:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

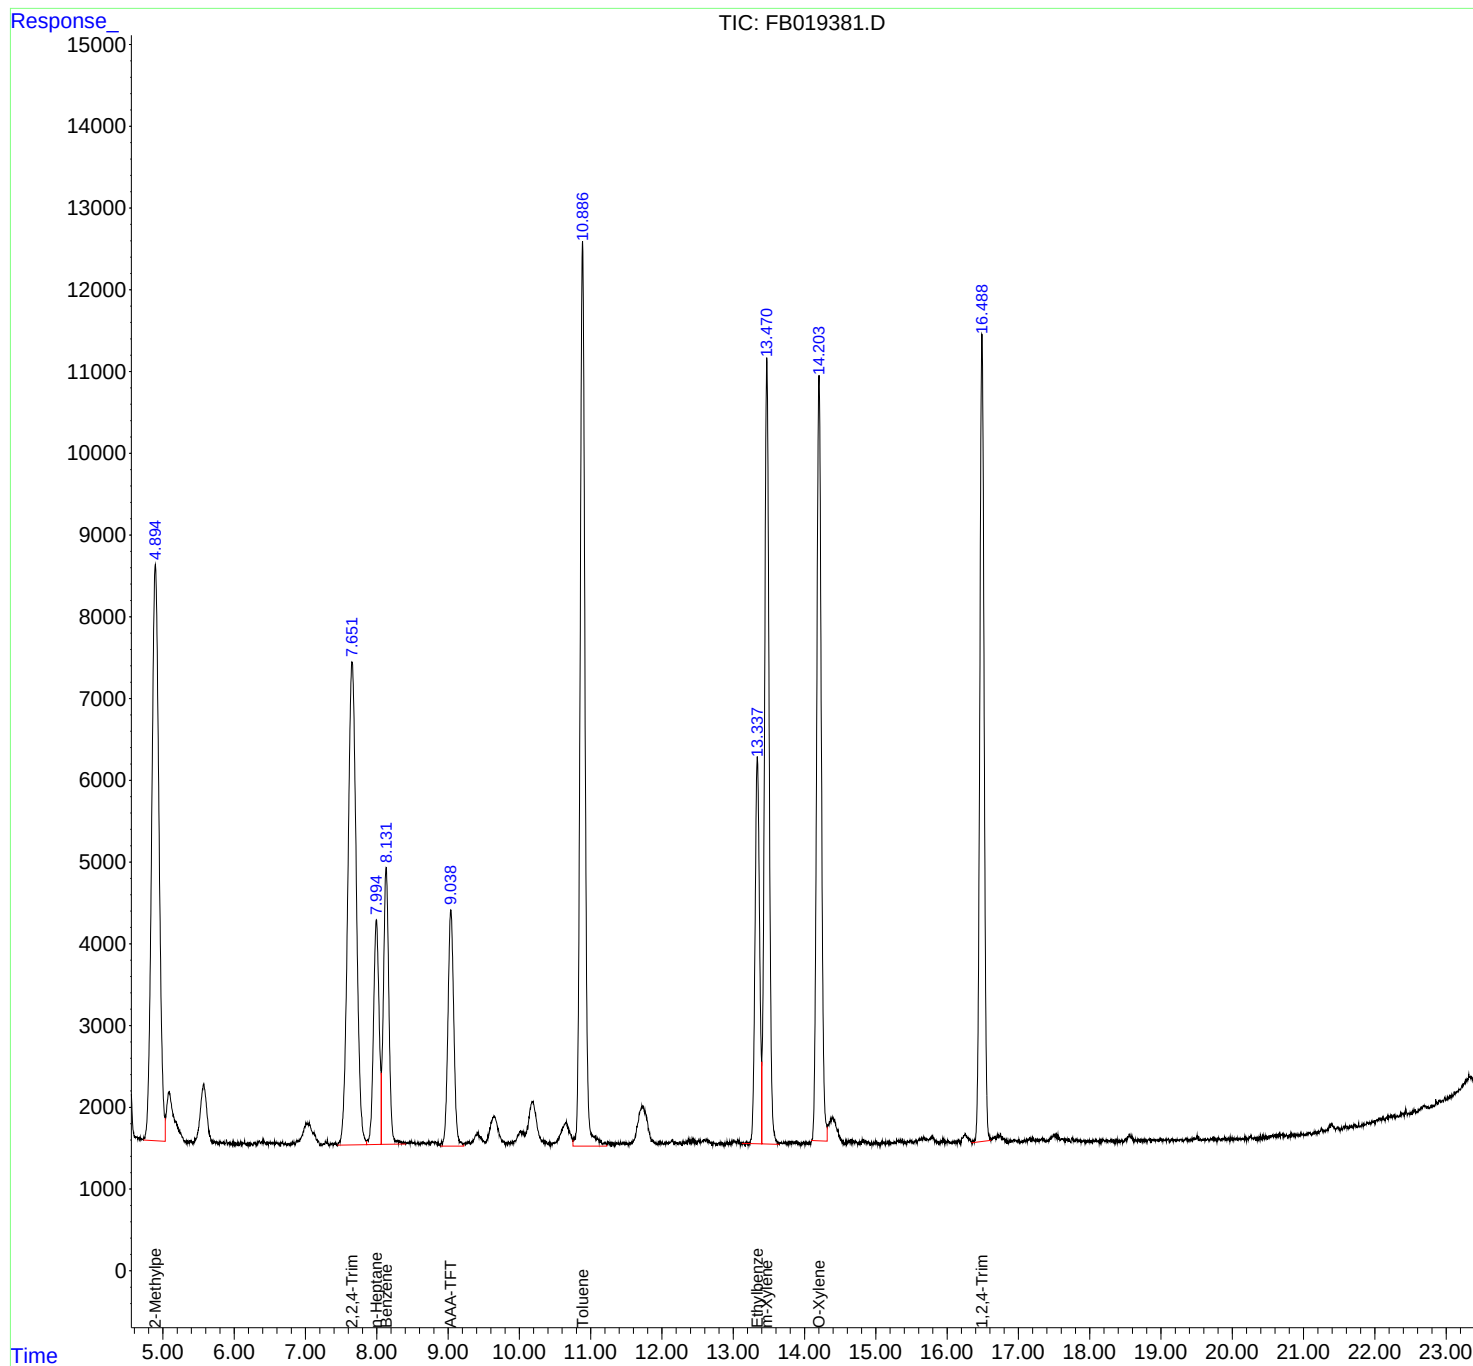


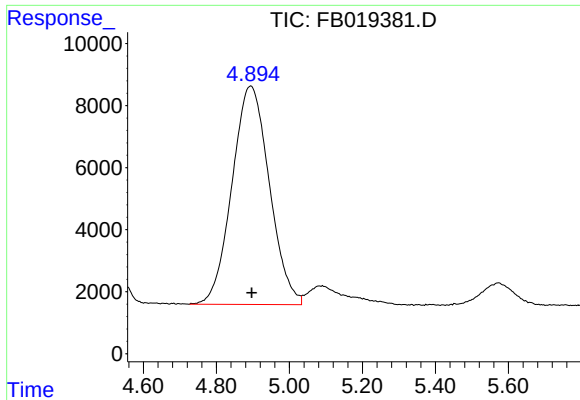

#1 2-Methylpentane


R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 500393
Conc: 25.12 ng/ml

Instrument :
FID_B
ClientSampleId :

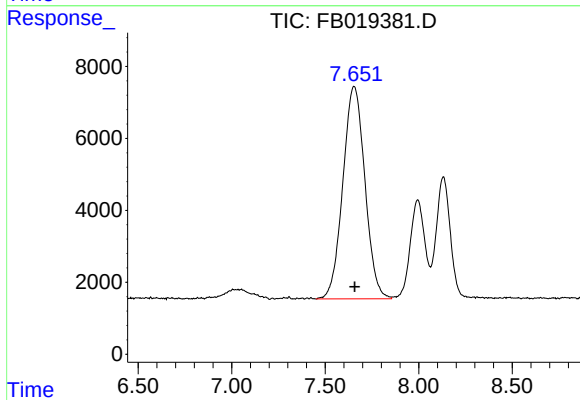


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.003 min
Response: 484203
Conc: 25.42 ng/ml

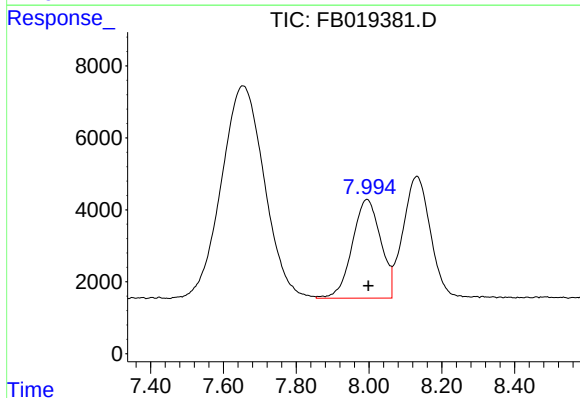


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.003 min
Response: 149273
Conc: 8.56 ng/ml

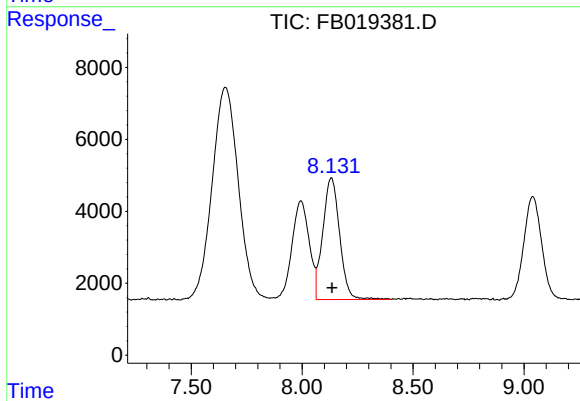

#4 Benzene


R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 178708
Conc: 9.10 ng/ml

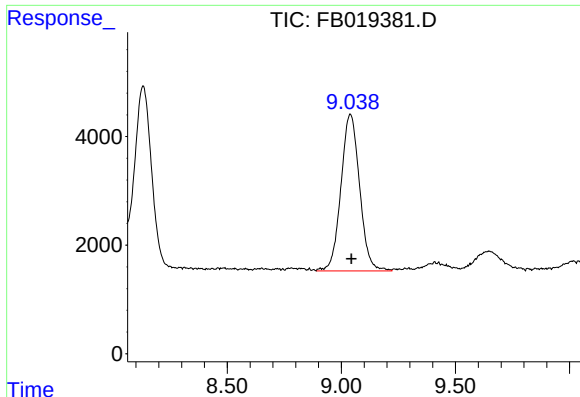

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: -0.004 min
Response: 164231
Conc: 18.48 ng/ml

Instrument :
FID_B
ClientSampleId :

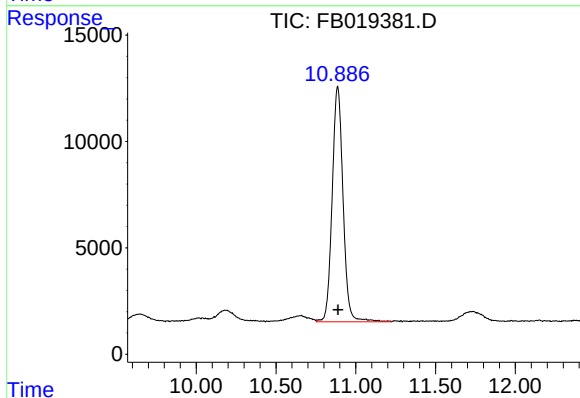


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.004 min
Response: 525698
Conc: 29.06 ng/ml

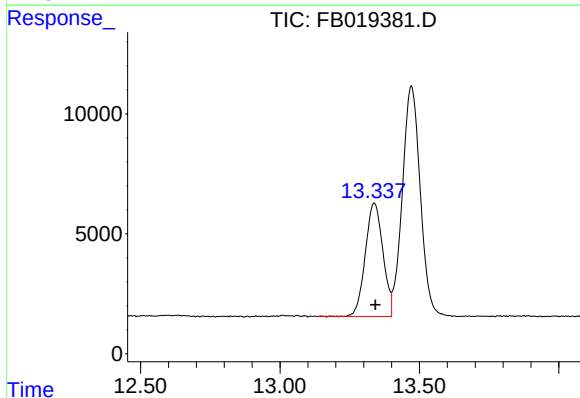


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.004 min
Response: 207426
Conc: 9.36 ng/ml

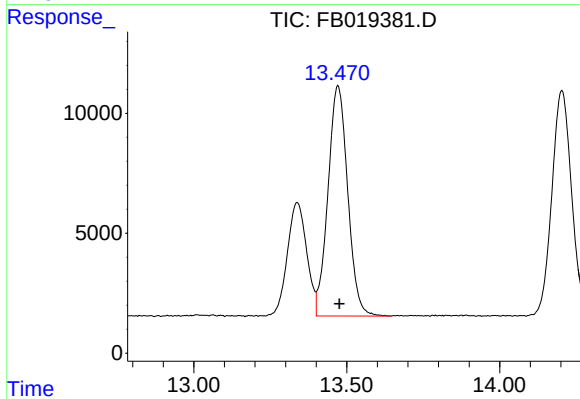

#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.004 min
Response: 430678
Conc: 18.77 ng/ml

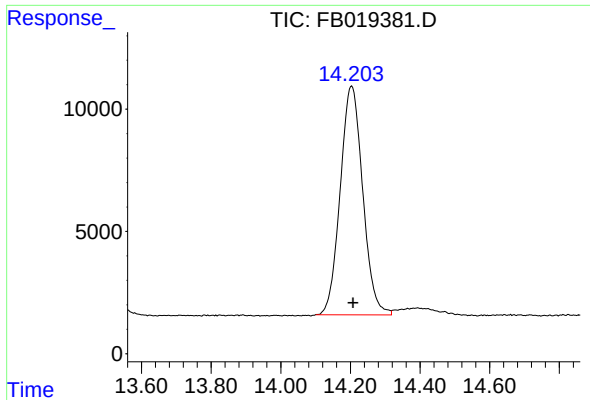

#9 O-Xylene


R.T.: 14.204 min

Delta R.T.: -0.004 min

Response: 419847

Conc: 18.71 ng/ml

Instrument :
FID_B
ClientSampleId :

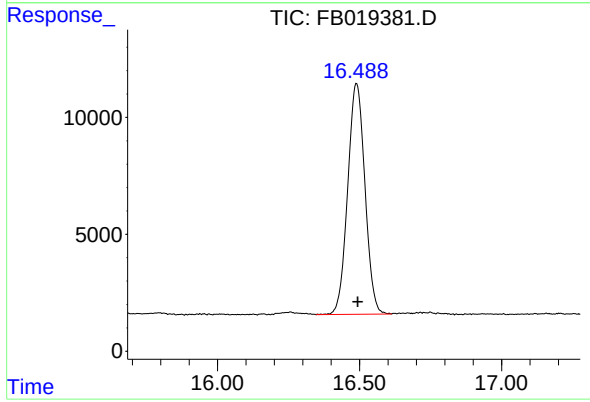

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min

Delta R.T.: -0.004 min

Response: 416302

Conc: 18.26 ng/ml