

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
 Data File : FB019372.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jan 2019 10:24
 Operator : MJ/SJ
 Sample : BSF0111S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 11 23:49:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.041	168957	19.014 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.895	559109	28.073 ng/ml
2) t	2,2,4-Trimethylpentane	7.654	542898	28.499 ng/ml
3) t	n-Heptane	7.996	165316	9.475 ng/ml
4) t	Benzene	8.132	190227	9.688 ng/ml
6) t	Toluene	10.887	543247	30.032 ng/ml
7) t	Ethylbenzene	13.340	219175	9.893 ng/ml
8) t	m-Xylene	13.472	450983	19.652 ng/ml
9) t	O-Xylene	14.205	438184	19.529 ng/ml
10) t	1,2,4-Trimethylbenzene	16.491	436085	19.125 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
Data File : FB019372.D
Signal(s) : FID2B.CH
Acq On : 11 Jan 2019 10:24
Operator : MJ/SJ
Sample : BSF0111S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 11 23:49:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

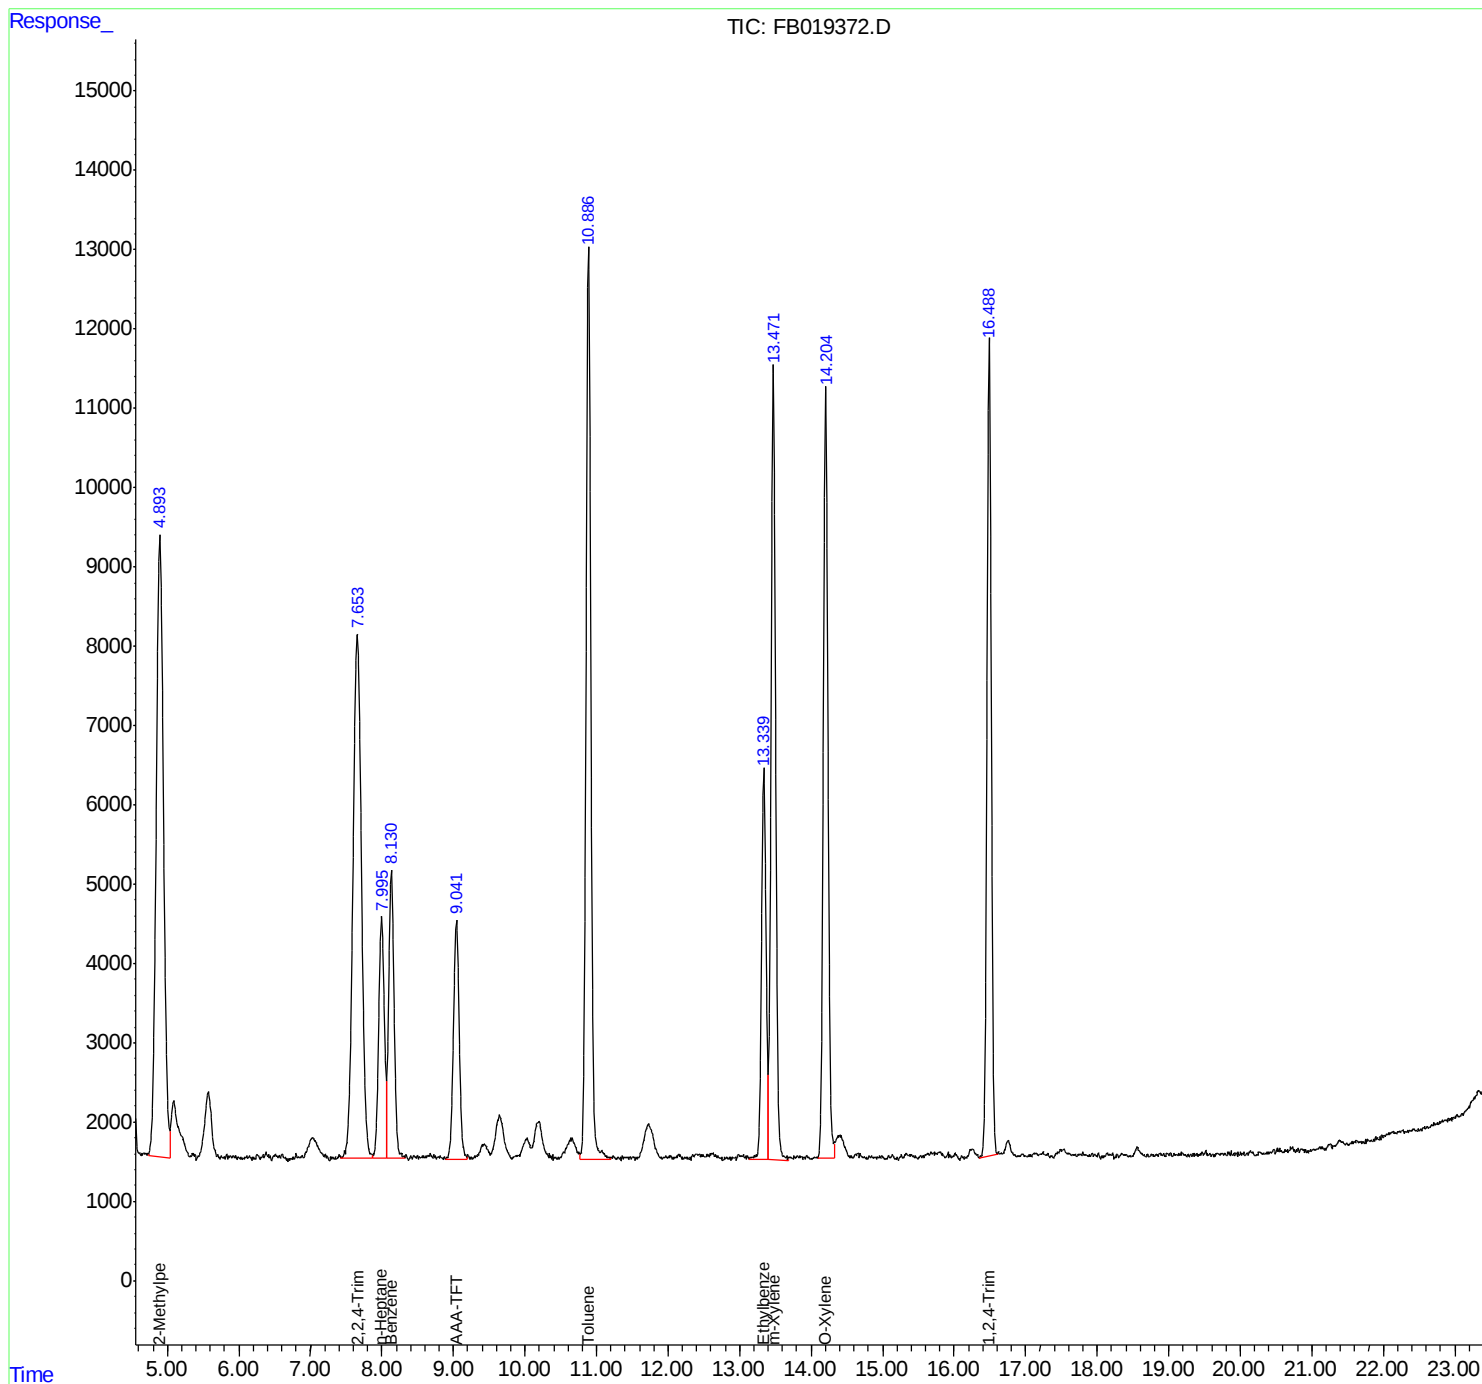


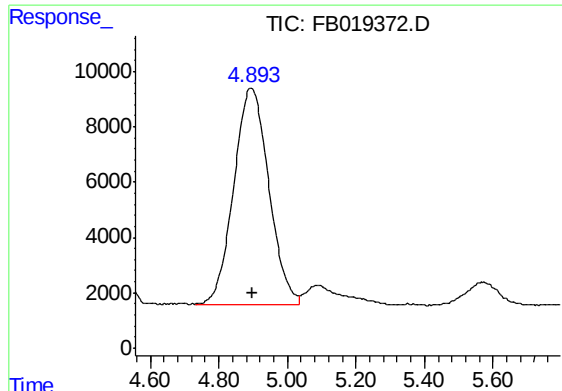

#1 2-Methylpentane


R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 559109
Conc: 28.07 ng/ml

Instrument :
FID_B
ClientSampleId :

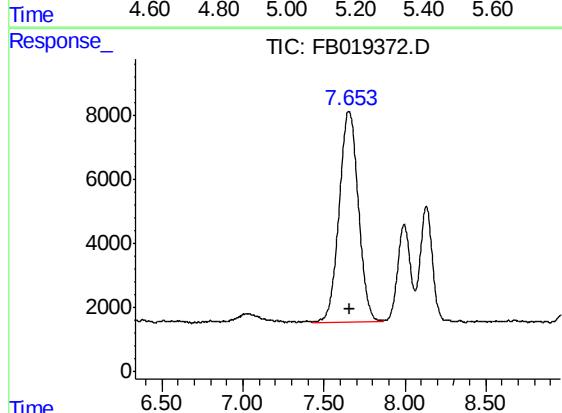


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.004 min
Response: 542898
Conc: 28.50 ng/ml

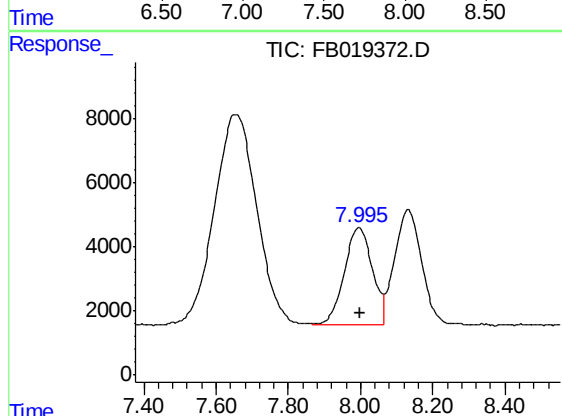


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 165316
Conc: 9.47 ng/ml

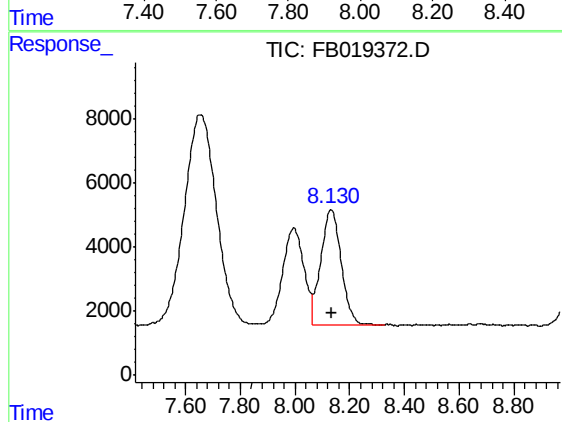

#4 Benzene


R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 190227
Conc: 9.69 ng/ml

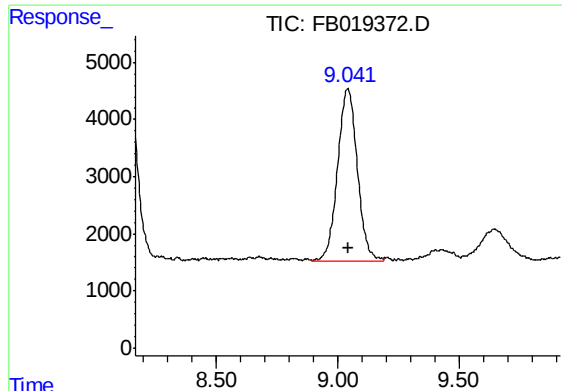

#5 AAA-TFT


R.T.: 9.041 min
Delta R.T.: -0.002 min
Response: 168957
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :

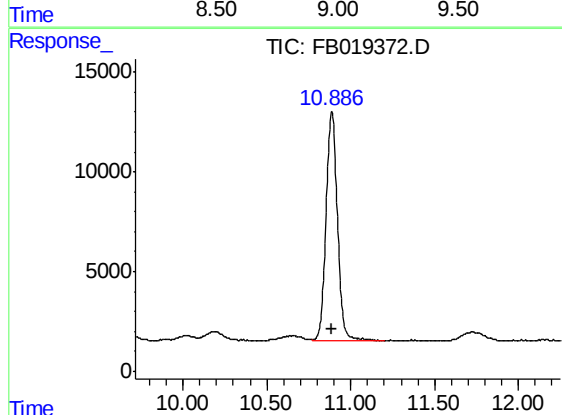


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.003 min
Response: 543247
Conc: 30.03 ng/ml

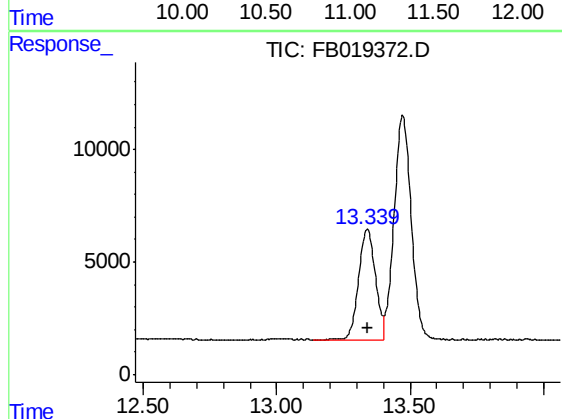


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.002 min
Response: 219175
Conc: 9.89 ng/ml

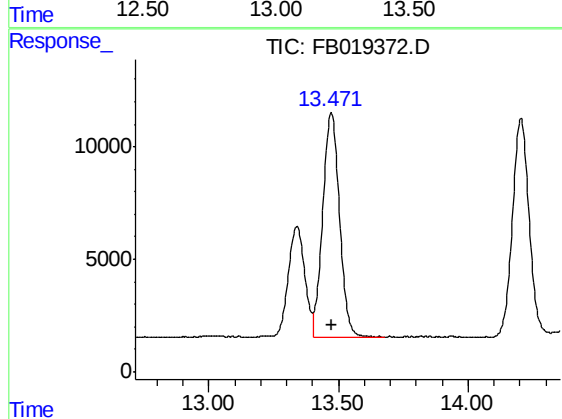

#8 m-Xylene


R.T.: 13.472 min
Delta R.T.: -0.003 min
Response: 450983
Conc: 19.65 ng/ml

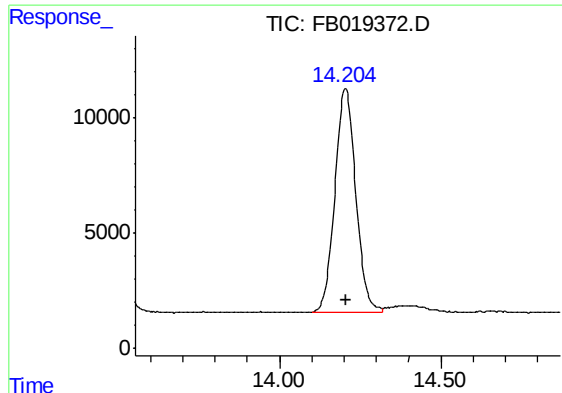

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: -0.003 min
Response: 438184
Conc: 19.53 ng/ml

Instrument :
FID_B
ClientSampleId :

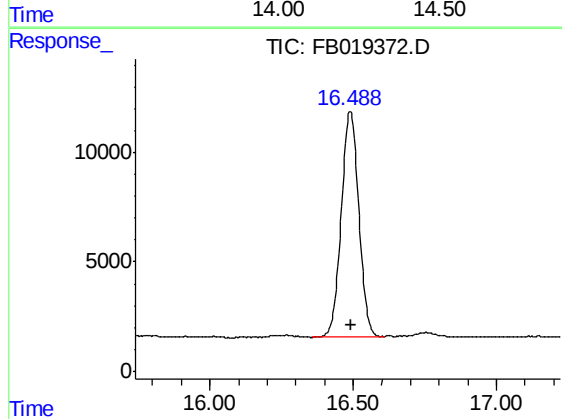

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: -0.003 min
Response: 436085
Conc: 19.12 ng/ml