

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
 Data File : FB019375.D
 Signal(s) : FID2B.CH
 Acq On : 11 Jan 2019 17:18
 Operator : MJ/SJ
 Sample : K1128-01MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RBR-200053MSD

Integration File: Calibration.e
 Quant Time: Jan 11 23:49:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	183372	20.636 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.896	535171	26.871 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	518015	27.192 ng/ml
3) t n-Heptane	7.996	153910	8.821 ng/ml
4) t Benzene	8.133	186299	9.488 ng/ml
6) t Toluene	10.888	529732	29.285 ng/ml
7) t Ethylbenzene	13.340	214916	9.700 ng/ml
8) t m-Xylene	13.473	447417	19.497 ng/ml
9) t O-Xylene	14.205	435864	19.426 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	434561	19.058 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011119\
Data File : FB019375.D
Signal(s) : FID2B.CH
Acq On : 11 Jan 2019 17:18
Operator : MJ/SJ
Sample : K1128-01MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RBR-200053MSD

Integration File: Calibration.e
Quant Time: Jan 11 23:49:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

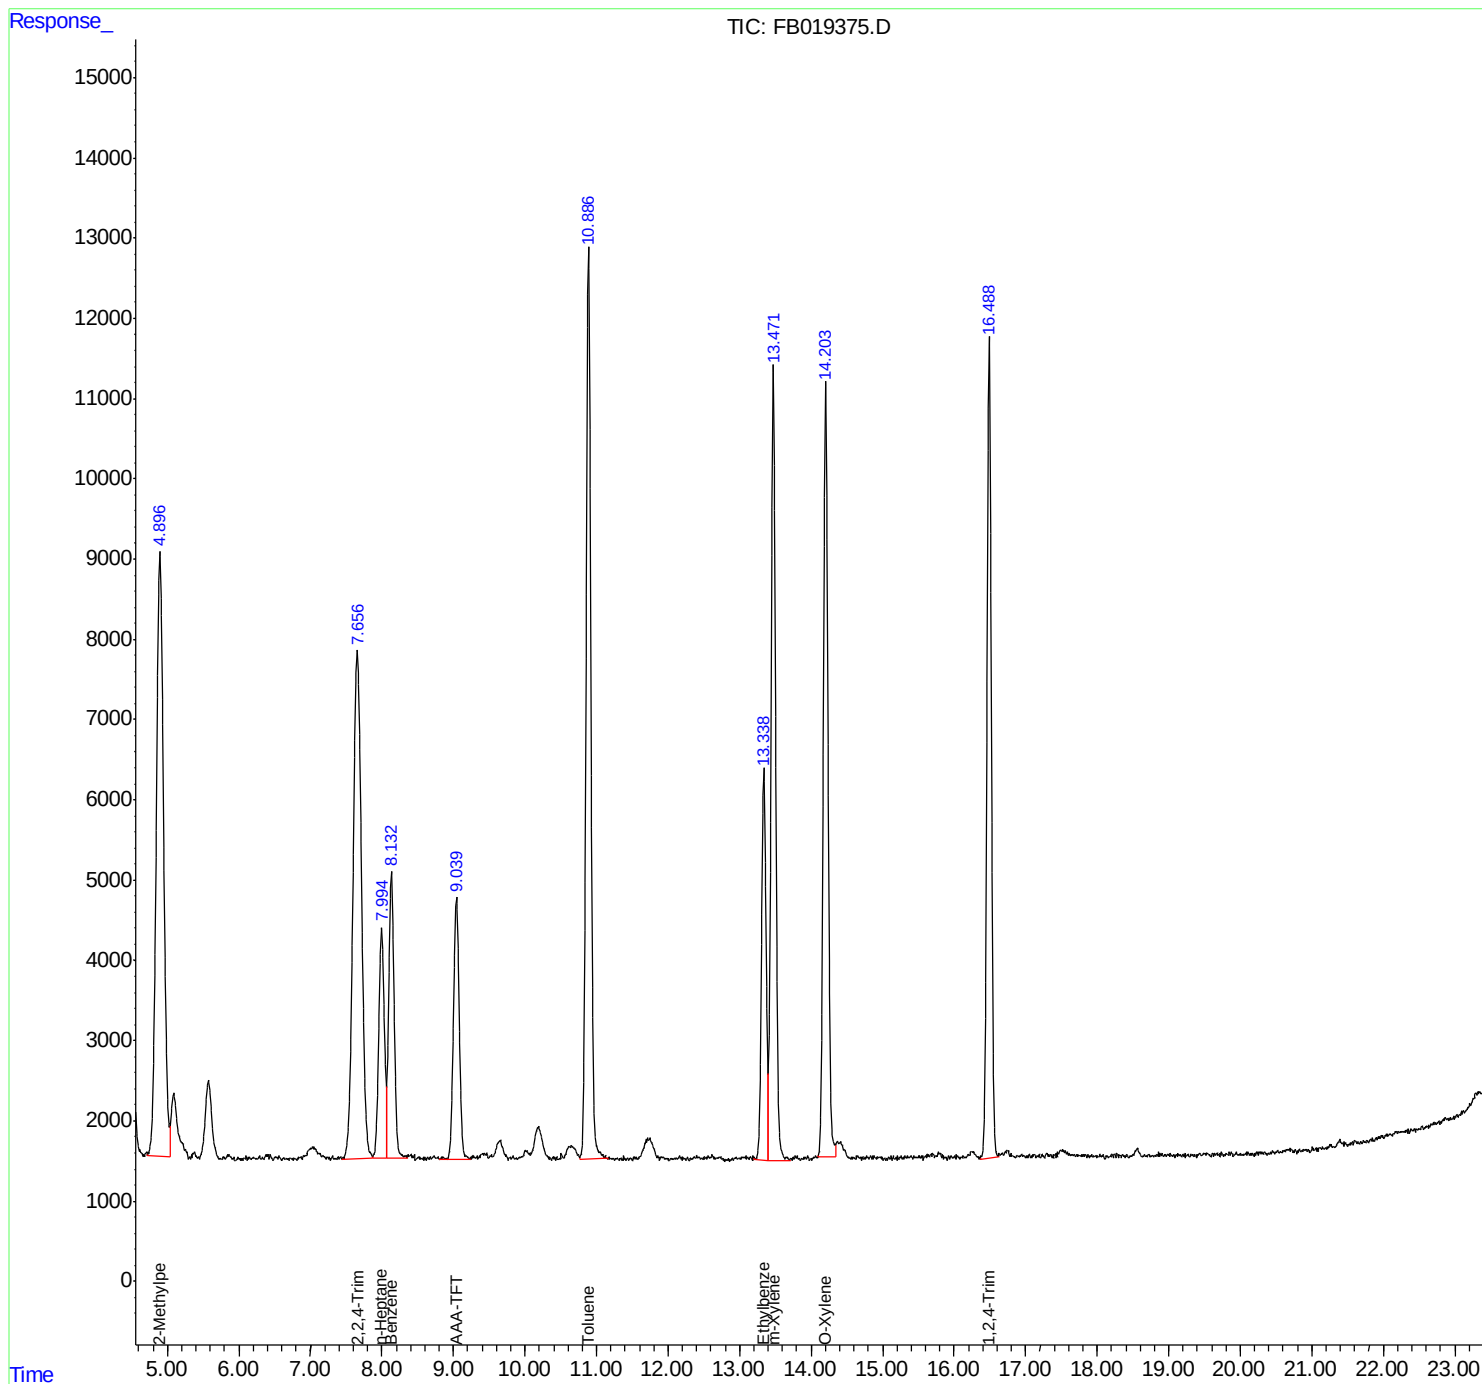


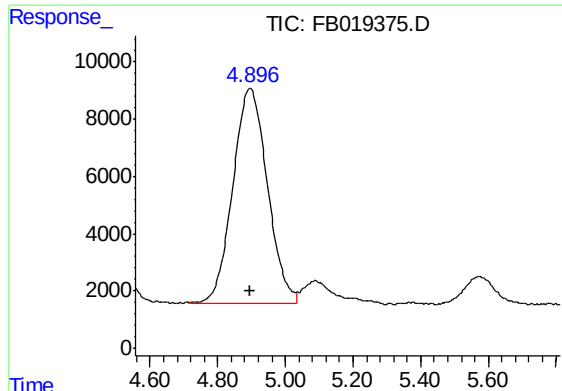

#1 2-Methylpentane


R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 535171
Conc: 26.87 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200053MSD

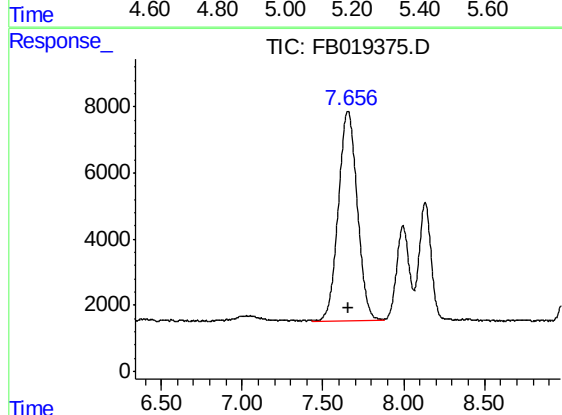


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: -0.001 min
Response: 518015
Conc: 27.19 ng/ml

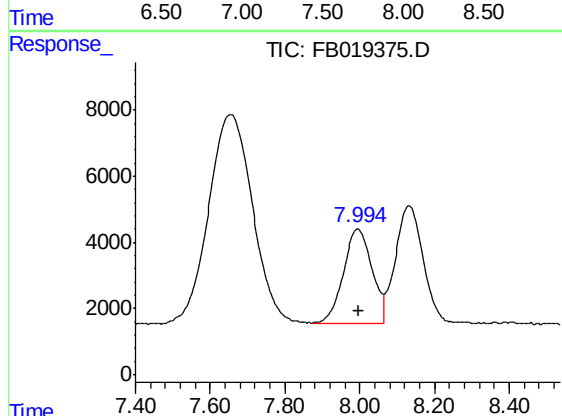


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 153910
Conc: 8.82 ng/ml

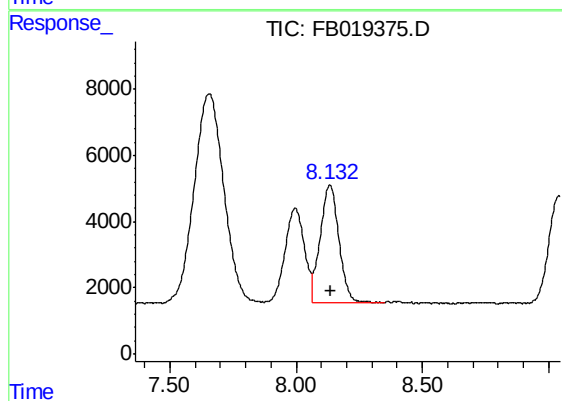

#4 Benzene


R.T.: 8.133 min
Delta R.T.: -0.002 min
Response: 186299
Conc: 9.49 ng/ml

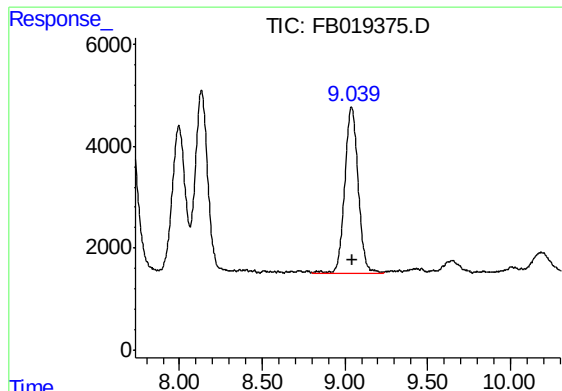

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: -0.003 min
Response: 183372
Conc: 20.64 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200053MSD

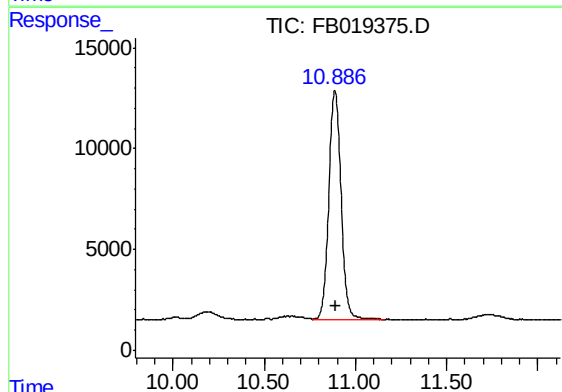


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.003 min
Response: 529732
Conc: 29.28 ng/ml

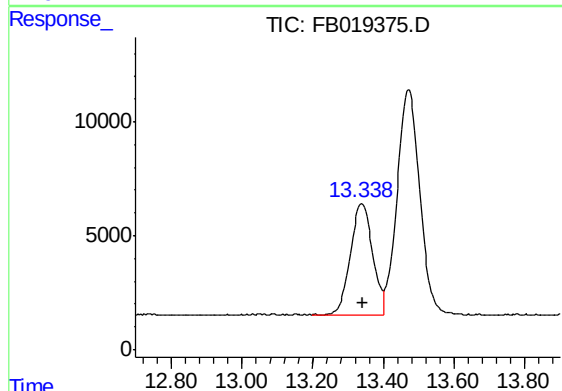


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.003 min
Response: 214916
Conc: 9.70 ng/ml

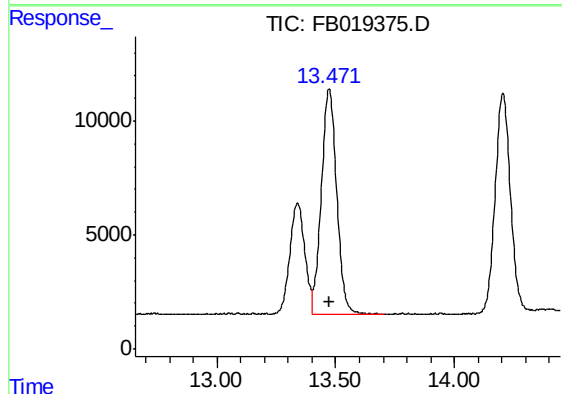

#8 m-Xylene


R.T.: 13.473 min
Delta R.T.: -0.003 min
Response: 447417
Conc: 19.50 ng/ml

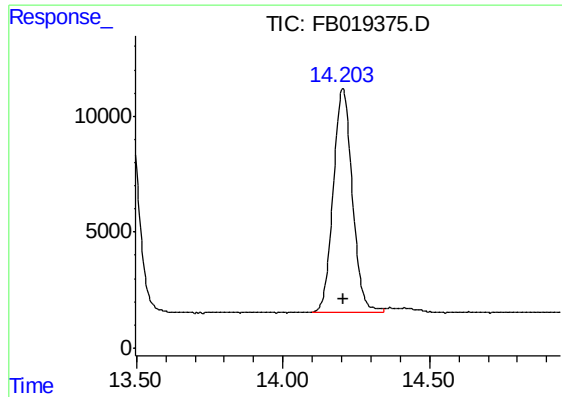

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: -0.003 min
Response: 435864
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :
RBR-200053MSD

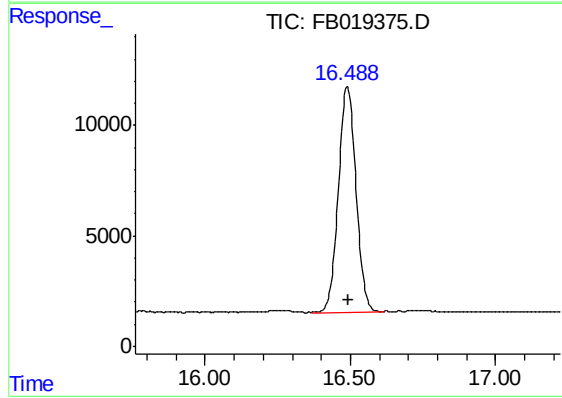

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: -0.004 min
Response: 434561
Conc: 19.06 ng/ml