

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011321\
 Data File : FB025390.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jan 2021 16:26
 Operator : DD/AJ
 Sample : BSF0113S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0113S1

Integration File: Calibration.e
 Quant Time: Jan 13 23:00:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	425712	18.924 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	938529	29.816 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1000259	31.550 ng/ml
3) t n-Heptane	7.758	324852	10.388 ng/ml
4) t Benzene	7.893	391188	9.950 ng/ml
6) t Toluene	10.631	1126067	29.997 ng/ml
7) t Ethylbenzene	13.072	358511	10.467 ng/ml
8) t m-Xylene	13.205	708493	20.708 ng/ml
9) t O-Xylene	13.933	695504	20.923 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	599815	20.858 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011321\
Data File : FB025390.D
Signal(s) : FID2B.CH
Acq On : 13 Jan 2021 16:26
Operator : DD/AJ
Sample : BSF0113S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0113S1

Integration File: Calibration.e
Quant Time: Jan 13 23:00:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

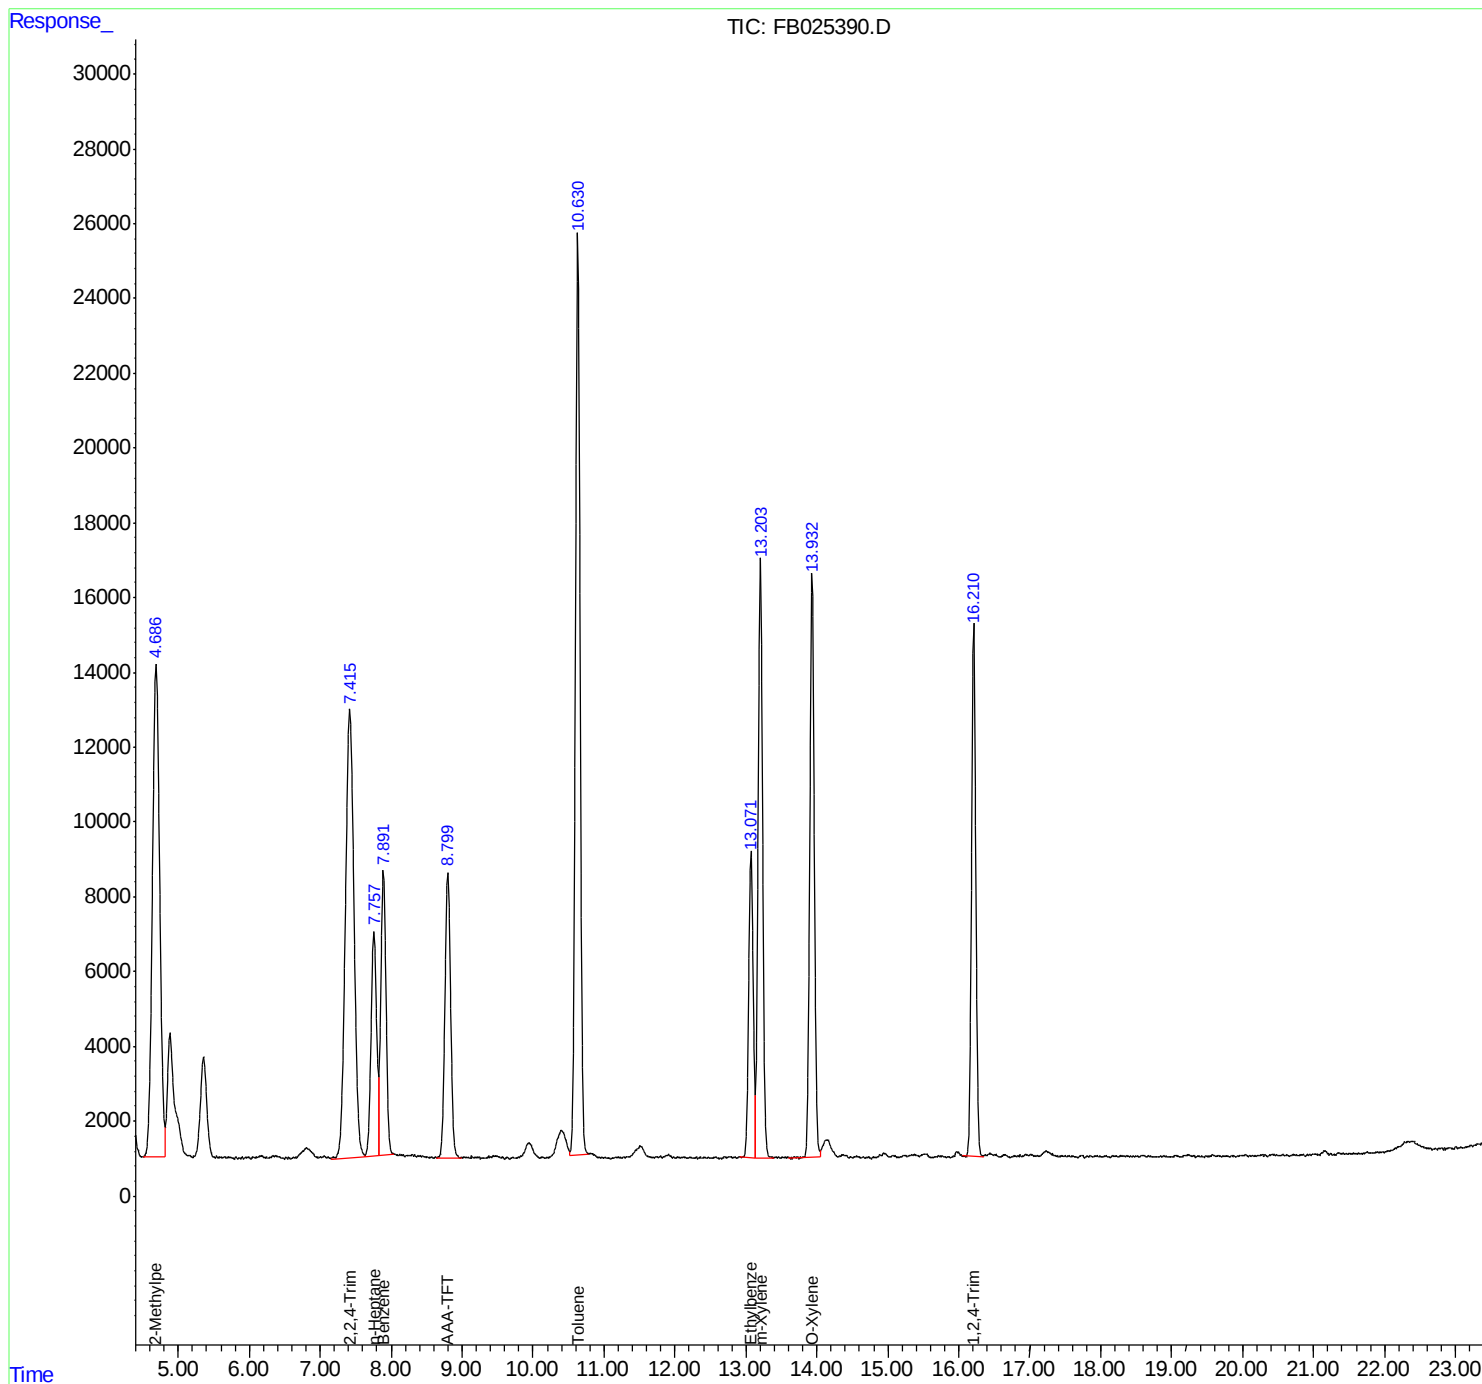


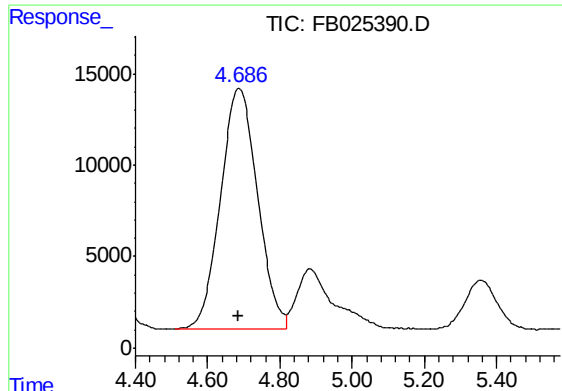

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.001 min
Response: 938529
Conc: 29.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0113S1

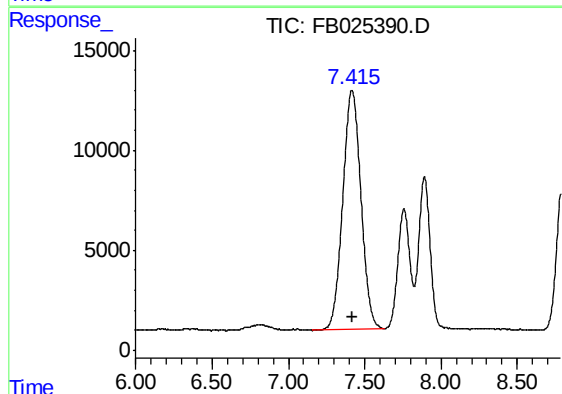


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1000259
Conc: 31.55 ng/ml

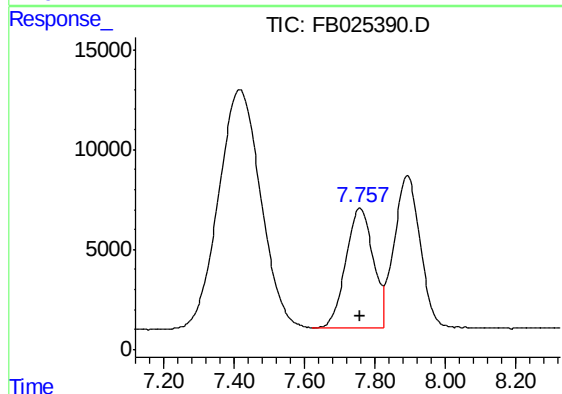


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.001 min
Response: 324852
Conc: 10.39 ng/ml

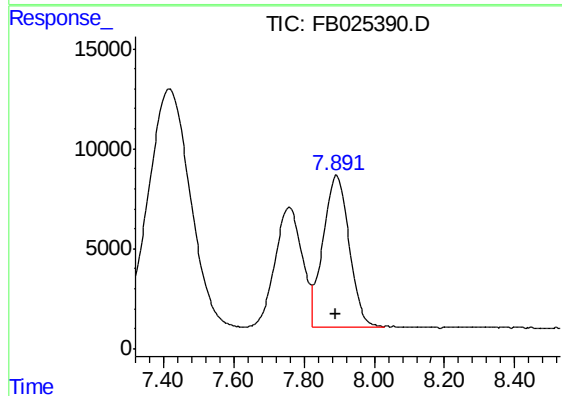

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 391188
Conc: 9.95 ng/ml

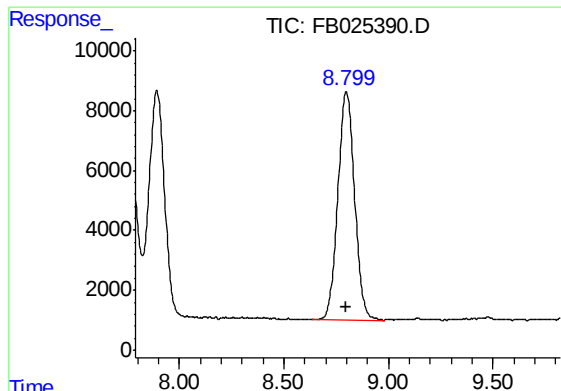

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 425712
Conc: 18.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0113S1

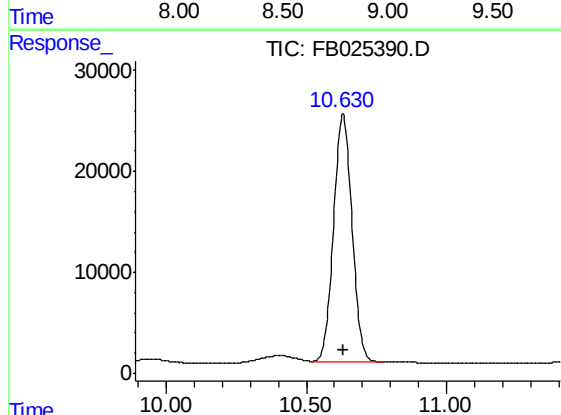


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1126067
Conc: 30.00 ng/ml

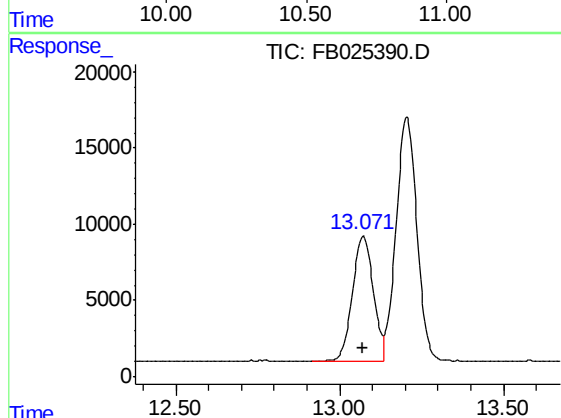


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 358511
Conc: 10.47 ng/ml

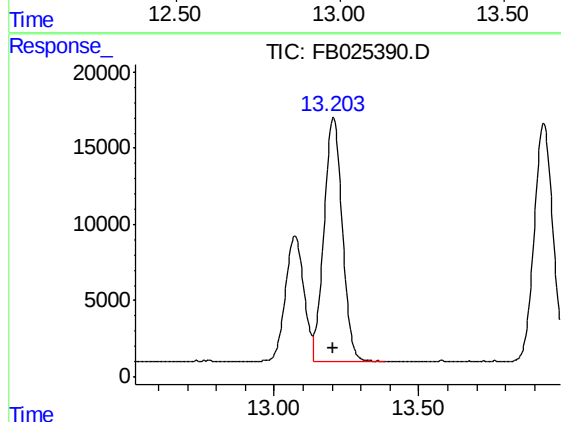

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 708493
Conc: 20.71 ng/ml

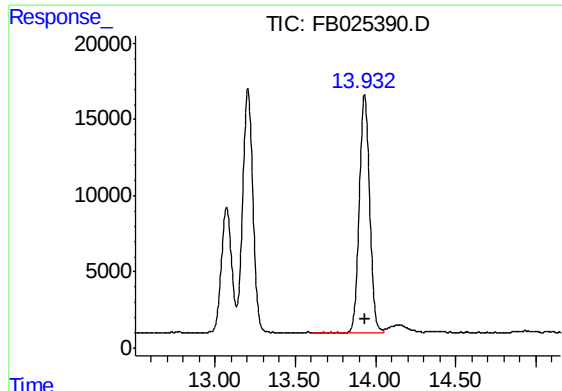

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 695504
Conc: 20.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0113S1

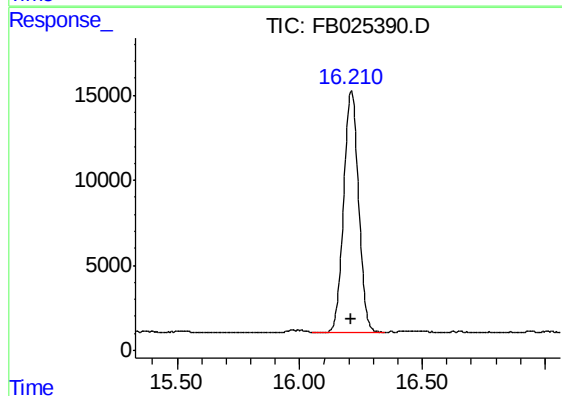

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 599815
Conc: 20.86 ng/ml