

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011321\
 Data File : FB025395.D
 Signal(s) : FID2B.CH
 Acq On : 13 Jan 2021 18:58
 Operator : DD/AJ
 Sample : M1123-02MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VW-SPMSD

Integration File: Calibration.e
 Quant Time: Jan 13 23:01:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	389433	17.312 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	717889	22.806 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	610455	19.255 ng/ml
3) t n-Heptane	7.758	194244	6.211 ng/ml
4) t Benzene	7.892	347585	8.841 ng/ml
6) t Toluene	10.631	959897	25.571 ng/ml
7) t Ethylbenzene	13.072	292448	8.538 ng/ml
8) t m-Xylene	13.205	578042	16.895 ng/ml
9) t O-Xylene	13.932	565691	17.018 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	458460	15.942 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011321\
Data File : FB025395.D
Signal(s) : FID2B.CH
Acq On : 13 Jan 2021 18:58
Operator : DD/AJ
Sample : M1123-02MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VW-SPMSD

Integration File: Calibration.e
Quant Time: Jan 13 23:01:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

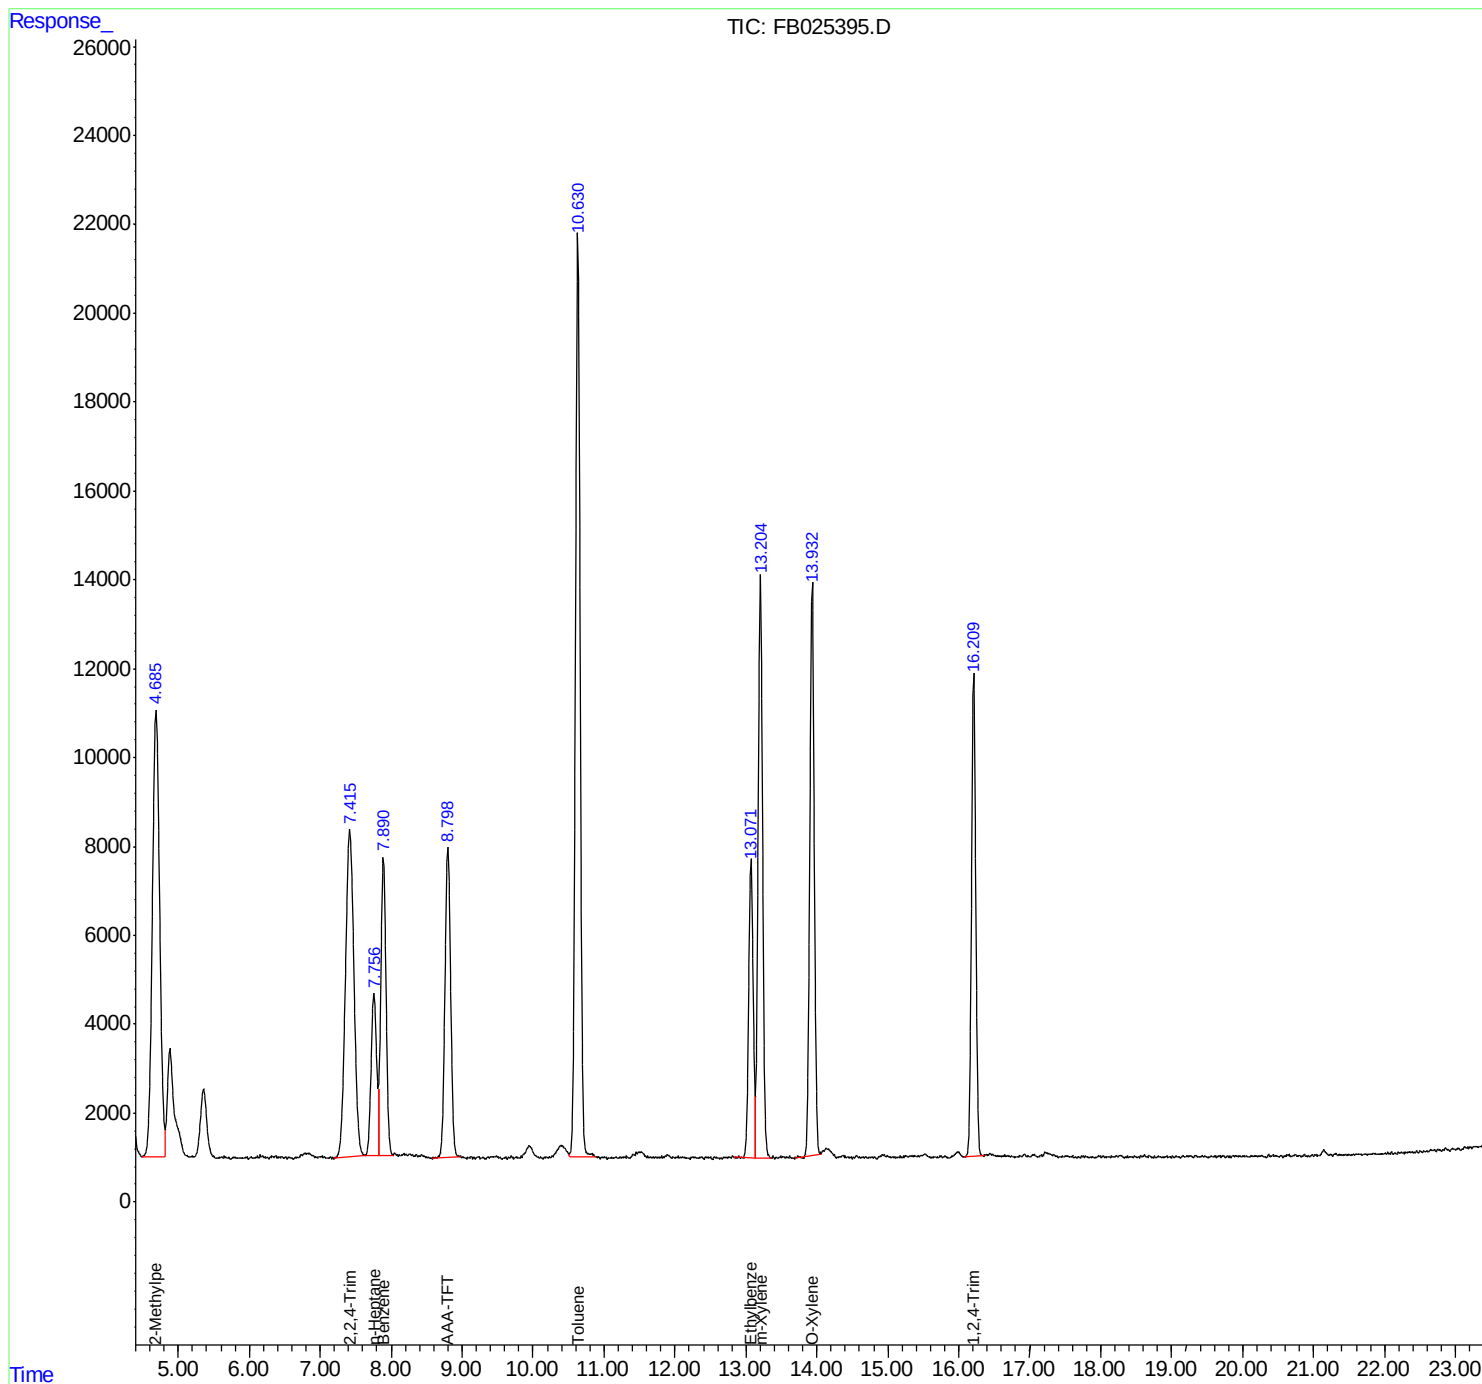


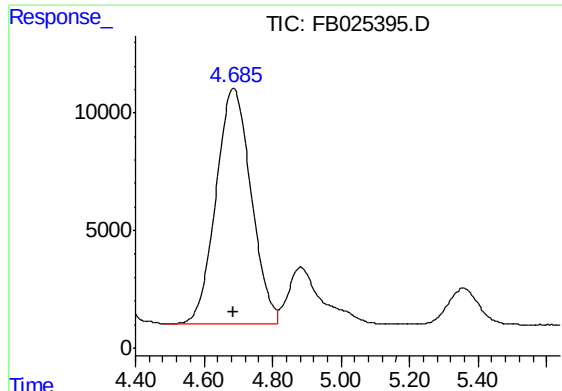

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: 0.000 min
Response: 717889
Conc: 22.81 ng/ml

Instrument :
FID_B
ClientSampleId :
VW-SPMSD

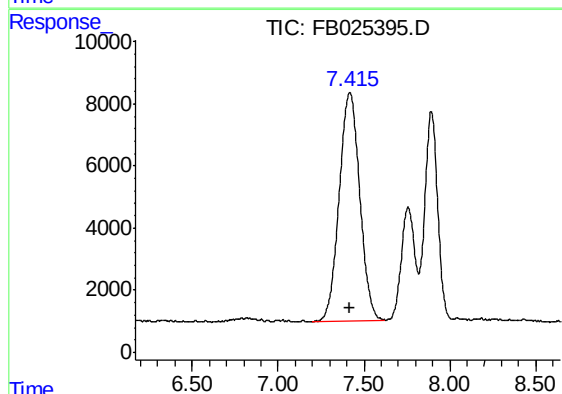


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 610455
Conc: 19.25 ng/ml

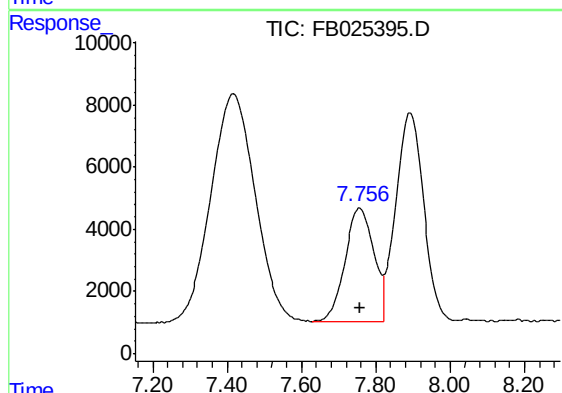


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 194244
Conc: 6.21 ng/ml

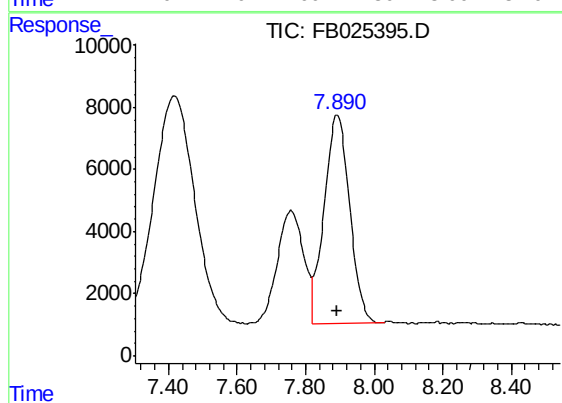

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 347585
Conc: 8.84 ng/ml

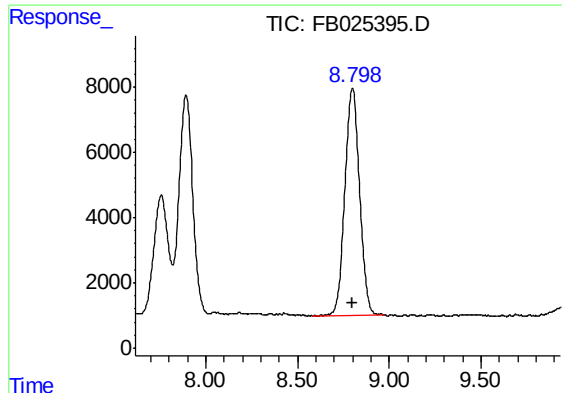

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 389433
Conc: 17.31 ng/ml

Instrument :
FID_B
ClientSampleId :
VW-SPMSD

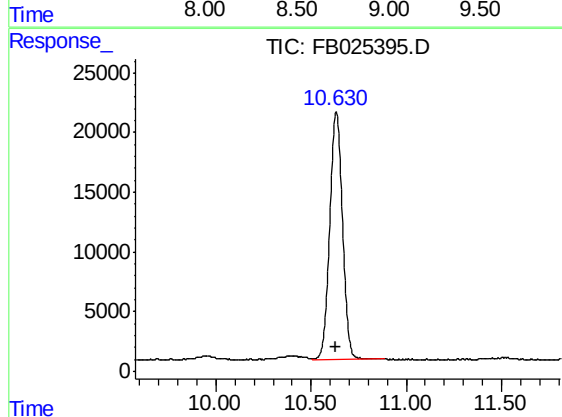


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 959897
Conc: 25.57 ng/ml

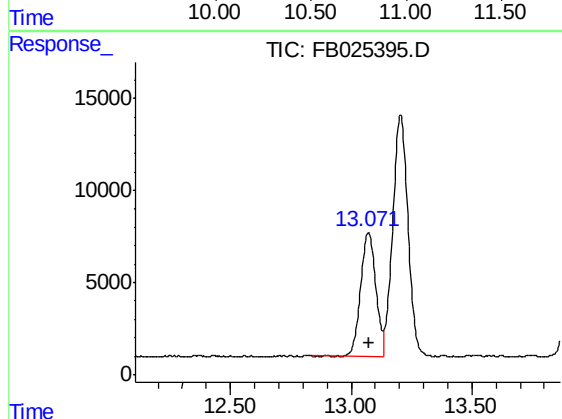


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 292448
Conc: 8.54 ng/ml

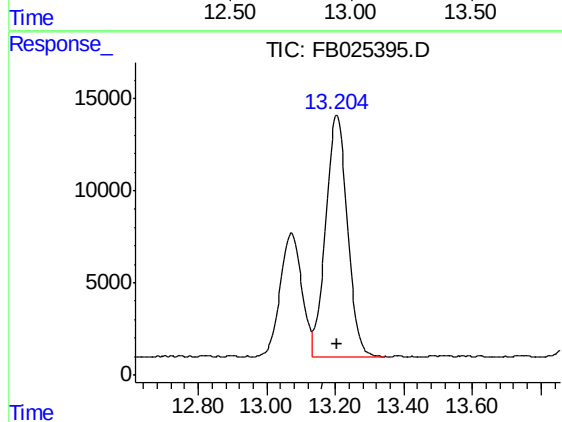

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 578042
Conc: 16.90 ng/ml

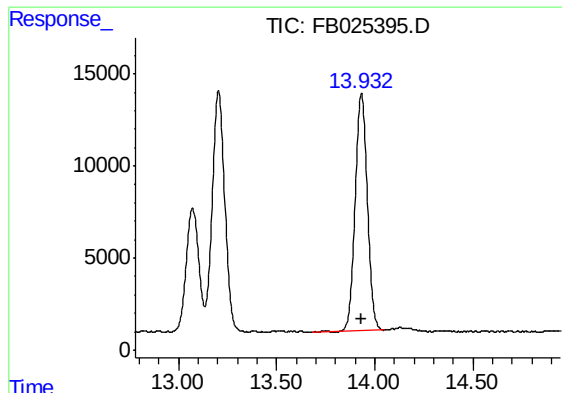

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 565691
Conc: 17.02 ng/ml

Instrument :
FID_B
ClientSampleId :
VW-SPMSD

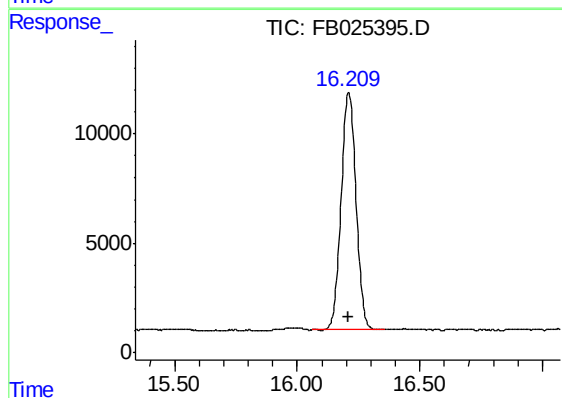

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 458460
Conc: 15.94 ng/ml