

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011419\
 Data File : FB019384.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jan 2019 9:58
 Operator : MJ/SJ
 Sample : BSF0114S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 14 22:37:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.040	178996	20.144 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.895	542112	27.219 ng/ml
2) t	2,2,4-Trimethylpentane	7.654	537131	28.196 ng/ml
3) t	n-Heptane	7.995	164460	9.426 ng/ml
4) t	Benzene	8.131	187798	9.564 ng/ml
6) t	Toluene	10.887	539403	29.819 ng/ml
7) t	Ethylbenzene	13.338	220995	9.975 ng/ml
8) t	m-Xylene	13.471	454949	19.825 ng/ml
9) t	O-Xylene	14.203	440640	19.639 ng/ml
10) t	1,2,4-Trimethylbenzene	16.489	448419	19.666 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011419\
Data File : FB019384.D
Signal(s) : FID2B.CH
Acq On : 14 Jan 2019 9:58
Operator : MJ/SJ
Sample : BSF0114S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 14 22:37:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

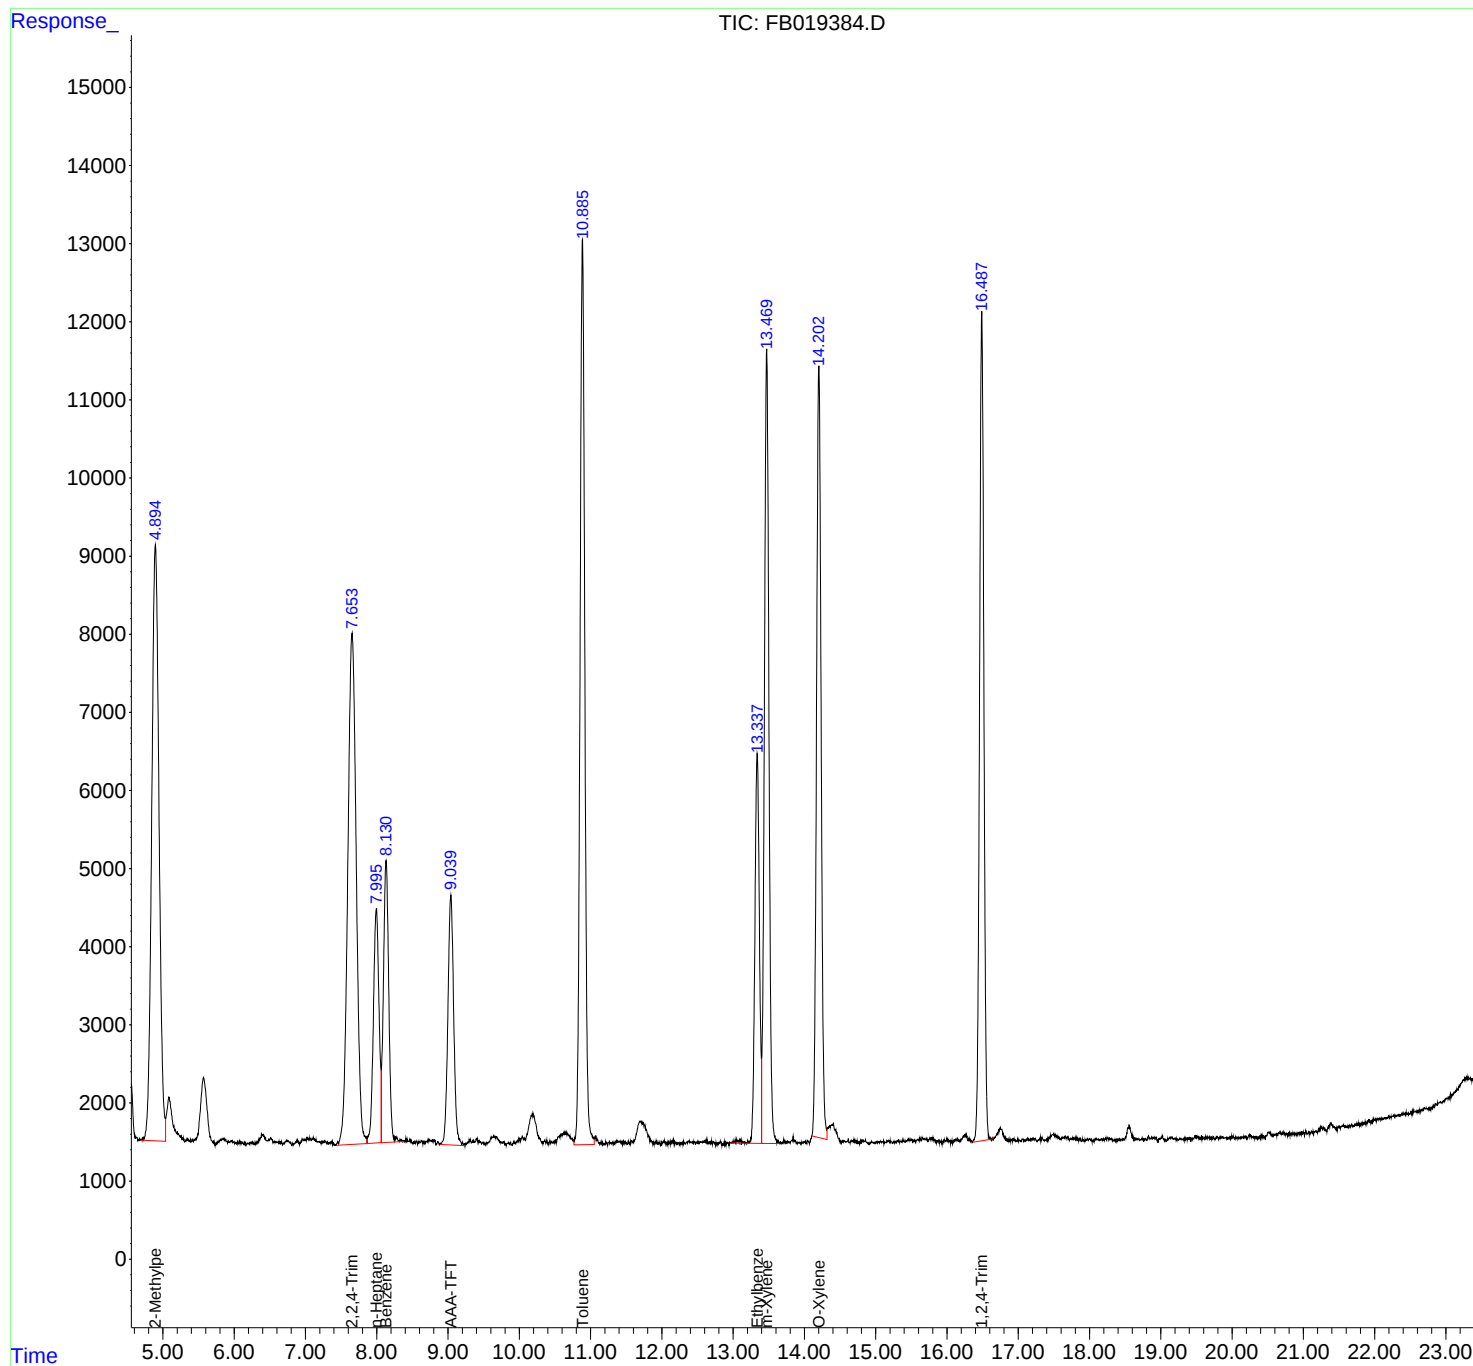

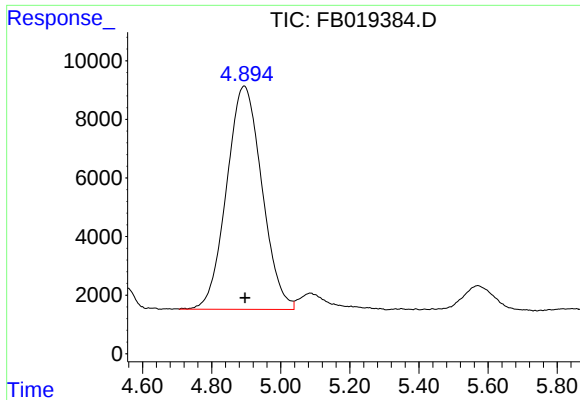


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 542112
Conc: 27.22 ng/ml

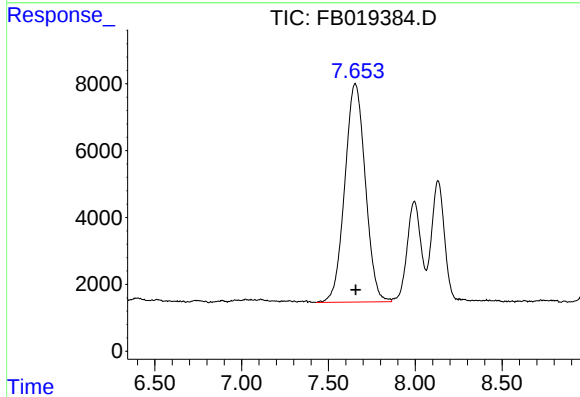


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.004 min
Response: 537131
Conc: 28.20 ng/ml

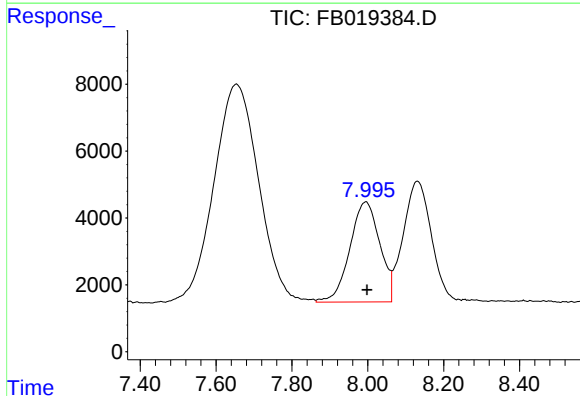


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.003 min
Response: 164460
Conc: 9.43 ng/ml

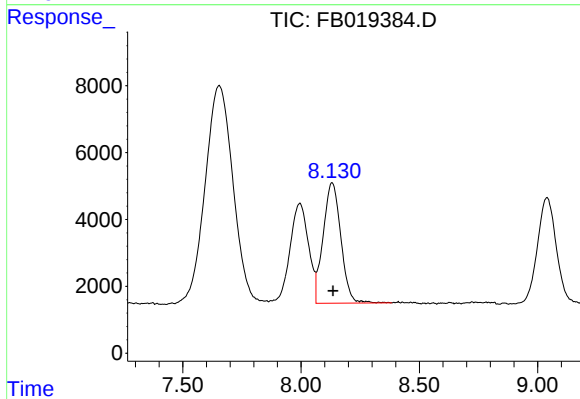


#4 Benzene

R.T.: 8.131 min
Delta R.T.: -0.004 min
Response: 187798
Conc: 9.56 ng/ml

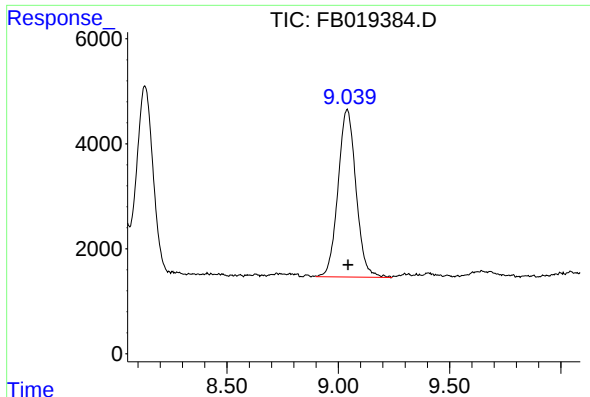


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.004 min
Response: 178996
Conc: 20.14 ng/ml

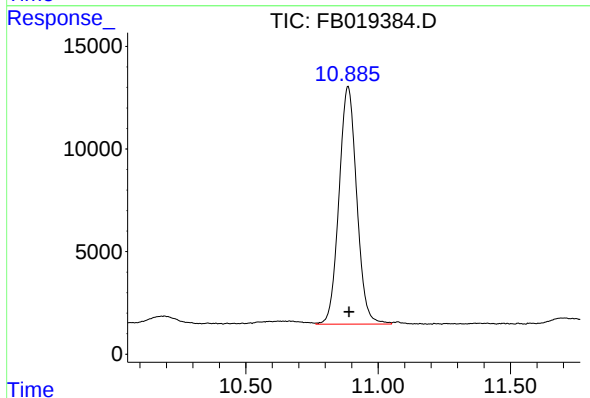


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.004 min
Response: 539403
Conc: 29.82 ng/ml

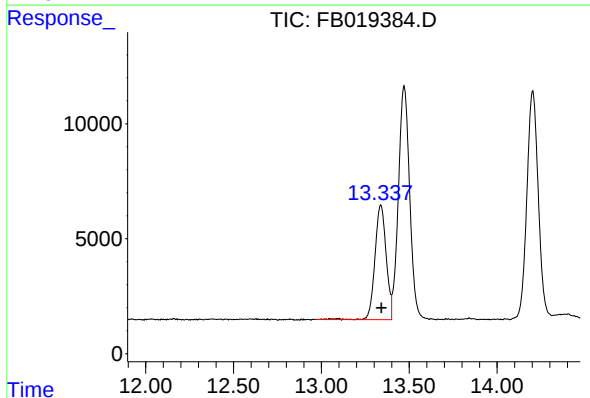


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.004 min
Response: 220995
Conc: 9.97 ng/ml

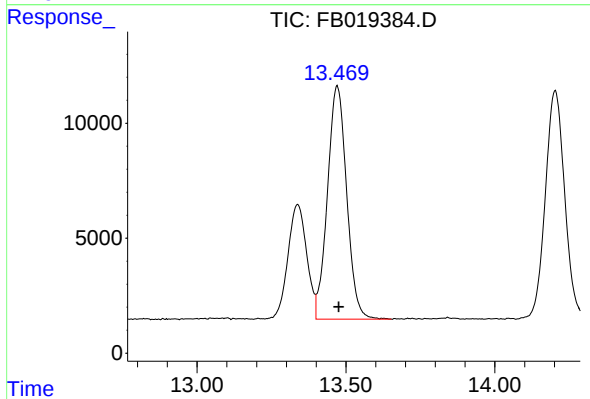


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.005 min
Response: 454949
Conc: 19.82 ng/ml

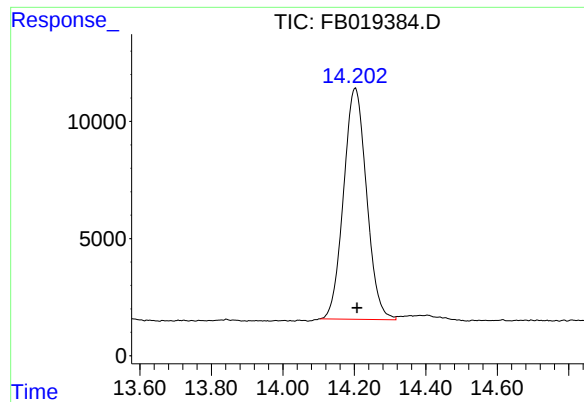

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.005 min
Response: 440640
Conc: 19.64 ng/ml

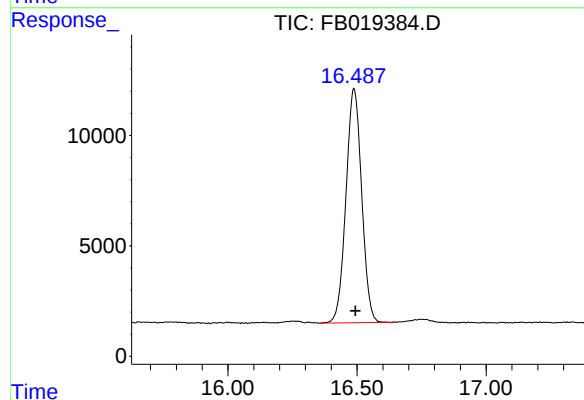

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.005 min
Response: 448419
Conc: 19.67 ng/ml