

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011419\
 Data File : FB019387.D
 Signal(s) : FID2B.CH
 Acq On : 14 Jan 2019 11:58
 Operator : MJ/SJ
 Sample : K1015-05MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 14 22:38:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.040	173844	19.564 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.895	480456	24.124 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	452659	23.762 ng/ml
3) t	n-Heptane	7.995	135220	7.750 ng/ml
4) t	Benzene	8.132	177111	9.020 ng/ml
6) t	Toluene	10.887	521833	28.848 ng/ml
7) t	Ethylbenzene	13.340	209755	9.467 ng/ml
8) t	m-Xylene	13.473	432906	18.864 ng/ml
9) t	O-Xylene	14.204	421939	18.805 ng/ml
10) t	1,2,4-Trimethylbenzene	16.490	413013	18.113 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011419\
Data File : FB019387.D
Signal(s) : FID2B.CH
Acq On : 14 Jan 2019 11:58
Operator : MJ/SJ
Sample : K1015-05MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 14 22:38:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

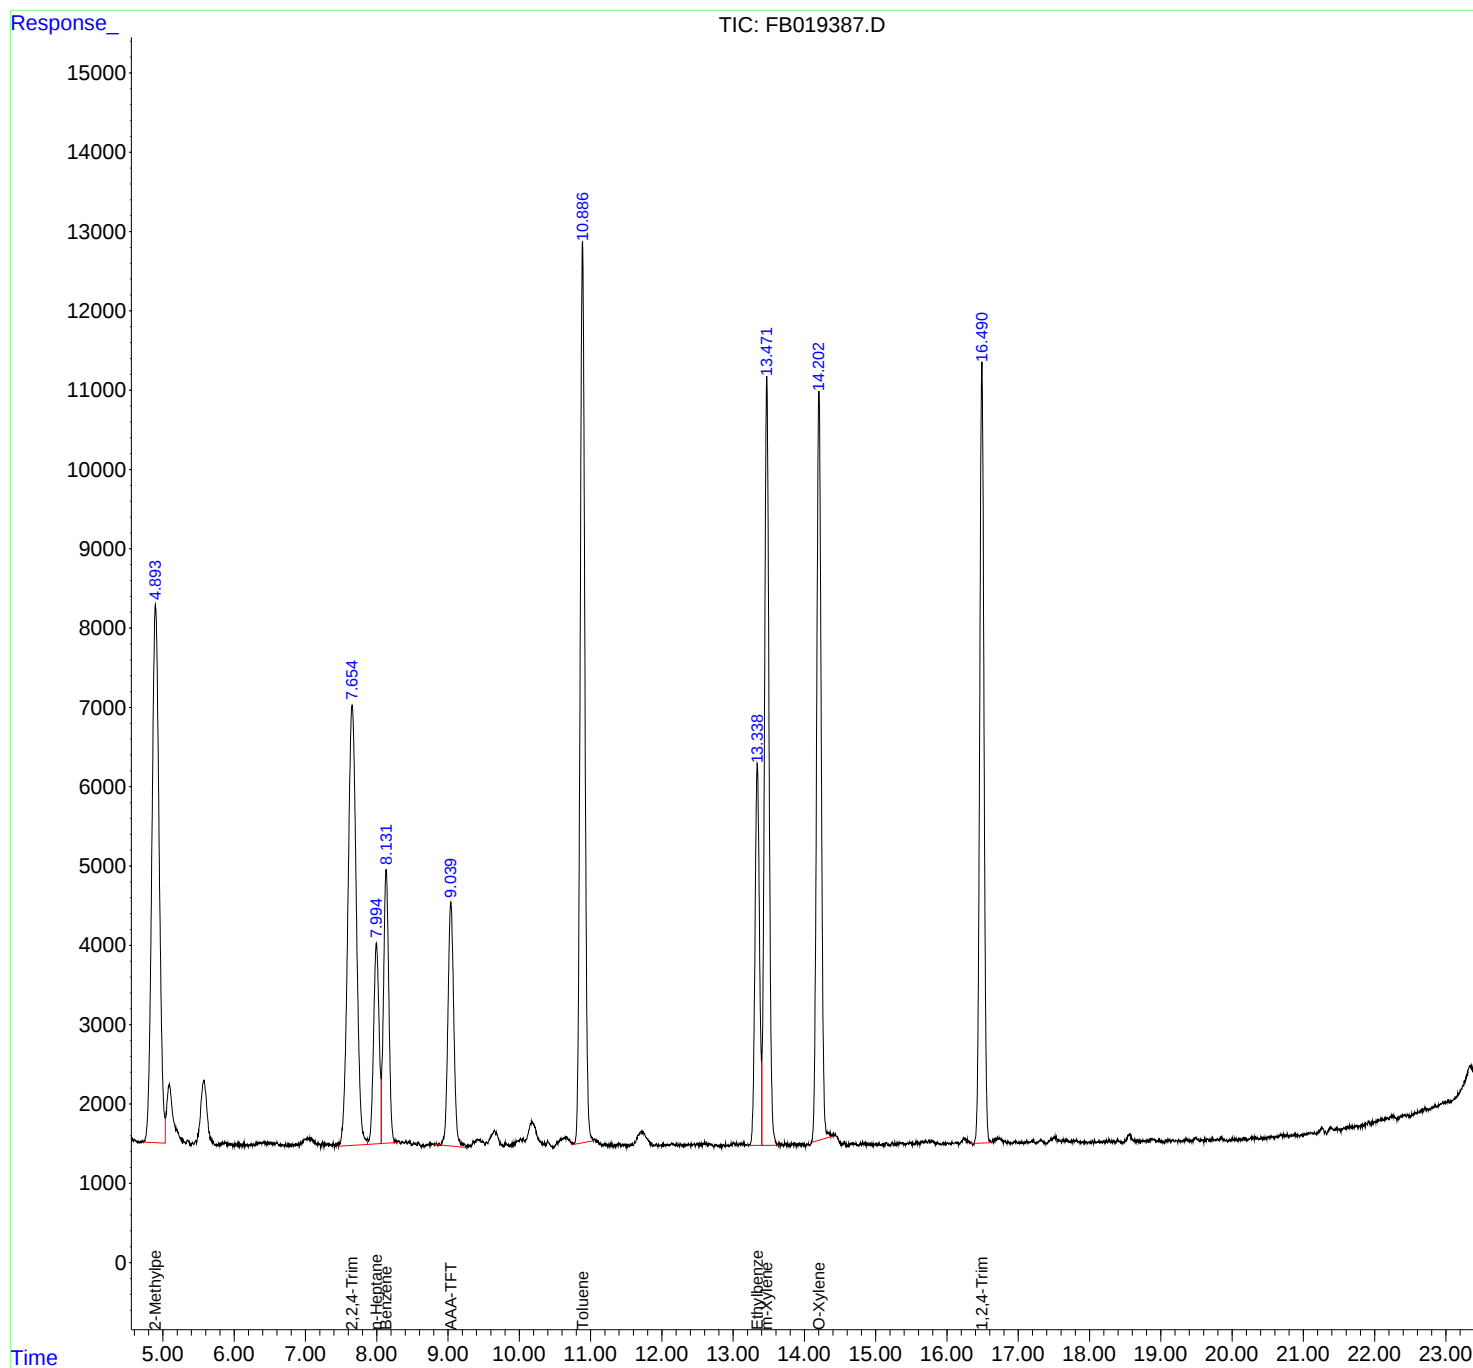

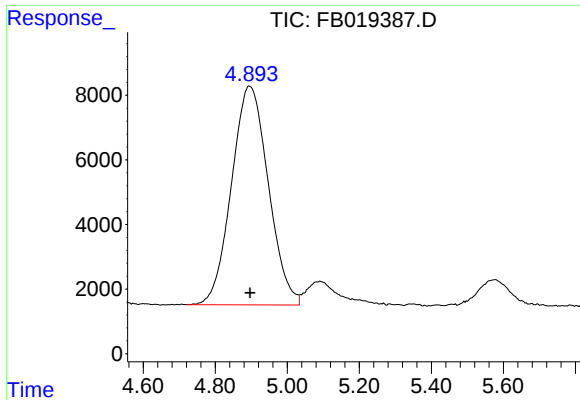


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 480456
Conc: 24.12 ng/ml

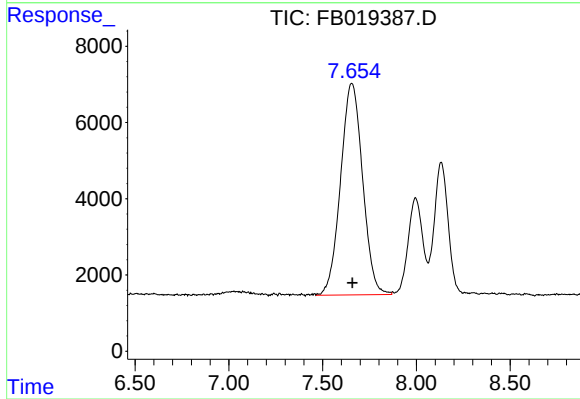


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.003 min
Response: 452659
Conc: 23.76 ng/ml

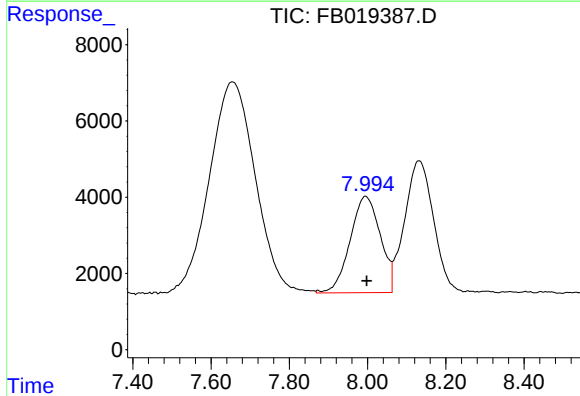


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.003 min
Response: 135220
Conc: 7.75 ng/ml

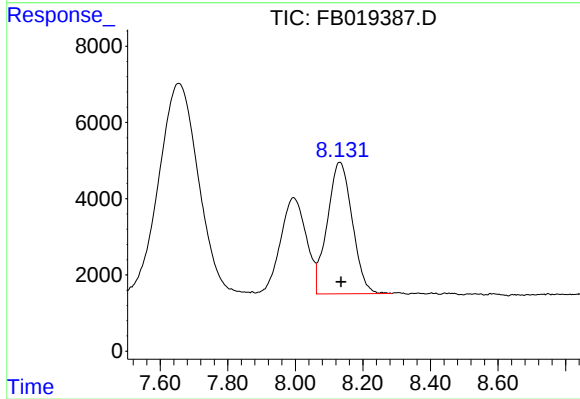


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 177111
Conc: 9.02 ng/ml

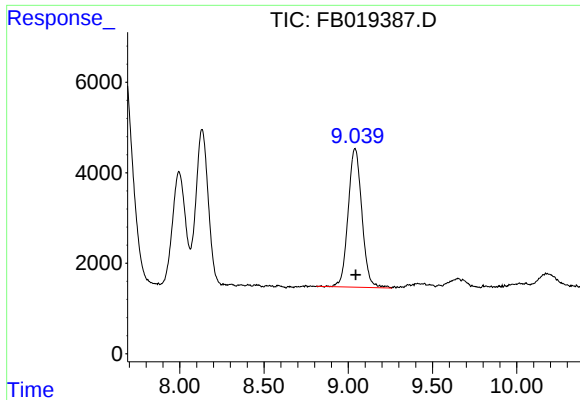


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.004 min
Response: 173844
Conc: 19.56 ng/ml

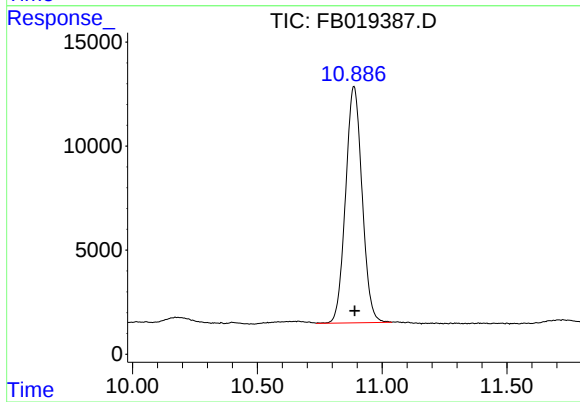


#6 Toluene

R.T.: 10.887 min
Delta R.T.: -0.003 min
Response: 521833
Conc: 28.85 ng/ml

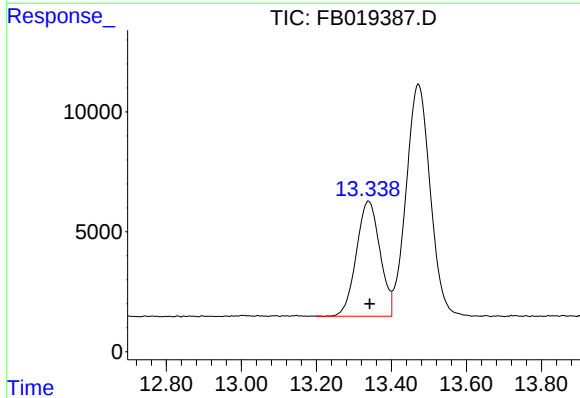


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.003 min
Response: 209755
Conc: 9.47 ng/ml

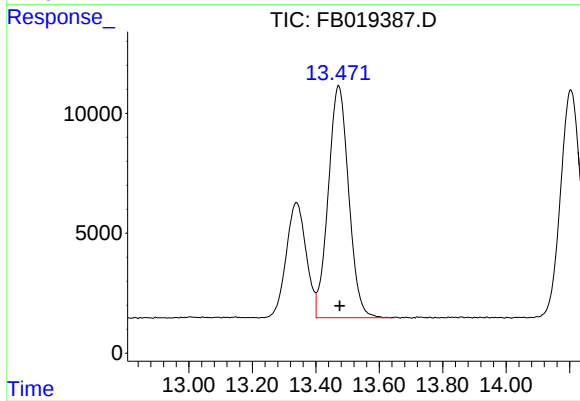


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.003 min
Response: 432906
Conc: 18.86 ng/ml

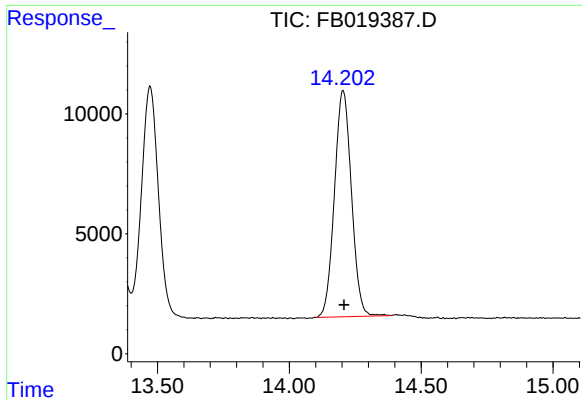

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: -0.003 min
Response: 421939
Conc: 18.81 ng/ml

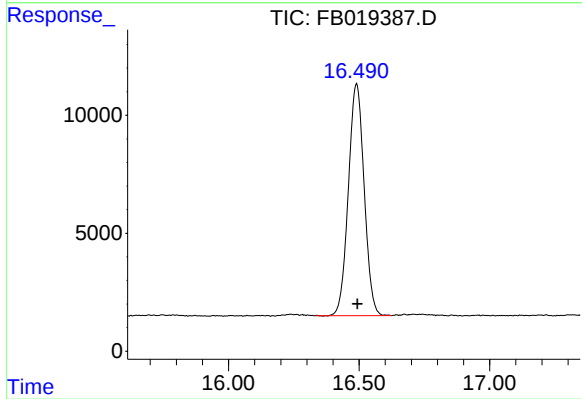

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: -0.003 min
Response: 413013
Conc: 18.11 ng/ml