

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB011519\
Data File : FB019411.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2019 10:09
Operator : MJ/SJ
Sample : BSF0115S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 13:49:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.040	169808	19.110 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.894	523737	26.297 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	521177	27.358 ng/ml
3) t	n-Heptane	7.995	159763	9.157 ng/ml
4) t	Benzene	8.131	186805	9.514 ng/ml
6) t	Toluene	10.886	557533	30.822 ng/ml
7) t	Ethylbenzene	13.338	223339	10.081 ng/ml
8) t	m-Xylene	13.471	463362	20.191 ng/ml
9) t	O-Xylene	14.203	451398	20.118 ng/ml
10) t	1,2,4-Trimethylbenzene	16.489	446484	19.581 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB011519\
Data File : FB019411.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2019 10:09
Operator : MJ/SJ
Sample : BSF0115S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 13:49:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

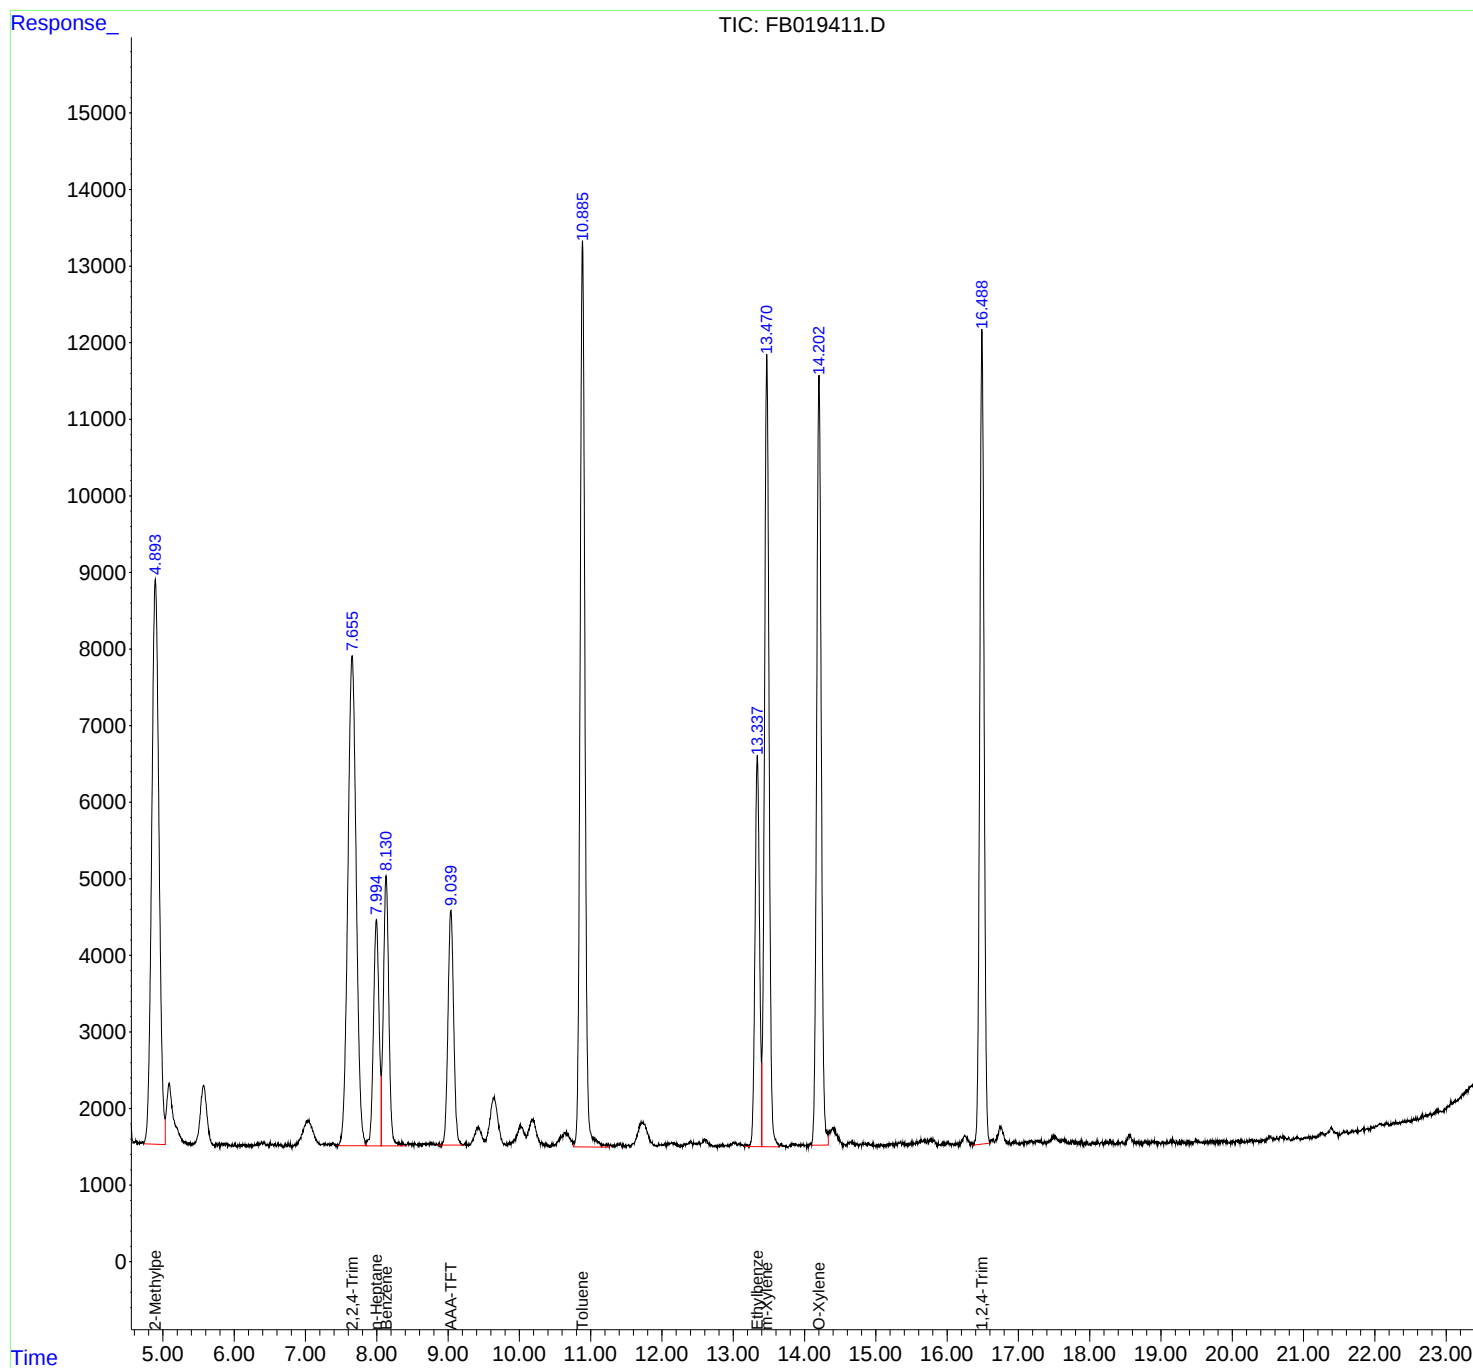

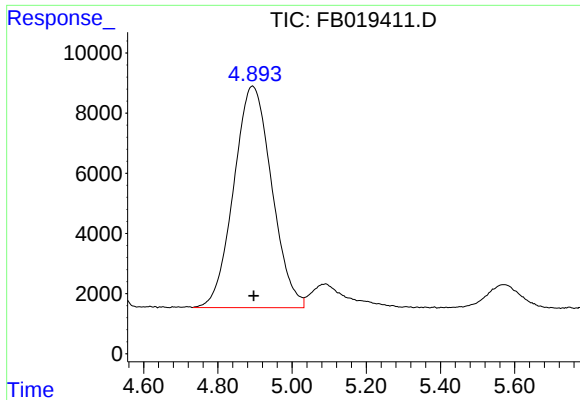


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 523737
Conc: 26.30 ng/ml

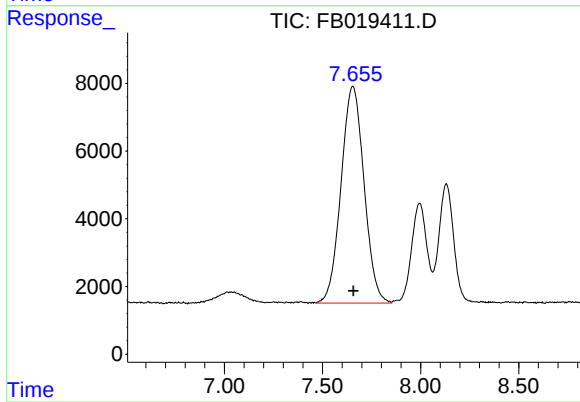


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.003 min
Response: 521177
Conc: 27.36 ng/ml

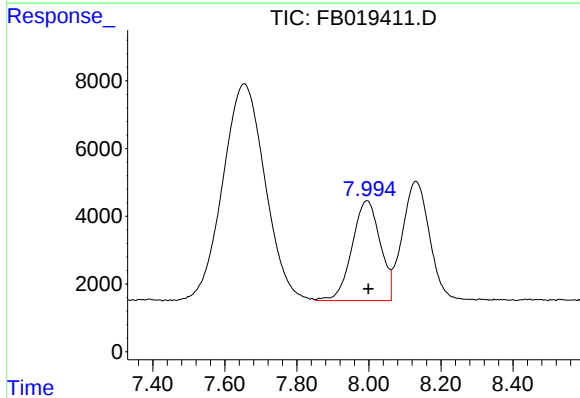


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.003 min
Response: 159763
Conc: 9.16 ng/ml

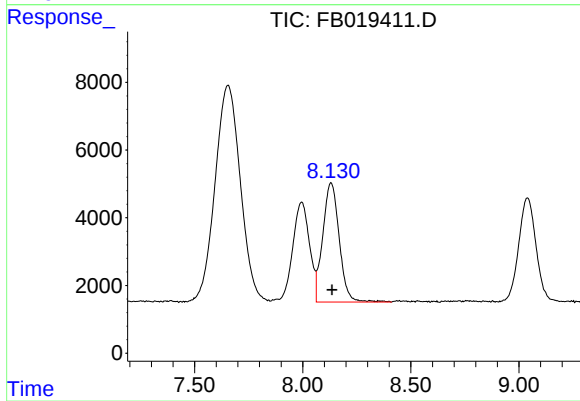


#4 Benzene

R.T.: 8.131 min
Delta R.T.: -0.004 min
Response: 186805
Conc: 9.51 ng/ml

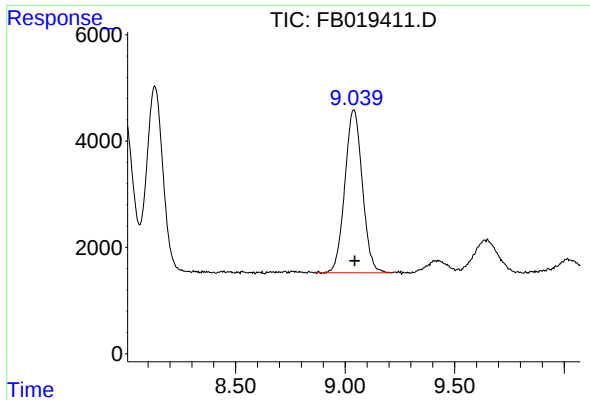


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.004 min
Response: 169808
Conc: 19.11 ng/ml

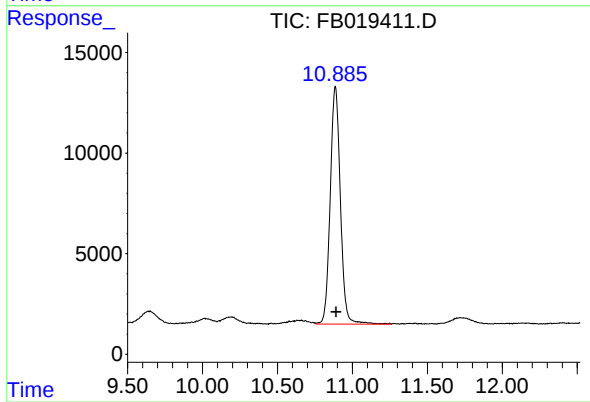


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.004 min
Response: 557533
Conc: 30.82 ng/ml

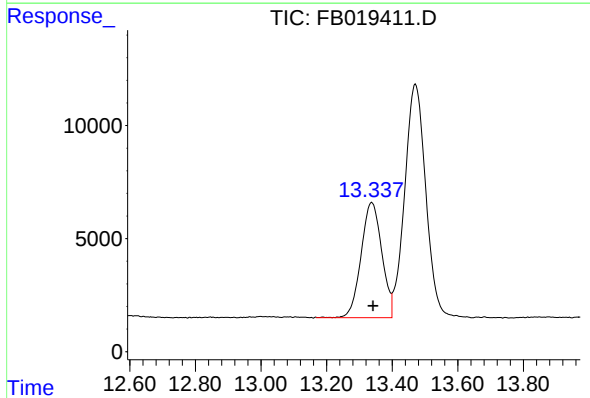


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.004 min
Response: 223339
Conc: 10.08 ng/ml

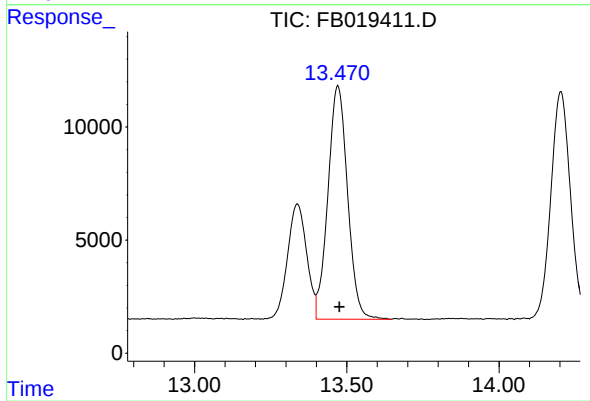

#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.005 min
Response: 463362
Conc: 20.19 ng/ml

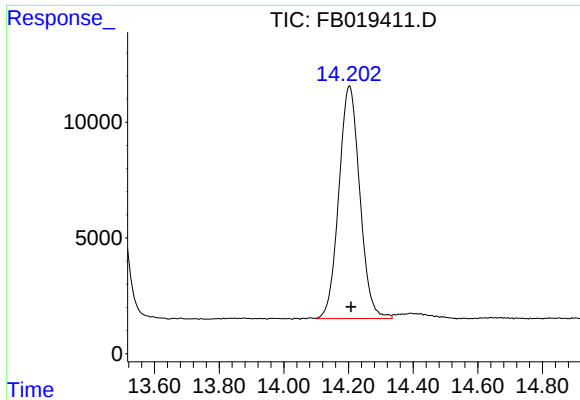


#9 O-Xylene

R.T.: 14.203 min

Delta R.T.: -0.004 min

Response: 451398

Conc: 20.12 ng/ml

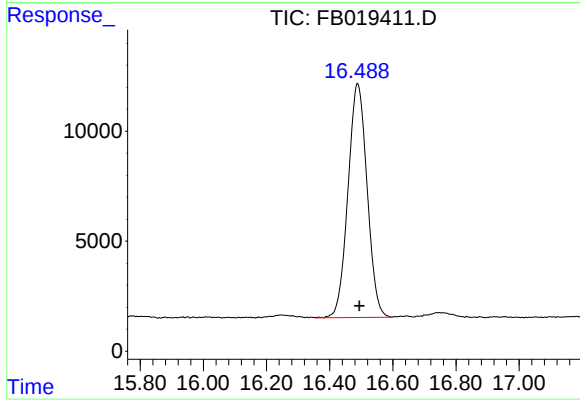

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min

Delta R.T.: -0.005 min

Response: 446484

Conc: 19.58 ng/ml