

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB011519\
Data File : FB019415.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2019 12:28
Operator : MJ/SJ
Sample : K1007-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 13:50:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.041	212541	23.919 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.895	506782	25.445 ng/ml
2) t	2,2,4-Trimethylpentane	7.655	431874	22.671 ng/ml
3) t	n-Heptane	7.997	137557	7.884 ng/ml
4) t	Benzene	8.133	182521	9.295 ng/ml
6) t	Toluene	10.888	527017	29.135 ng/ml
7) t	Ethylbenzene	13.340	206978	9.342 ng/ml
8) t	m-Xylene	13.473	430056	18.740 ng/ml
9) t	O-Xylene	14.206	424178	18.905 ng/ml
10) t	1,2,4-Trimethylbenzene	16.492	424393	18.612 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB011519\
Data File : FB019415.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2019 12:28
Operator : MJ/SJ
Sample : K1007-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 13:50:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

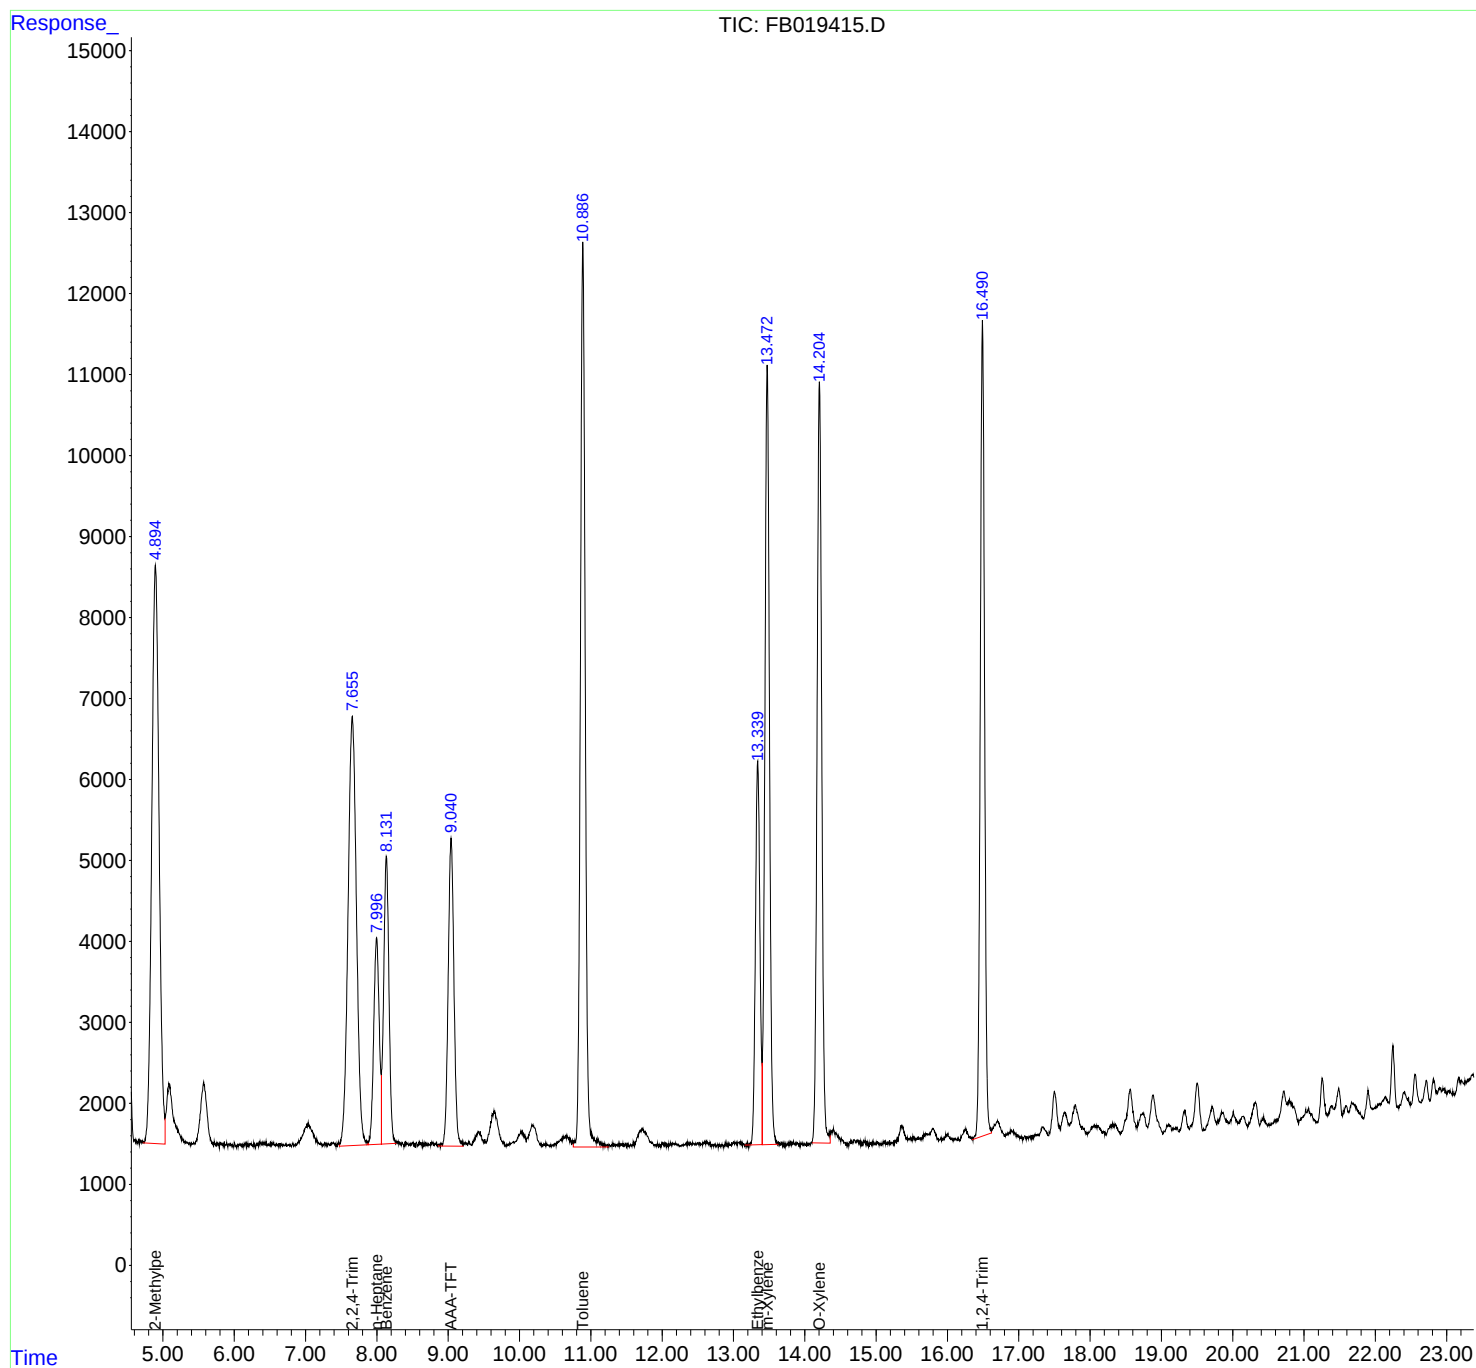

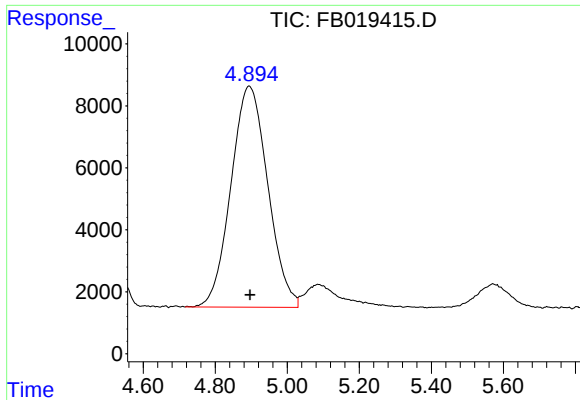


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 506782
Conc: 25.45 ng/ml

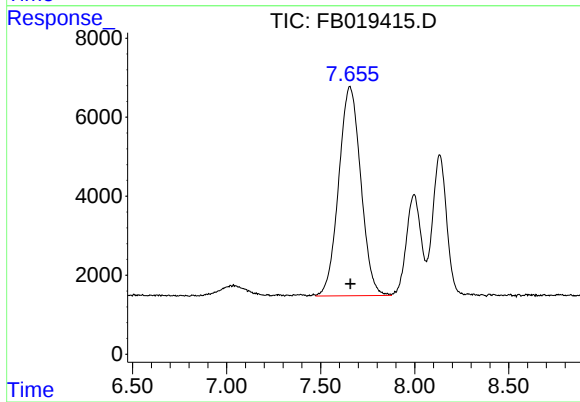


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.003 min
Response: 431874
Conc: 22.67 ng/ml

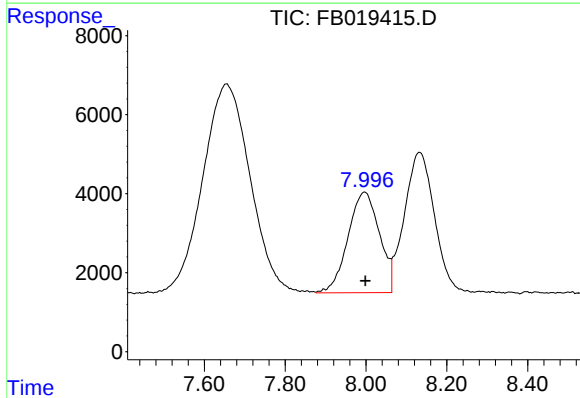


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: -0.001 min
Response: 137557
Conc: 7.88 ng/ml

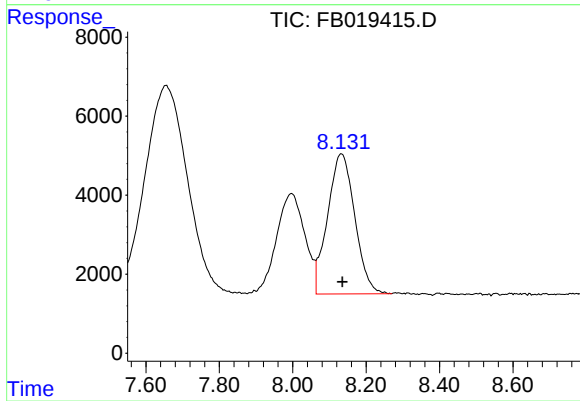


#4 Benzene

R.T.: 8.133 min
Delta R.T.: -0.002 min
Response: 182521
Conc: 9.30 ng/ml

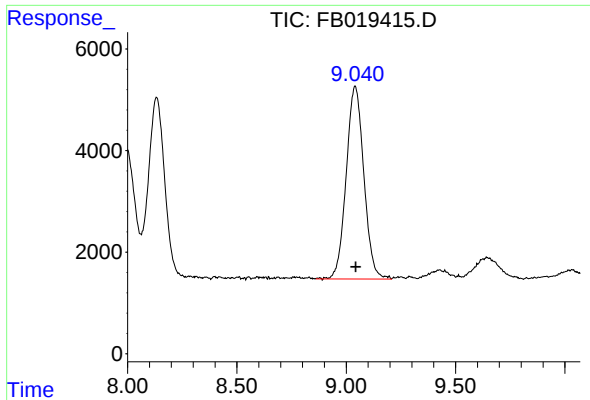


#5 AAA-TFT

R.T.: 9.041 min
Delta R.T.: -0.002 min
Response: 212541
Conc: 23.92 ng/ml

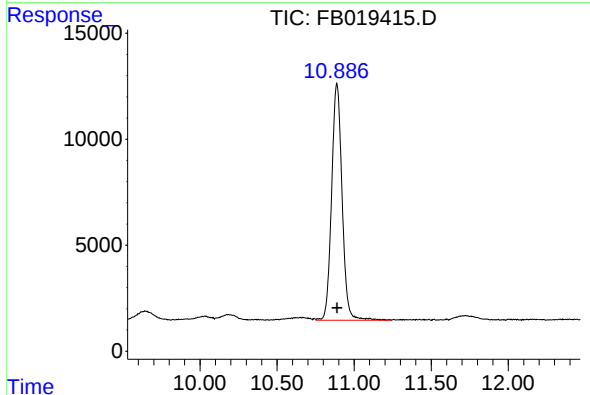


#6 Toluene

R.T.: 10.888 min
Delta R.T.: -0.002 min
Response: 527017
Conc: 29.13 ng/ml

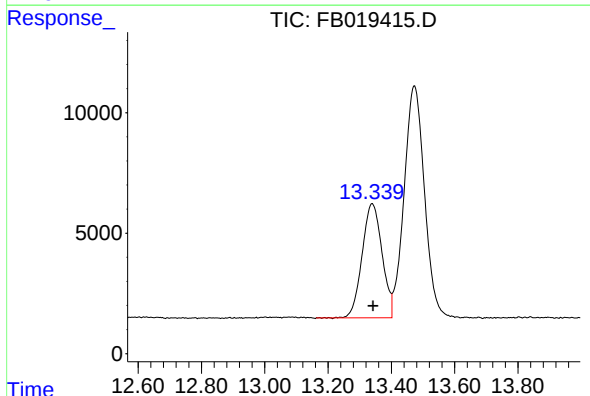


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: -0.002 min
Response: 206978
Conc: 9.34 ng/ml

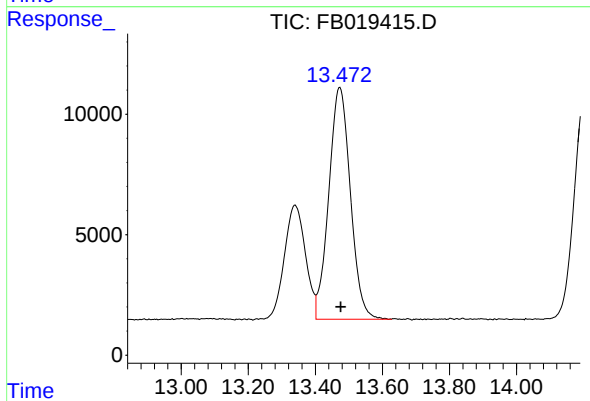


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.002 min
Response: 430056
Conc: 18.74 ng/ml

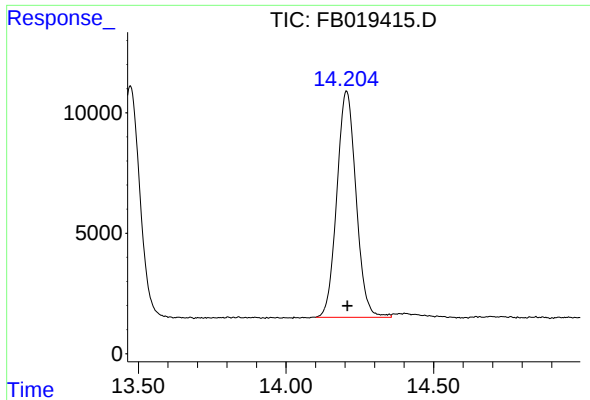

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.002 min
Response: 424178
Conc: 18.90 ng/ml

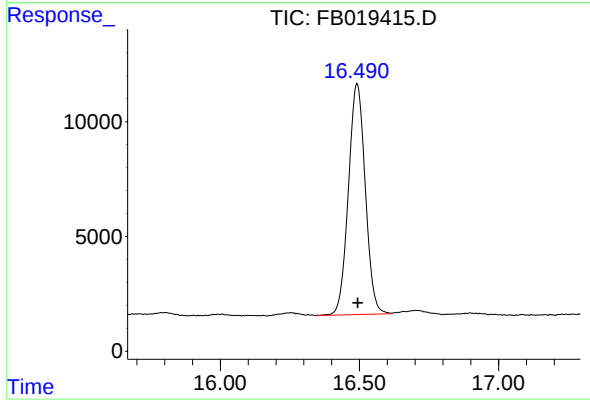

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: -0.002 min
Response: 424393
Conc: 18.61 ng/ml