

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
 Data File : FB023414.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2020 9:14
 Operator : DD/AJ
 Sample : BSF0115S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0115S1

Integration File: Calibration.e
 Quant Time: Jan 16 00:09:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	494391	20.848 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	887511	28.676 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1031050	30.864 ng/ml
3) t n-Heptane	7.753	330739	10.027 ng/ml
4) t Benzene	7.887	405312	10.150 ng/ml
6) t Toluene	10.625	1172780	30.459 ng/ml
7) t Ethylbenzene	13.065	369631	10.184 ng/ml
8) t m-Xylene	13.198	702801	20.247 ng/ml
9) t O-Xylene	13.926	677198	20.105 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	579109	20.640 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
Data File : FB023414.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2020 9:14
Operator : DD/AJ
Sample : BSF0115S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0115S1

Integration File: Calibration.e
Quant Time: Jan 16 00:09:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

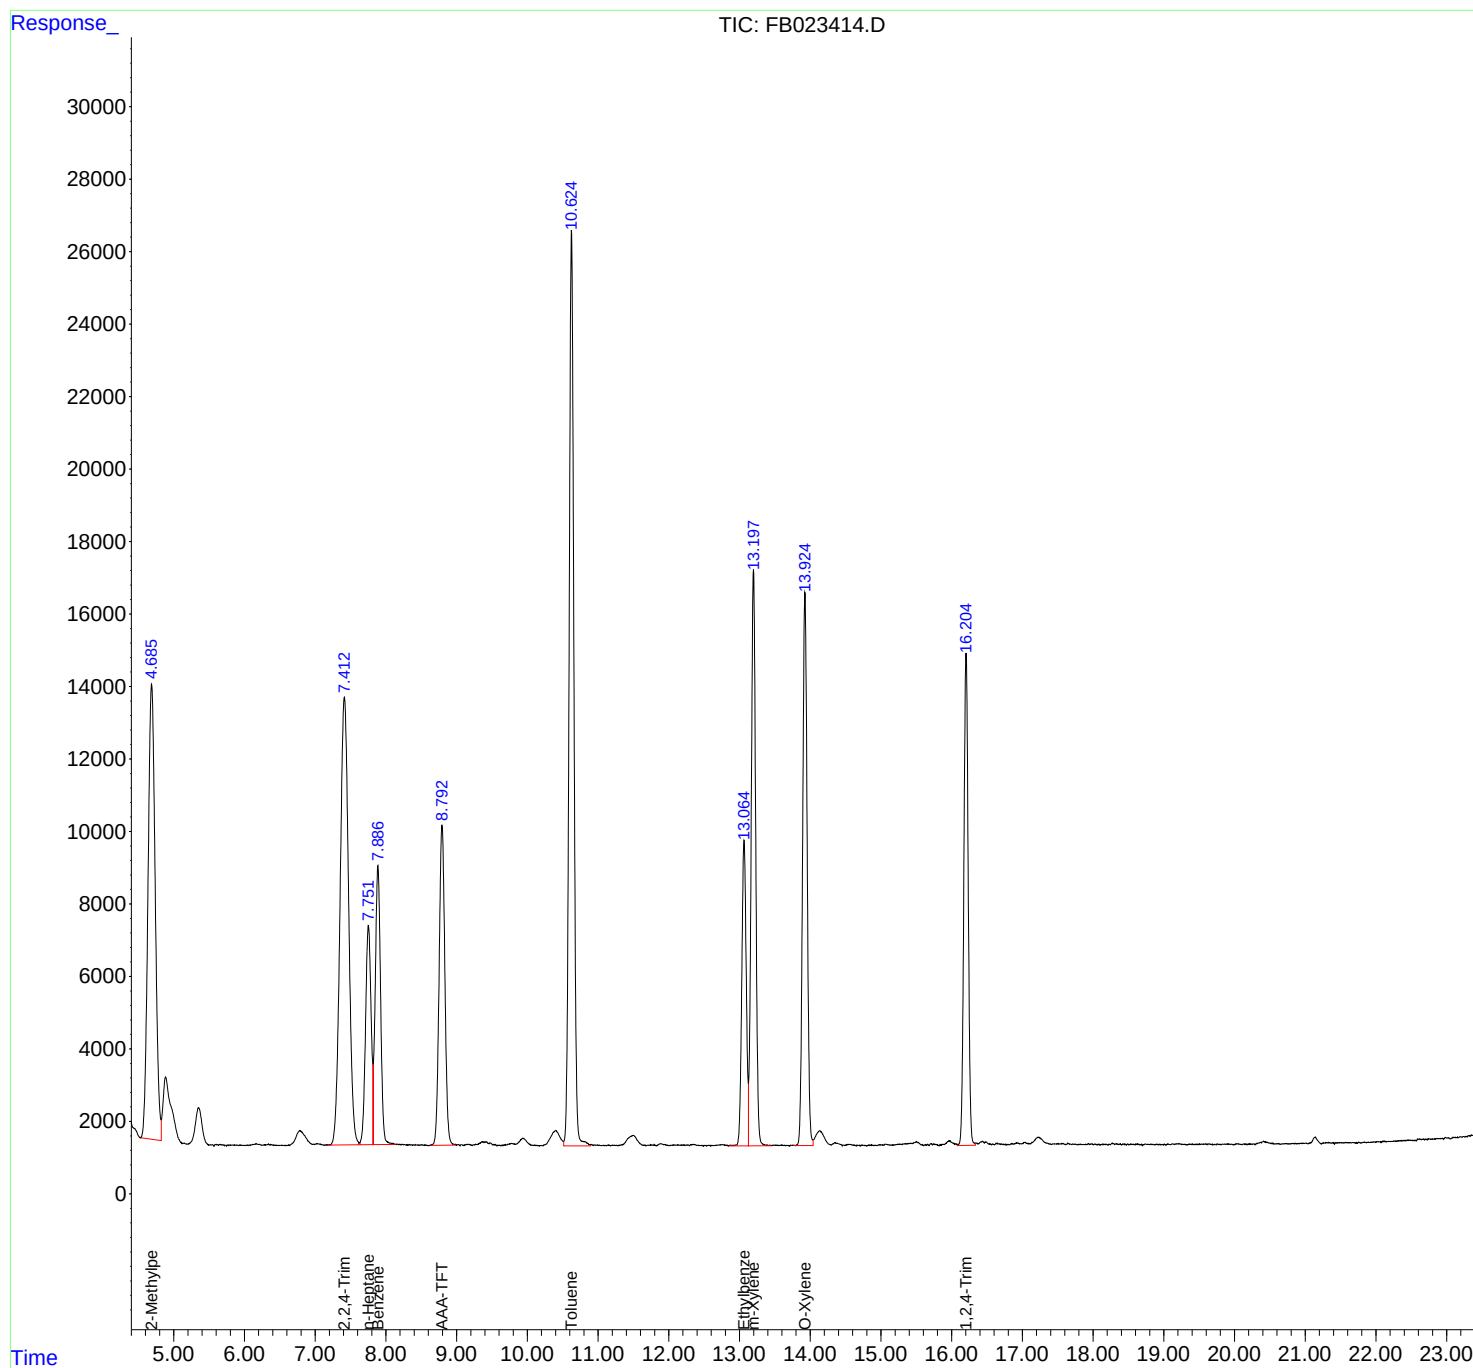


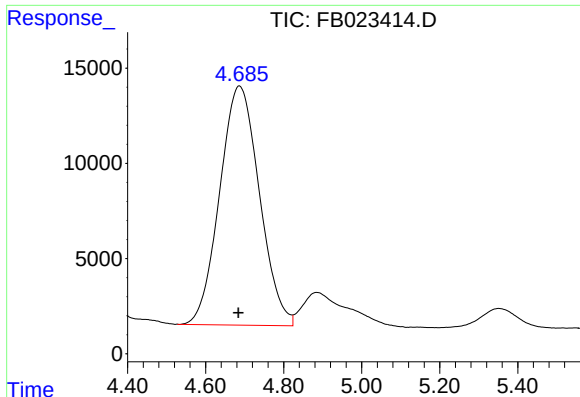

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.003 min
Response: 887511
Conc: 28.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0115S1

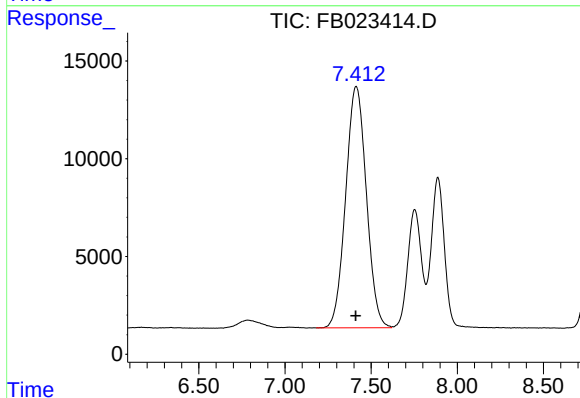


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.002 min
Response: 1031050
Conc: 30.86 ng/ml

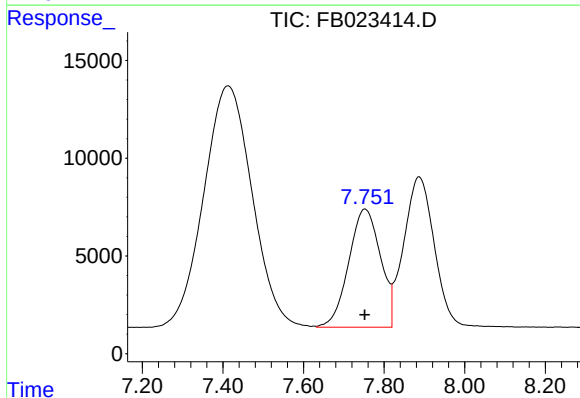


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.001 min
Response: 330739
Conc: 10.03 ng/ml

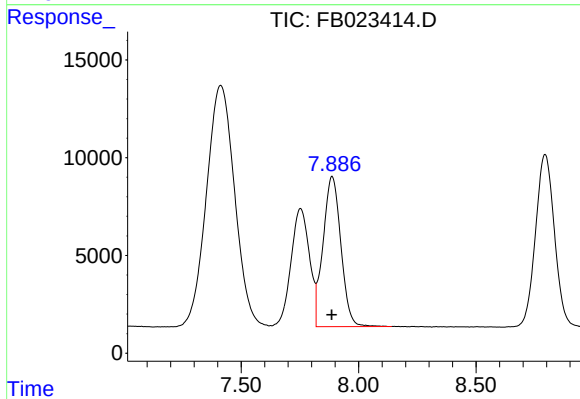

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 405312
Conc: 10.15 ng/ml

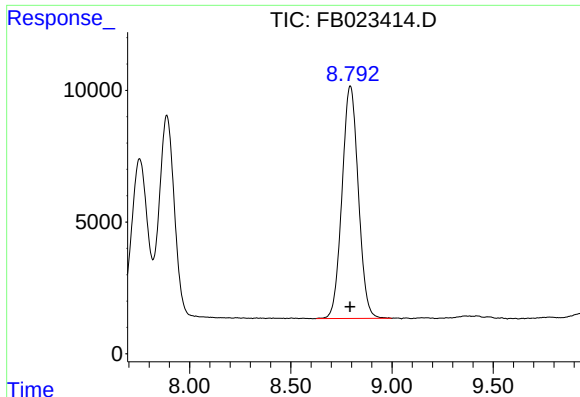

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 494391
Conc: 20.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0115S1

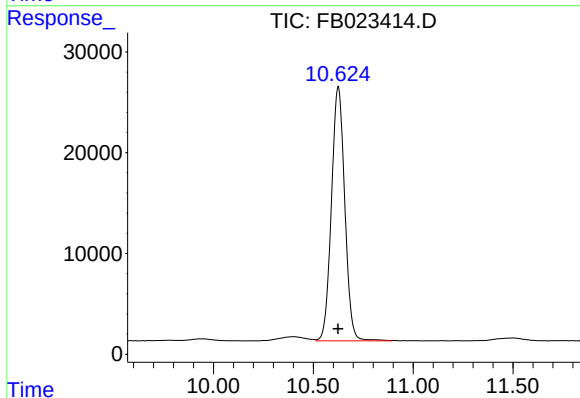


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.001 min
Response: 1172780
Conc: 30.46 ng/ml

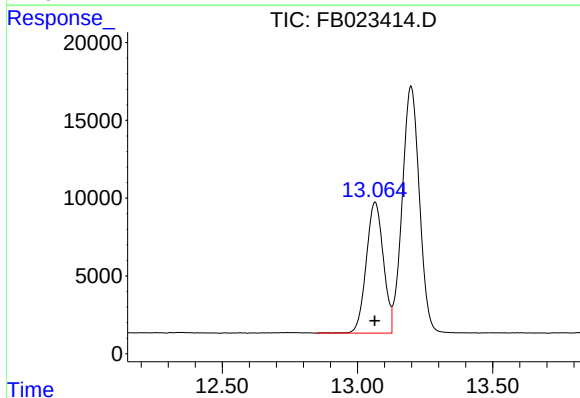


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.002 min
Response: 369631
Conc: 10.18 ng/ml

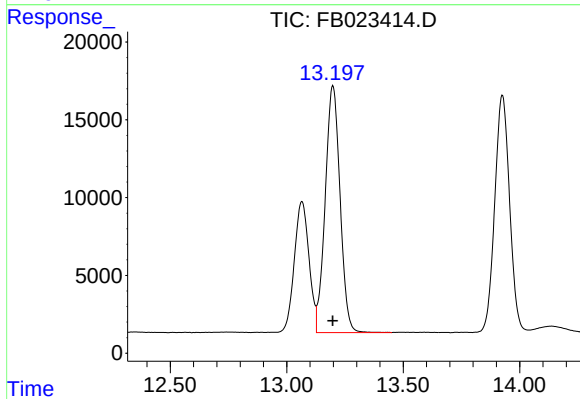

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: 0.001 min
Response: 702801
Conc: 20.25 ng/ml

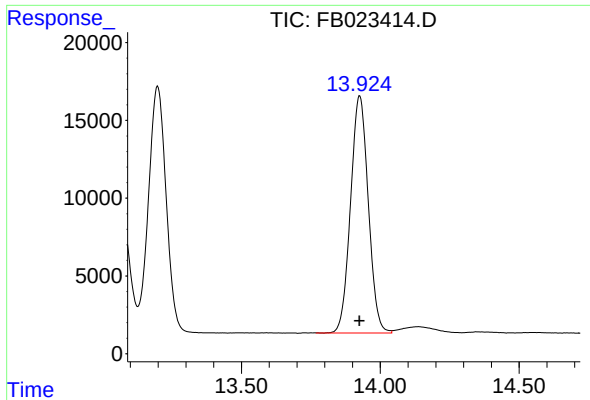

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.001 min
Response: 677198
Conc: 20.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0115S1

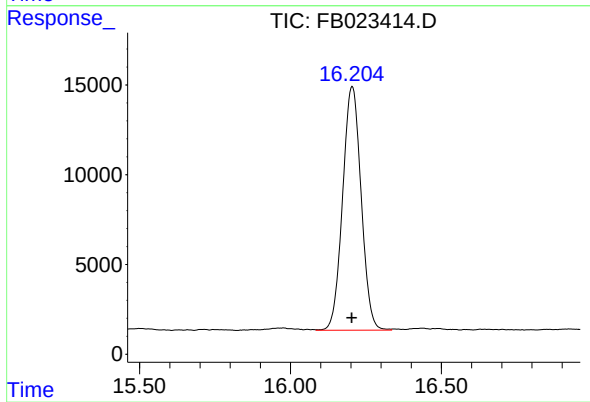

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.001 min
Response: 579109
Conc: 20.64 ng/ml