

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB011520\  
Data File : FB023415.D  
Signal(s) : FID2B.CH  
Acq On : 15 Jan 2020 9:44  
Operator : DD/AJ  
Sample : L1123-02  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-01-COMP

Integration File: Calibration.e  
Quant Time: Jan 16 00:09:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB121919.M  
Quant Title :  
QLast Update : Thu Dec 19 12:43:06 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB011520\  
Data File : FB023415.D  
Signal(s) : FID2B.CH  
Acq On : 15 Jan 2020 9:44  
Operator : DD/AJ  
Sample : L1123-02  
Misc : 5.02g/5.00ml DI WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
SB-01-COMP

Integration File: Calibration.e  
Quant Time: Jan 16 00:09:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB121919.M  
Quant Title :  
QLast Update : Thu Dec 19 12:43:06 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

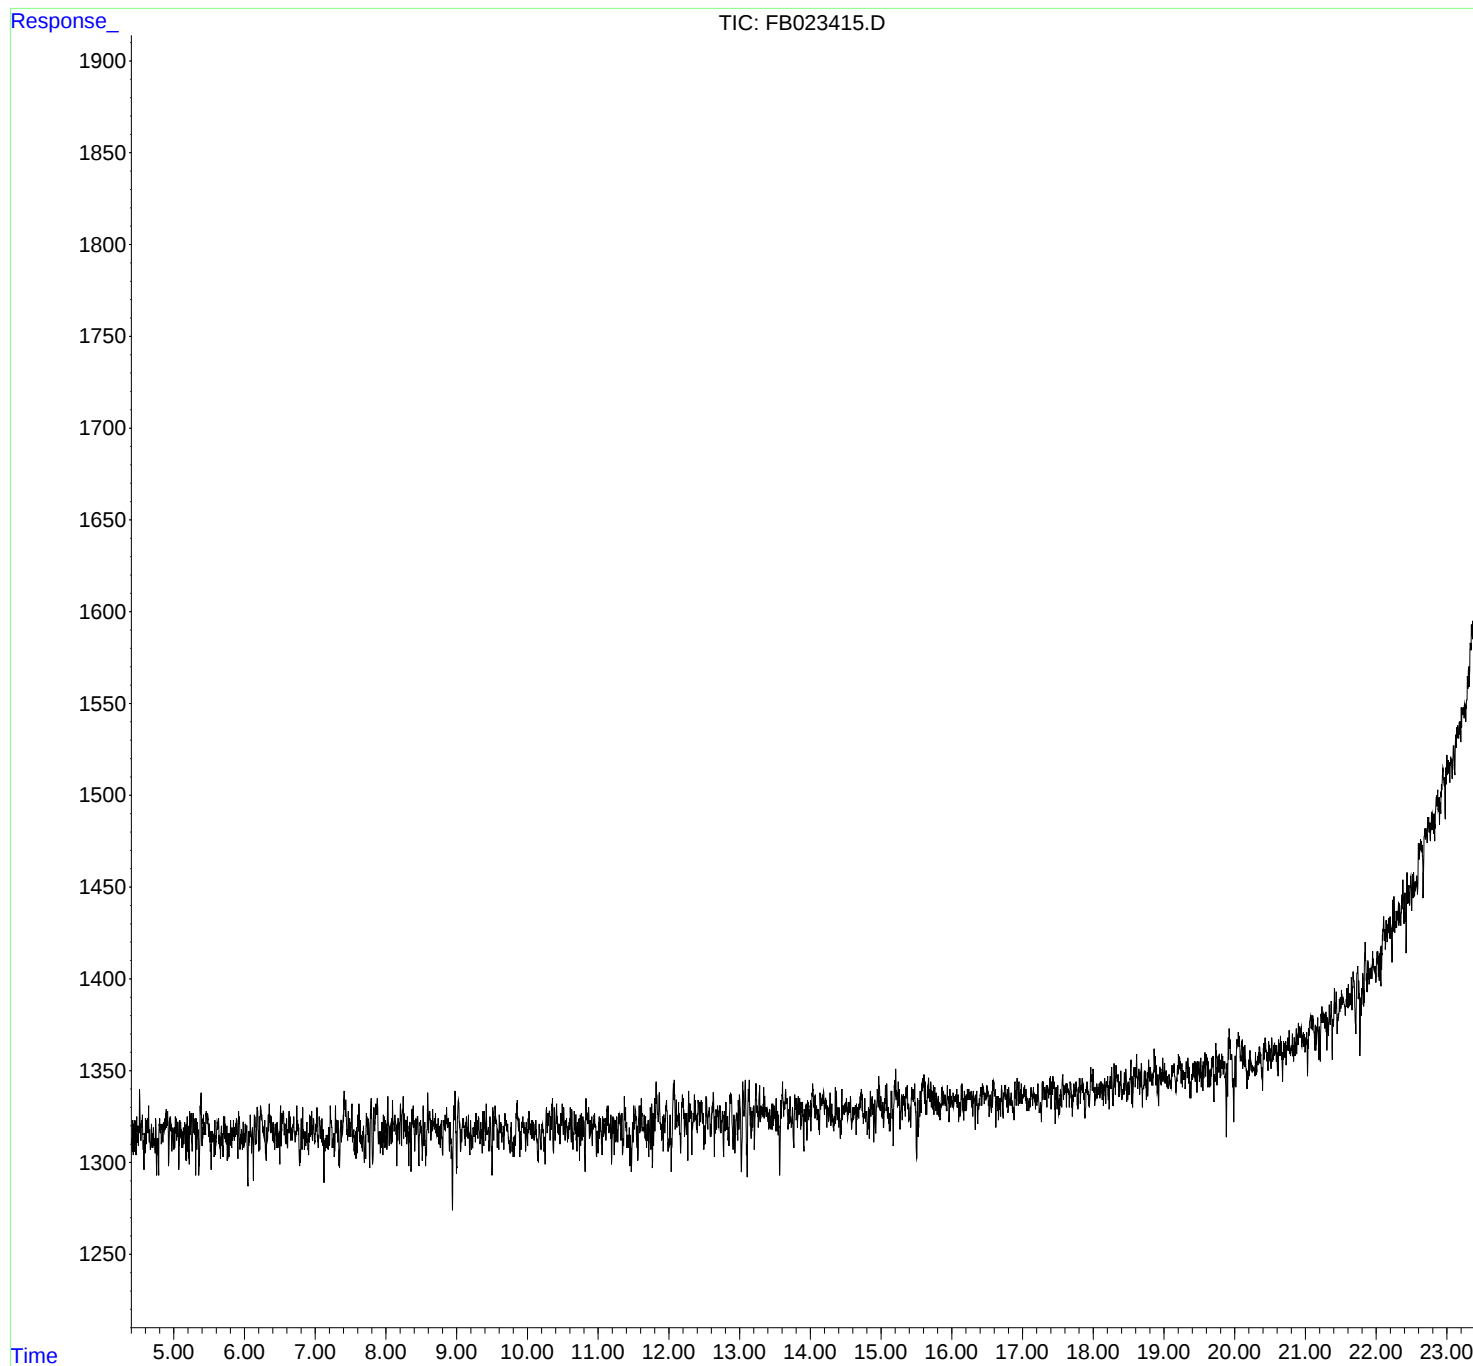

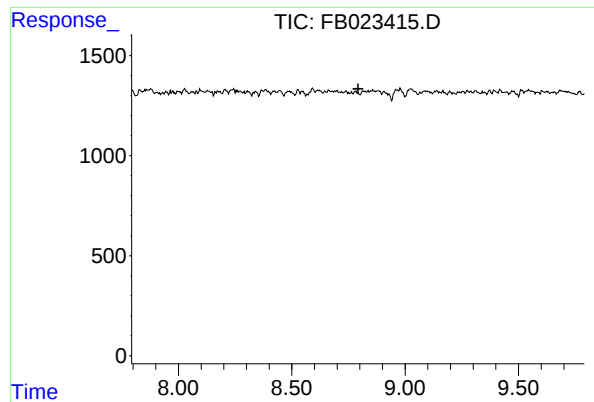

#5 AAA-TFT

R.T.: 0.000 min  
Exp R.T.: 8.793 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_B  
ClientSampleId :  
SB-01-COMP