

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
 Data File : FB023421.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2020 12:45
 Operator : DD/AJ
 Sample : L1005-02MSD
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 HR-05-011420MSD

Integration File: Calibration.e
 Quant Time: Jan 16 00:10:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	495166	20.881 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	701070	22.652 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	693103	20.748 ng/ml
3) t n-Heptane	7.755	122402	3.711 ng/ml
4) t Benzene	7.889	341705	8.557 ng/ml
6) t Toluene	10.627	980518	25.466 ng/ml
7) t Ethylbenzene	13.066	347550	9.575 ng/ml
8) t m-Xylene	13.200	453987	13.079 ng/ml
9) t O-Xylene	13.928	636424	18.895 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	375929	13.398 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
Data File : FB023421.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2020 12:45
Operator : DD/AJ
Sample : L1005-02MSD
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
HR-05-011420MSD

Integration File: Calibration.e
Quant Time: Jan 16 00:10:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

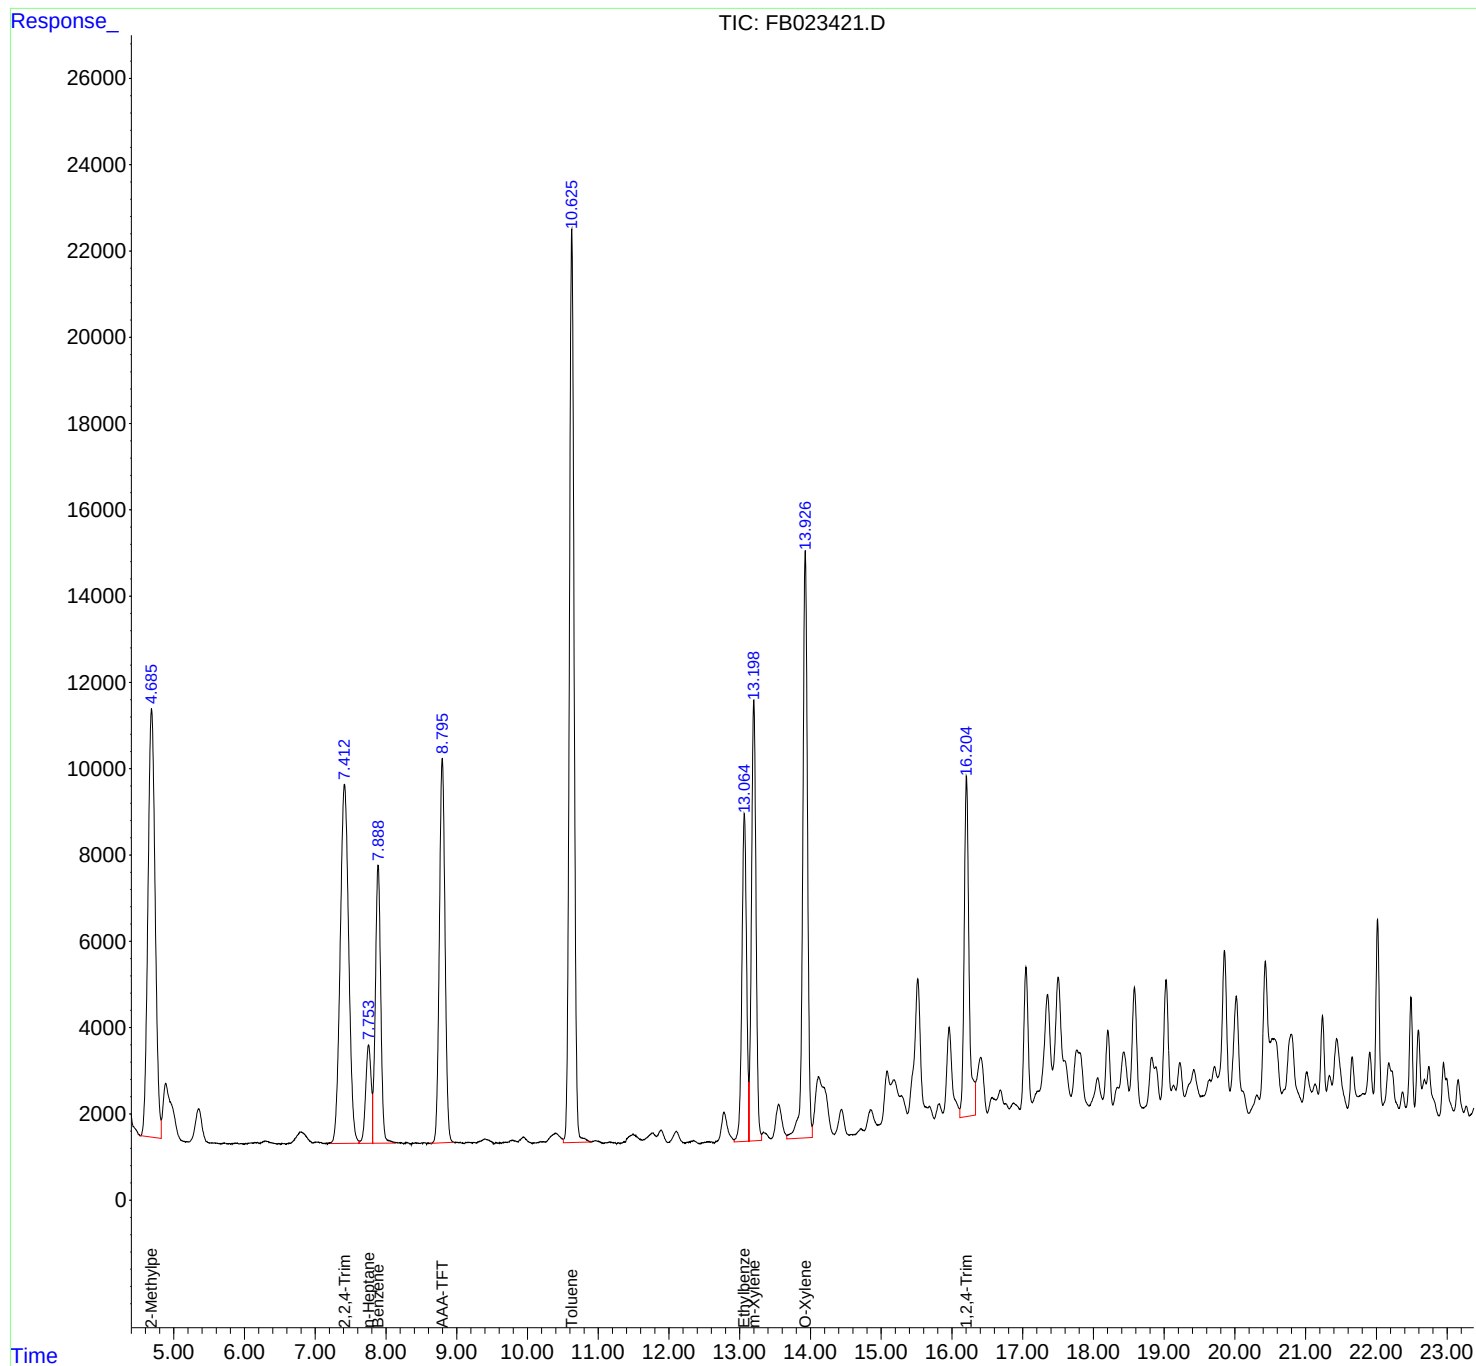


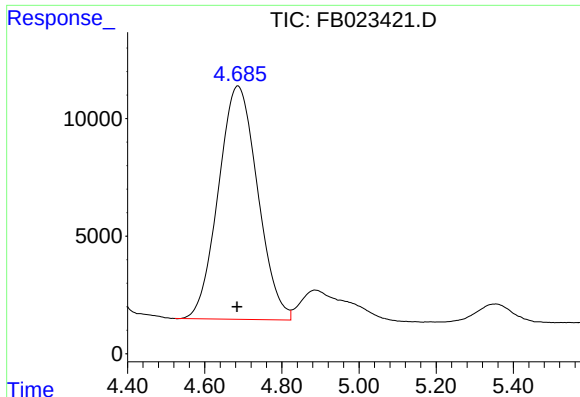

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.003 min
Response: 701070
Conc: 22.65 ng/ml

Instrument :
FID_B
ClientSampleId :
HR-05-011420MSD

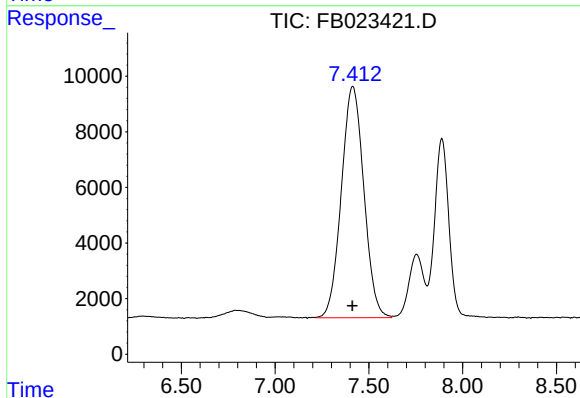


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.002 min
Response: 693103
Conc: 20.75 ng/ml

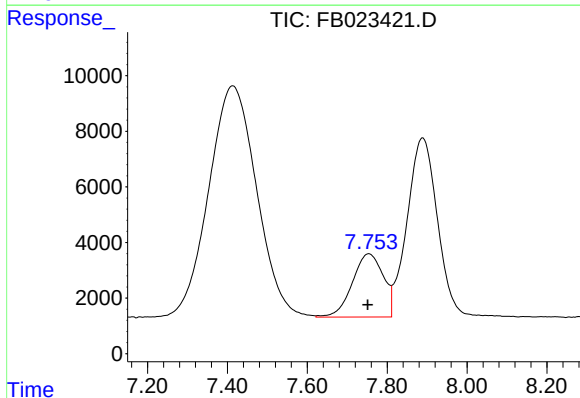


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 122402
Conc: 3.71 ng/ml

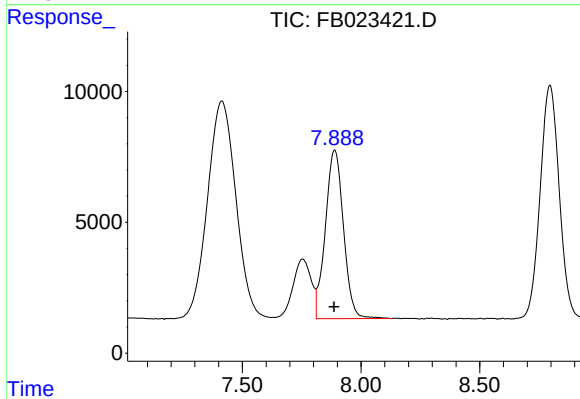

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 341705
Conc: 8.56 ng/ml

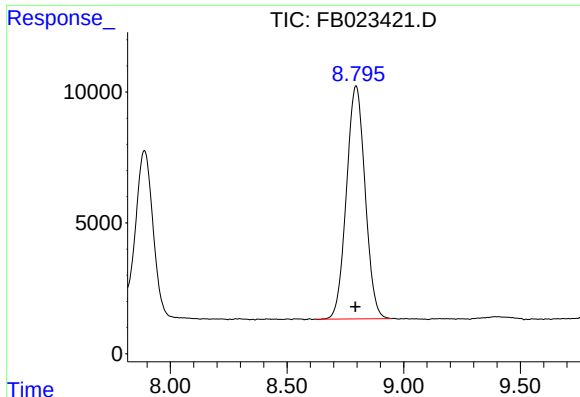

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.003 min
Response: 495166
Conc: 20.88 ng/ml

Instrument :
FID_B
ClientSampleId :
HR-05-011420MSD

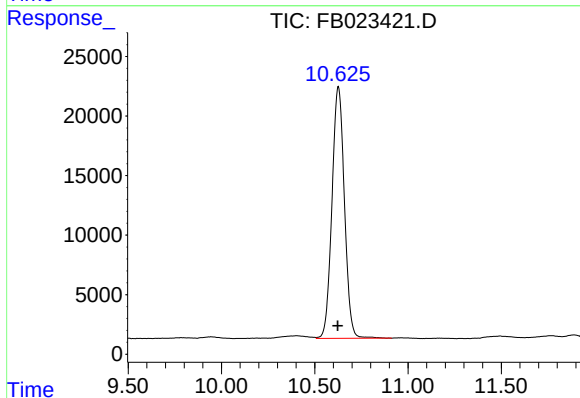


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.003 min
Response: 980518
Conc: 25.47 ng/ml

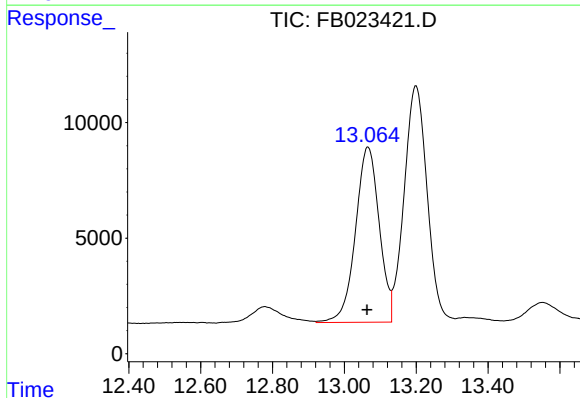


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.002 min
Response: 347550
Conc: 9.58 ng/ml

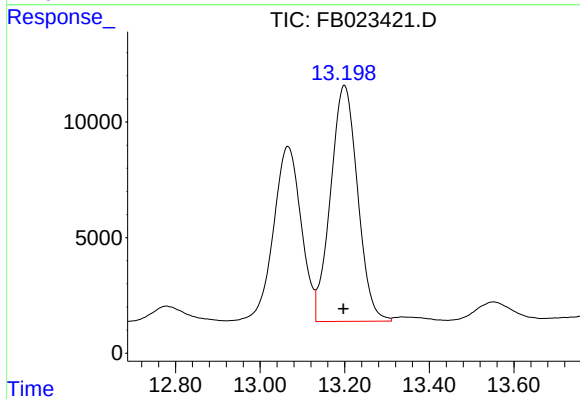

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.003 min
Response: 453987
Conc: 13.08 ng/ml

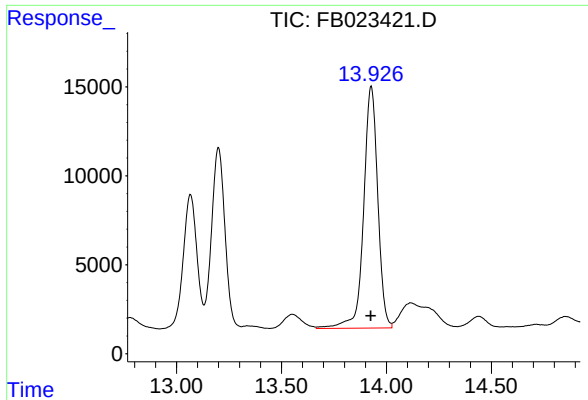

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.003 min
Response: 636424
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
HR-05-011420MSD

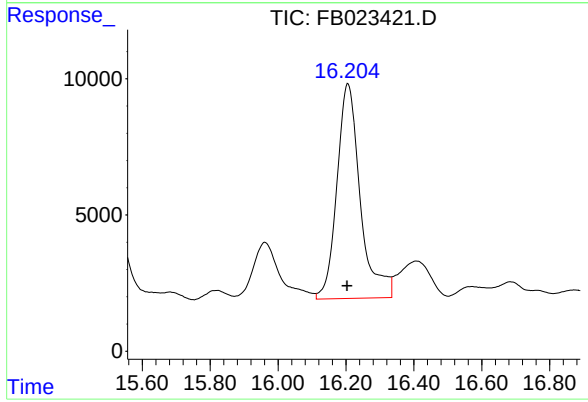

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.003 min
Response: 375929
Conc: 13.40 ng/ml