

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
 Data File : FB023423.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2020 13:46
 Operator : DD/AJ
 Sample : L1123-08 50X
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-04-COMP

Manual Integrations
 APPROVED

Ankita
 1/16/2020 9:59:38 AM

Integration File: Calibration.e
 Quant Time: Jan 16 00:10:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	1111938	46.890 ng/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011520\
Data File : FB023423.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2020 13:46
Operator : DD/AJ
Sample : L1123-08 50X
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Ankita
1/16/2020 9:59:38 AM

Integration File: Calibration.e
Quant Time: Jan 16 00:10:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

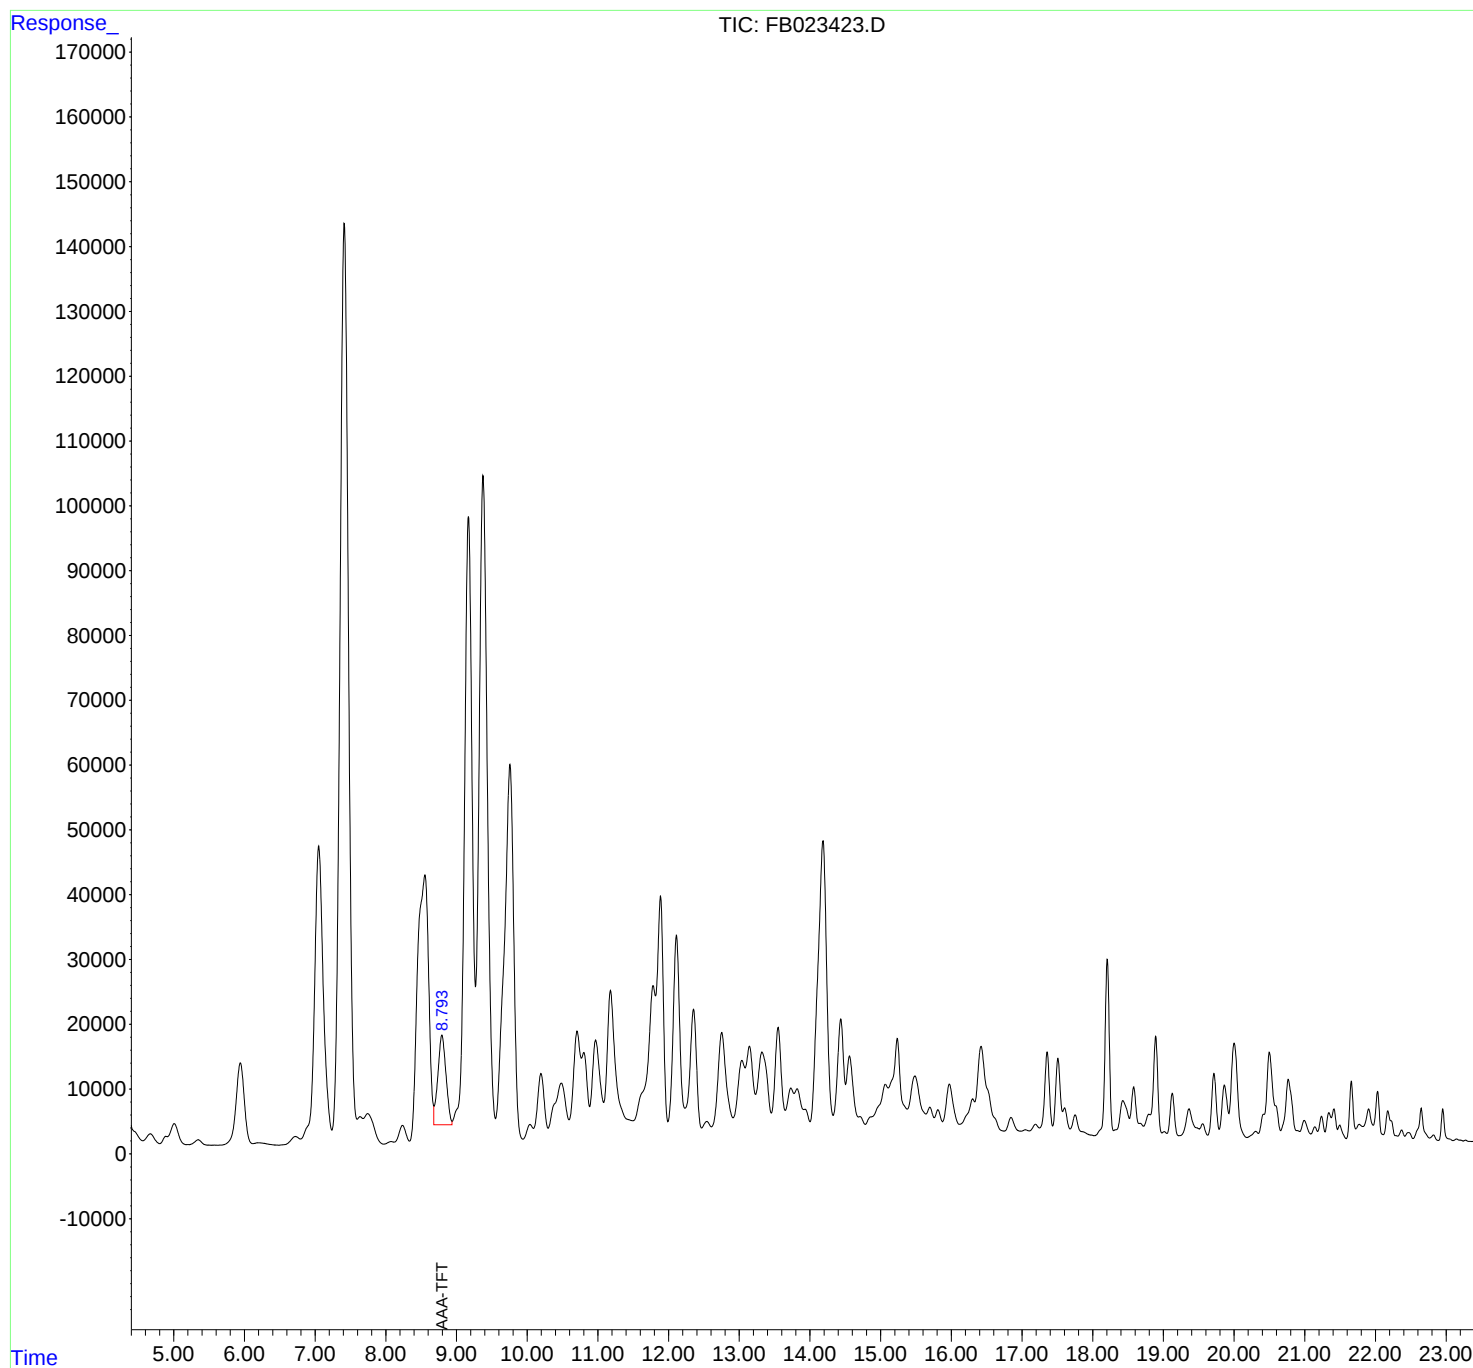

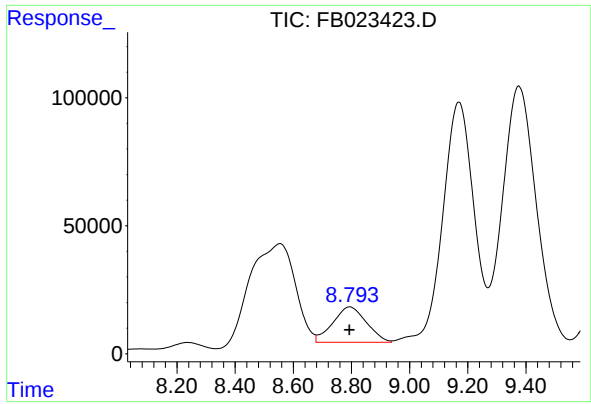

#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 1111938
Conc: 46.89 ng/ml m

Instrument :
FID_B
ClientSampleId :
SB-04-COMP

Manual Integrations
APPROVED

Ankita
1/16/2020 9:59:38 AM