

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011521\
 Data File : FB025399.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2021 10:48
 Operator : DD/AJ
 Sample : BSF0115S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 15 21:47:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	412119	18.320 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	898958	28.559 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	953649	30.080 ng/ml
3) t n-Heptane	7.759	309827	9.908 ng/ml
4) t Benzene	7.894	377079	9.591 ng/ml
6) t Toluene	10.632	1068989	28.477 ng/ml
7) t Ethylbenzene	13.072	332913	9.720 ng/ml
8) t m-Xylene	13.204	666240	19.473 ng/ml
9) t O-Xylene	13.932	641990	19.313 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	558532	19.422 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011521\
Data File : FB025399.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2021 10:48
Operator : DD/AJ
Sample : BSF0115S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 21:47:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

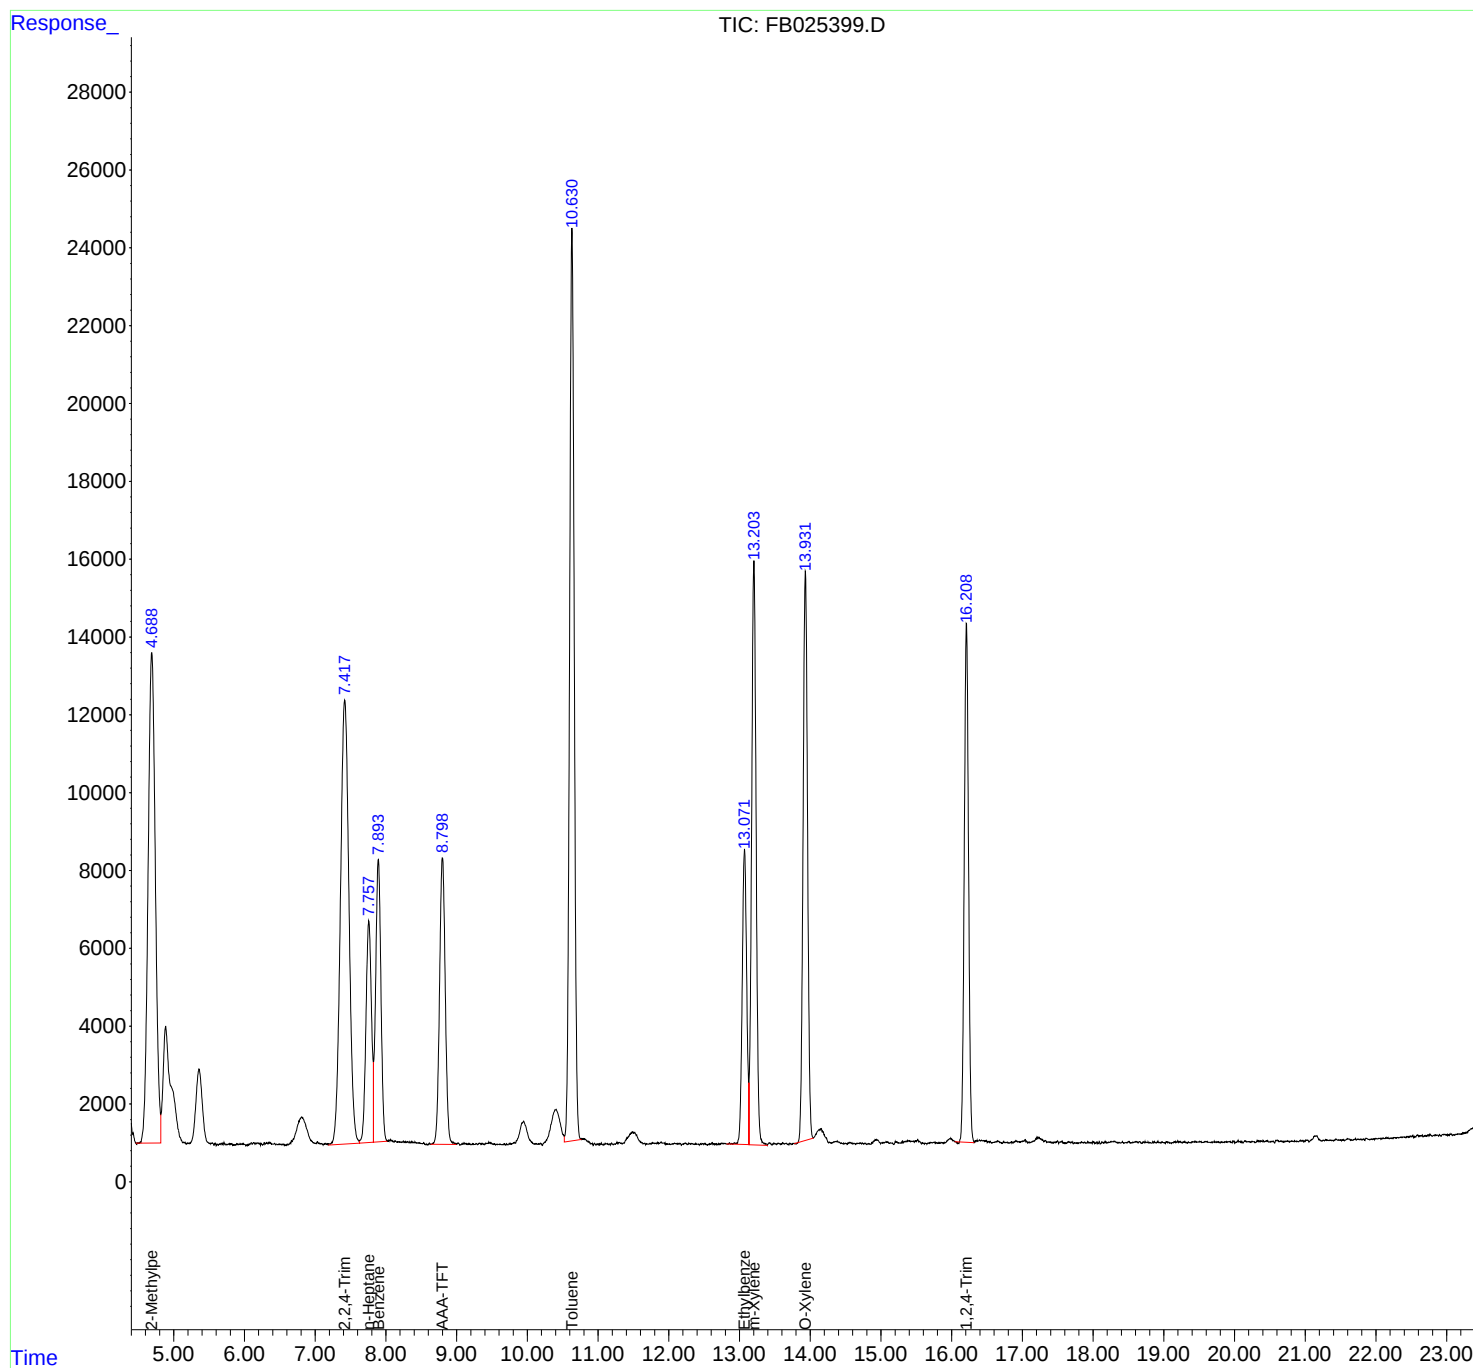

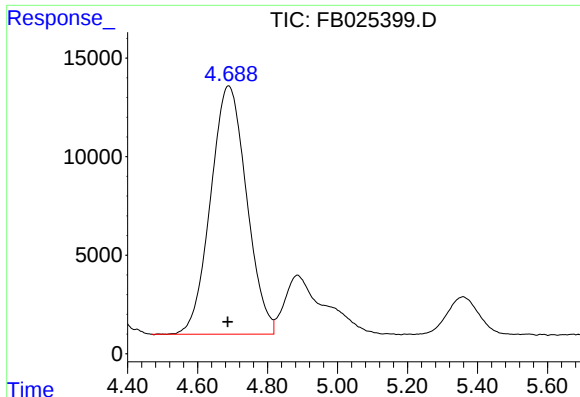


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.003 min
Response: 898958
Conc: 28.56 ng/ml

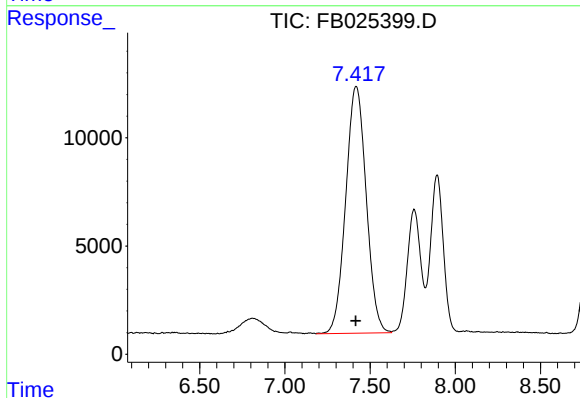


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 953649
Conc: 30.08 ng/ml

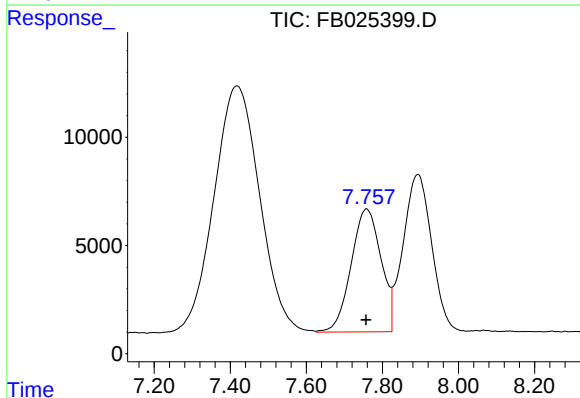


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.002 min
Response: 309827
Conc: 9.91 ng/ml

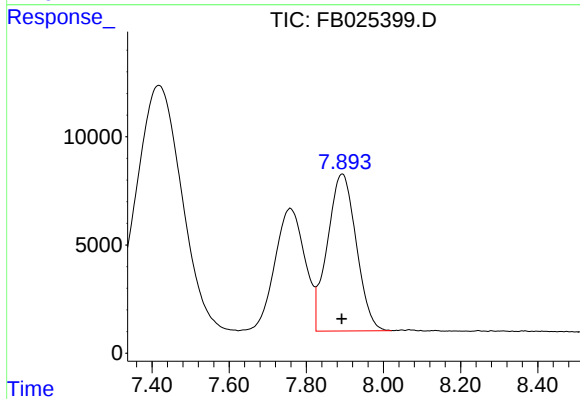


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 377079
Conc: 9.59 ng/ml

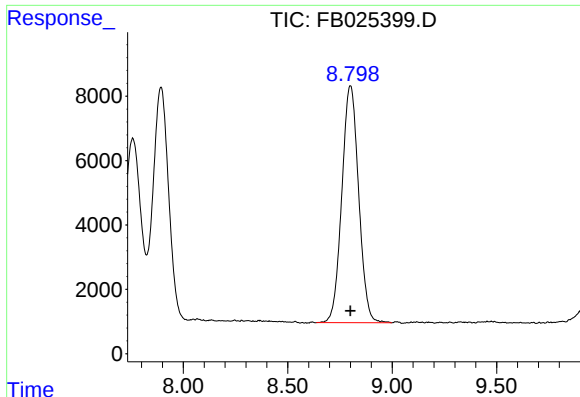


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 412119
Conc: 18.32 ng/ml

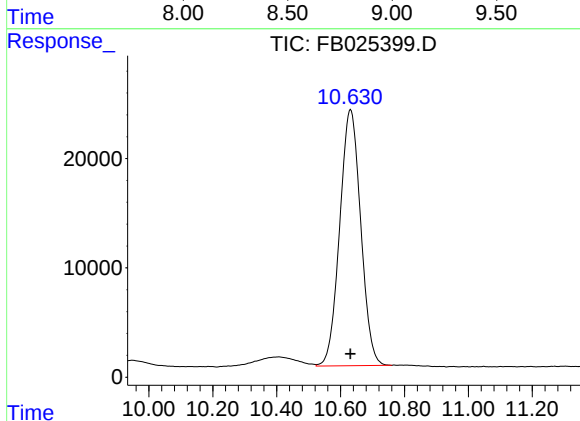


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1068989
Conc: 28.48 ng/ml

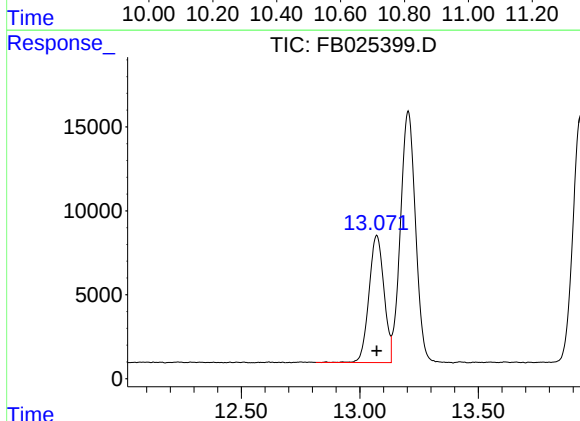


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 332913
Conc: 9.72 ng/ml

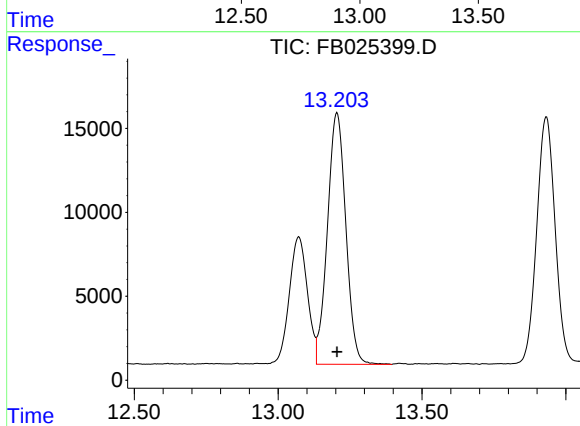

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 666240
Conc: 19.47 ng/ml

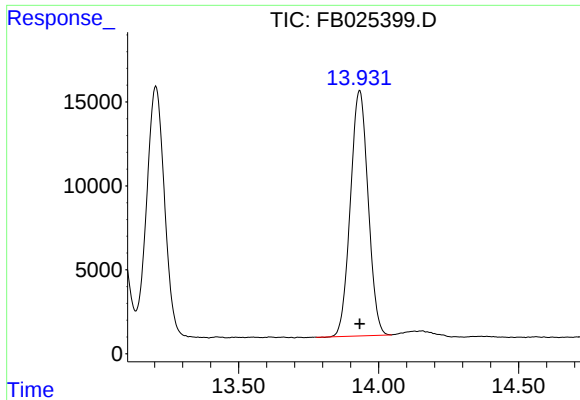


#9 O-Xylene

R.T.: 13.932 min

Delta R.T.: 0.000 min

Response: 641990

Conc: 19.31 ng/ml

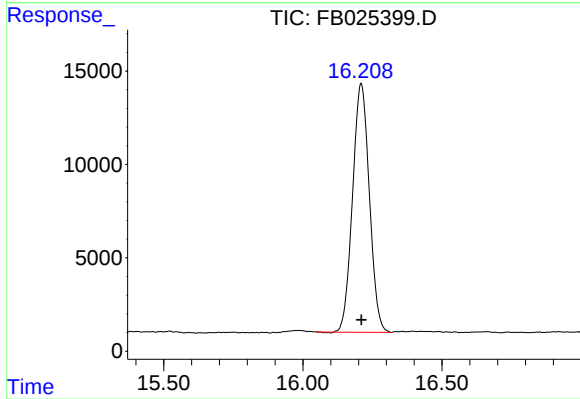

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: 0.000 min

Response: 558532

Conc: 19.42 ng/ml