

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011521\
 Data File : FB025404.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2021 13:49
 Operator : DD/AJ
 Sample : M1120-02MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 15 21:48:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
 Quant Title :
 QLast Update : Mon Jan 04 13:09:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	364596	16.207 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	745220	23.675 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	757104	23.880 ng/ml
3) t n-Heptane	7.759	246517	7.883 ng/ml
4) t Benzene	7.894	321885	8.187 ng/ml
6) t Toluene	10.632	932901	24.851 ng/ml
7) t Ethylbenzene	13.073	293099	8.557 ng/ml
8) t m-Xylene	13.206	578247	16.901 ng/ml
9) t O-Xylene	13.933	562669	16.927 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	479935	16.689 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011521\
Data File : FB025404.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2021 13:49
Operator : DD/AJ
Sample : M1120-02MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 15 21:48:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010421.M
Quant Title :
QLast Update : Mon Jan 04 13:09:59 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

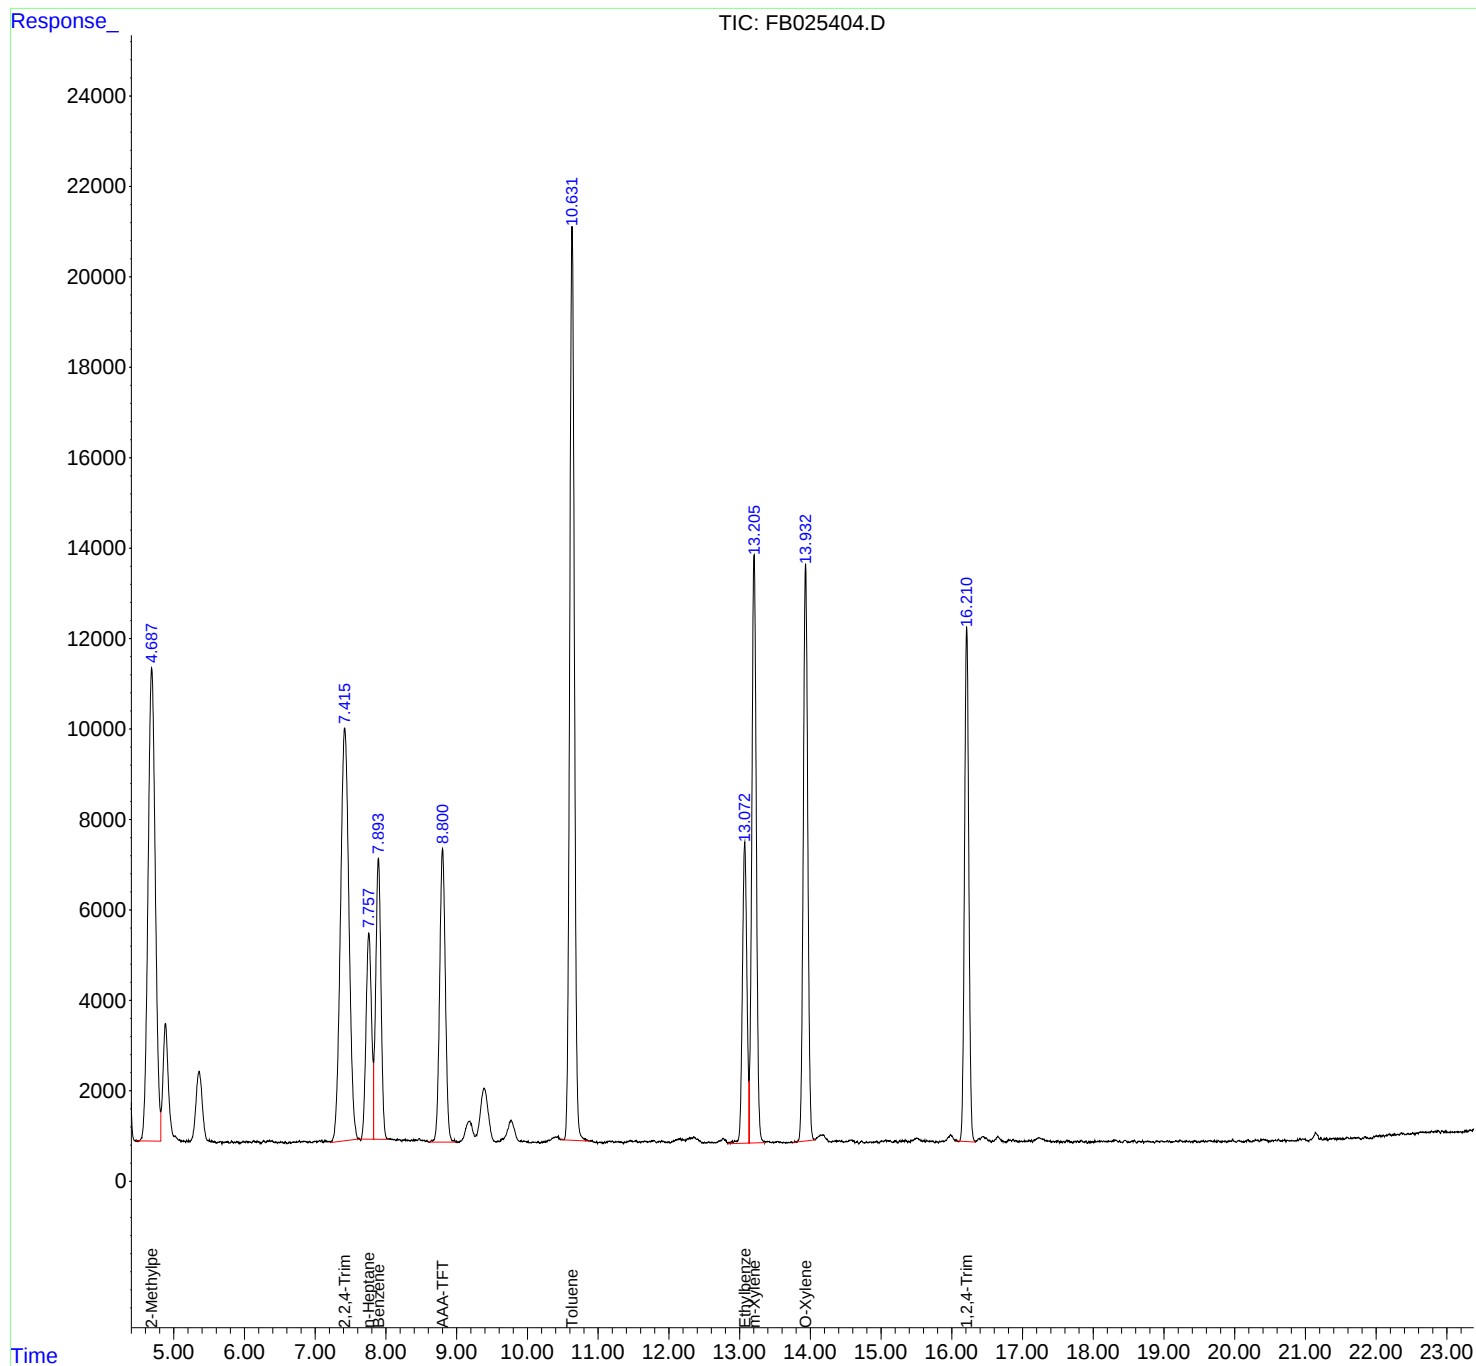

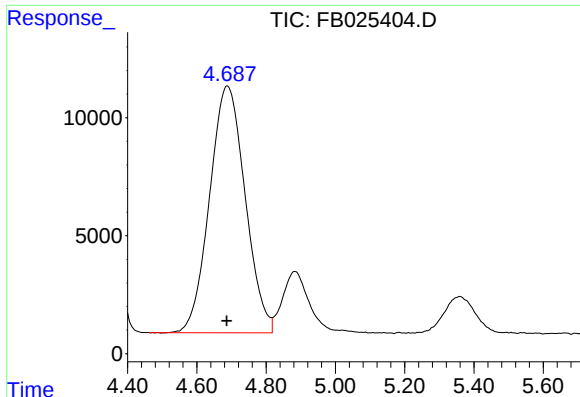


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.002 min
Response: 745220
Conc: 23.67 ng/ml

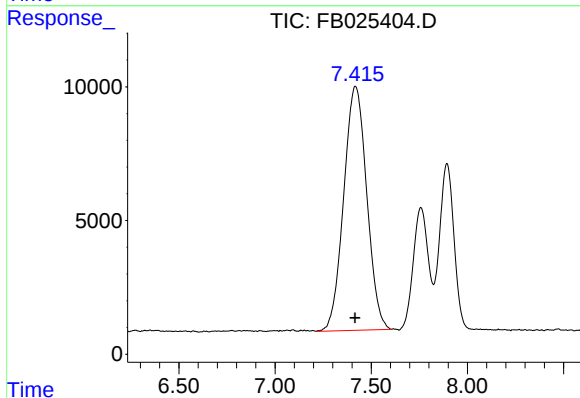


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 757104
Conc: 23.88 ng/ml

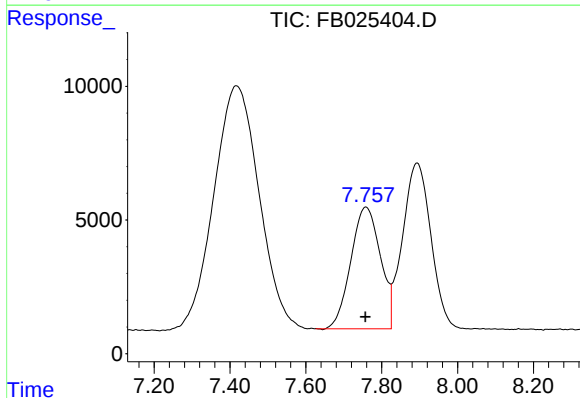


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.002 min
Response: 246517
Conc: 7.88 ng/ml

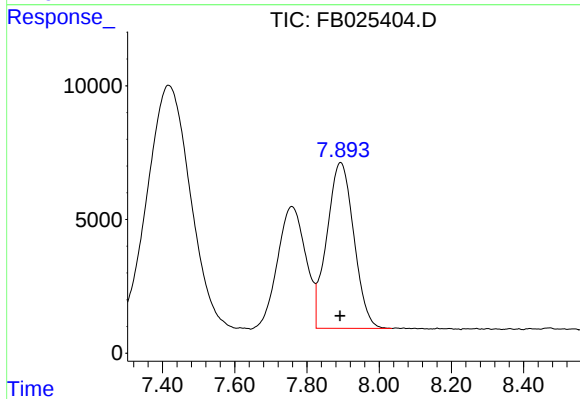


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 321885
Conc: 8.19 ng/ml

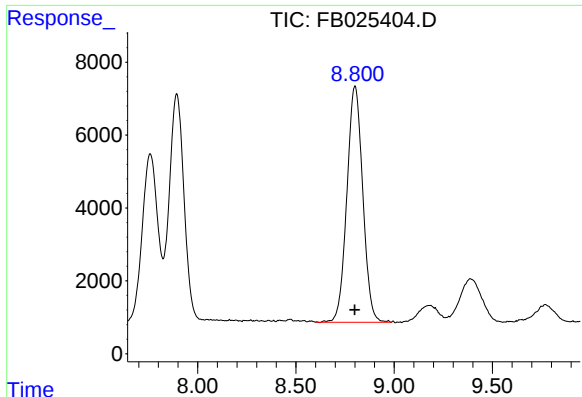


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 364596
Conc: 16.21 ng/ml

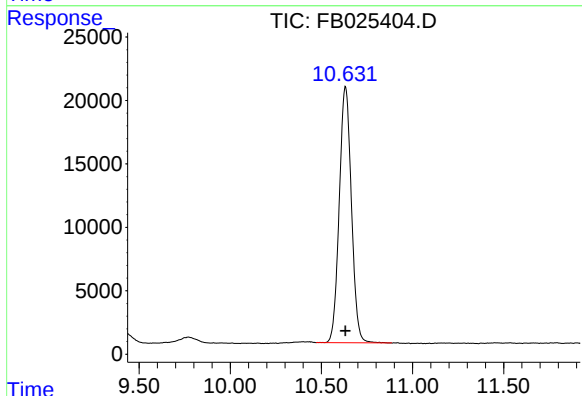


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 932901
Conc: 24.85 ng/ml

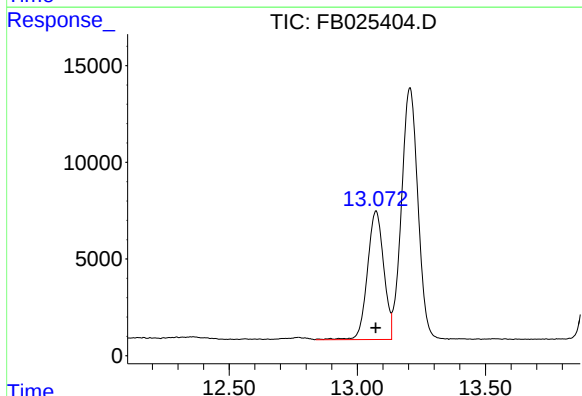


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.002 min
Response: 293099
Conc: 8.56 ng/ml

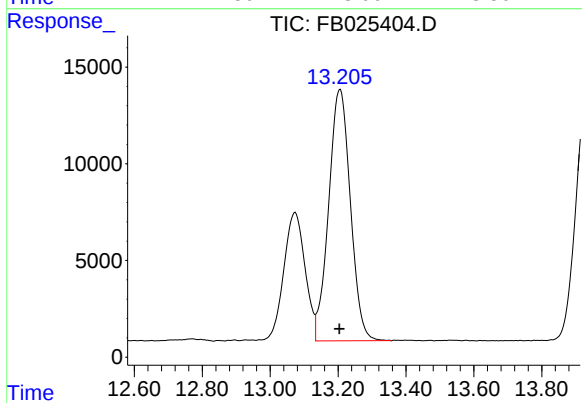


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.001 min
Response: 578247
Conc: 16.90 ng/ml

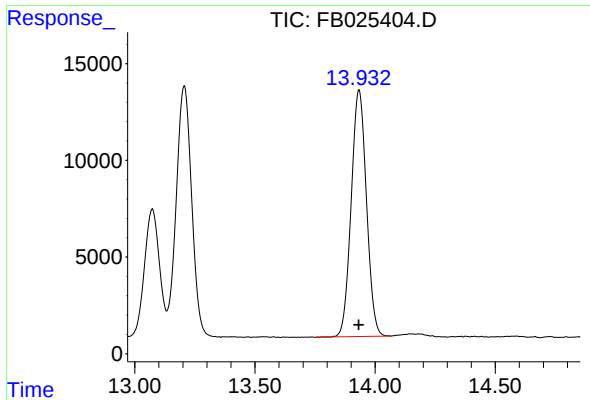

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.001 min
Response: 562669
Conc: 16.93 ng/ml

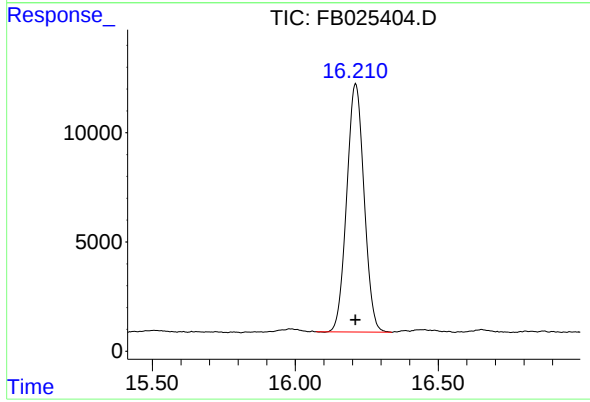

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.001 min
Response: 479935
Conc: 16.69 ng/ml