

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011525\
 Data File : FB031307.D
 Signal(s) : FID2B.CH
 Acq On : 15 Jan 2025 10:20
 Operator : YP/AJ
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 15 11:20:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
 Quant Title :
 QLast Update : Wed Jan 15 11:19:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	115906	4.680 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	233598	7.655 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	275493	7.888 ng/ml
3) t n-Heptane	7.745	76823	2.289 ng/ml
4) t Benzene	7.885	96940	2.457 ng/ml
6) t Toluene	10.613	281739	7.767 ng/ml
7) t Ethylbenzene	13.049	90664	2.859 ng/ml
8) t m-Xylene	13.183	196650	5.784 ng/ml
9) t O-Xylene	13.911	197897	6.226 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	169444	6.606 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011525\
Data File : FB031307.D
Signal(s) : FID2B.CH
Acq On : 15 Jan 2025 10:20
Operator : YP/AJ
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 15 11:20:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 11:19:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

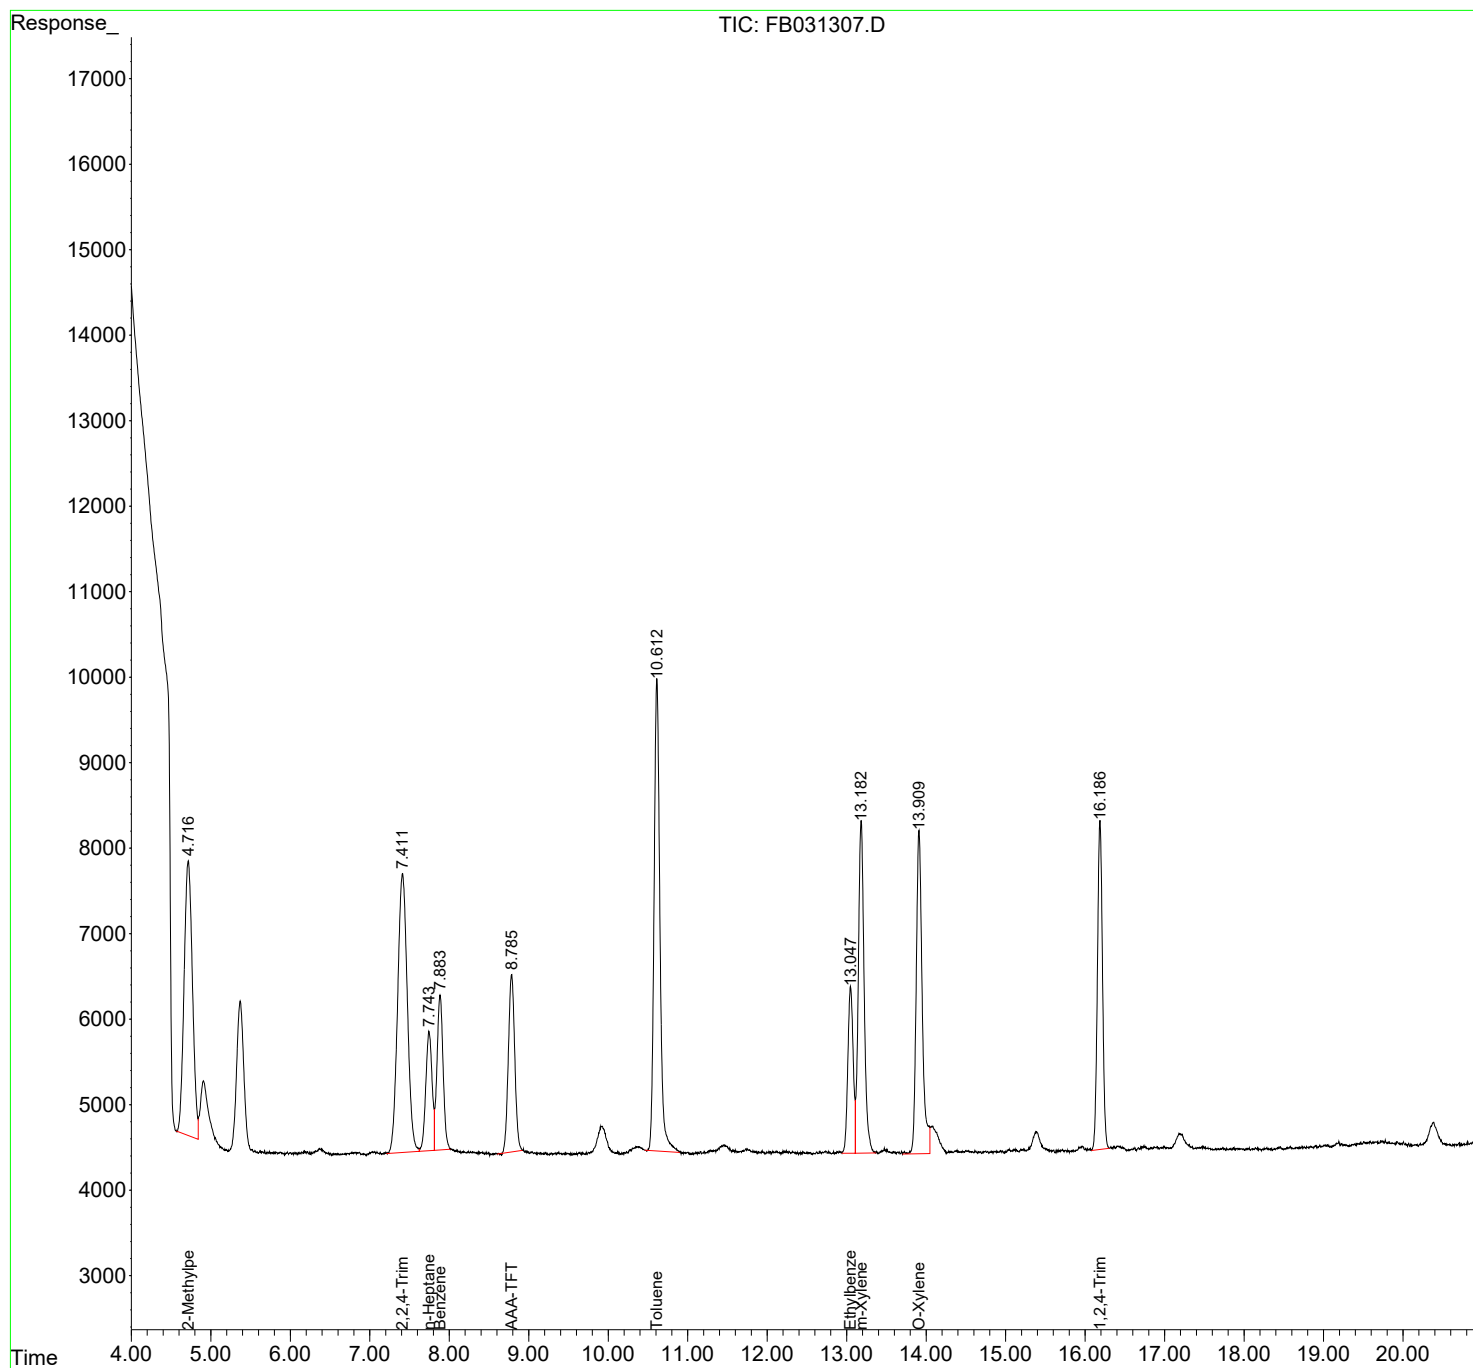


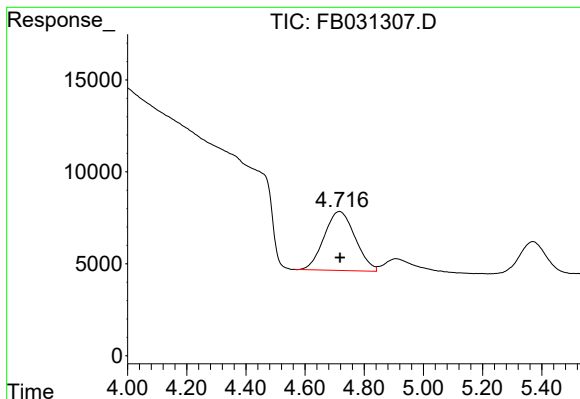

#1 2-Methylpentane


R.T.: 4.718 min
Delta R.T.: 0.000 min
Response: 233598
Conc: 7.65 ng/ml

Instrument :
FID_B
ClientSampleId :

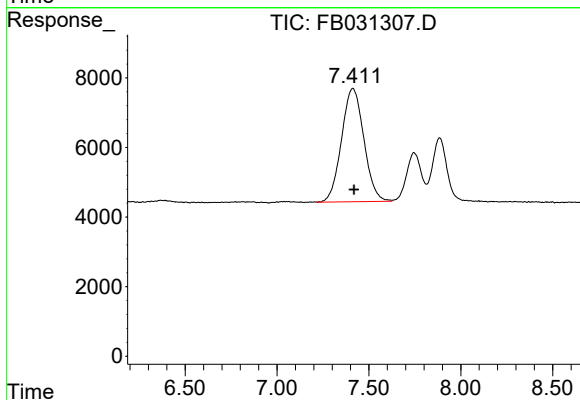


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.007 min
Response: 275493
Conc: 7.89 ng/ml

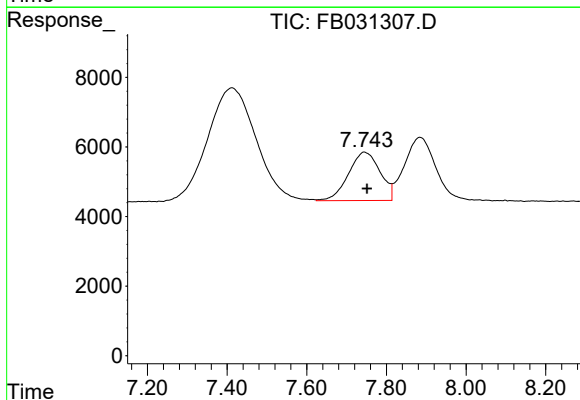


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.006 min
Response: 76823
Conc: 2.29 ng/ml

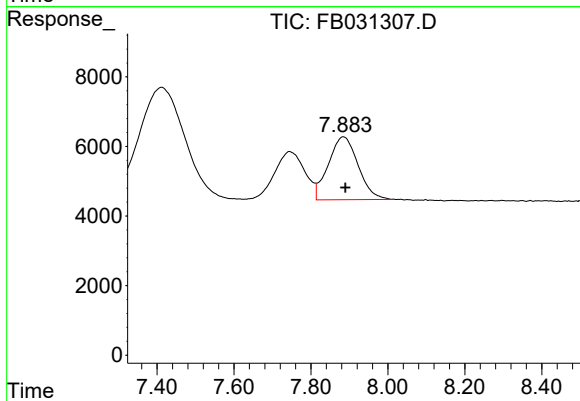

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.005 min
Response: 96940
Conc: 2.46 ng/ml

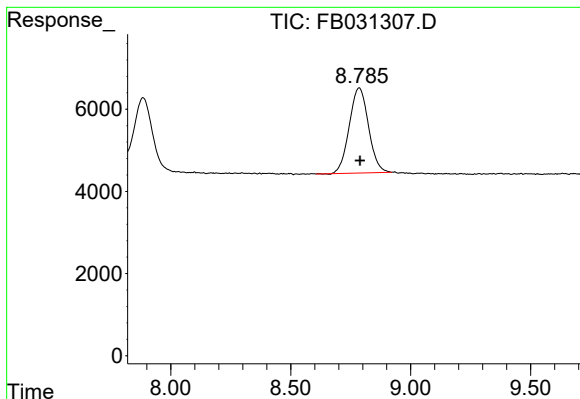

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: -0.003 min
Response: 115906
Conc: 4.68 ng/ml

Instrument :
FID_B
ClientSampleId :

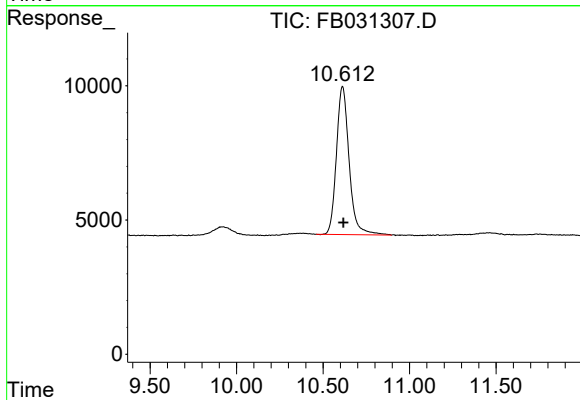


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.005 min
Response: 281739
Conc: 7.77 ng/ml

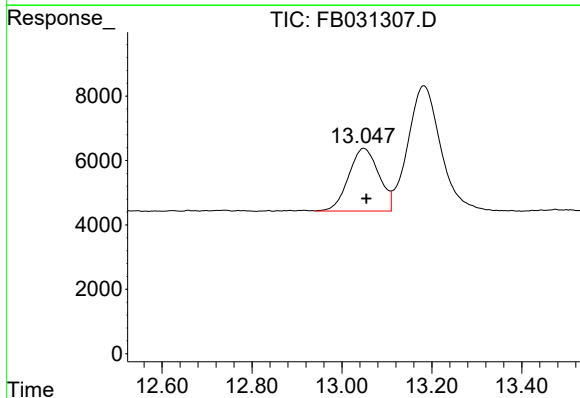


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.005 min
Response: 90664
Conc: 2.86 ng/ml

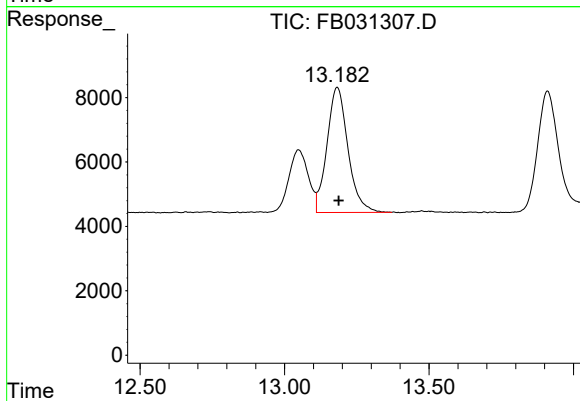

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.005 min
Response: 196650
Conc: 5.78 ng/ml

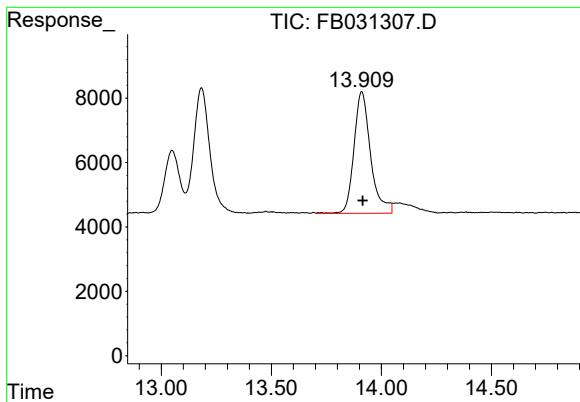

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 197897
Conc: 6.23 ng/ml

Instrument :
FID_B
ClientSampleId :

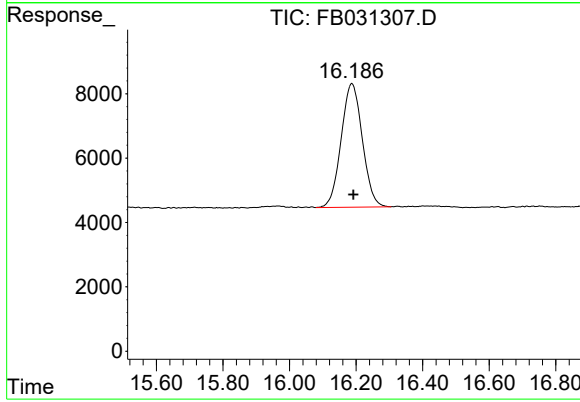

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.004 min
Response: 169444
Conc: 6.61 ng/ml