

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011619\
 Data File : FB019419.D
 Signal(s) : FID2B.CH
 Acq On : 16 Jan 2019 8:59
 Operator : MJ/SJ
 Sample : BSF0116S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 17 00:53:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	162178	18.251 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	544289	27.329 ng/ml
2) t 2,2,4-Trimethylpentane	7.657	533260	27.993 ng/ml
3) t n-Heptane	7.996	164893	9.451 ng/ml
4) t Benzene	8.134	192209	9.789 ng/ml
6) t Toluene	10.889	565416	31.258 ng/ml
7) t Ethylbenzene	13.341	229088	10.340 ng/ml
8) t m-Xylene	13.473	474812	20.690 ng/ml
9) t O-Xylene	14.206	461545	20.570 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	458502	20.108 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011619\
Data File : FB019419.D
Signal(s) : FID2B.CH
Acq On : 16 Jan 2019 8:59
Operator : MJ/SJ
Sample : BSF0116S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 17 00:53:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

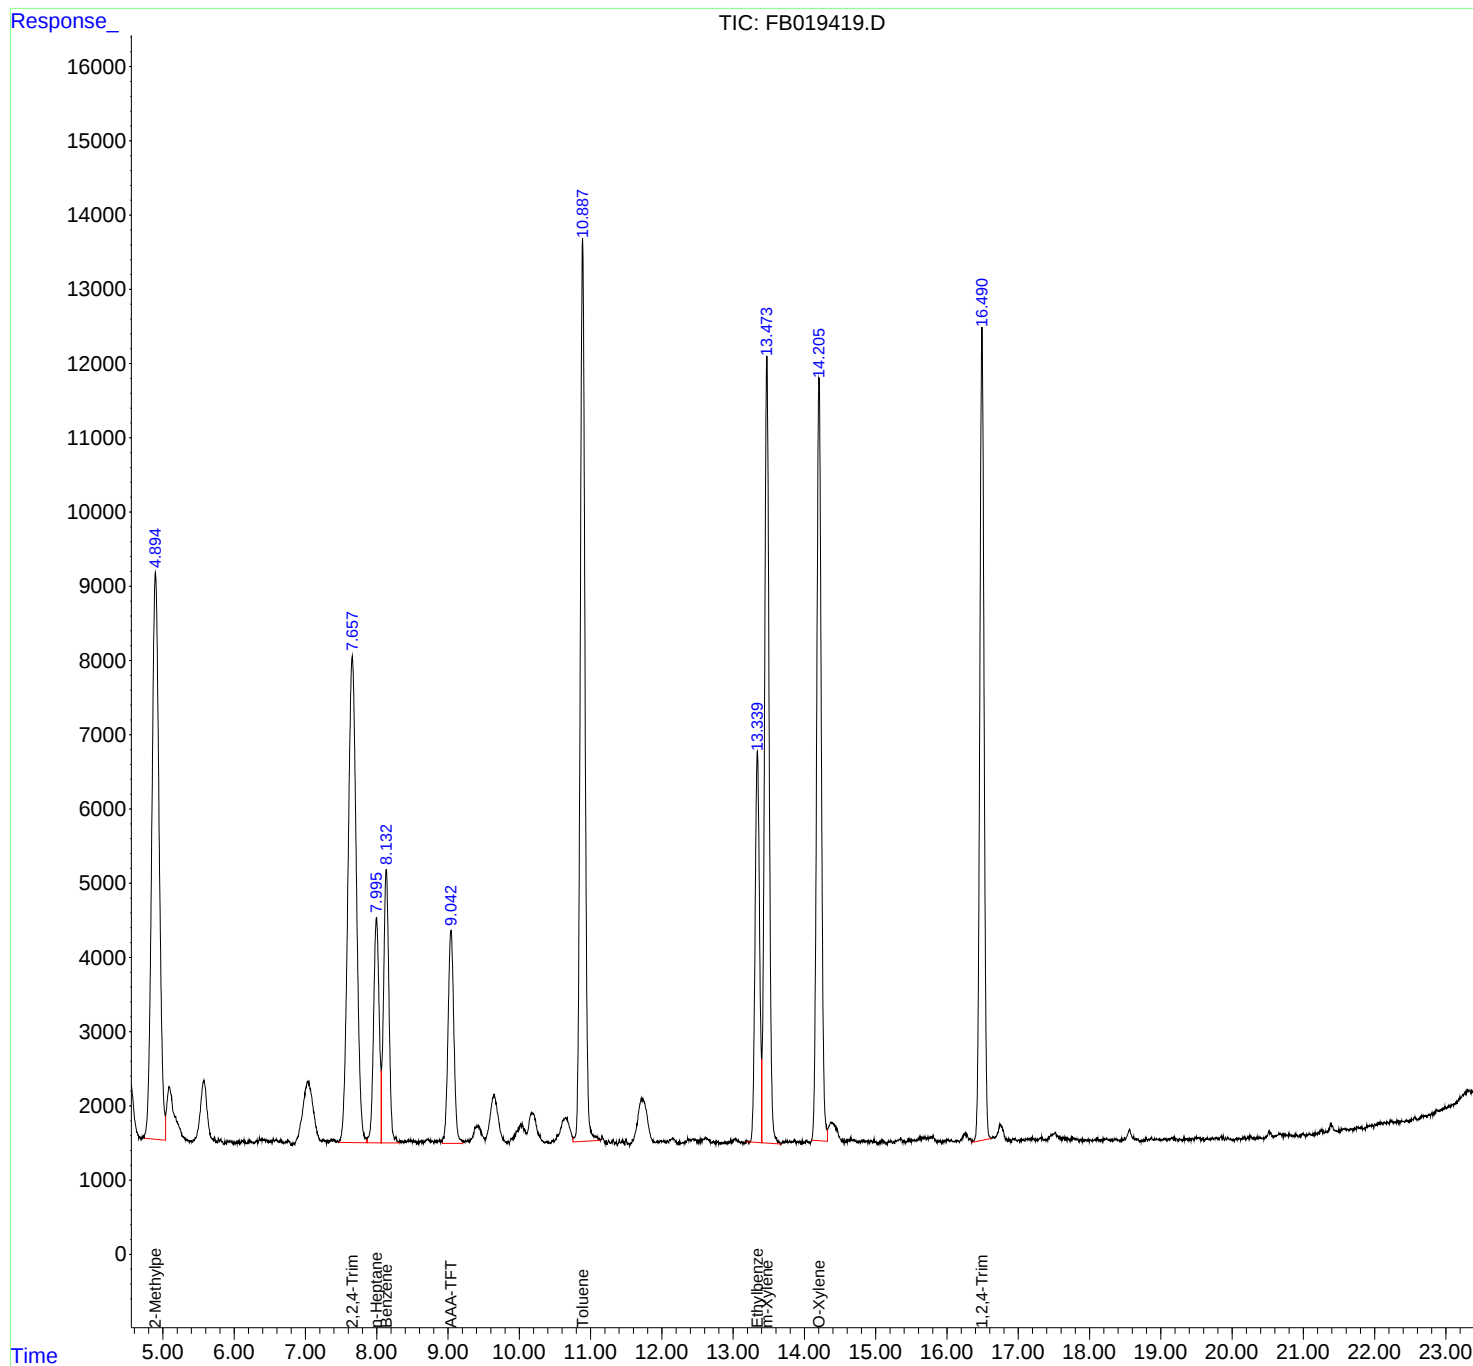

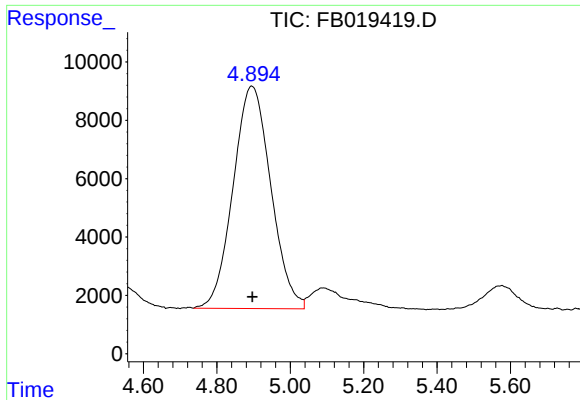


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 544289
Conc: 27.33 ng/ml

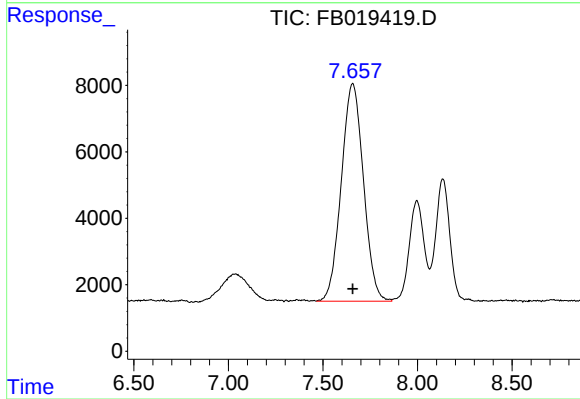


#2 2,2,4-Trimethylpentane

R.T.: 7.657 min
Delta R.T.: 0.000 min
Response: 533260
Conc: 27.99 ng/ml

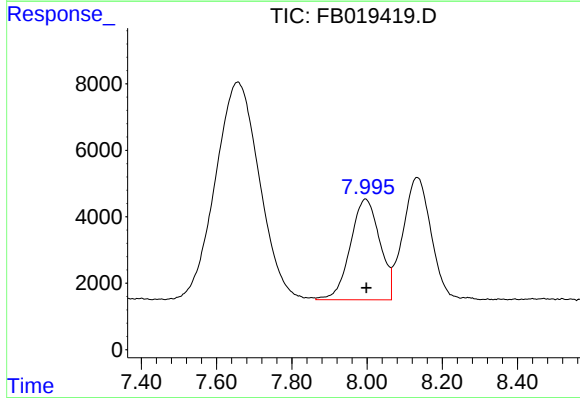


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: -0.002 min
Response: 164893
Conc: 9.45 ng/ml

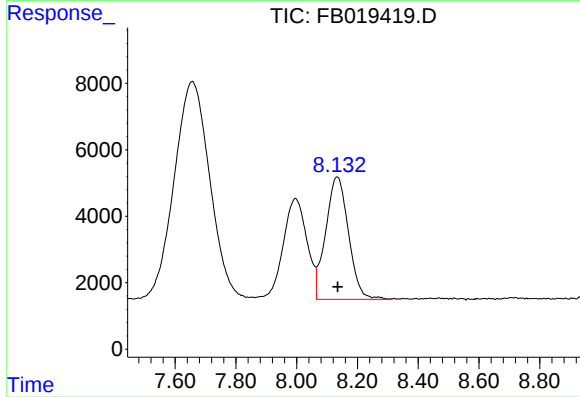


#4 Benzene

R.T.: 8.134 min
Delta R.T.: -0.001 min
Response: 192209
Conc: 9.79 ng/ml

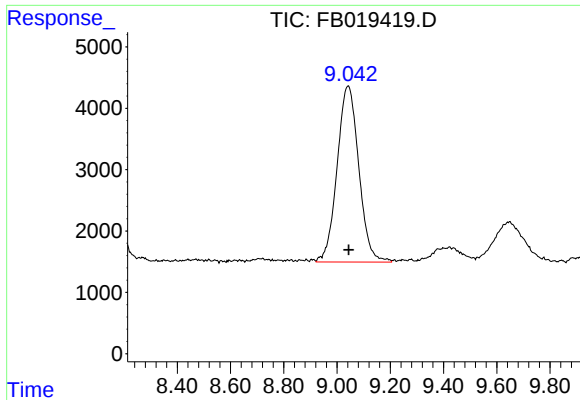


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 162178
Conc: 18.25 ng/ml

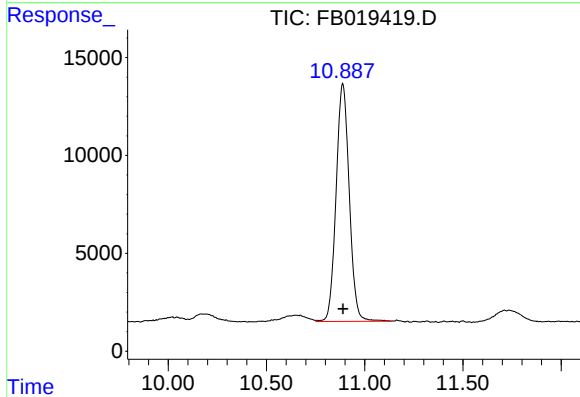


#6 Toluene

R.T.: 10.889 min
Delta R.T.: -0.002 min
Response: 565416
Conc: 31.26 ng/ml

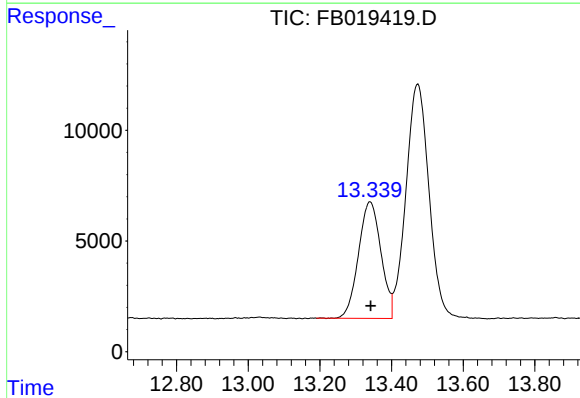


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: -0.001 min
Response: 229088
Conc: 10.34 ng/ml

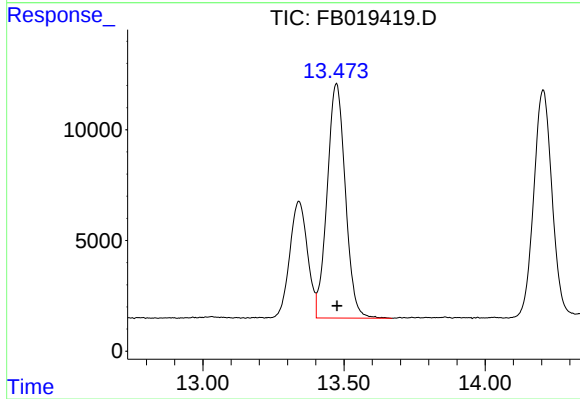


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: -0.002 min
Response: 474812
Conc: 20.69 ng/ml

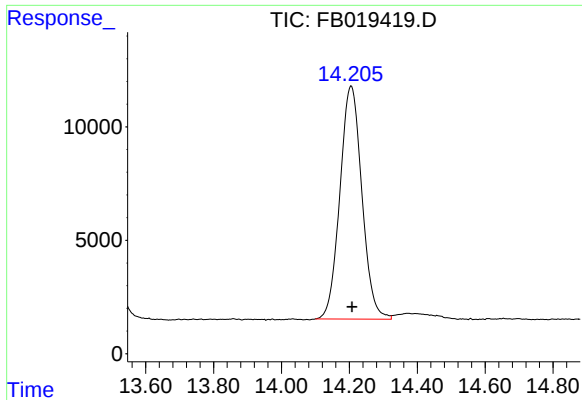

#9 O-Xylene

R.T.: 14.206 min
Delta R.T.: -0.002 min
Response: 461545
Conc: 20.57 ng/ml

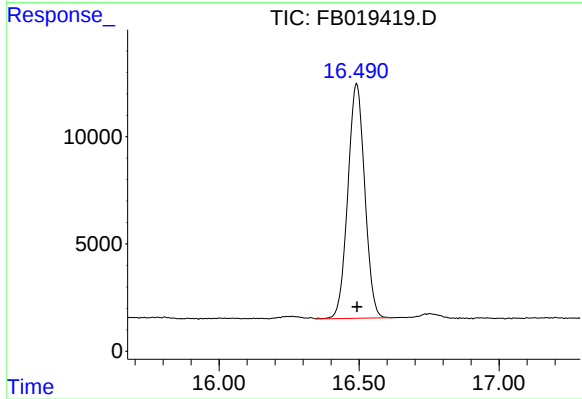

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: -0.002 min
Response: 458502
Conc: 20.11 ng/ml