

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011620\
Data File : FB023441.D
Signal(s) : FID2B.CH
Acq On : 16 Jan 2020 17:21
Operator : DD/AJ
Sample : L1017-05
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 17 00:08:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	385057	16.210 ng/ml
Target Compounds				
6) t	Toluene	10.627	4800	0.121 ng/ml
8) t	m-Xylene	13.200	3693	0.104 ng/ml
9) t	O-Xylene	13.916	338	0.010 ng/ml
10) t	1,2,4-Trimethylbenzene	16.215	4154	0.142 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011620\
Data File : FB023441.D
Signal(s) : FID2B.CH
Acq On : 16 Jan 2020 17:21
Operator : DD/AJ
Sample : L1017-05
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 17 00:08:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

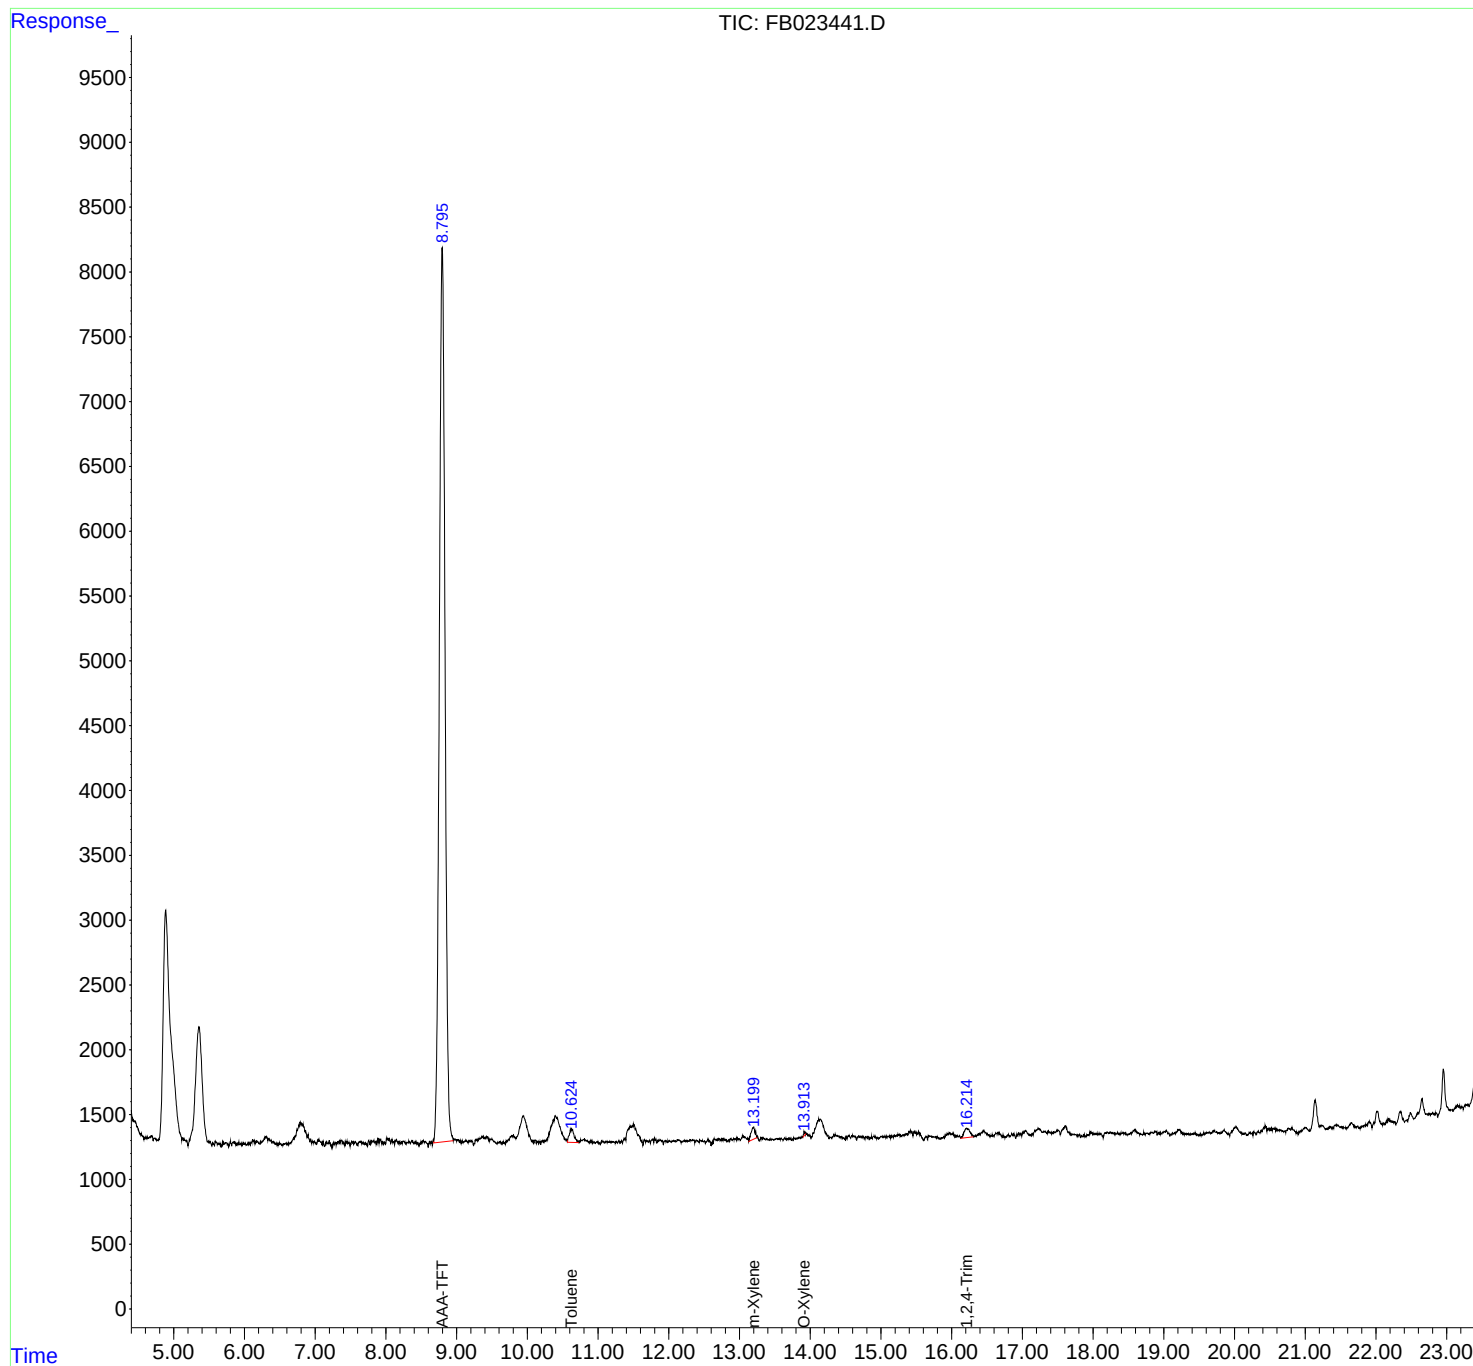

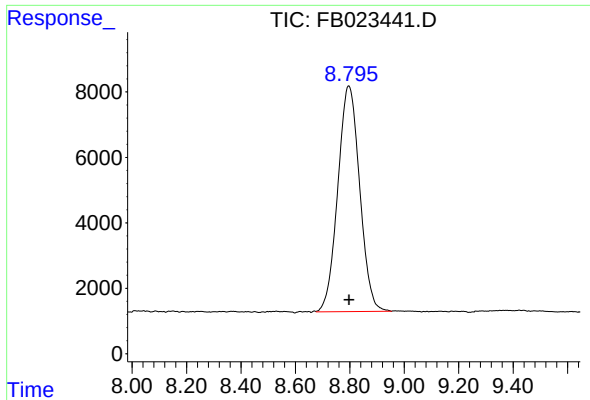


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 385057
Conc: 16.21 ng/ml

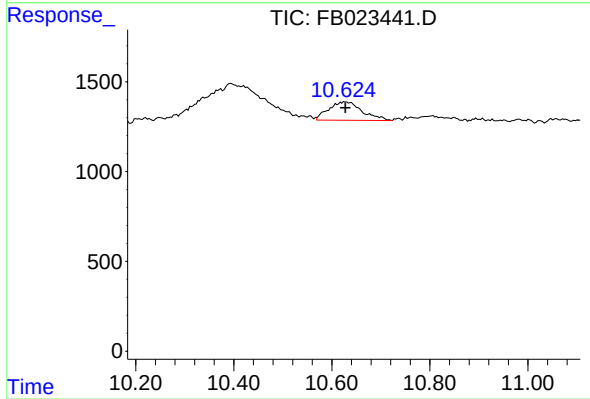


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.000 min
Response: 4800
Conc: 0.12 ng/ml

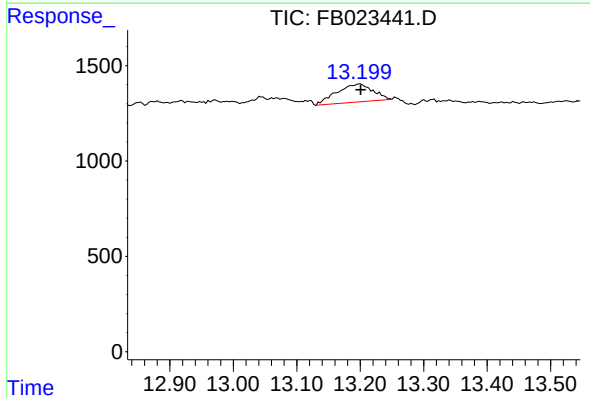


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: 0.000 min
Response: 3693
Conc: 0.10 ng/ml

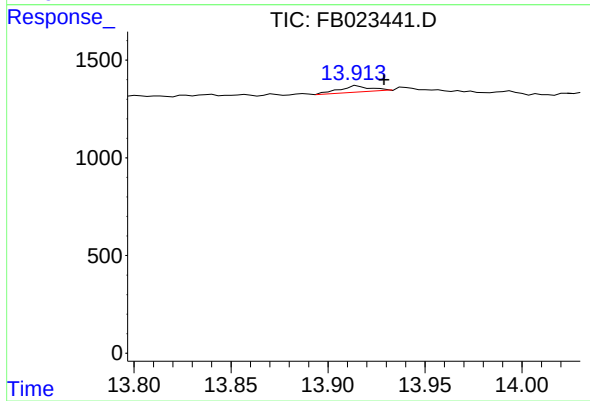

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.013 min
Response: 338
Conc: 0.01 ng/ml

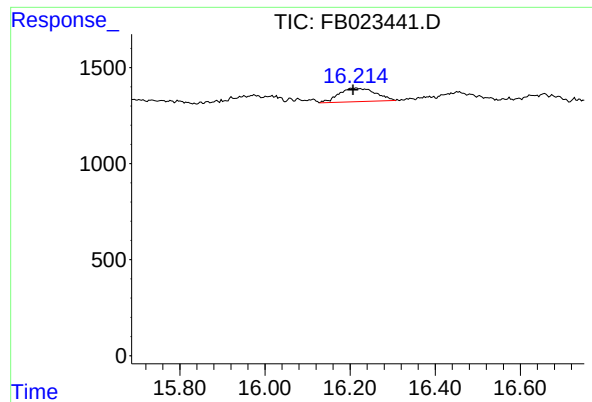

#10 1,2,4-Trimethylbenzene

R.T.: 16.215 min
Delta R.T.: 0.009 min
Response: 4154
Conc: 0.14 ng/ml