

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011719\
 Data File : FB019449.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2019 9:26
 Operator : MJ/SJ
 Sample : BSF0117S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 18 02:47:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	161191	18.140 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.893	513266	25.771 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	516308	27.103 ng/ml
3) t n-Heptane	7.994	158262	9.070 ng/ml
4) t Benzene	8.131	185065	9.425 ng/ml
6) t Toluene	10.885	566361	31.310 ng/ml
7) t Ethylbenzene	13.337	228000	10.291 ng/ml
8) t m-Xylene	13.470	468754	20.426 ng/ml
9) t O-Xylene	14.202	451941	20.142 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	451703	19.810 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011719\
Data File : FB019449.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2019 9:26
Operator : MJ/SJ
Sample : BSF0117S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 18 02:47:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

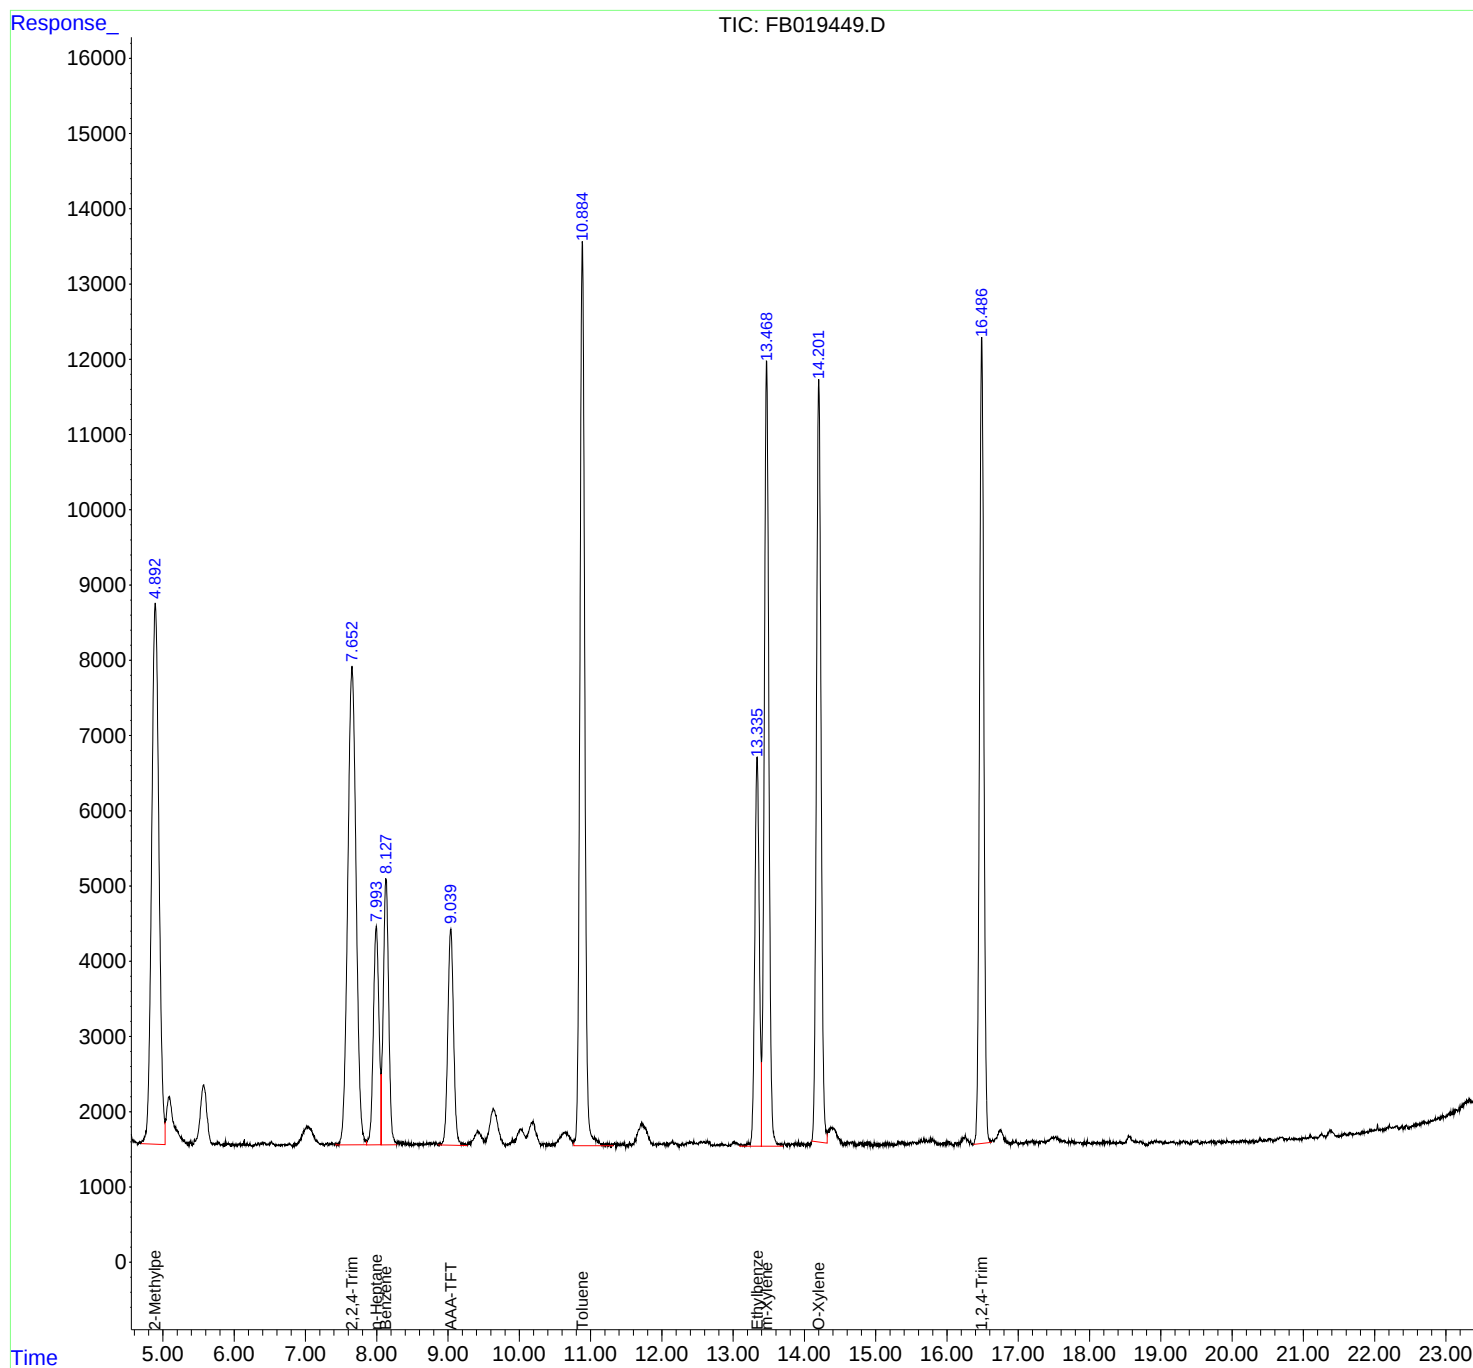

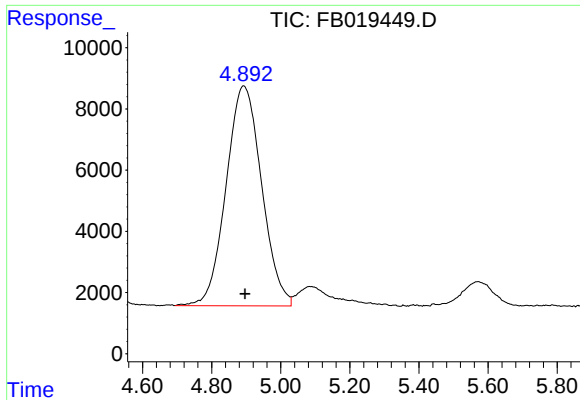


#1 2-Methylpentane

R.T.: 4.893 min
Delta R.T.: -0.004 min
Response: 513266
Conc: 25.77 ng/ml

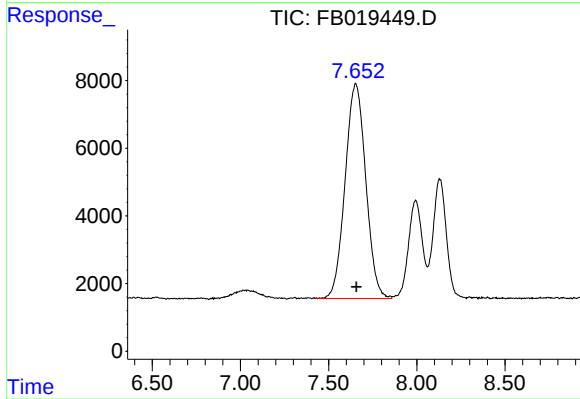


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.004 min
Response: 516308
Conc: 27.10 ng/ml

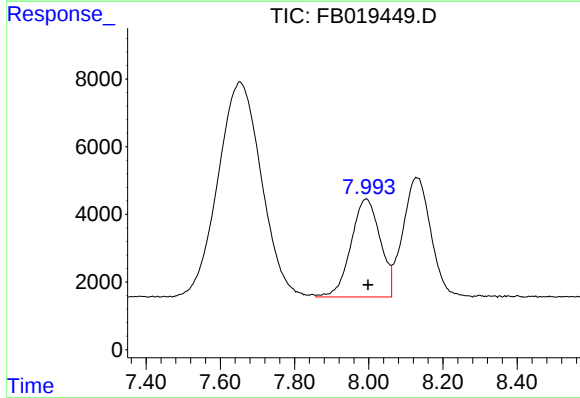


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: -0.005 min
Response: 158262
Conc: 9.07 ng/ml

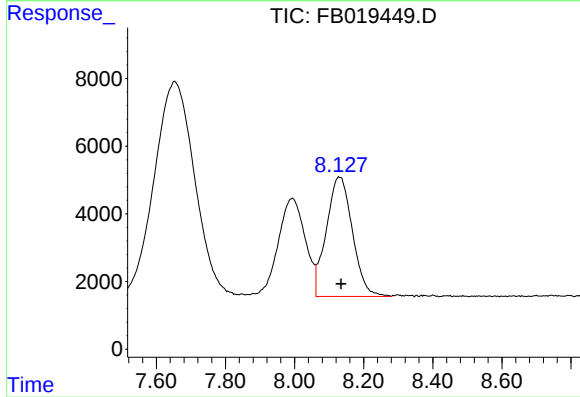


#4 Benzene

R.T.: 8.131 min
Delta R.T.: -0.005 min
Response: 185065
Conc: 9.42 ng/ml

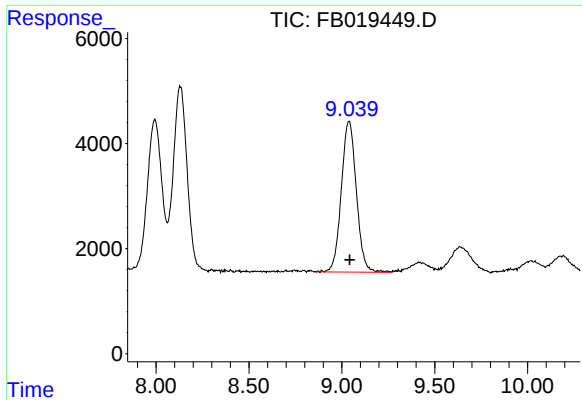


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: -0.005 min
Response: 161191
Conc: 18.14 ng/ml

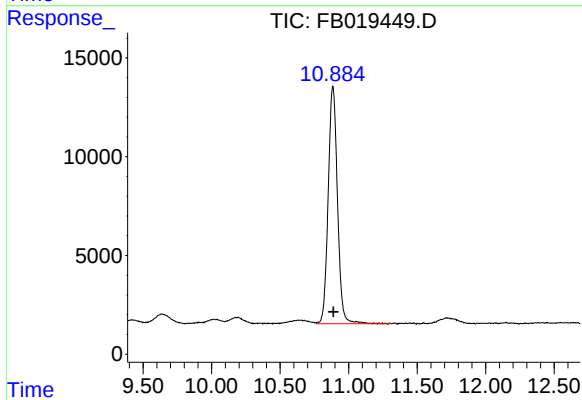


#6 Toluene

R.T.: 10.885 min
Delta R.T.: -0.005 min
Response: 566361
Conc: 31.31 ng/ml

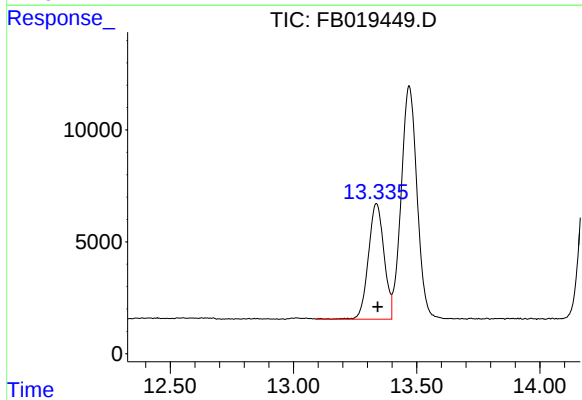


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: -0.005 min
Response: 228000
Conc: 10.29 ng/ml

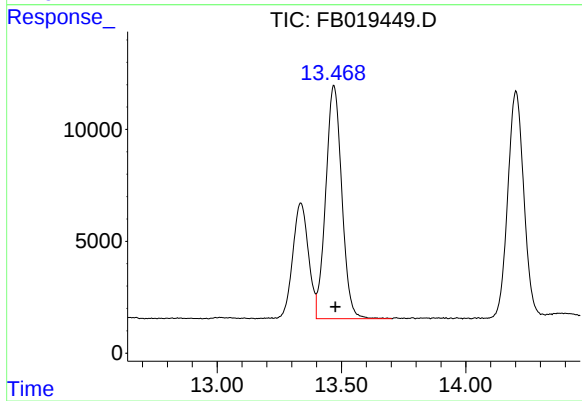


#8 m-Xylene

R.T.: 13.470 min
Delta R.T.: -0.006 min
Response: 468754
Conc: 20.43 ng/ml

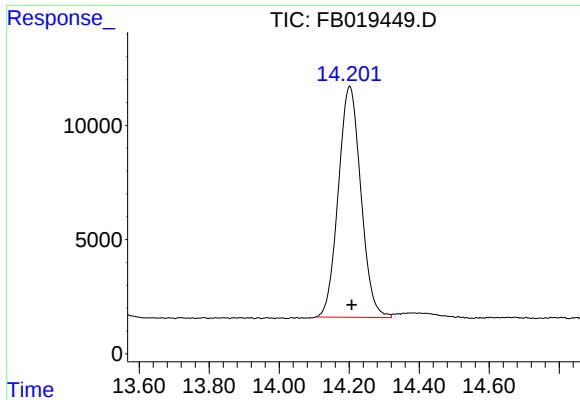

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: -0.006 min
Response: 451941
Conc: 20.14 ng/ml

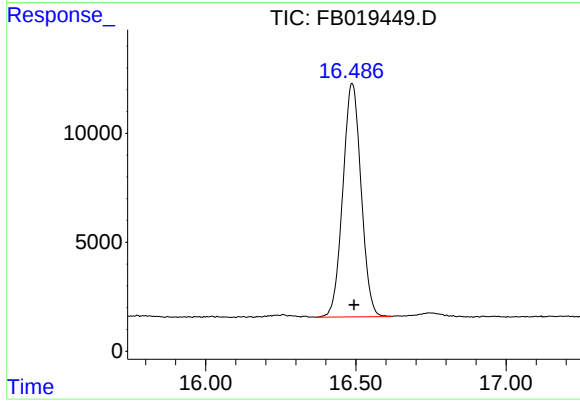

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.006 min
Response: 451703
Conc: 19.81 ng/ml