

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011719\
 Data File : FB019452.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2019 11:23
 Operator : MJ/SJ
 Sample : K1153-01MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 18 02:47:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	173382	19.512 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.895	443214	22.254 ng/ml
2) t 2,2,4-Trimethylpentane	7.654	433315	22.746 ng/ml
3) t n-Heptane	7.995	114954	6.588 ng/ml
4) t Benzene	8.132	179413	9.137 ng/ml
6) t Toluene	10.886	517892	28.630 ng/ml
7) t Ethylbenzene	13.338	205963	9.296 ng/ml
8) t m-Xylene	13.472	424558	18.500 ng/ml
9) t O-Xylene	14.203	420592	18.745 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	403234	17.684 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011719\
Data File : FB019452.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2019 11:23
Operator : MJ/SJ
Sample : K1153-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 18 02:47:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

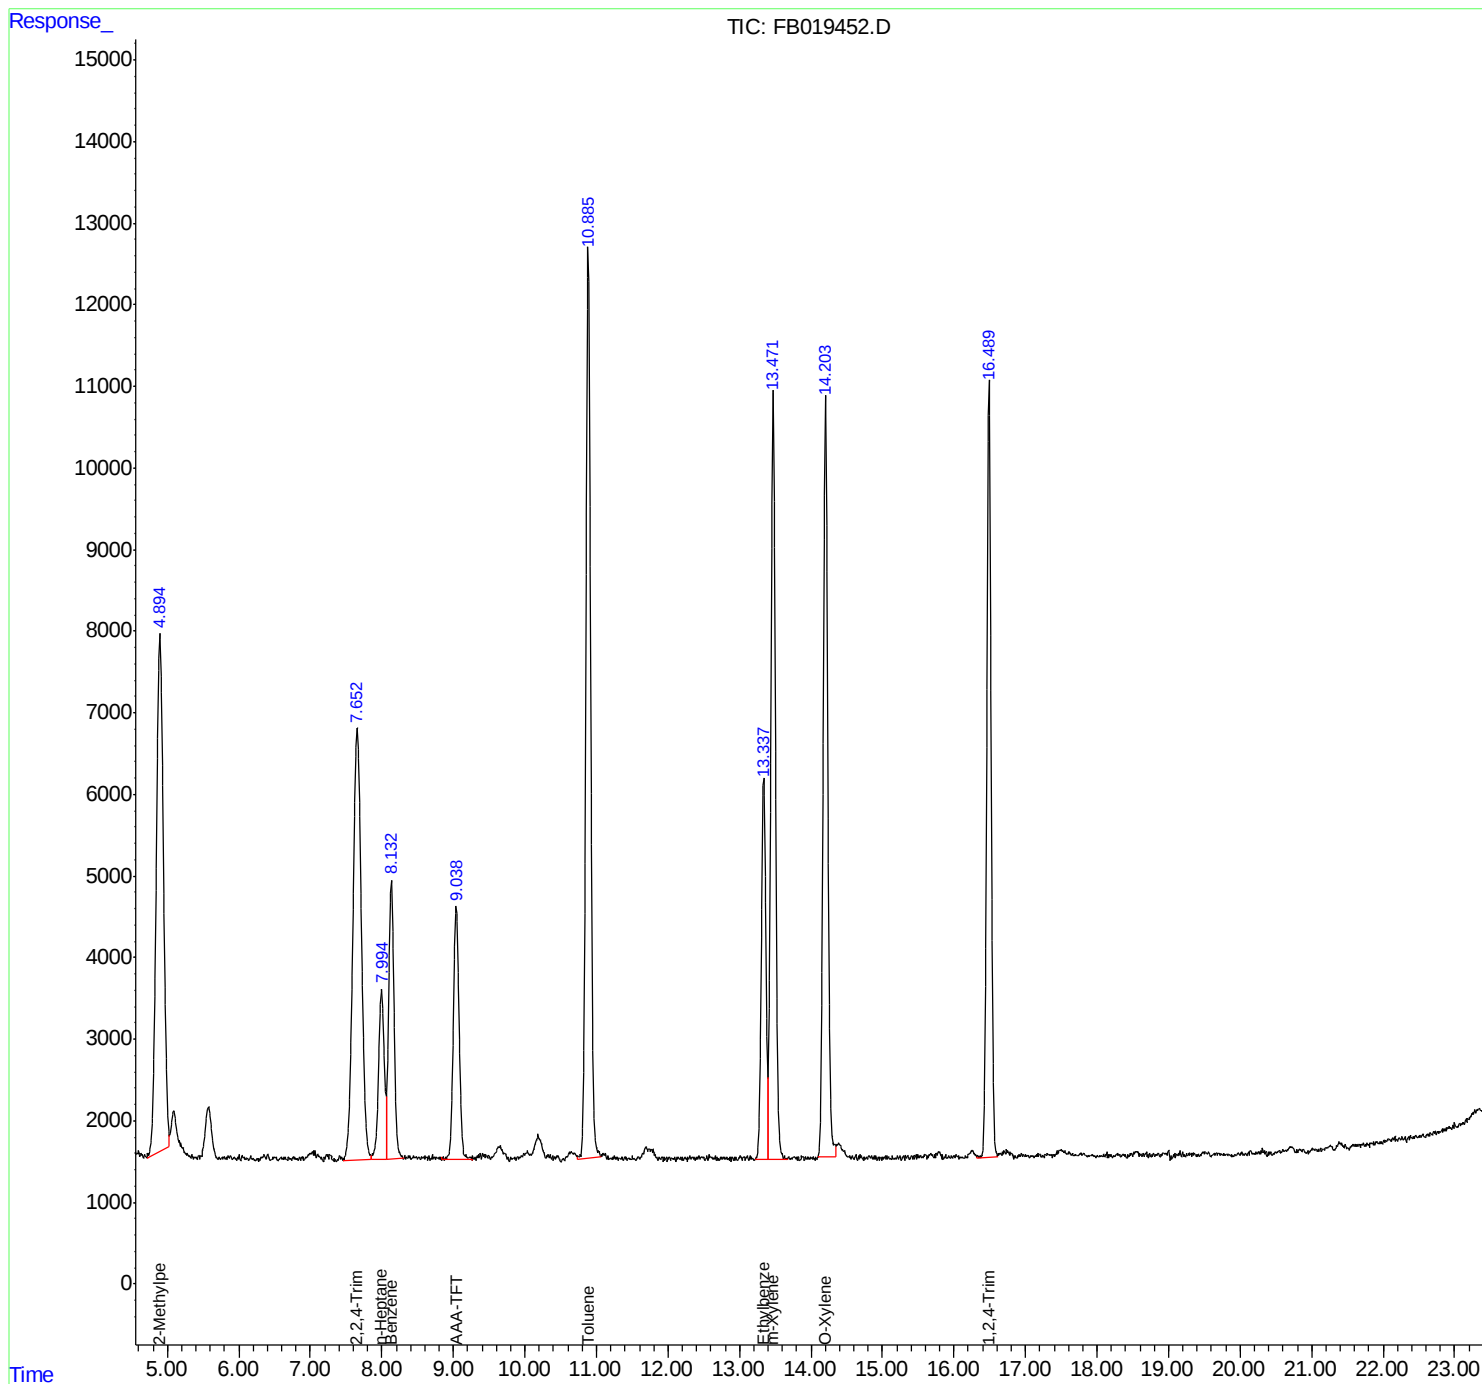

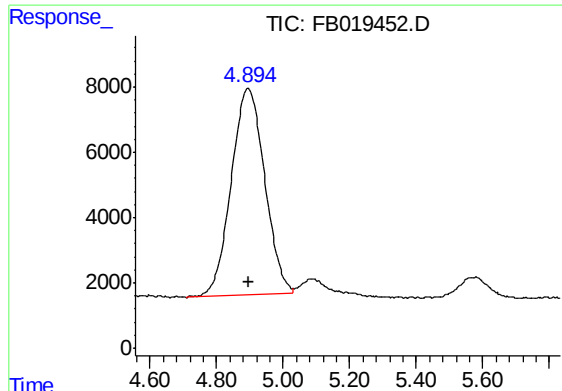


#1 2-Methylpentane

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 443214
Conc: 22.25 ng/ml

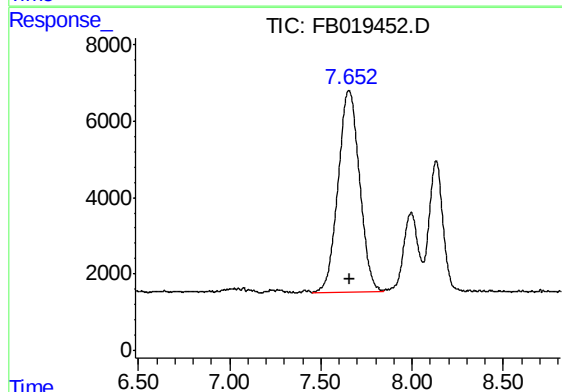


#2 2,2,4-Trimethylpentane

R.T.: 7.654 min
Delta R.T.: -0.004 min
Response: 433315
Conc: 22.75 ng/ml

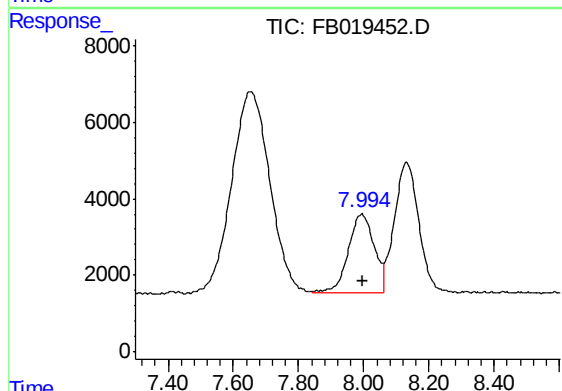


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: -0.004 min
Response: 114954
Conc: 6.59 ng/ml

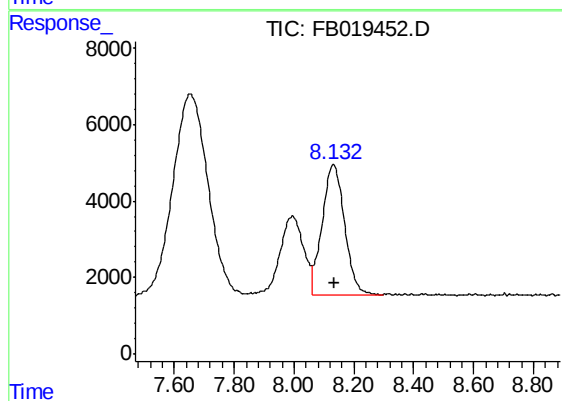


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.003 min
Response: 179413
Conc: 9.14 ng/ml

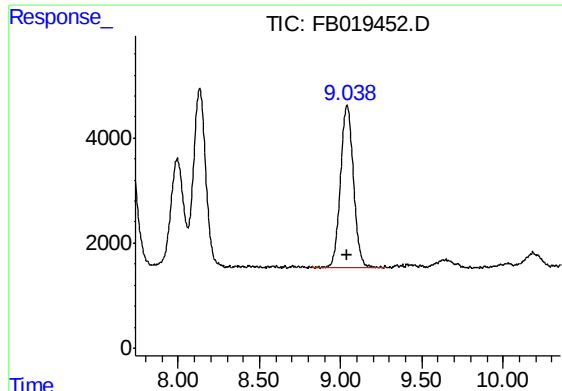


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: -0.004 min
Response: 173382
Conc: 19.51 ng/ml

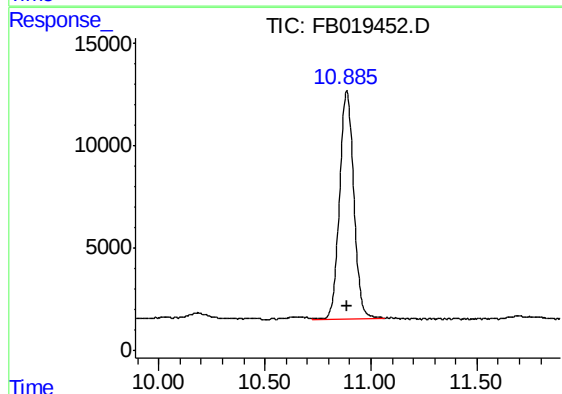


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.004 min
Response: 517892
Conc: 28.63 ng/ml

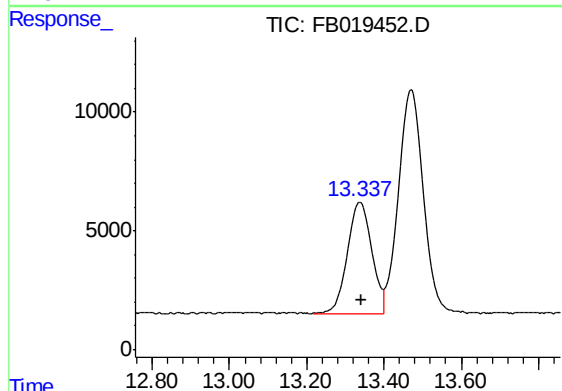


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.004 min
Response: 205963
Conc: 9.30 ng/ml

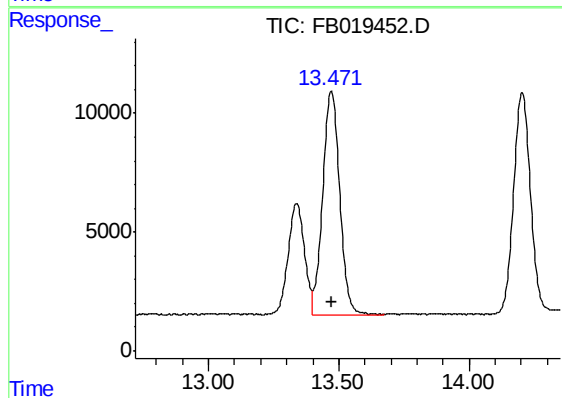


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.004 min
Response: 424558
Conc: 18.50 ng/ml

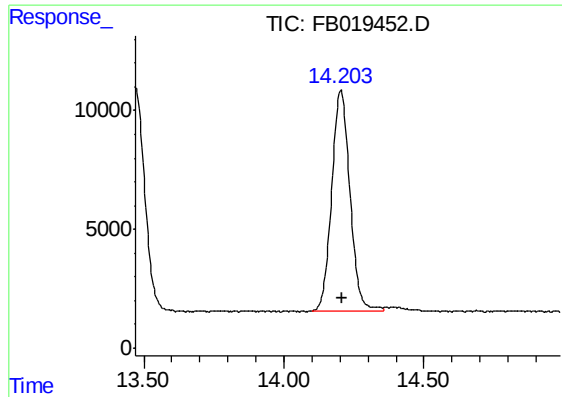

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.004 min
Response: 420592
Conc: 18.75 ng/ml

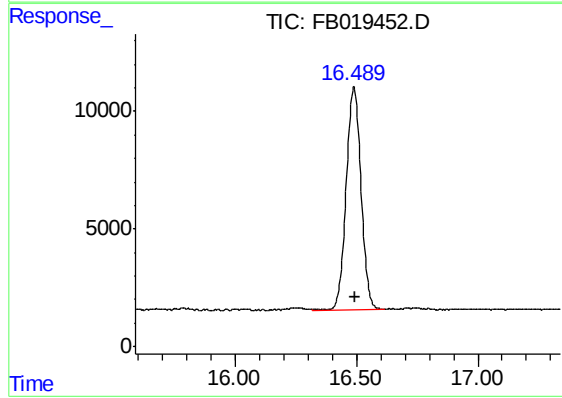

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: -0.004 min
Response: 403234
Conc: 17.68 ng/ml