

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011720\
 Data File : FB023451.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2020 12:34
 Operator : DD/AJ
 Sample : L1008-09MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 17 21:40:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	520303	21.904 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	937118	29.655 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	972011	28.628 ng/ml
3) t n-Heptane	7.751	322484	9.630 ng/ml
4) t Benzene	7.885	408927	10.013 ng/ml
6) t Toluene	10.623	1207270	30.550 ng/ml
7) t Ethylbenzene	13.063	374002	10.014 ng/ml
8) t m-Xylene	13.196	711023	19.995 ng/ml
9) t O-Xylene	13.924	686826	19.877 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	582009	19.904 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011720\
Data File : FB023451.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2020 12:34
Operator : DD/AJ
Sample : L1008-09MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 17 21:40:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

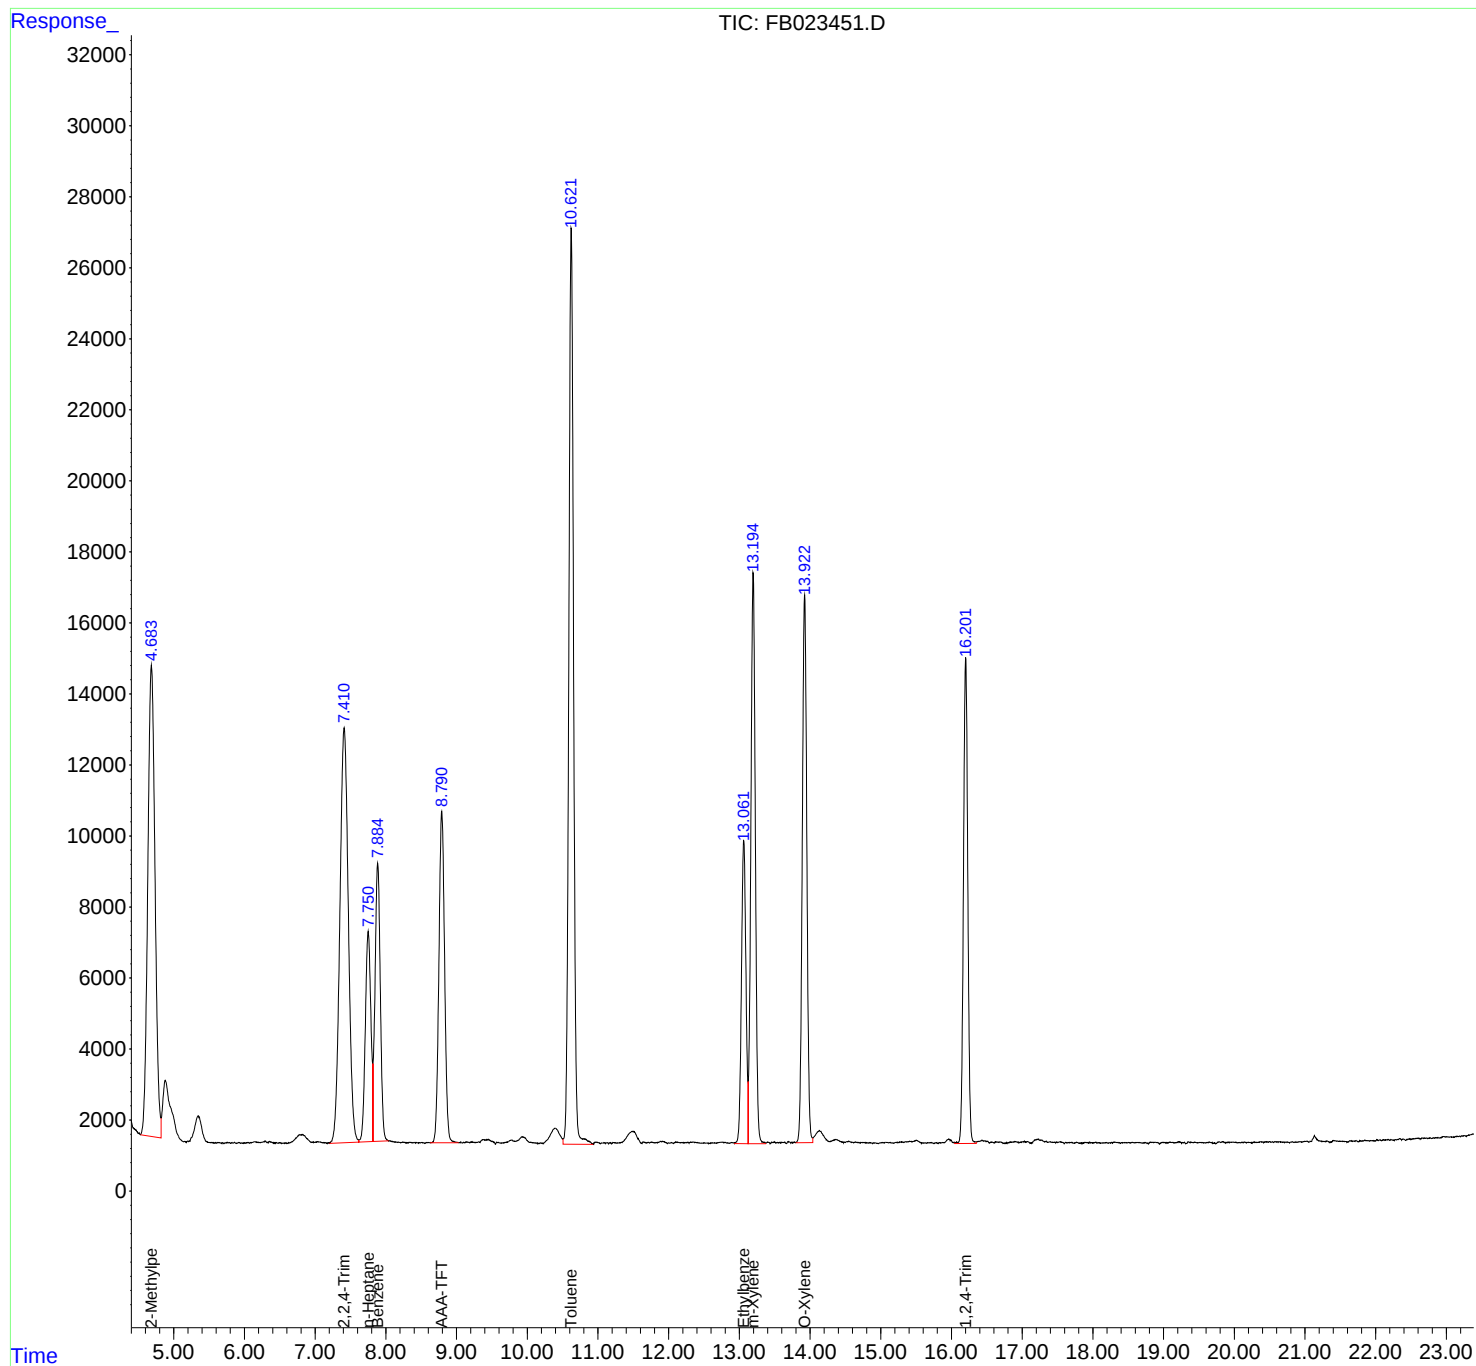

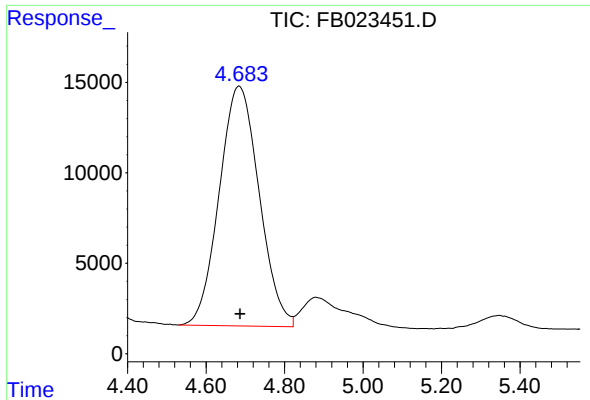


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: -0.003 min
Response: 937118
Conc: 29.65 ng/ml

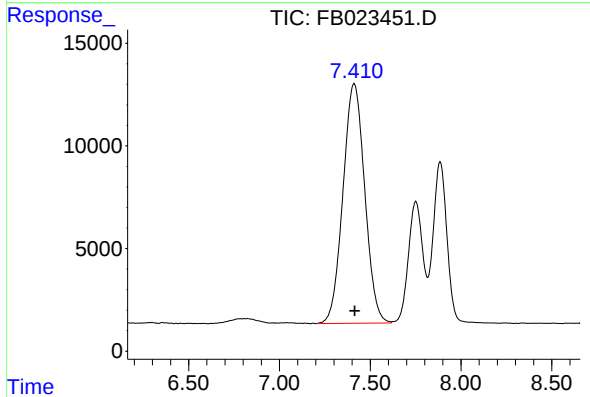


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.004 min
Response: 972011
Conc: 28.63 ng/ml

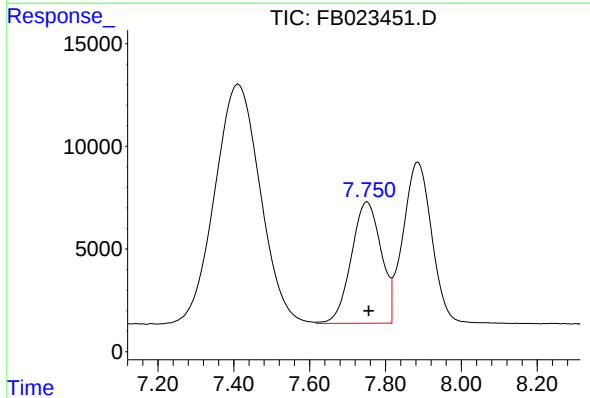


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 322484
Conc: 9.63 ng/ml

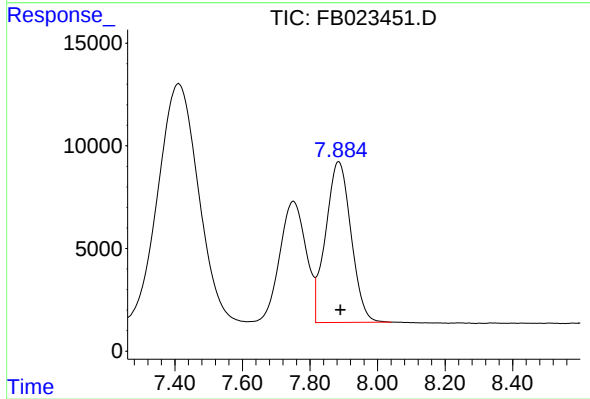


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.004 min
Response: 408927
Conc: 10.01 ng/ml

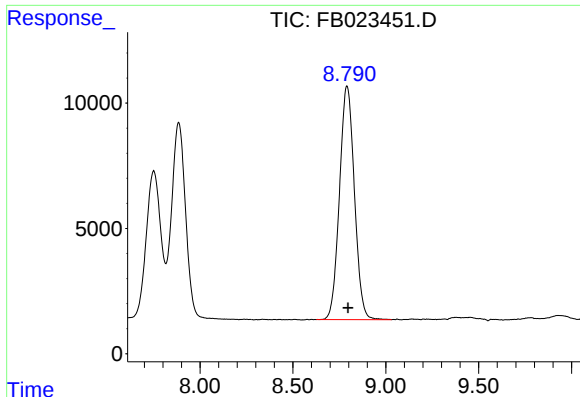


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.005 min
Response: 520303
Conc: 21.90 ng/ml

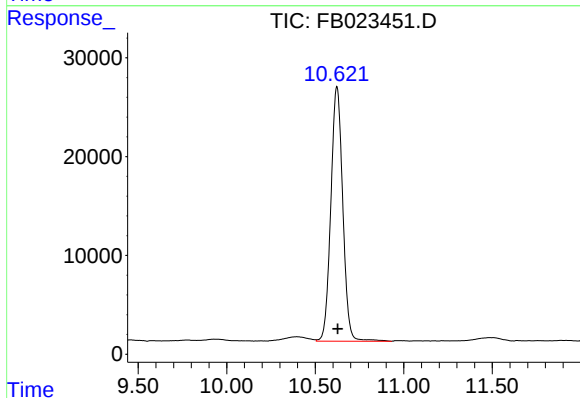


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 1207270
Conc: 30.55 ng/ml

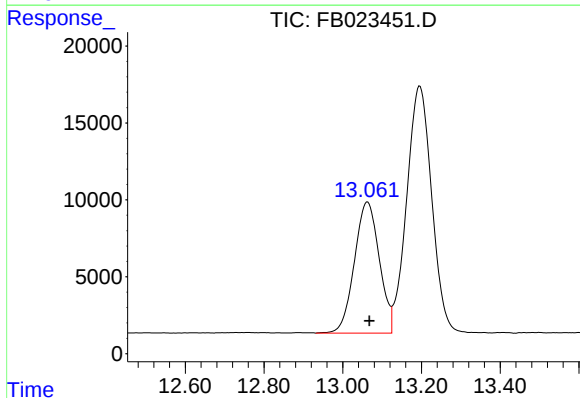


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.005 min
Response: 374002
Conc: 10.01 ng/ml

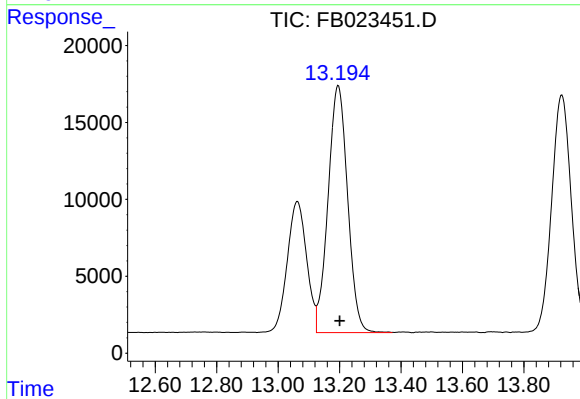


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.005 min
Response: 711023
Conc: 19.99 ng/ml

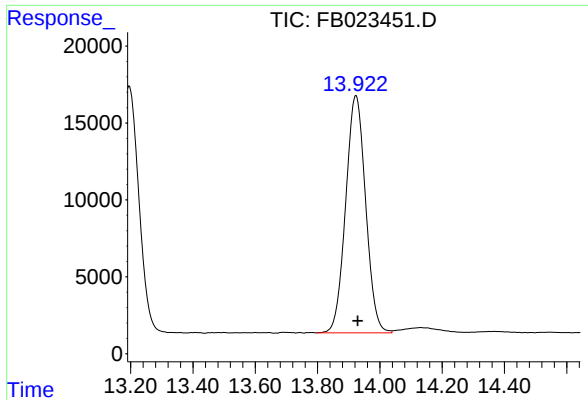

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.005 min
Response: 686826
Conc: 19.88 ng/ml

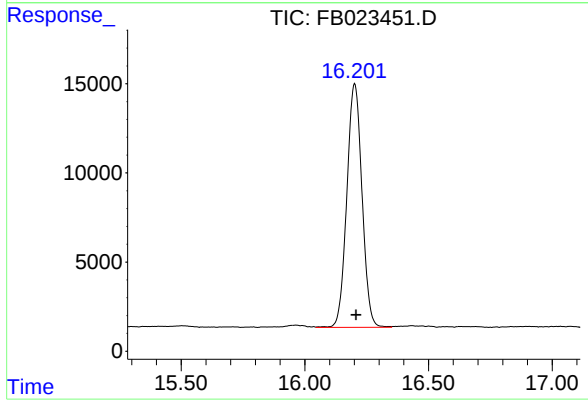

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 582009
Conc: 19.90 ng/ml