

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011720\
 Data File : FB023452.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2020 13:04
 Operator : DD/AJ
 Sample : L1008-09MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 17 21:40:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
 Quant Title :
 QLast Update : Thu Jan 16 11:42:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	541960	22.816 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	954633	30.209 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	988487	29.113 ng/ml
3) t n-Heptane	7.751	325494	9.720 ng/ml
4) t Benzene	7.886	416411	10.197 ng/ml
6) t Toluene	10.623	1216216	30.776 ng/ml
7) t Ethylbenzene	13.063	385749	10.328 ng/ml
8) t m-Xylene	13.196	736127	20.700 ng/ml
9) t O-Xylene	13.924	707777	20.483 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	591749	20.237 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011720\
Data File : FB023452.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2020 13:04
Operator : DD/AJ
Sample : L1008-09MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 17 21:40:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011620.M
Quant Title :
QLast Update : Thu Jan 16 11:42:55 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

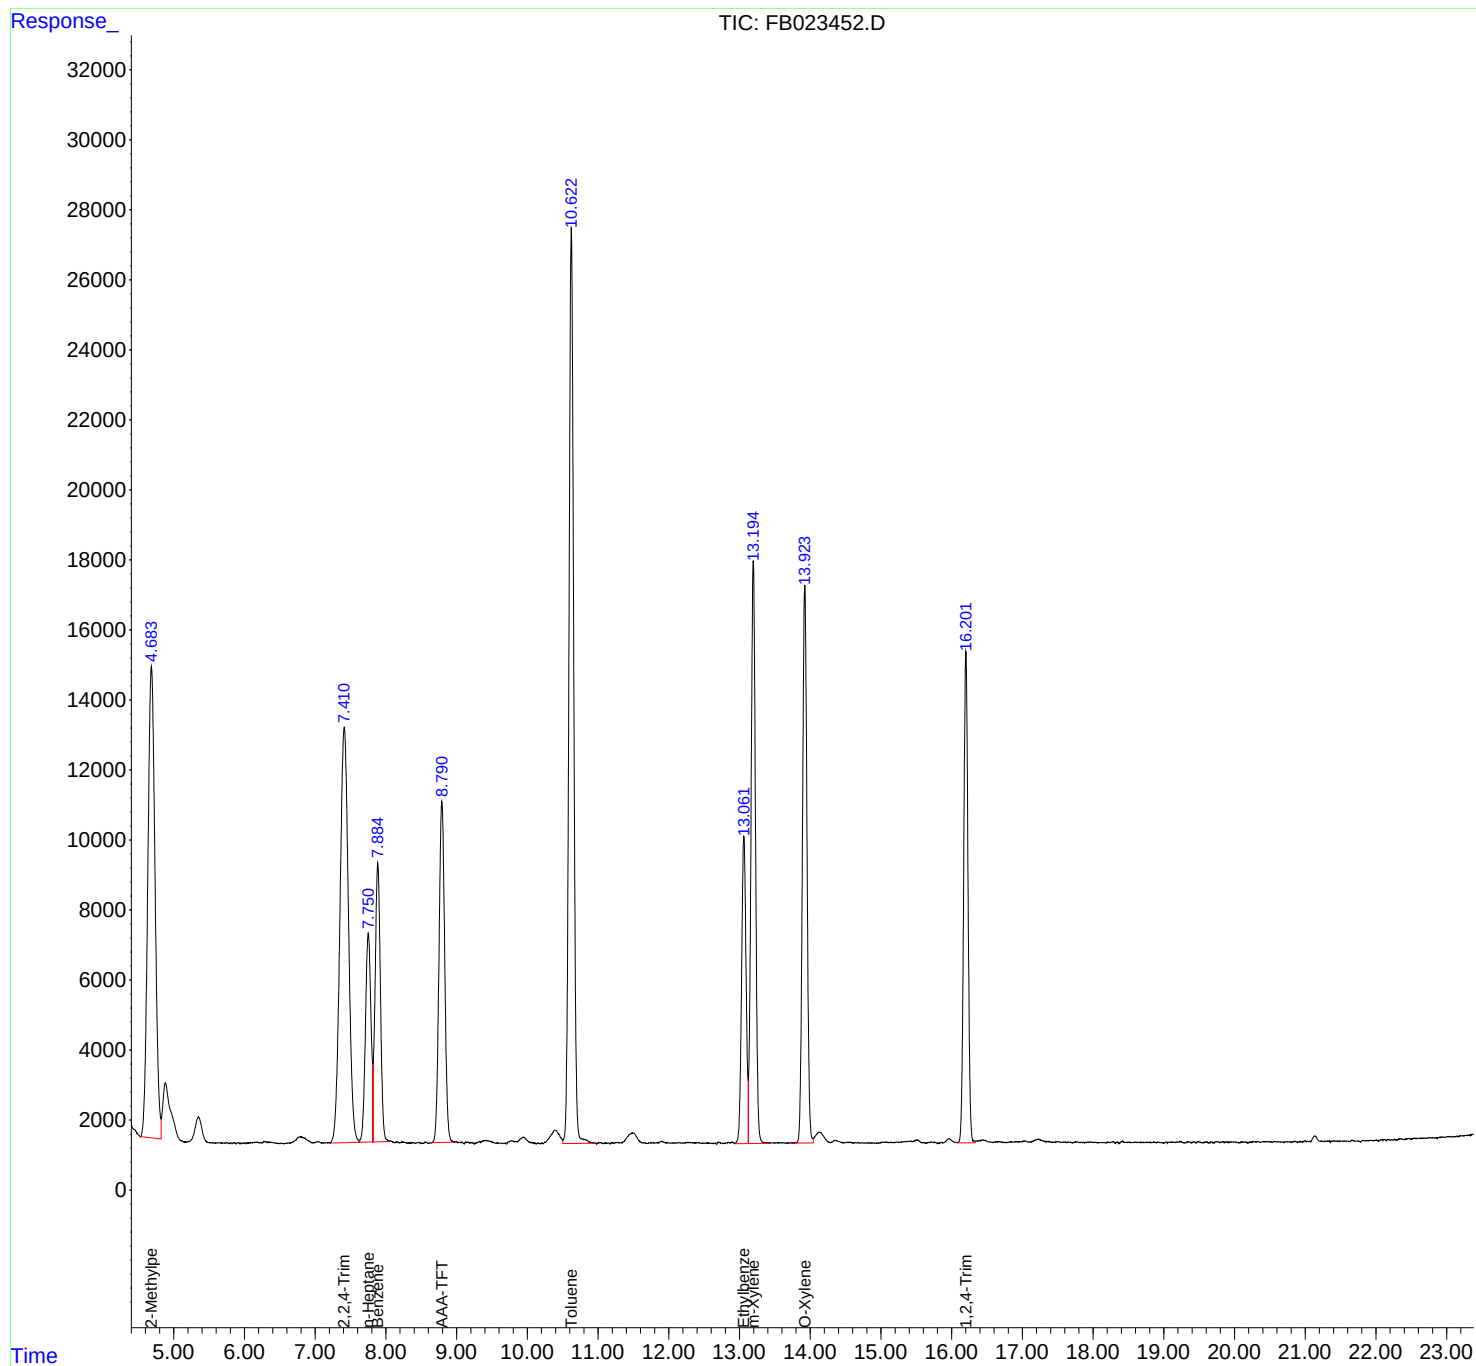

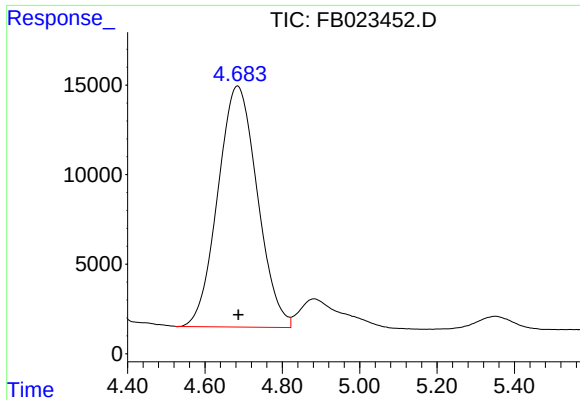


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: -0.002 min
Response: 954633
Conc: 30.21 ng/ml

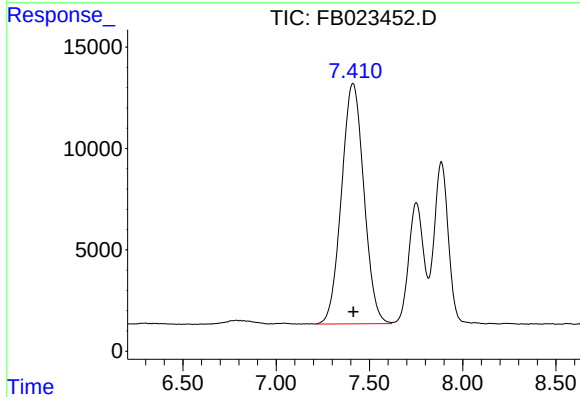


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.004 min
Response: 988487
Conc: 29.11 ng/ml

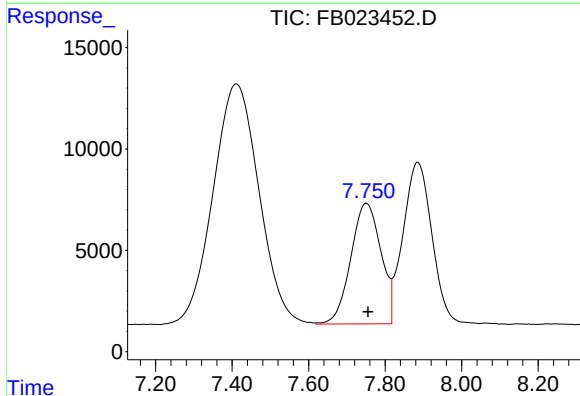


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.004 min
Response: 325494
Conc: 9.72 ng/ml

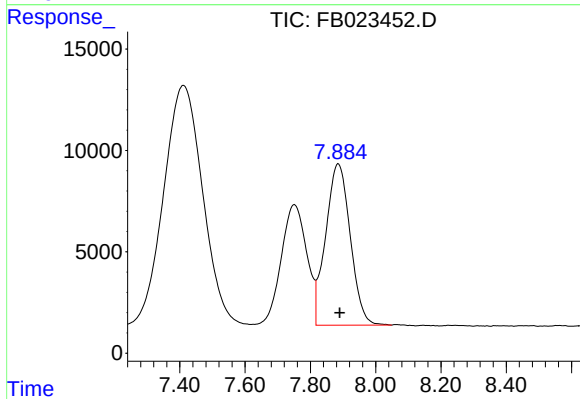


#4 Benzene

R.T.: 7.886 min
Delta R.T.: -0.004 min
Response: 416411
Conc: 10.20 ng/ml

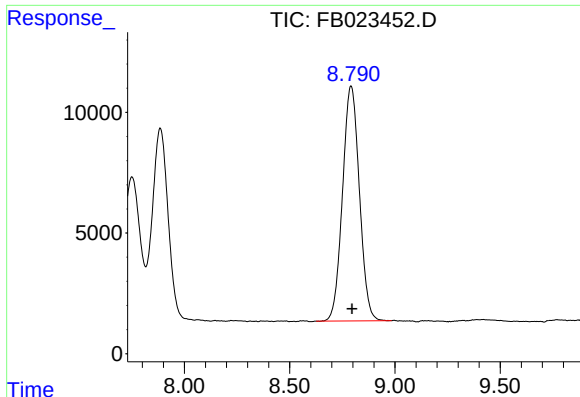


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.005 min
Response: 541960
Conc: 22.82 ng/ml

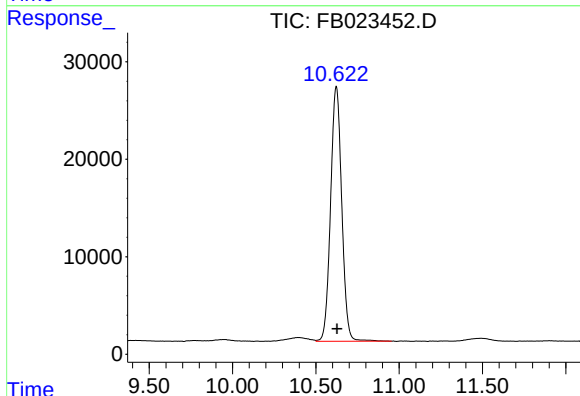


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.005 min
Response: 1216216
Conc: 30.78 ng/ml

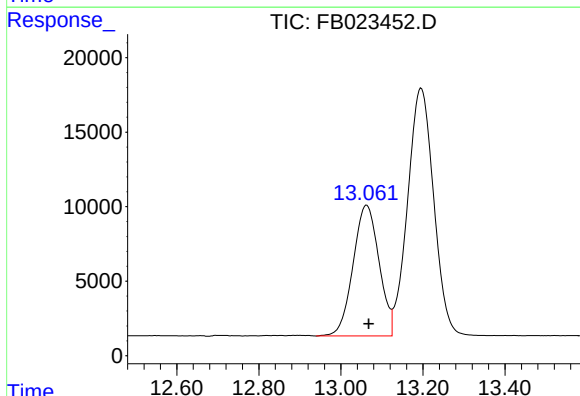


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: -0.005 min
Response: 385749
Conc: 10.33 ng/ml

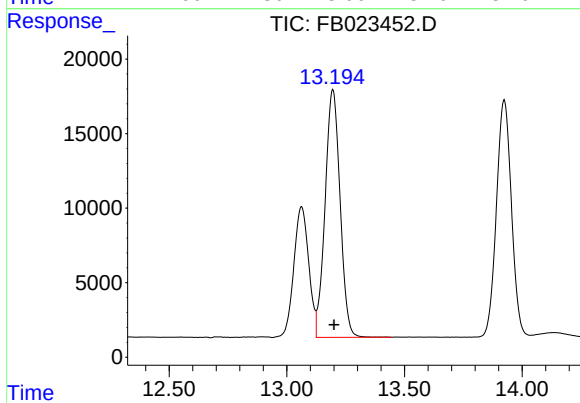


#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.005 min
Response: 736127
Conc: 20.70 ng/ml

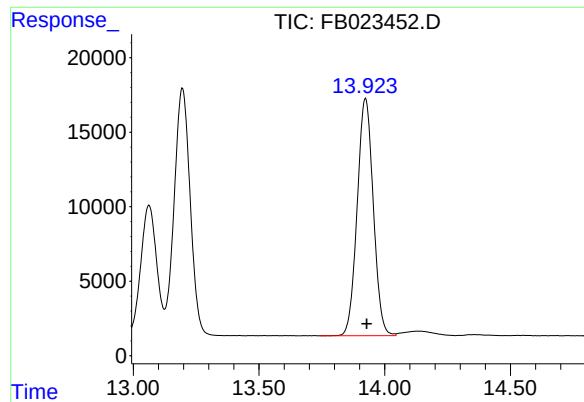

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: -0.005 min
Response: 707777
Conc: 20.48 ng/ml

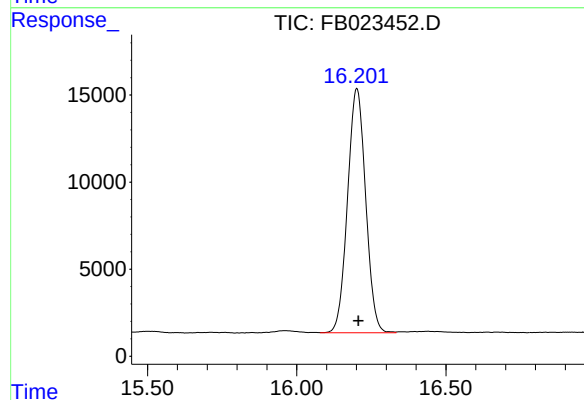

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: -0.005 min
Response: 591749
Conc: 20.24 ng/ml