

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011723\
 Data File : FB029117.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2023 10:30
 Operator : AJ/MA
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jan 17 10:39:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 10:39:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	270400	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	489452	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	536752	30.000 ng/ml
3) t n-Heptane	7.748	183446	10.000 ng/ml
4) t Benzene	7.885	221809	10.000 ng/ml
6) t Toluene	10.618	645260	30.000 ng/ml
7) t Ethylbenzene	13.054	199306	10.000 ng/ml
8) t m-Xylene	13.187	395702	20.000 ng/ml
9) t O-Xylene	13.914	385951	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	384435	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011723\
Data File : FB029117.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2023 10:30
Operator : AJ/MA
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 17 10:39:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 10:39:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

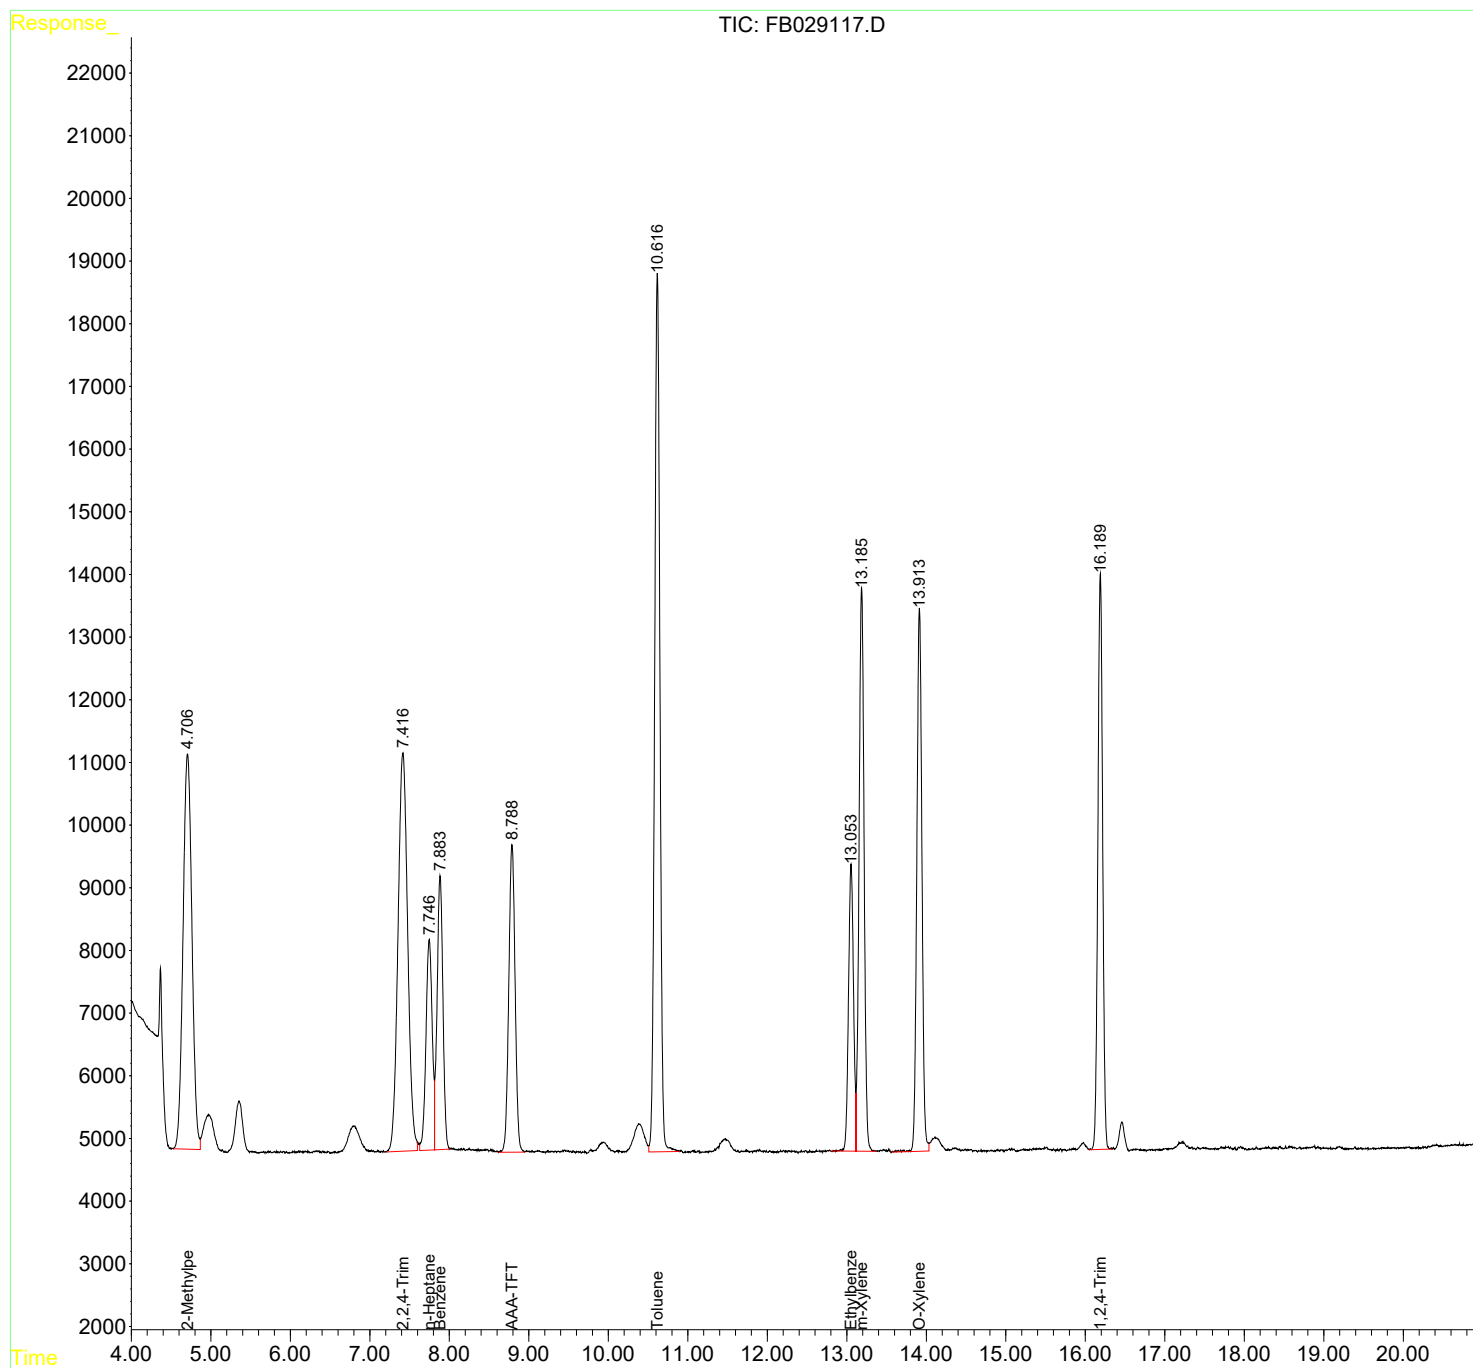


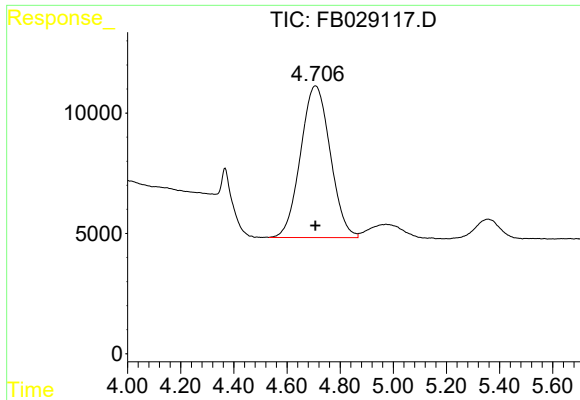

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 489452
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

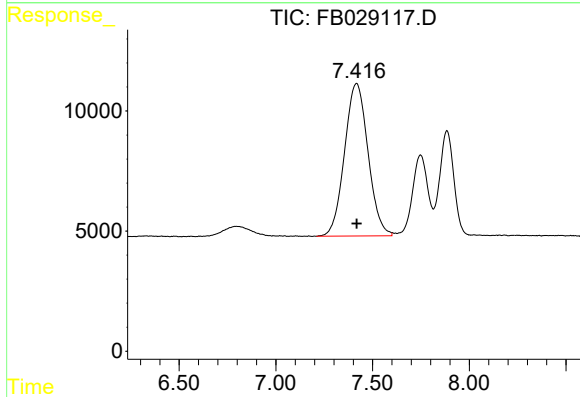


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 536752
Conc: 30.00 ng/ml

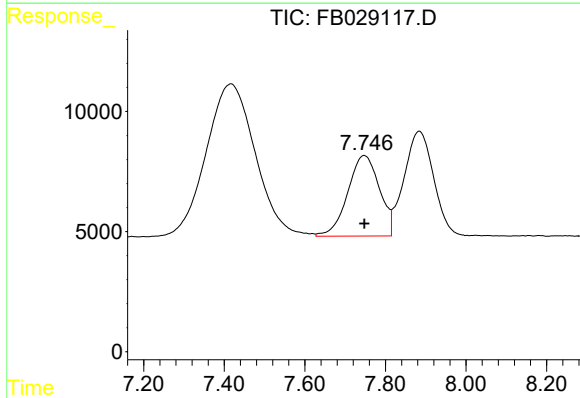


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 183446
Conc: 10.00 ng/ml

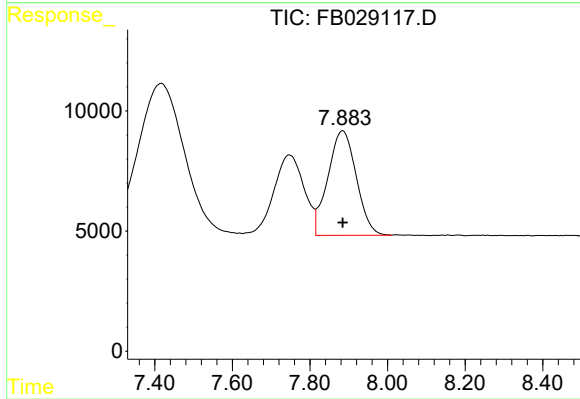

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 221809
Conc: 10.00 ng/ml

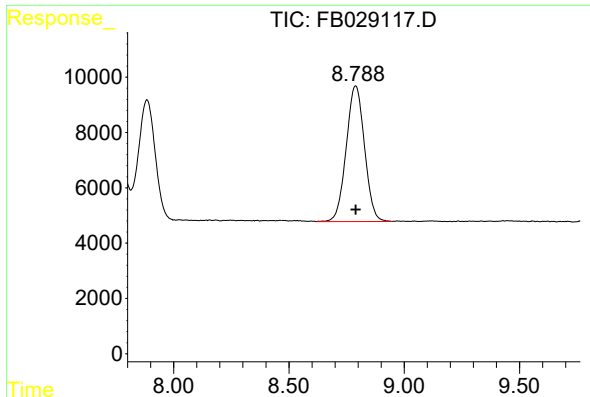

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 270400
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

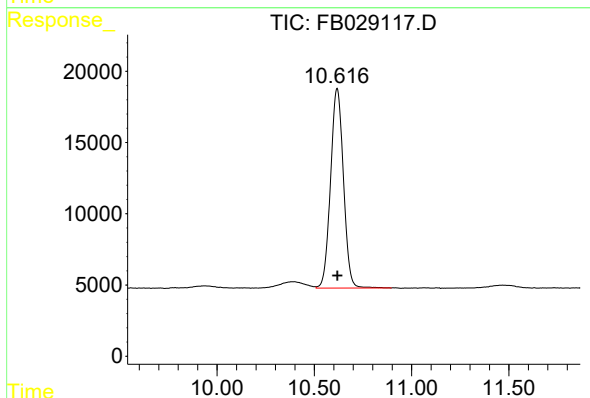


#6 Toluene

R.T.: 10.618 min
Delta R.T.: 0.000 min
Response: 645260
Conc: 30.00 ng/ml

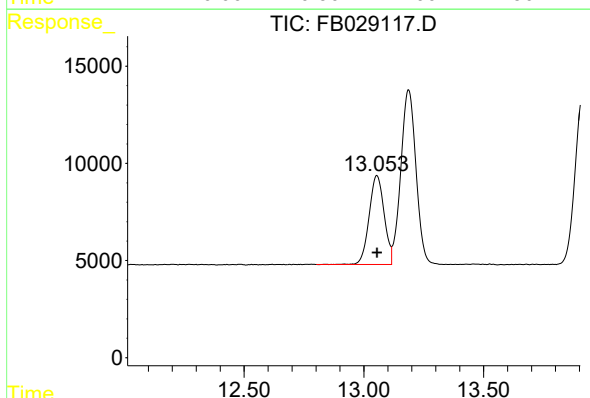


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: 0.000 min
Response: 199306
Conc: 10.00 ng/ml

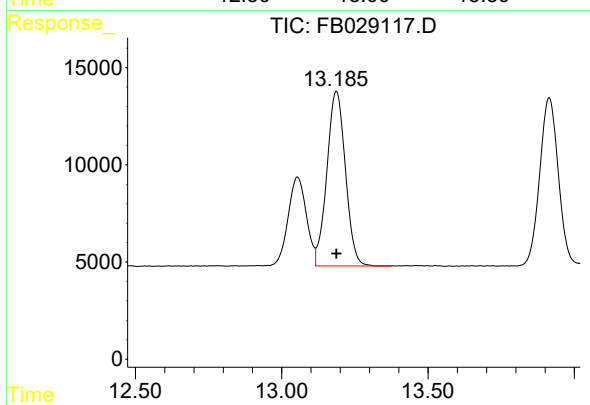

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: 0.000 min
Response: 395702
Conc: 20.00 ng/ml

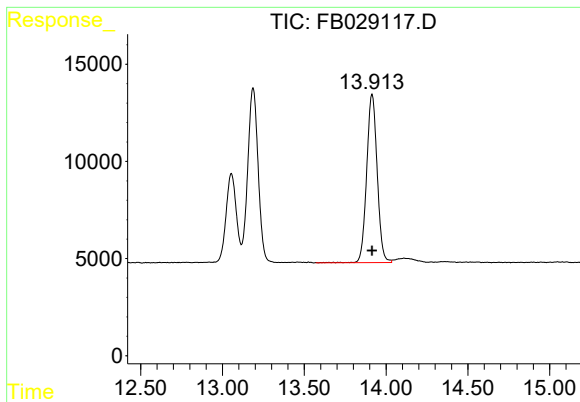

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: 0.000 min
Response: 385951
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

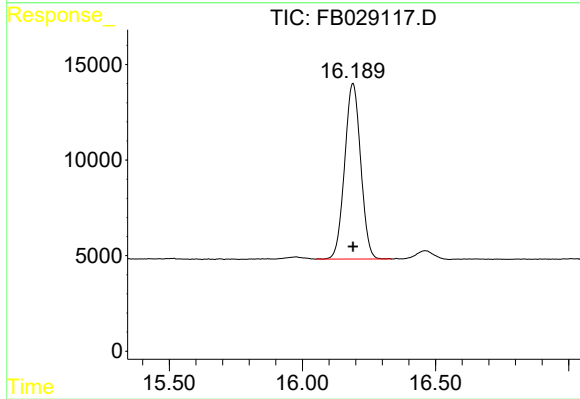

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: 0.000 min
Response: 384435
Conc: 20.00 ng/ml