

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011723\
 Data File : FB029115.D
 Signal(s) : FID2B.CH
 Acq On : 17 Jan 2023 9:03
 Operator : AJ/MA
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Jan 17 10:41:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
 Quant Title :
 QLast Update : Tue Jan 17 10:39:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	47910	3.544 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	81869	5.018 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	86066	4.810 ng/ml
3) t n-Heptane	7.743	30486	1.662 ng/ml
4) t Benzene	7.882	44721	2.016 ng/ml
6) t Toluene	10.615	115822	5.385 ng/ml
7) t Ethylbenzene	13.049	40869	2.051 ng/ml
8) t m-Xylene	13.183	75813	3.832 ng/ml
9) t O-Xylene	13.911	71353	3.697 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	75990	3.953 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011723\
Data File : FB029115.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2023 9:03
Operator : AJ/MA
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Jan 17 10:41:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011723.M
Quant Title :
QLast Update : Tue Jan 17 10:39:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

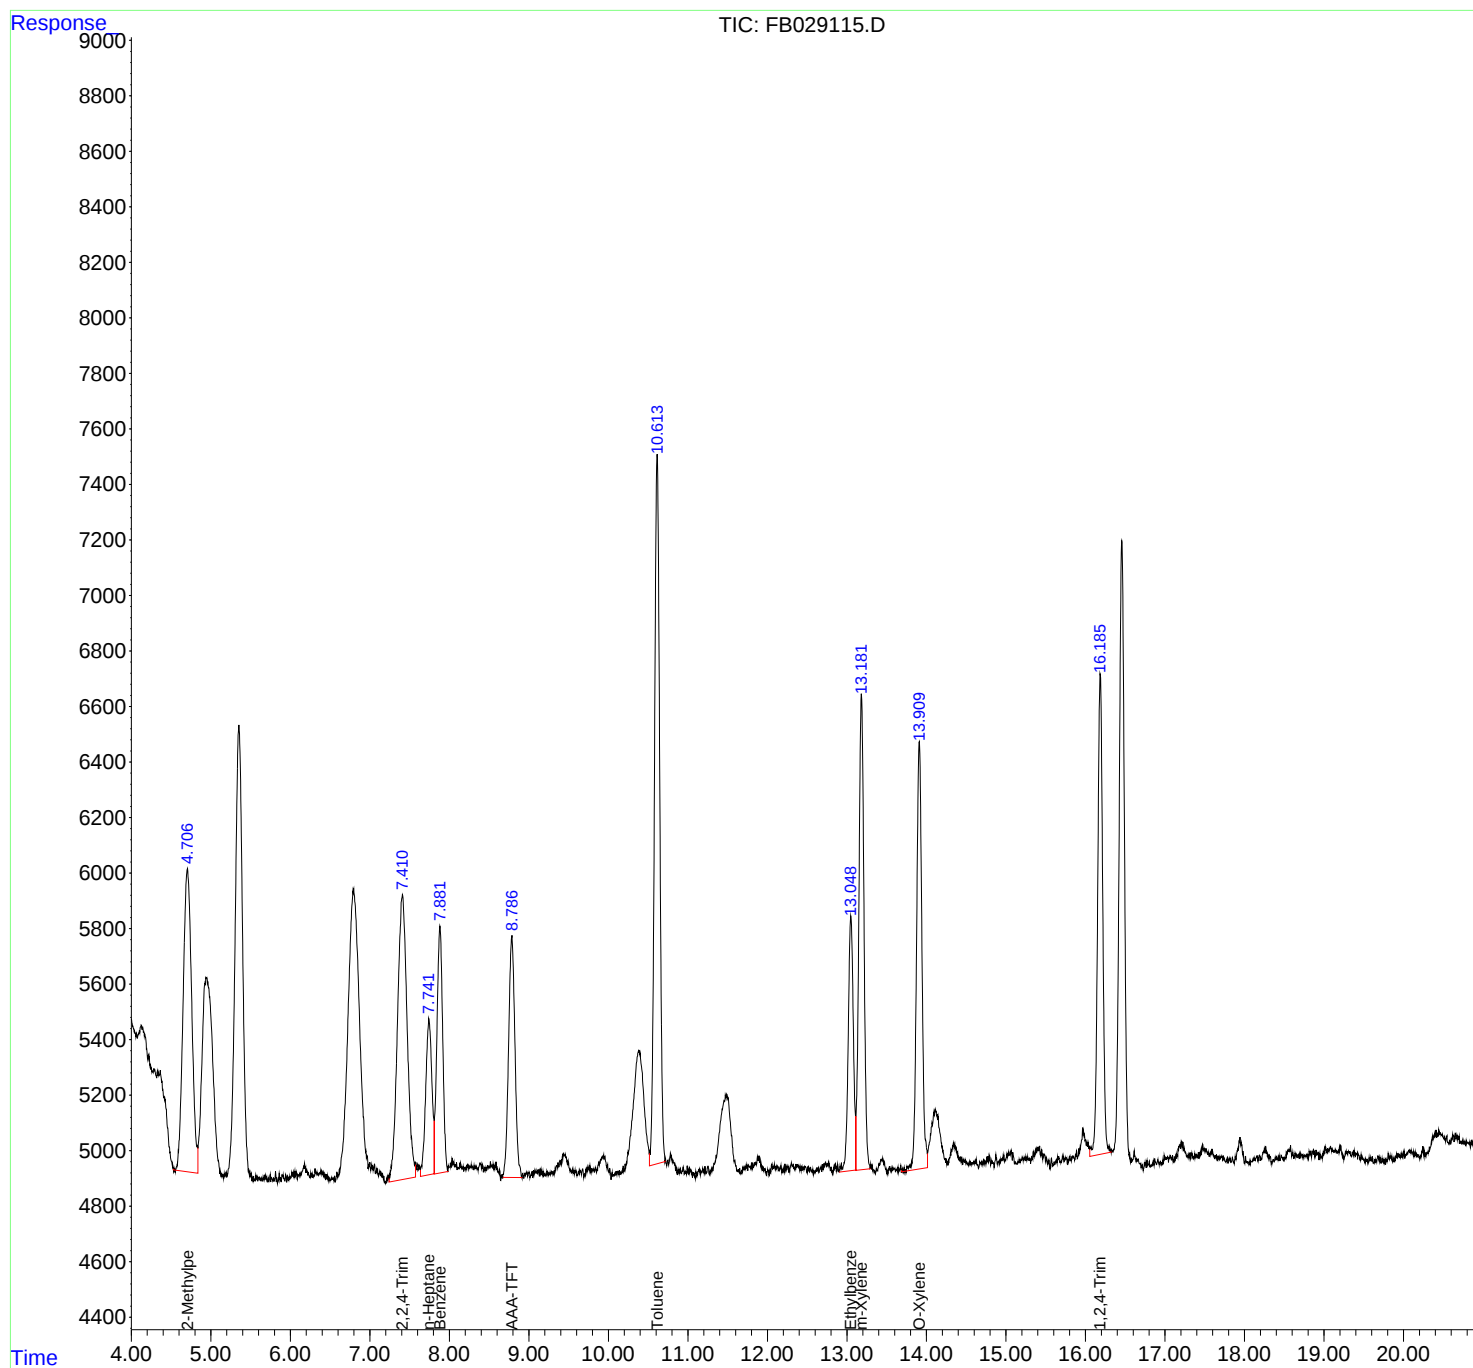


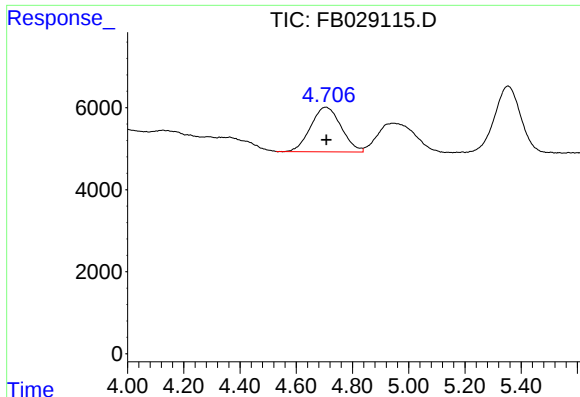

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 81869
Conc: 5.02 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

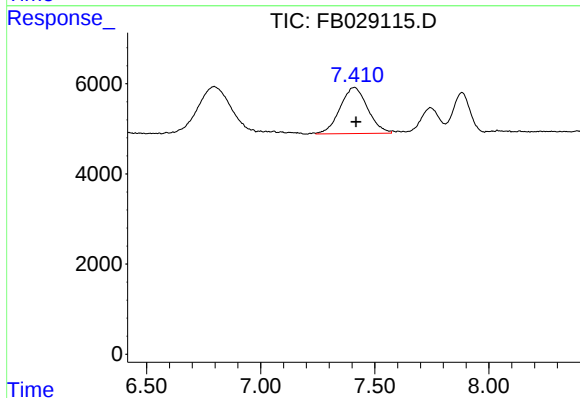


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.006 min
Response: 86066
Conc: 4.81 ng/ml

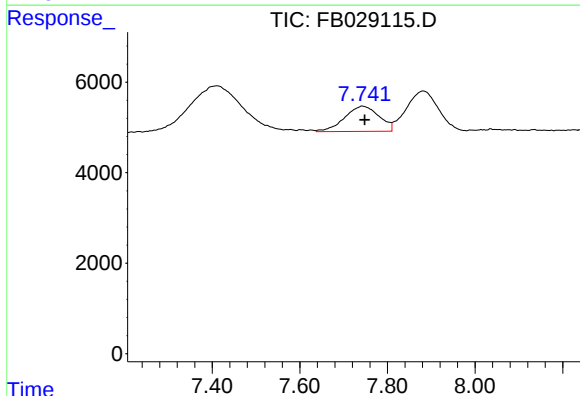


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.005 min
Response: 30486
Conc: 1.66 ng/ml

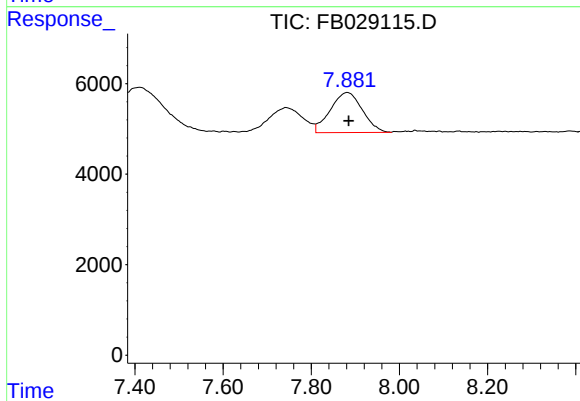

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.002 min
Response: 44721
Conc: 2.02 ng/ml

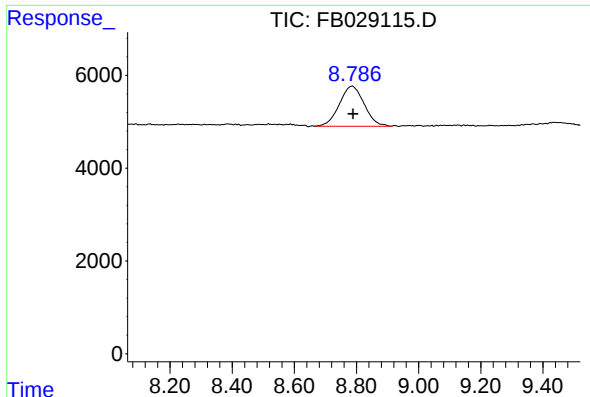

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.002 min
Response: 47910
Conc: 3.54 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

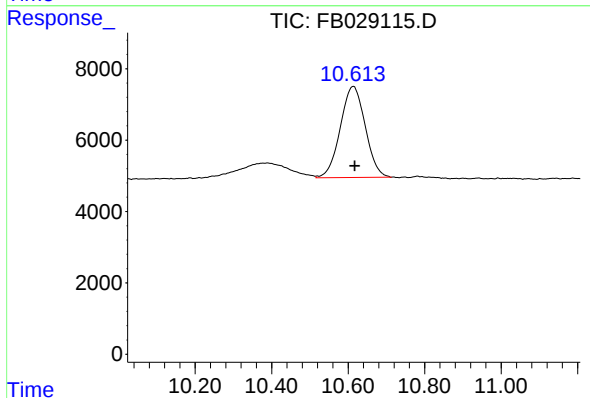


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.003 min
Response: 115822
Conc: 5.38 ng/ml

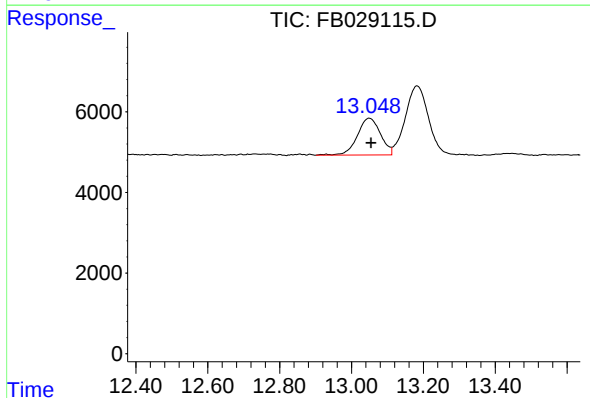


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.005 min
Response: 40869
Conc: 2.05 ng/ml

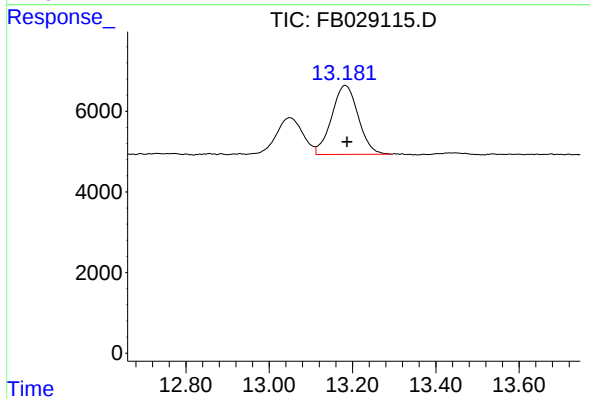

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.004 min
Response: 75813
Conc: 3.83 ng/ml

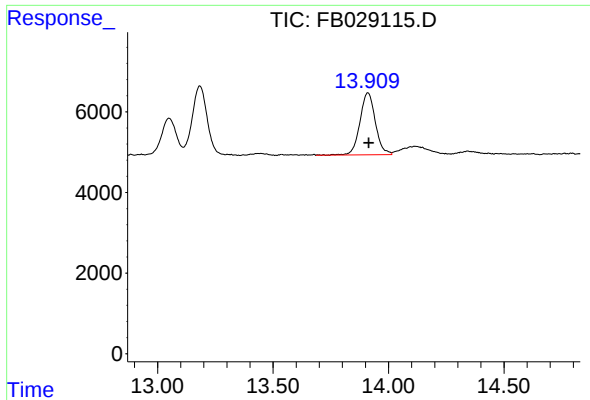

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.003 min
Response: 71353
Conc: 3.70 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

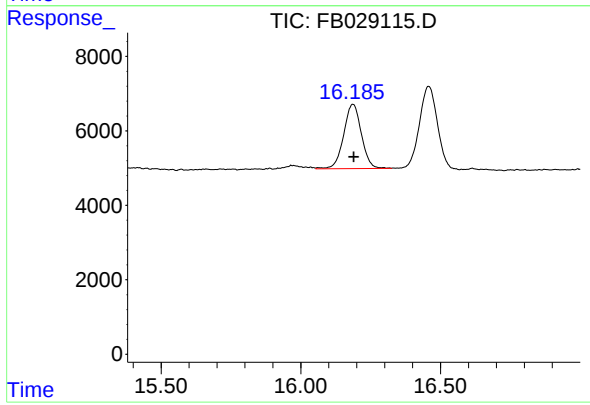

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.003 min
Response: 75990
Conc: 3.95 ng/ml