

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011725\
Data File : FB031314.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2025 9:35
Operator : YP/AJ
Sample : VBF0117W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 18 01:27:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	440337	18.461 ng/ml
Target Compounds			
6) t Toluene	10.605	4487	0.115 ng/ml
8) t m-Xylene	13.188	5295	0.142 ng/ml
9) t O-Xylene	13.918	6604	0.185 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	12416	0.438 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011725\
Data File : FB031314.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2025 9:35
Operator : YP/AJ
Sample : VBF0117W1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 18 01:27:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

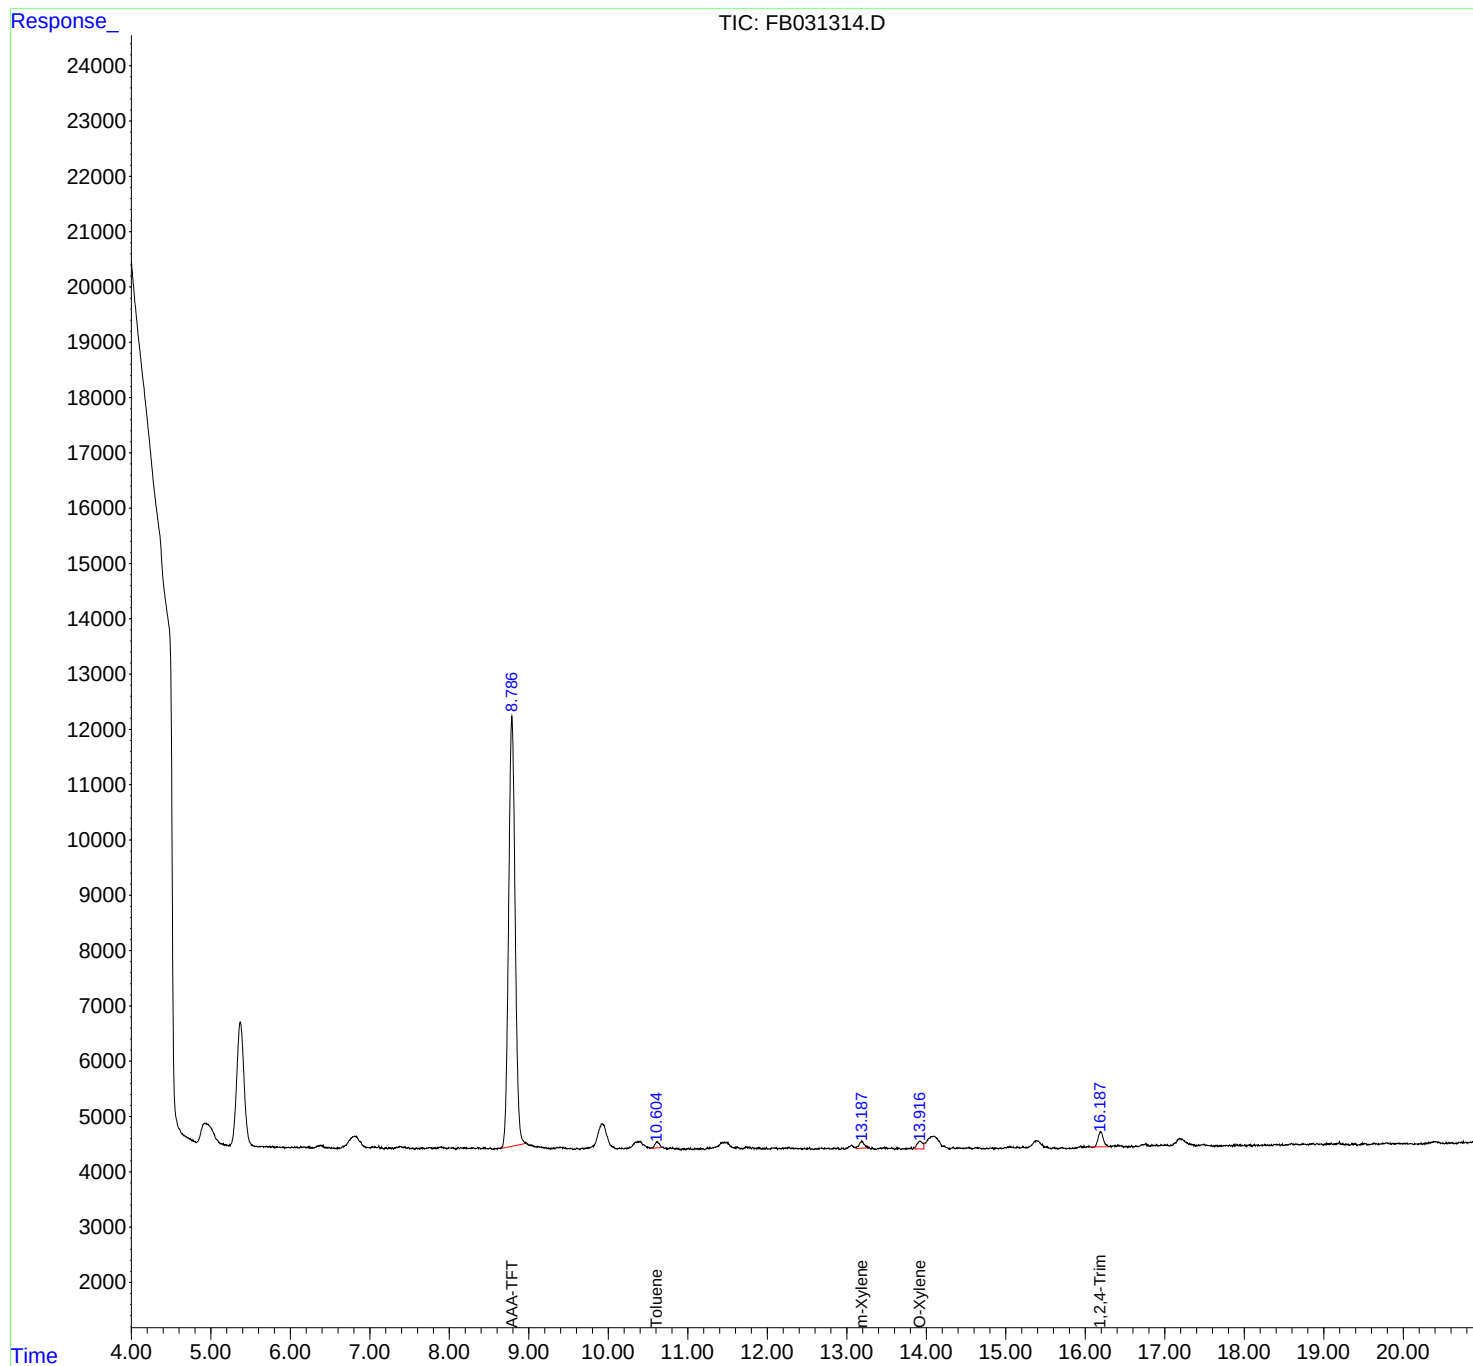


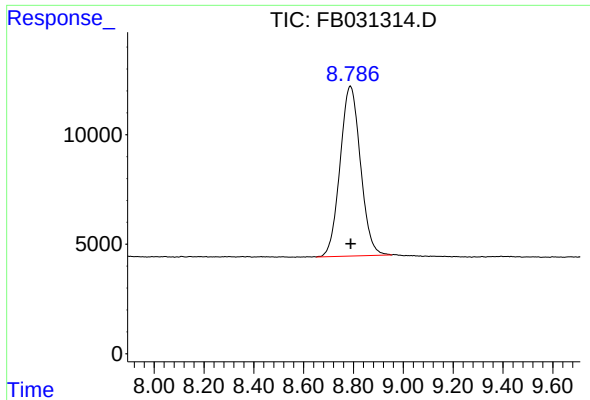

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.002 min
Response: 440337
Conc: 18.46 ng/ml

Instrument :
FID_B
ClientSampleId :

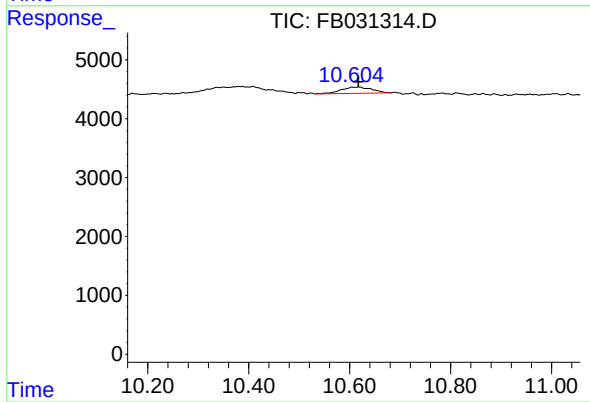


#6 Toluene

R.T.: 10.605 min
Delta R.T.: -0.012 min
Response: 4487
Conc: 0.11 ng/ml

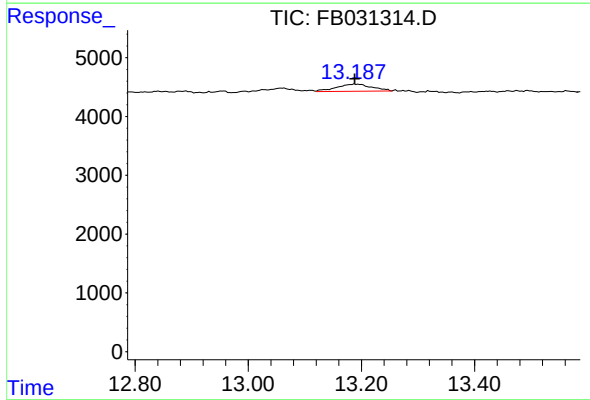


#8 m-Xylene

R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 5295
Conc: 0.14 ng/ml

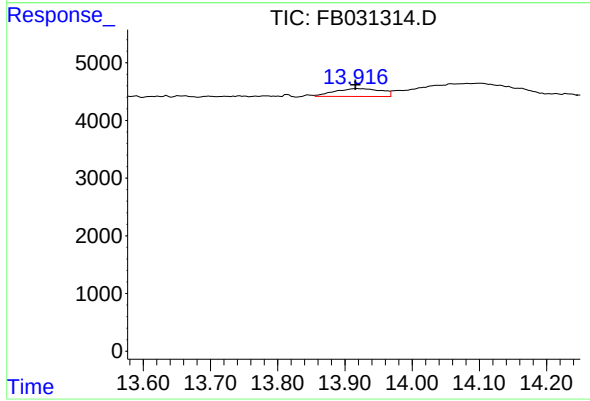

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.003 min
Response: 6604
Conc: 0.19 ng/ml

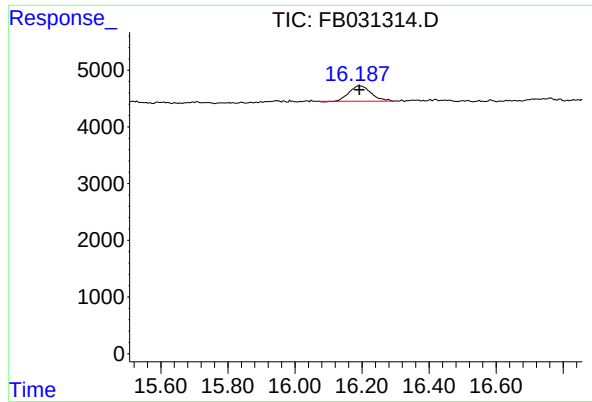

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 12416
Conc: 0.44 ng/ml

Instrument :
FID_B
ClientSampleId :