

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011725\
Data File : FB031317.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2025 11:05
Operator : YP/AJ
Sample : Q1109-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 18 01:28:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	444549	18.637 ng/ml
Target Compounds			
6) t Toluene	10.624	6849	0.175 ng/ml
8) t m-Xylene	13.194	9267	0.248 ng/ml
9) t O-Xylene	13.920	6294	0.177 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	12183	0.430 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011725\
Data File : FB031317.D
Signal(s) : FID2B.CH
Acq On : 17 Jan 2025 11:05
Operator : YP/AJ
Sample : Q1109-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jan 18 01:28:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB011525.M
Quant Title :
QLast Update : Wed Jan 15 12:01:08 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

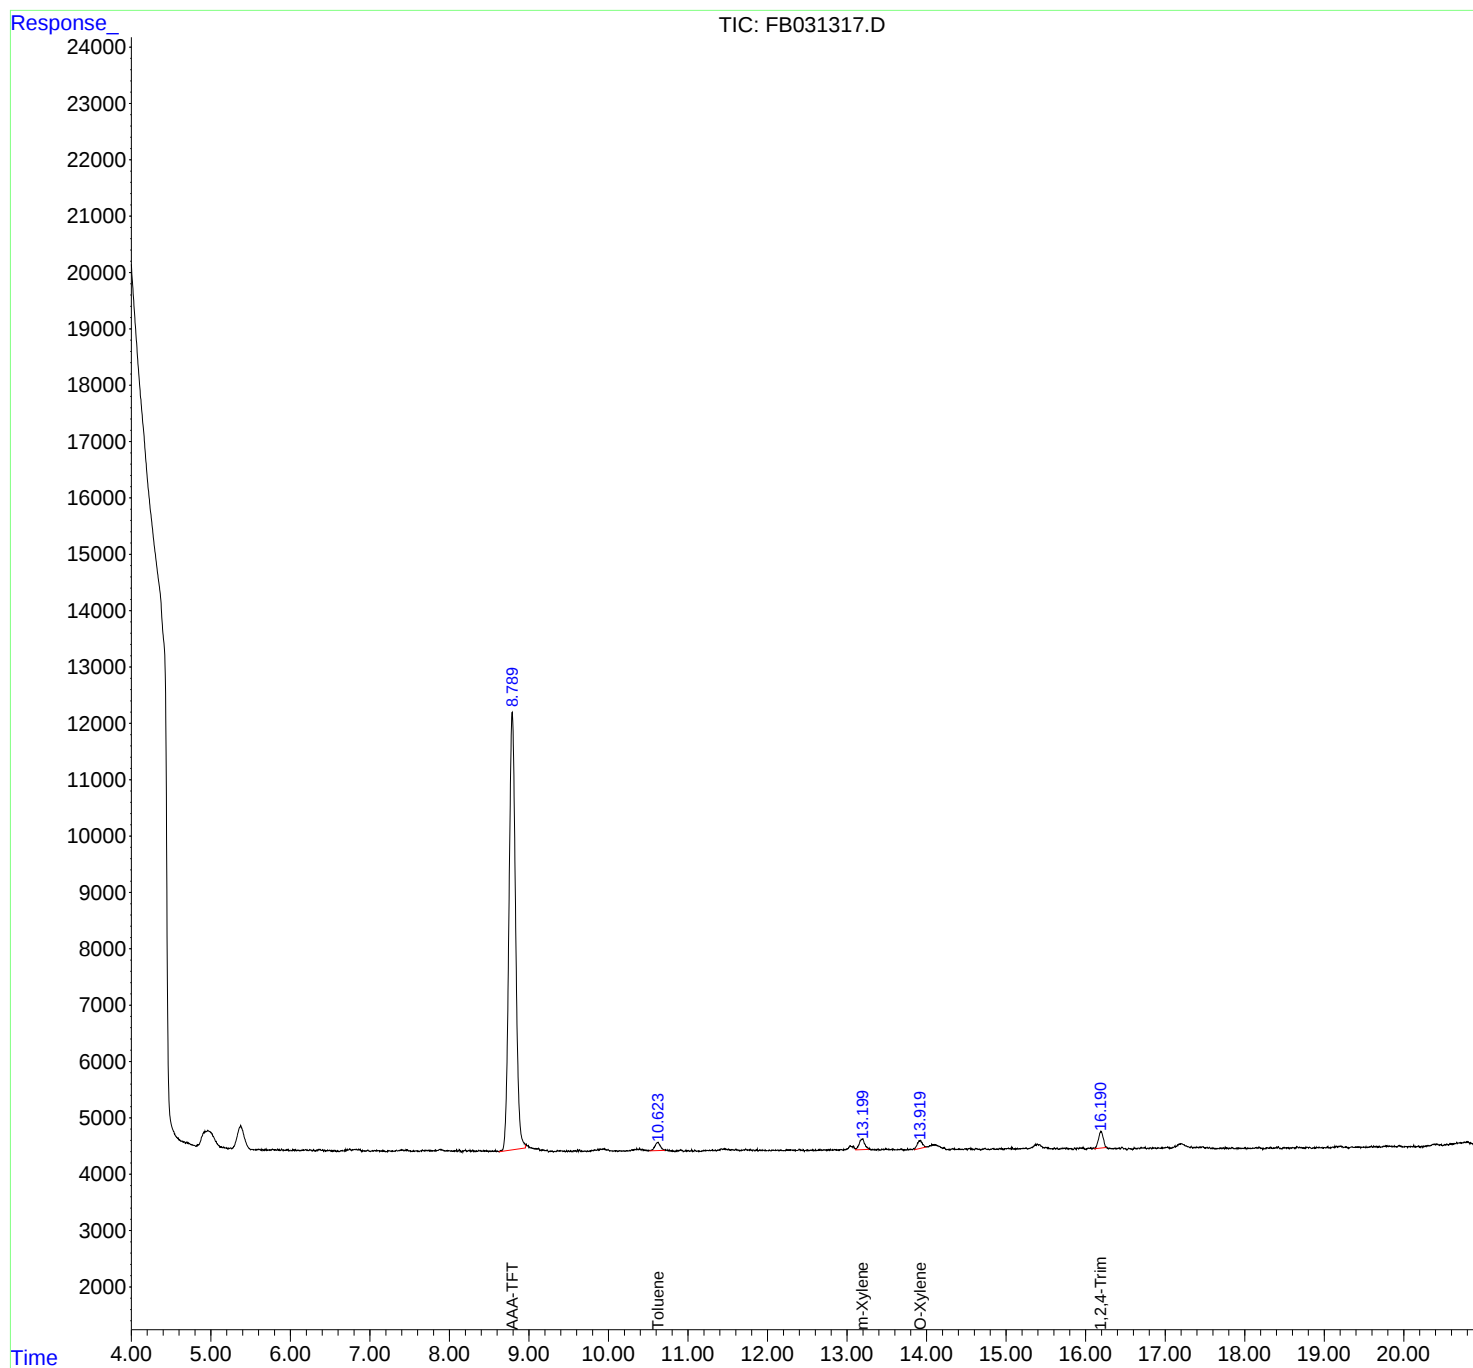


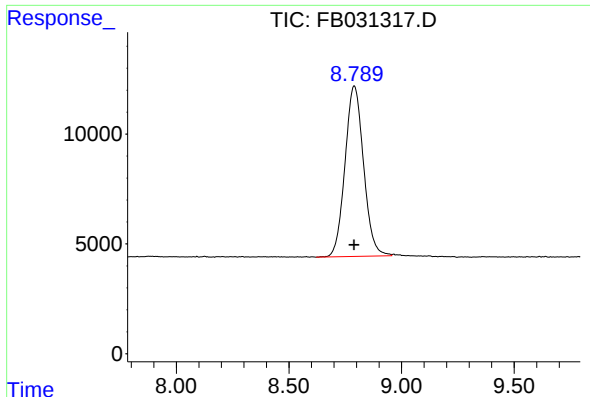

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 444549
Conc: 18.64 ng/ml

Instrument :
FID_B
ClientSampleId :

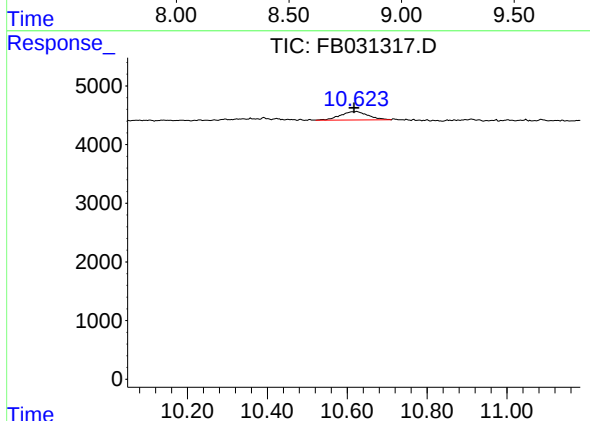


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.007 min
Response: 6849
Conc: 0.18 ng/ml

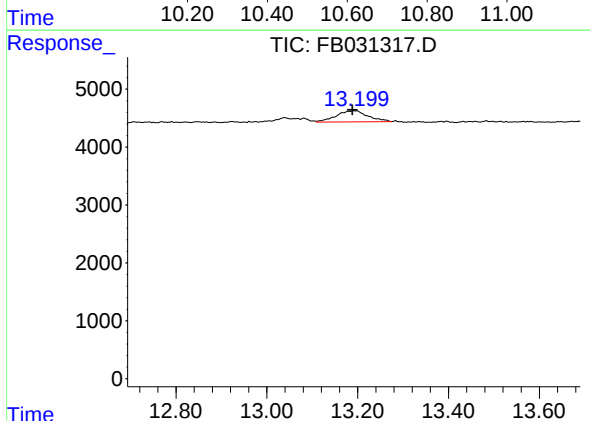


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.006 min
Response: 9267
Conc: 0.25 ng/ml

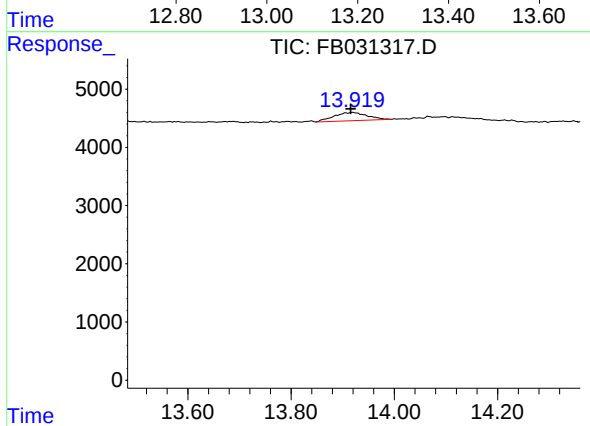

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 6294
Conc: 0.18 ng/ml

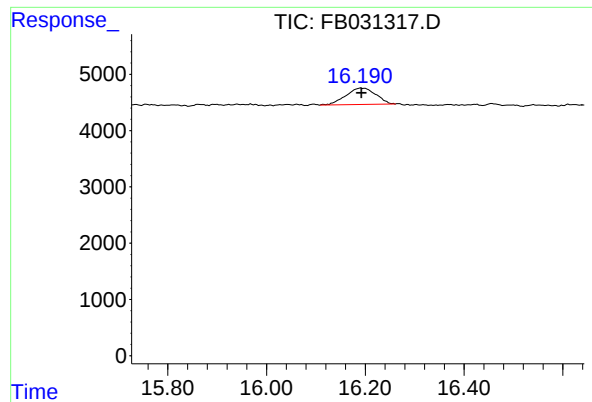

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 12183
Conc: 0.43 ng/ml

Instrument :

FID_B

ClientSampleId :