

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011819\
 Data File : FB019469.D
 Signal(s) : FID2B.CH
 Acq On : 18 Jan 2019 15:51
 Operator : MJ/SJ
 Sample : K1180-01MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jan 18 21:48:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
 Quant Title :
 QLast Update : Wed Jan 09 07:19:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.043	169678	19.095 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.897	530461	26.634 ng/ml
2) t 2,2,4-Trimethylpentane	7.658	528782	27.758 ng/ml
3) t n-Heptane	7.998	155173	8.893 ng/ml
4) t Benzene	8.135	190382	9.696 ng/ml
6) t Toluene	10.890	550959	30.458 ng/ml
7) t Ethylbenzene	13.341	222920	10.062 ng/ml
8) t m-Xylene	13.475	461980	20.131 ng/ml
9) t O-Xylene	14.206	444911	19.829 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	448948	19.689 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB011819\
Data File : FB019469.D
Signal(s) : FID2B.CH
Acq On : 18 Jan 2019 15:51
Operator : MJ/SJ
Sample : K1180-01MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jan 18 21:48:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB010819.M
Quant Title :
QLast Update : Wed Jan 09 07:19:31 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

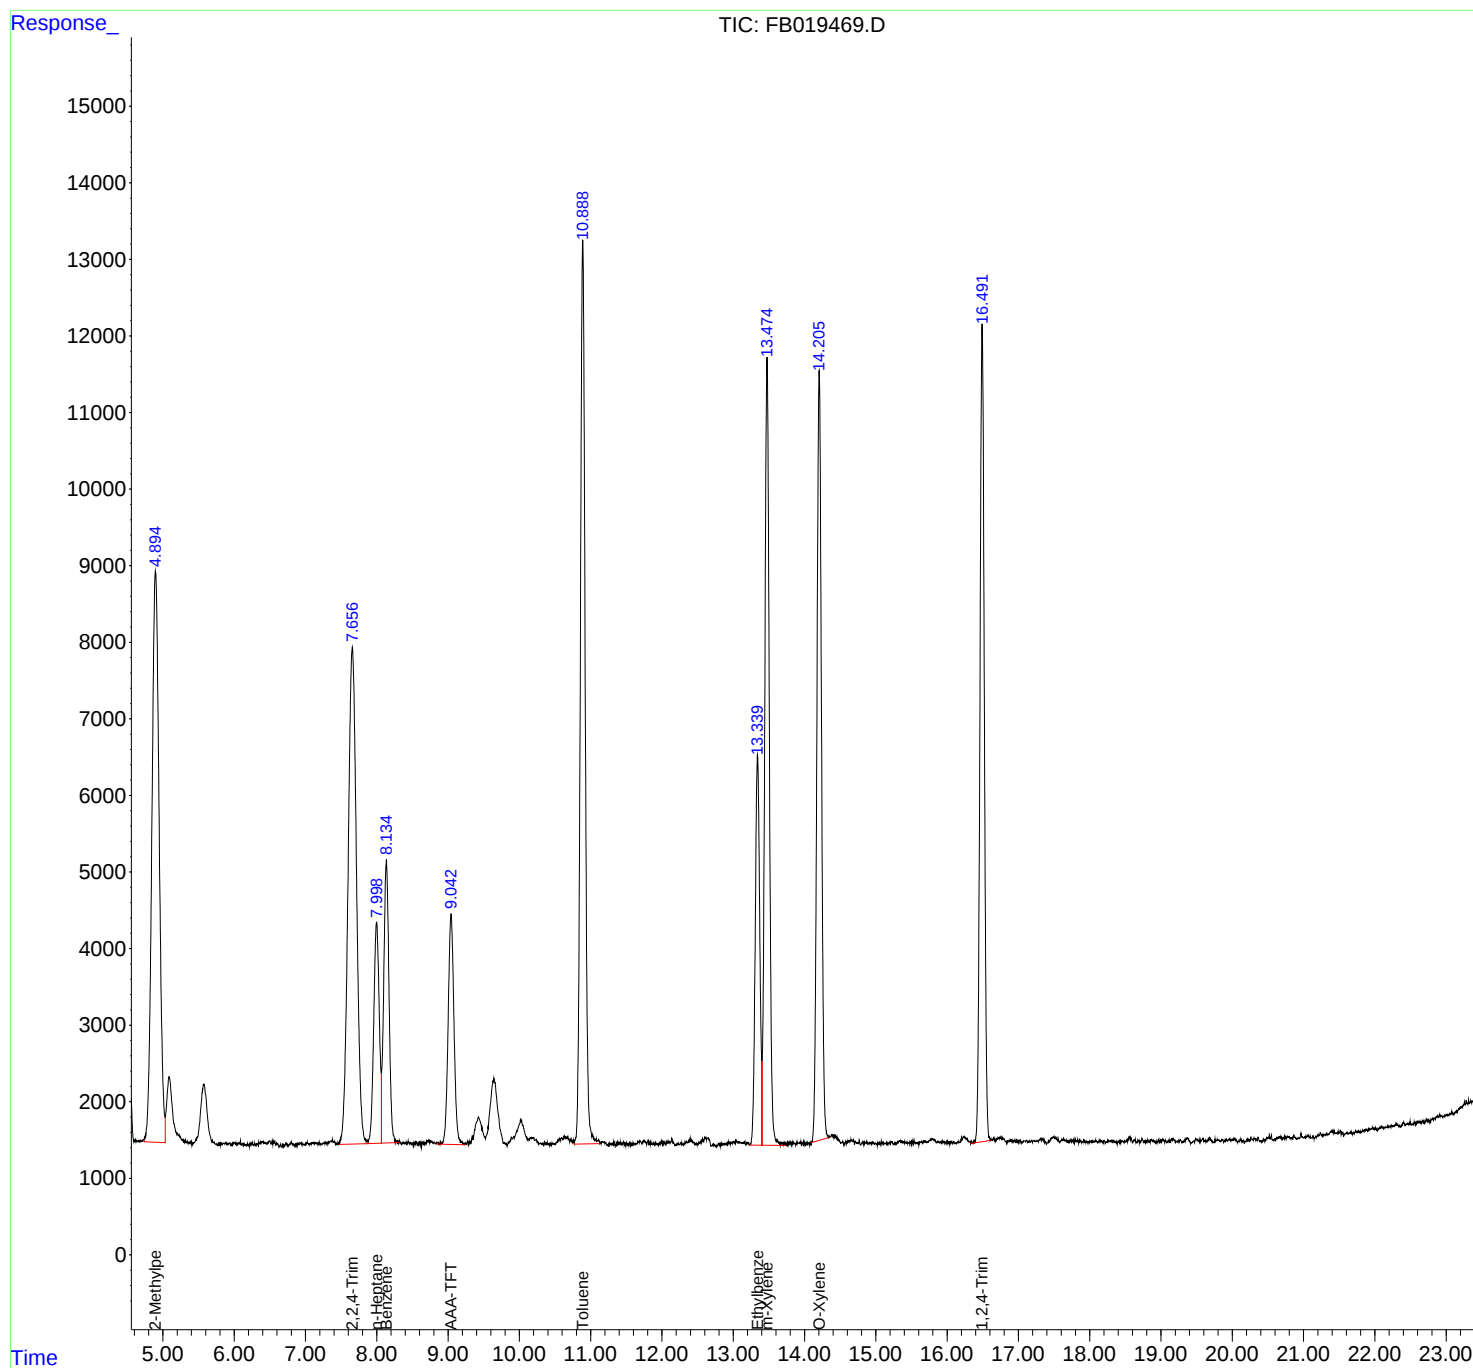

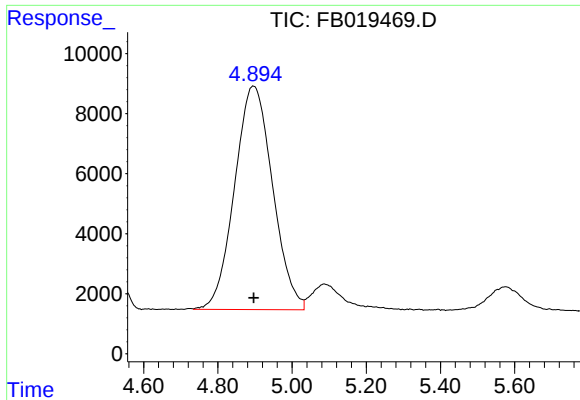


#1 2-Methylpentane

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 530461
Conc: 26.63 ng/ml

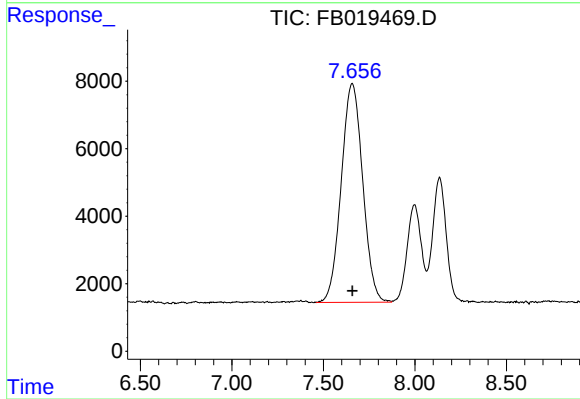


#2 2,2,4-Trimethylpentane

R.T.: 7.658 min
Delta R.T.: 0.000 min
Response: 528782
Conc: 27.76 ng/ml

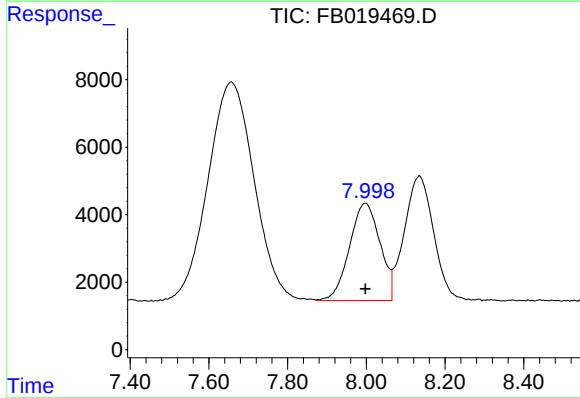


#3 n-Heptane

R.T.: 7.998 min
Delta R.T.: 0.000 min
Response: 155173
Conc: 8.89 ng/ml

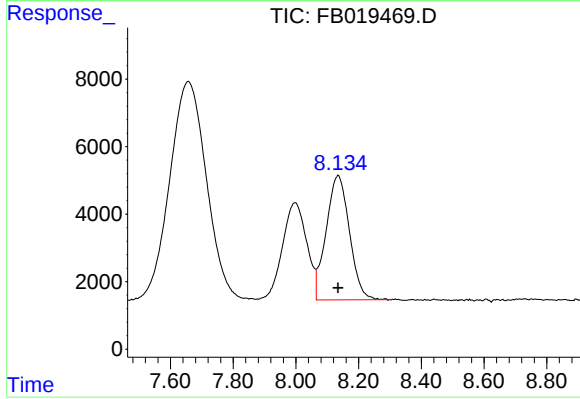


#4 Benzene

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 190382
Conc: 9.70 ng/ml

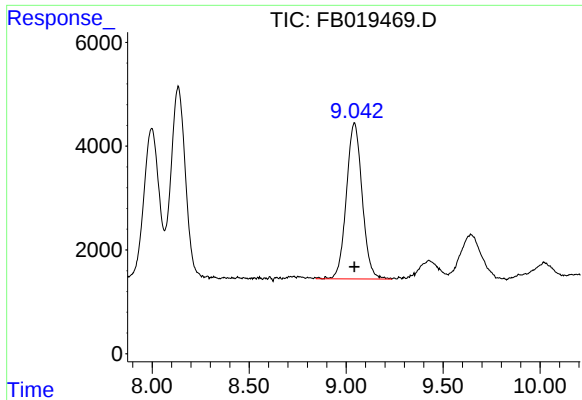


#5 AAA-TFT

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 169678
Conc: 19.10 ng/ml

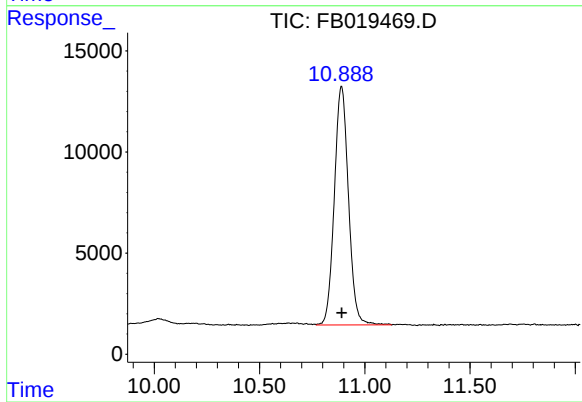


#6 Toluene

R.T.: 10.890 min
Delta R.T.: 0.000 min
Response: 550959
Conc: 30.46 ng/ml

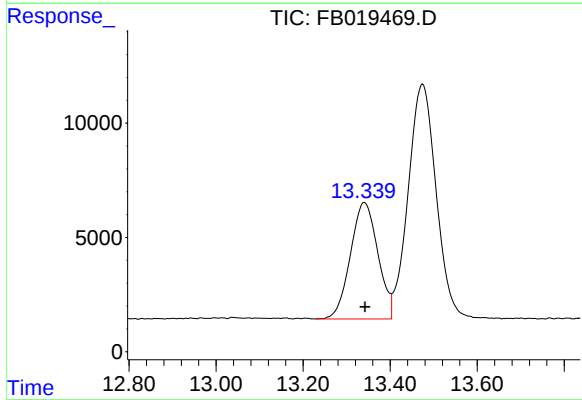


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: 0.000 min
Response: 222920
Conc: 10.06 ng/ml

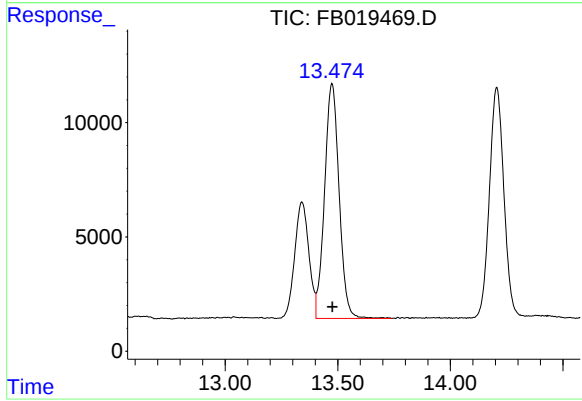

#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.000 min
Response: 461980
Conc: 20.13 ng/ml

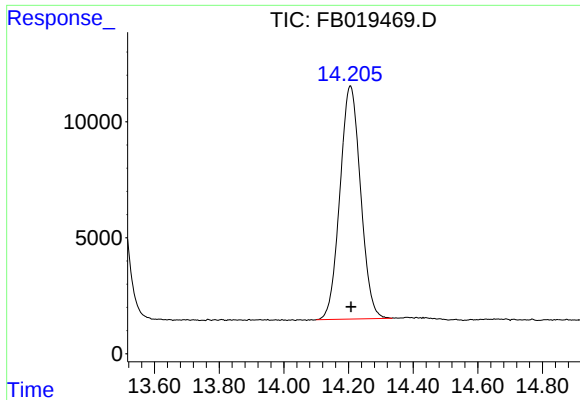


#9 O-Xylene

R.T.: 14.206 min

Delta R.T.: -0.001 min

Response: 444911

Conc: 19.83 ng/ml

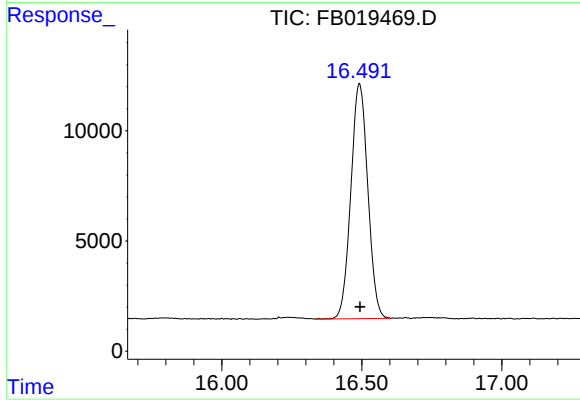

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min

Delta R.T.: -0.002 min

Response: 448948

Conc: 19.69 ng/ml